


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
 Data File : BF135199.D
 Acq On : 13 Sep 2023 01:17
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 12 00:19:07 2023

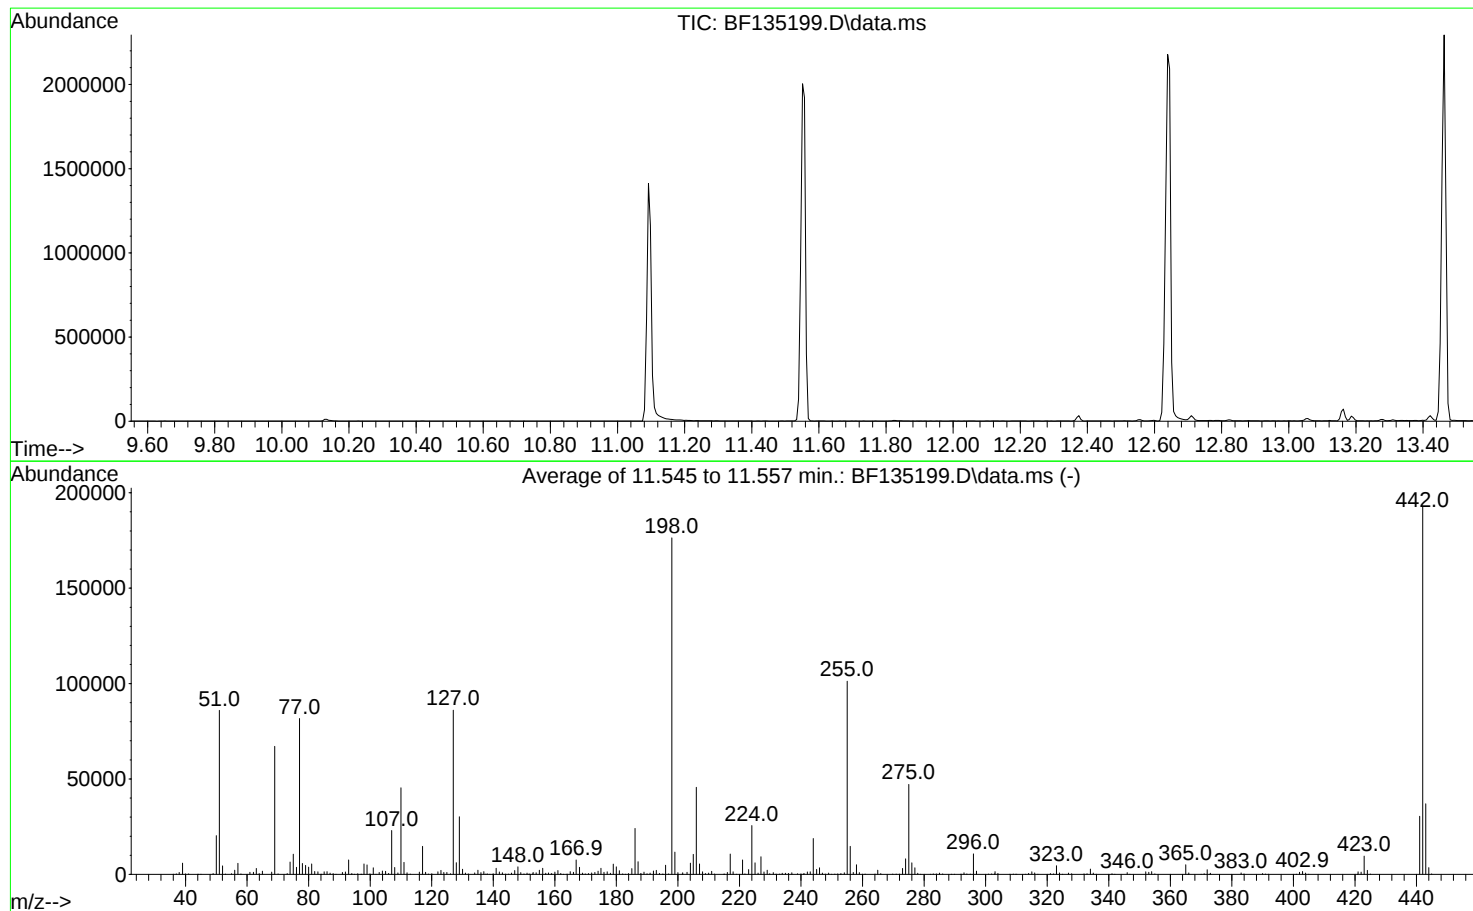




AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.7	85936	PASS
68	69	0.00	2	1.8	1198	PASS
69	198	0.00	100	38.0	67061	PASS
70	69	0.00	2	0.4	283	PASS
127	198	10	80	48.8	86008	PASS
197	198	0.00	2	0.2	285	PASS
198	198	100	100	100.0	176357	PASS
199	198	5	9	6.6	11676	PASS
275	198	10	60	26.7	47155	PASS
365	198	1	100	2.9	5073	PASS
441	198	0.01	100	17.3	30430	PASS
442	442	50	100	100.0	192813	PASS
443	442	15	24	19.2	36953	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF0911223\
Data File : BF135199.D
Acq On : 13 Sep 2023 01:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 13 05:59:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

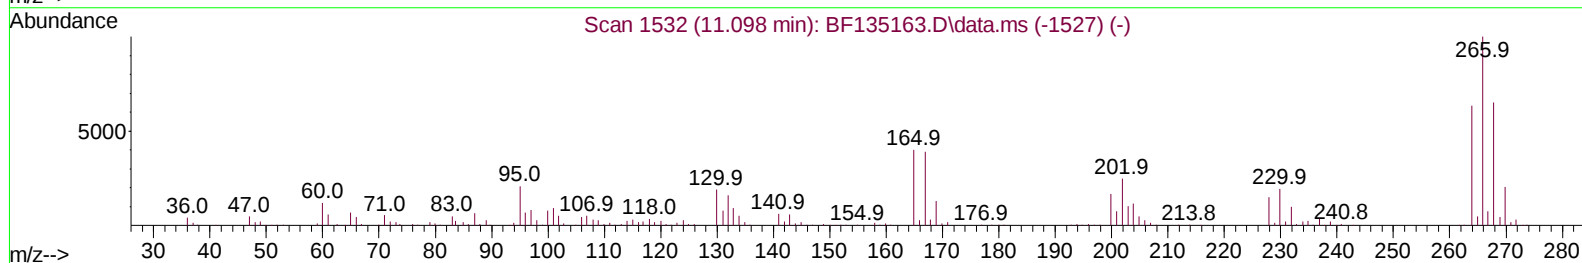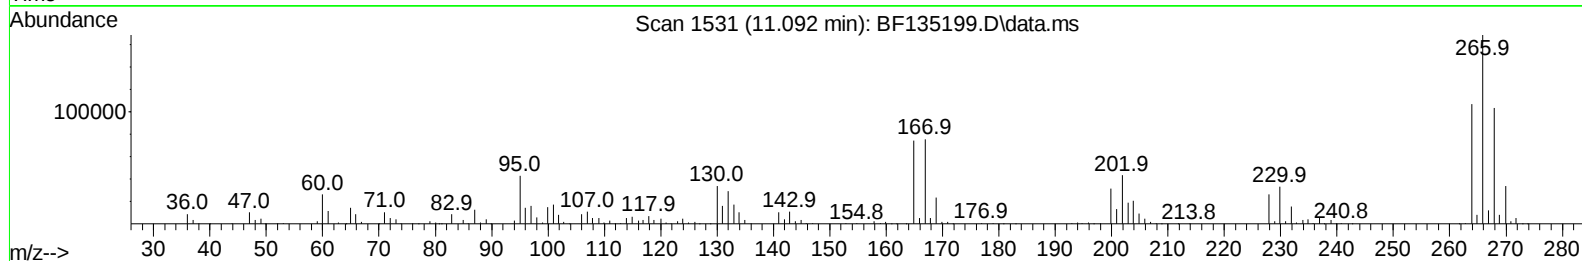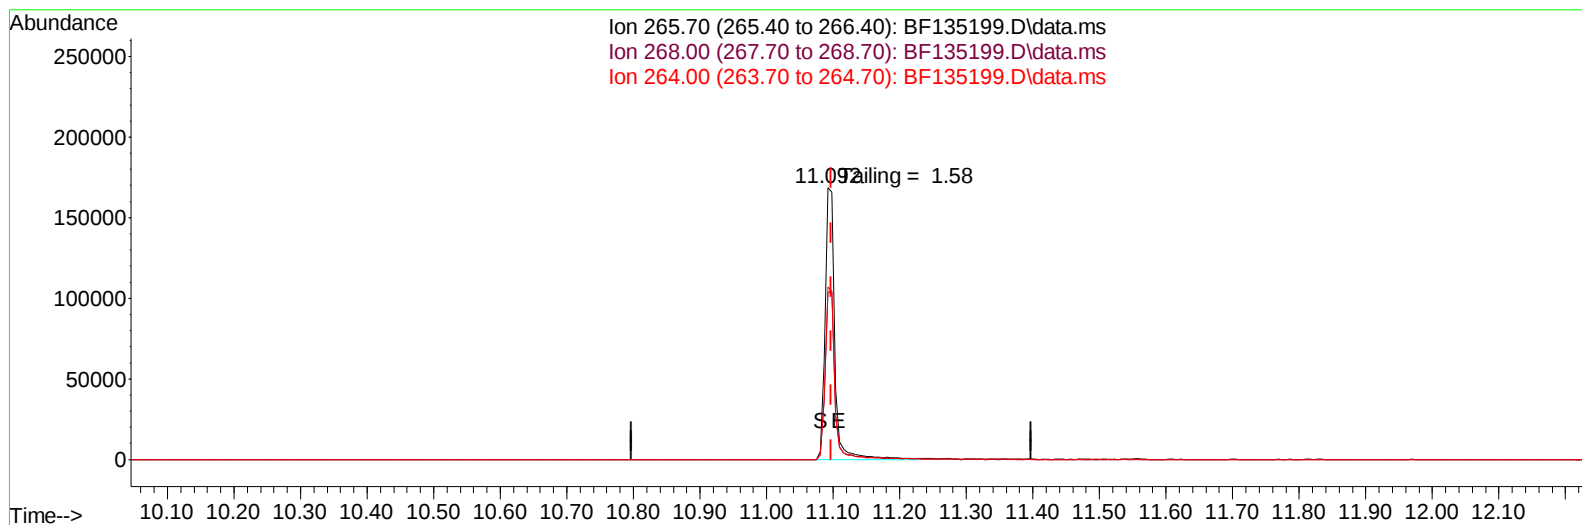

TIC: BF135199.D\data.ms

(70) Pentachlorophenol (C)

11.092min (-0.006) 37200.08 ng




response 173421

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	61.46
264.00	63.50	63.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091223\
 Data File : BF135199.D
 Acq On : 13 Sep 2023 01:17
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 13 05:59:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 12 00:19:07 2023
 Response via : Initial Calibration

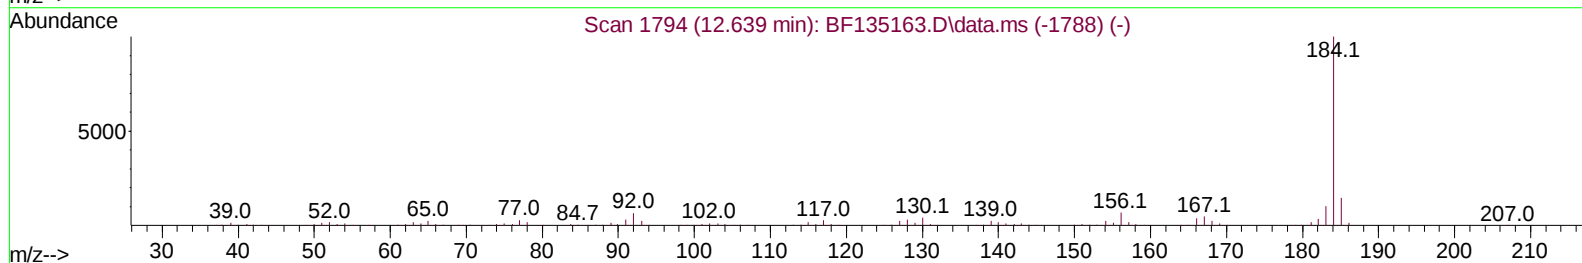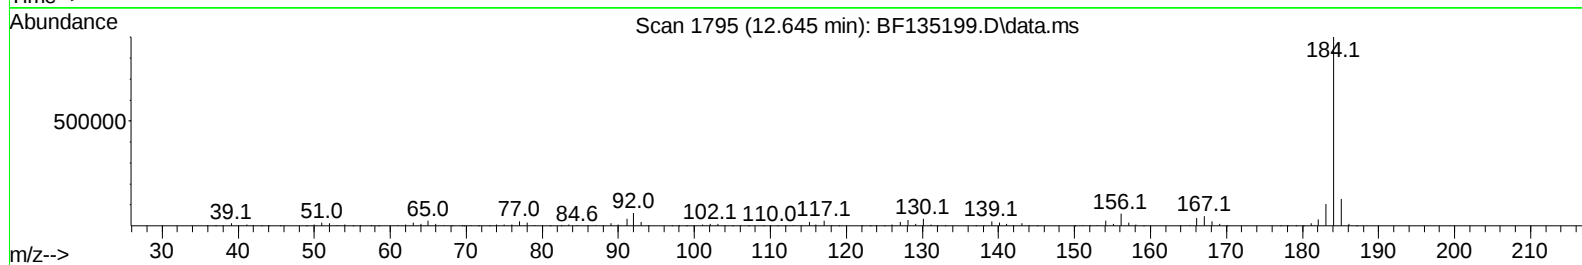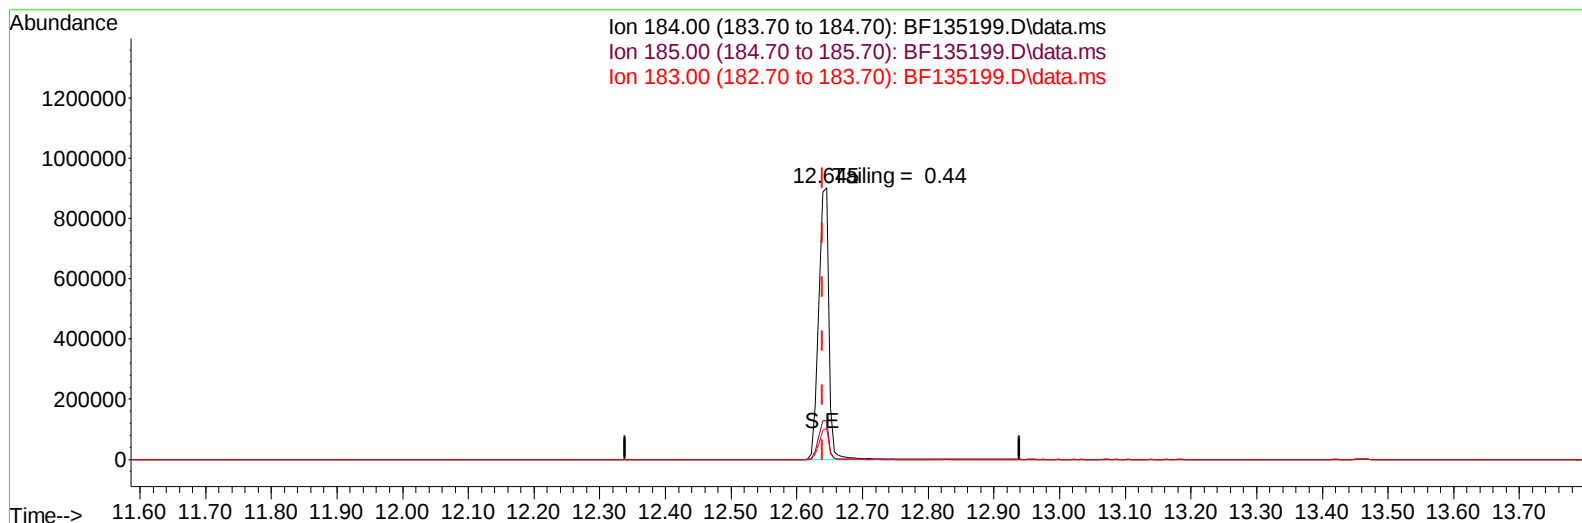

TIC: BF135199.D\data.ms

(77) Benzidine

12.645min (+ 0.006) 0.00 ng

response 982241

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.23
183.00	10.30	11.40
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/12/2023	BNA_F	<u>BF135199.D</u>
Compound Name	Response	Retention Time
DDT	406184	13.463
DDD	17257	13.163
DDE	991	12.822
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18248	424432	4.30

Instrument :
BNA_F
ClientSampleId :
DFTPP