


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091318\
 Data File : BF108962.D
 Acq On : 13 Sep 2018 13:15
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF090518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 05 18:03:31 2018

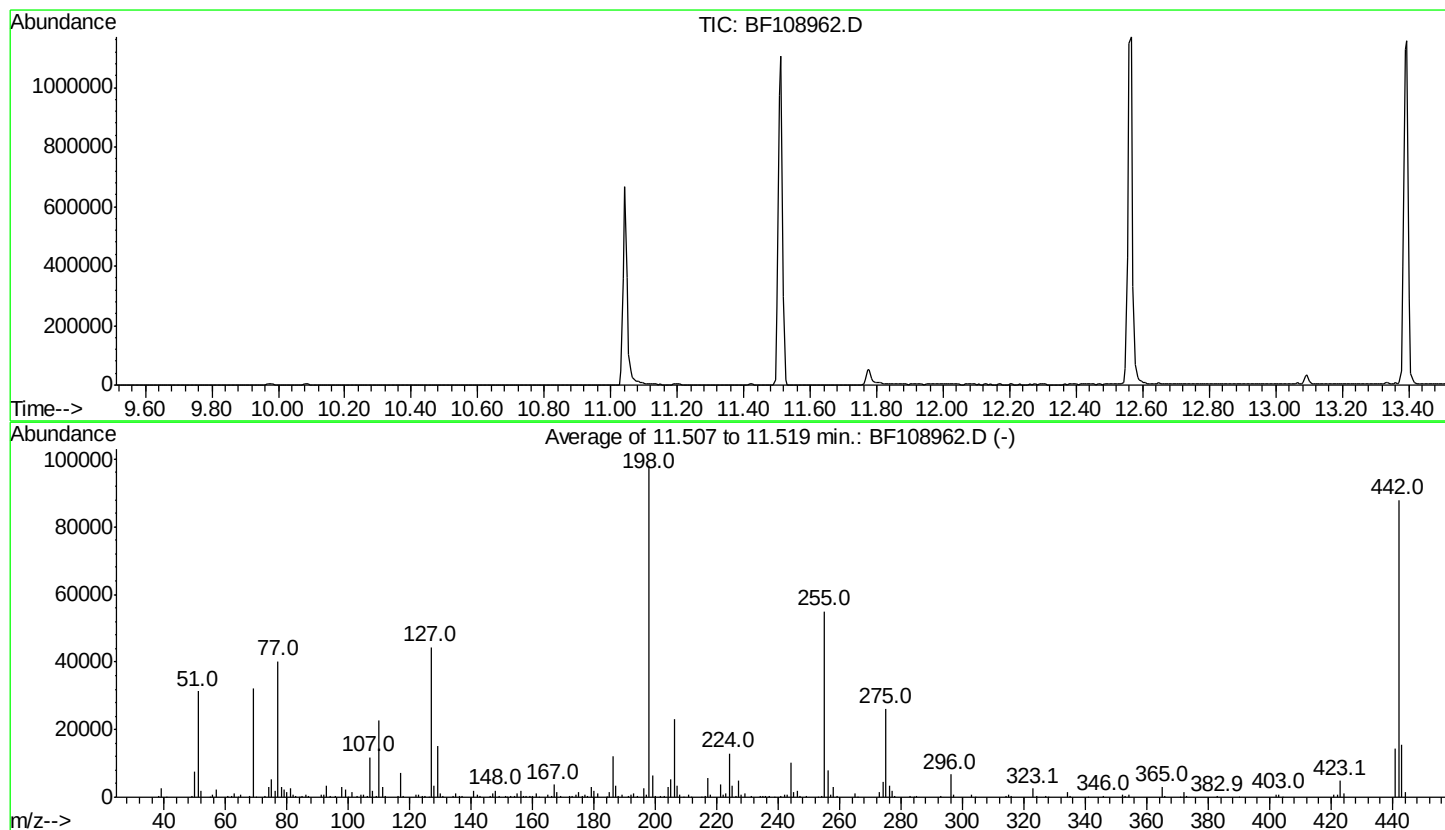

AutoFind: Scans 1559, 1560, 1561; Background Corrected with Scan 1554

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.9	31329	PASS
68	69	0.00	2	1.6	513	PASS
69	198	0.00	100	32.9	32279	PASS
70	69	0.00	2	0.3	100	PASS
127	198	10	80	45.2	44346	PASS
197	198	0.00	2	0.6	617	PASS
198	198	100	100	100.0	98072	PASS
199	198	5	9	6.5	6386	PASS
275	198	10	60	26.7	26181	PASS
365	198	1	100	3.3	3200	PASS
441	198	0.01	100	14.6	14291	PASS
442	198	50	100	89.7	87936	PASS
443	442	15	24	17.8	15689	PASS