
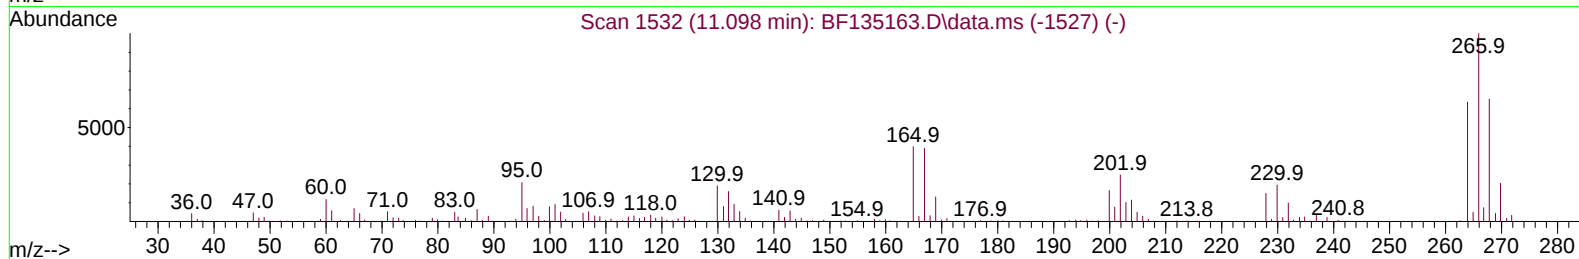
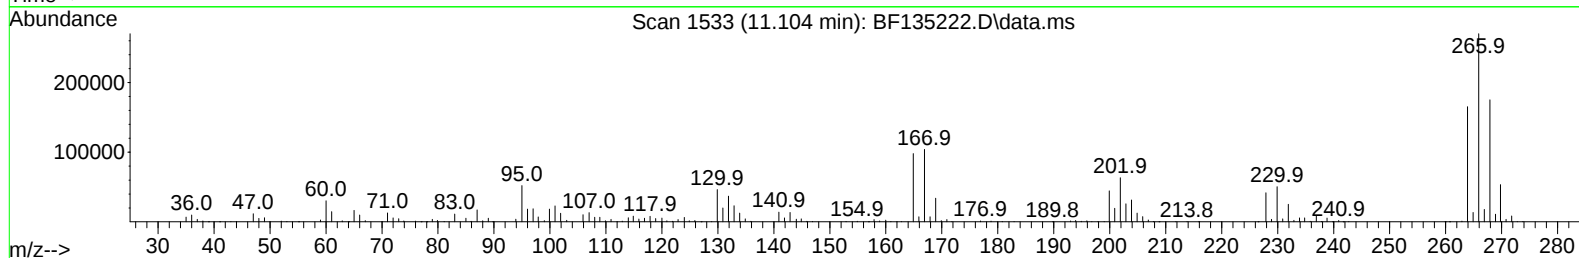


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091323\
Data File : BF135222.D
Acq On : 13 Sep 2023 14:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 03:02:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

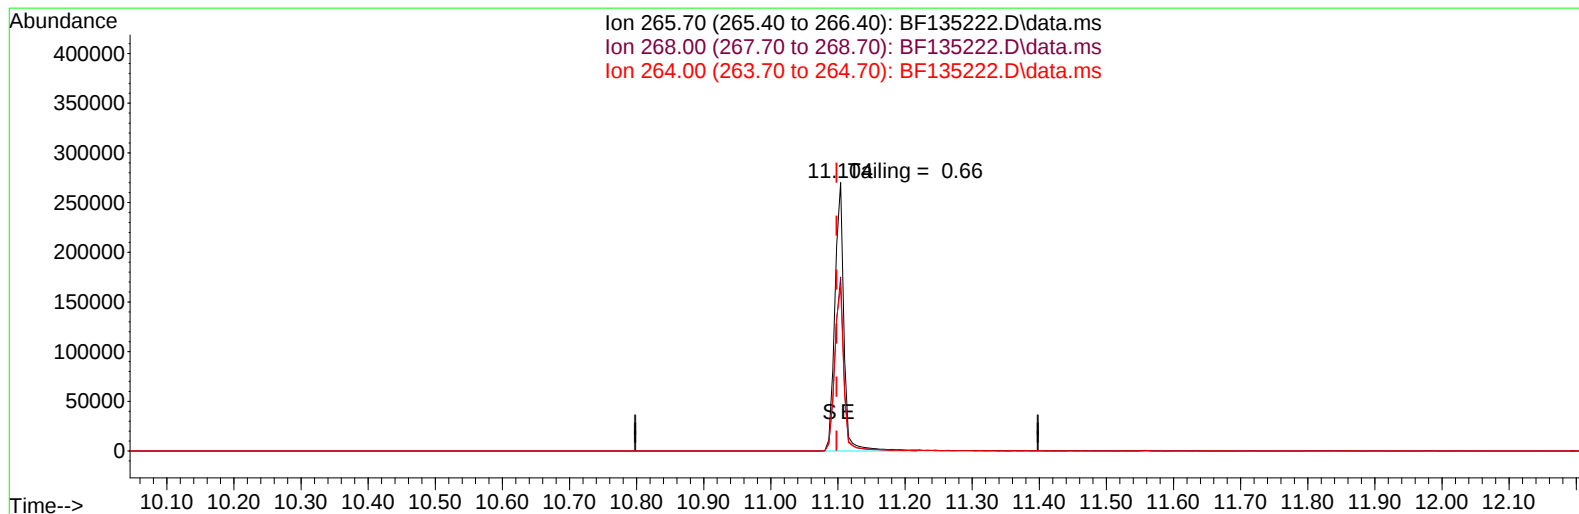

TIC: BF135222.D\data.ms

(70) Pentachlorophenol (C)




11.104min (+ 0.006) 401049.63 ng

response 252850

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	64.83
264.00	63.50	61.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091323\
Data File : BF135222.D
Acq On : 13 Sep 2023 14:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 03:02:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

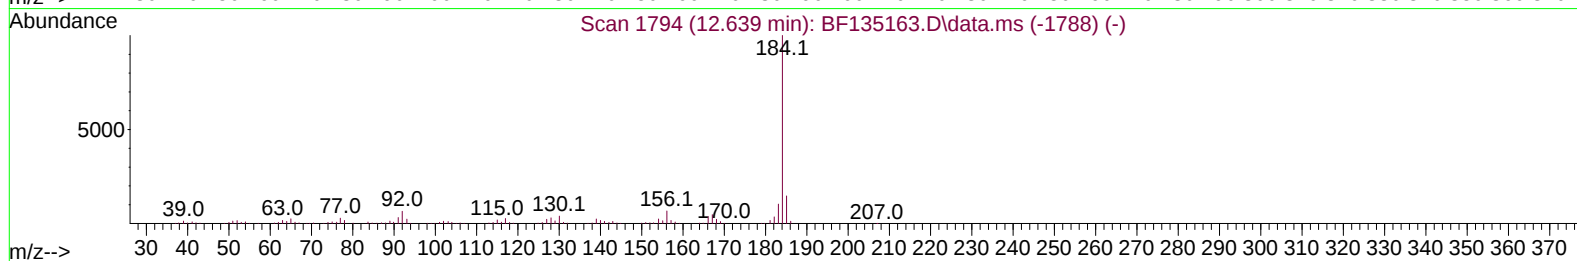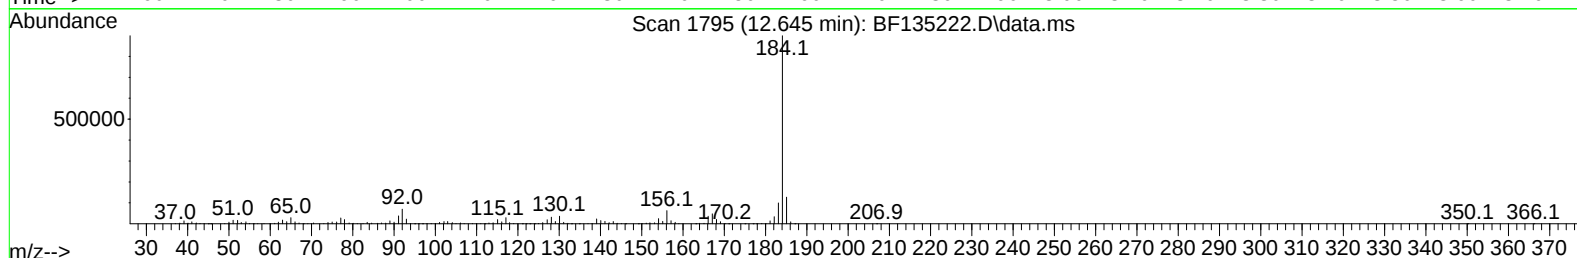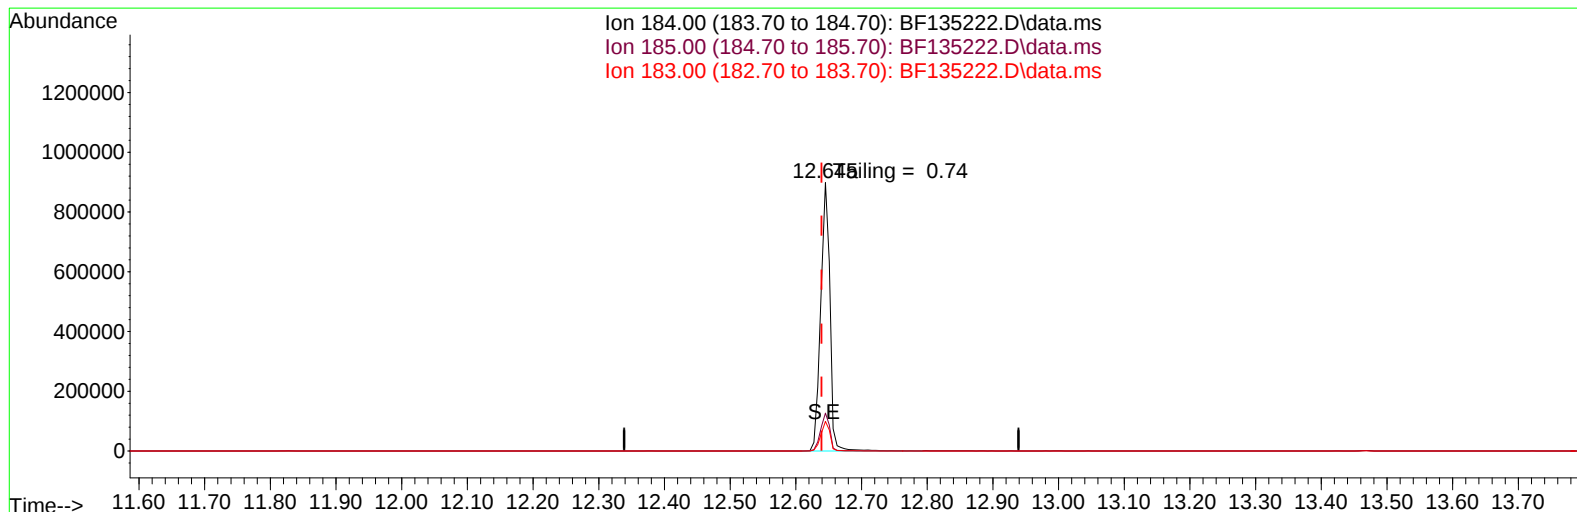

TIC: BF135222.D\data.ms

(77) Benzidine

12.645min (+ 0.006) 171275.13 ng

response 884239

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.16
183.00	10.30	11.04
0.00	0.00	0.00