
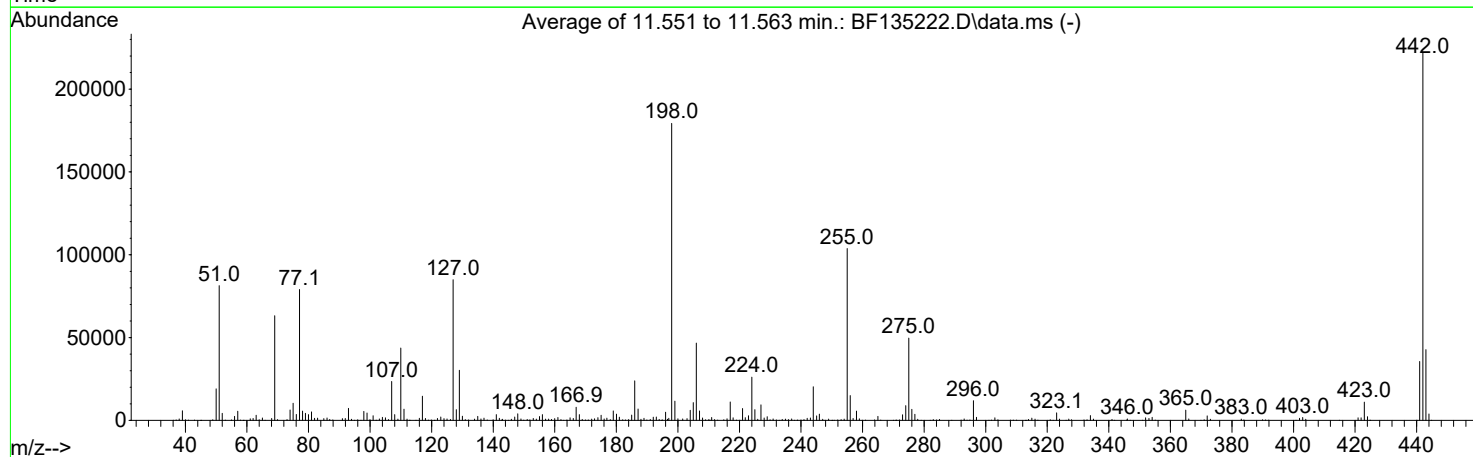


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF091323\  
Data File : BF135222.D  
Acq On : 13 Sep 2023 14:45  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF091123.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Tue Sep 12 00:19:07 2023

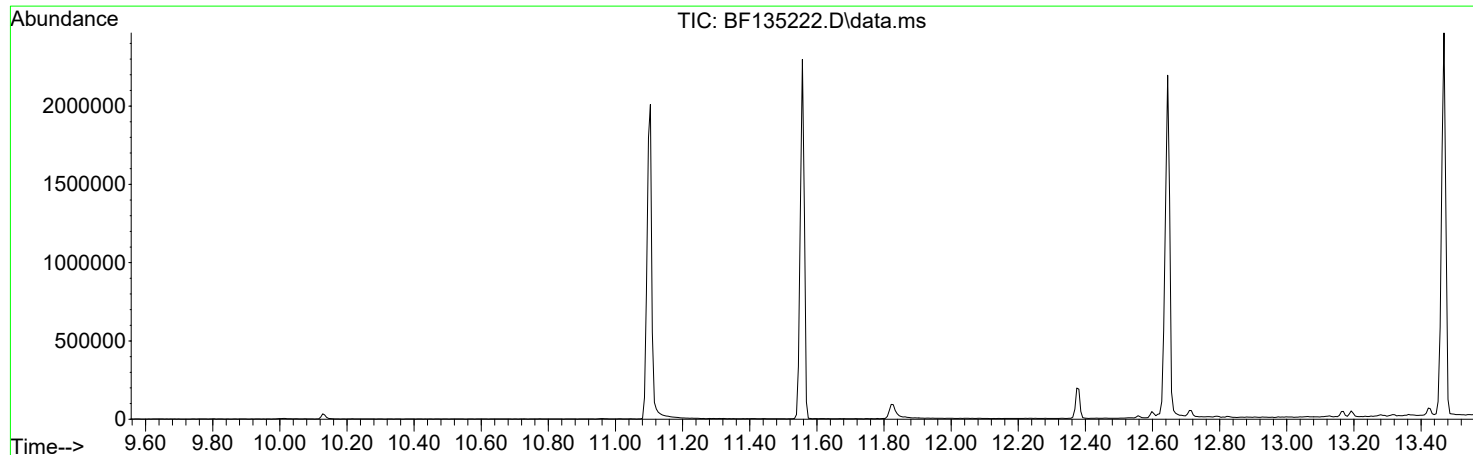




AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1604

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 45.4         | 81338      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.9          | 1179       | PASS                |
| 69             | 198             | 0.00            | 100             | 35.2         | 63147      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.7          | 440        | PASS                |
| 127            | 198             | 10              | 80              | 47.4         | 84944      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.7          | 1229       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 179344     | PASS                |
| 199            | 198             | 5               | 9               | 6.5          | 11568      | PASS                |
| 275            | 198             | 10              | 60              | 27.7         | 49712      | PASS                |
| 365            | 198             | 1               | 100             | 3.4          | 6170       | PASS                |
| 441            | 198             | 0.01            | 100             | 19.8         | 35587      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 222128     | PASS                |
| 443            | 442             | 15              | 24              | 19.2         | 42669      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF091323\  
Data File : BF135222.D  
Acq On : 13 Sep 2023 14:45  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Sep 14 03:02:09 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF091123.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Sep 12 00:19:07 2023  
Response via : Initial Calibration

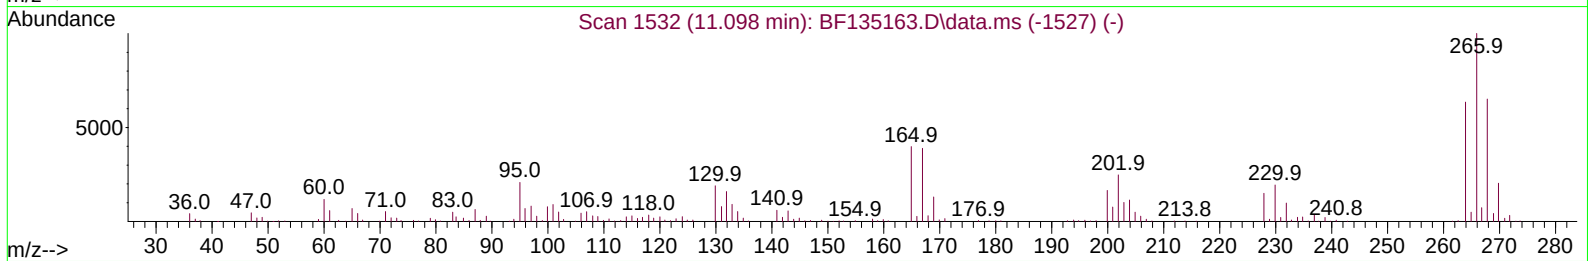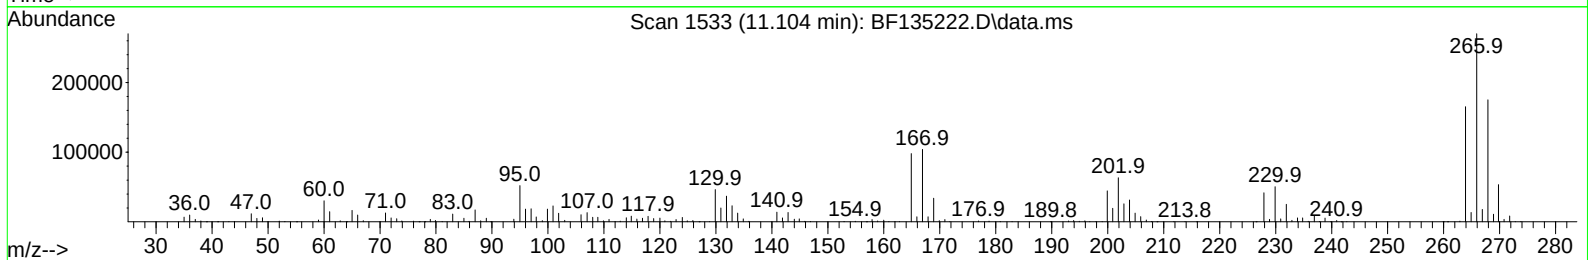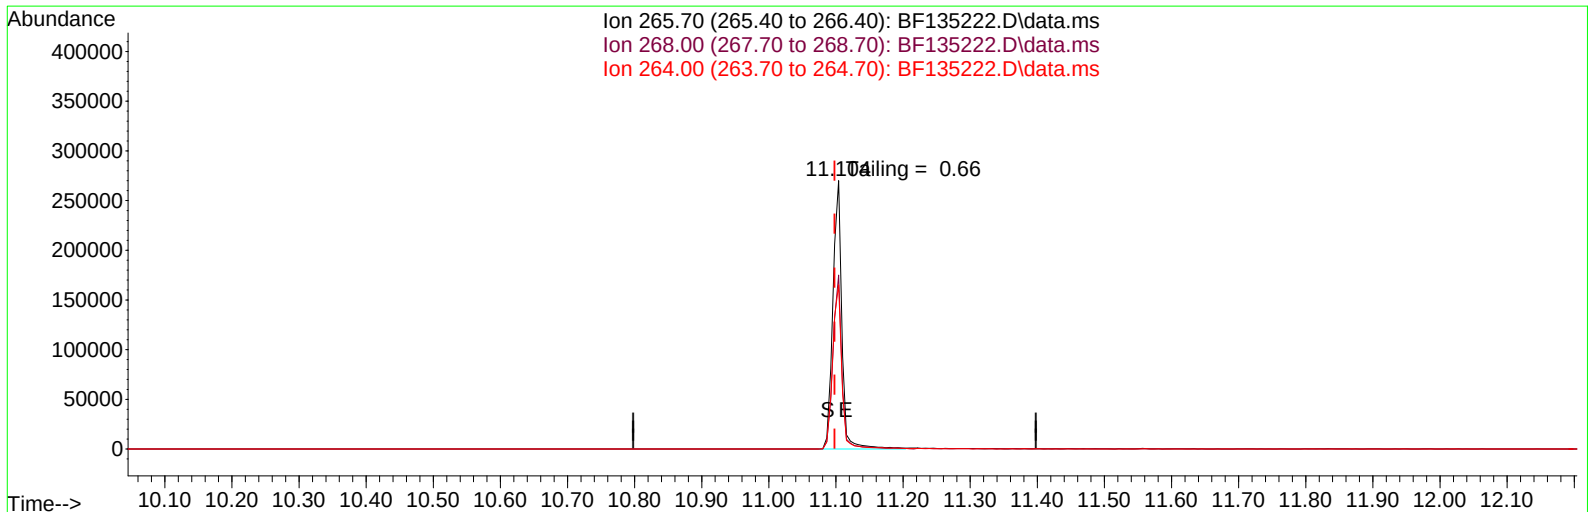

TIC: BF135222.D\data.ms

**(70) Pentachlorophenol (C)**

**11.104min (+ 0.006) 401049.63 ng**




**response 252850**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.10  | 64.83  |
| 264.00 | 63.50  | 61.18  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF091323\  
Data File : BF135222.D  
Acq On : 13 Sep 2023 14:45  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Sep 14 03:02:09 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF091123.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Sep 12 00:19:07 2023  
Response via : Initial Calibration

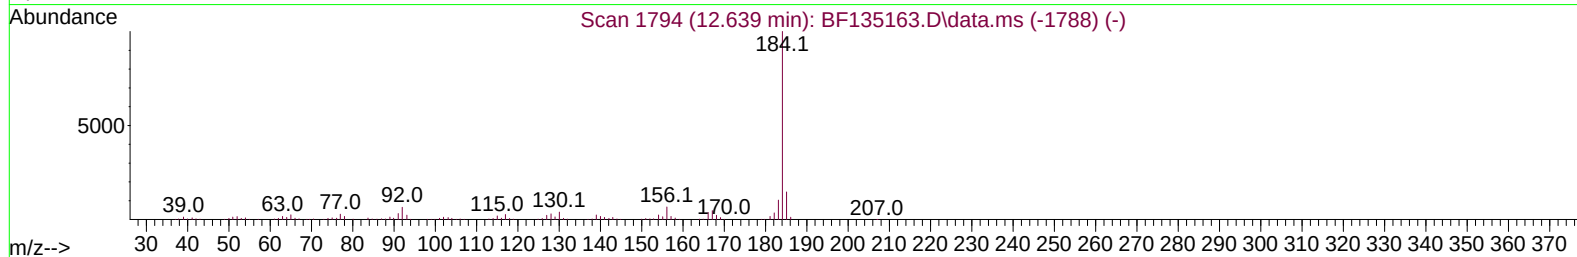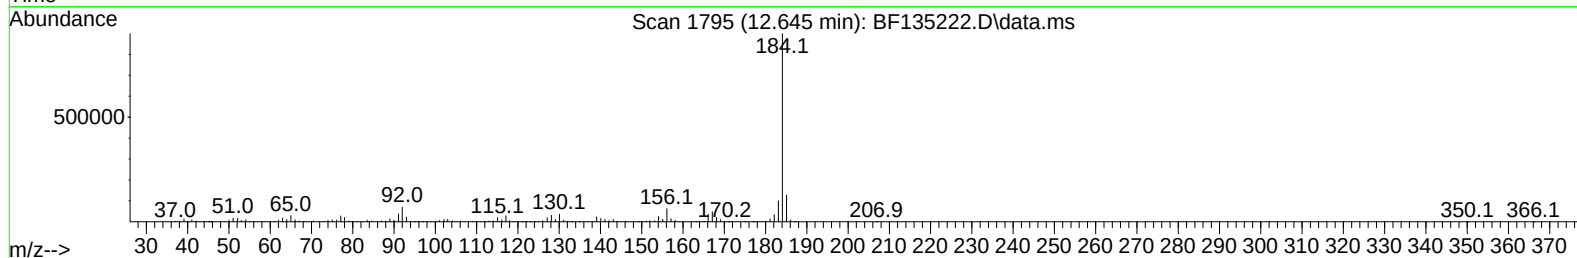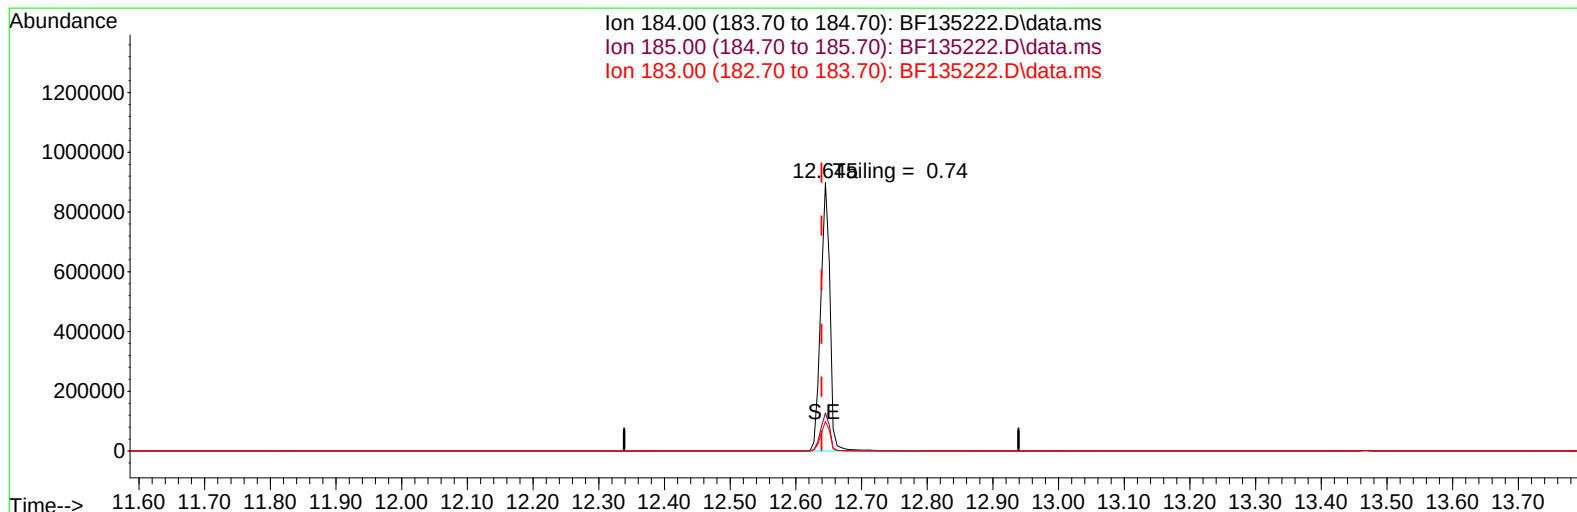

TIC: BF135222.D\data.ms

**(77) Benzidine**

**12.645min (+ 0.006) 171275.13 ng**

**response 884239**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.60  | 14.16  |
| 183.00 | 10.30  | 11.04  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 9/13/2023     | BNA_F            | <u>BF135222.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 425804           | 13.469             |
| DDD           | 11534            | 13.169             |
| DDE           | 521              | 12.827             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 12055         | 437859           | 2.75               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP