
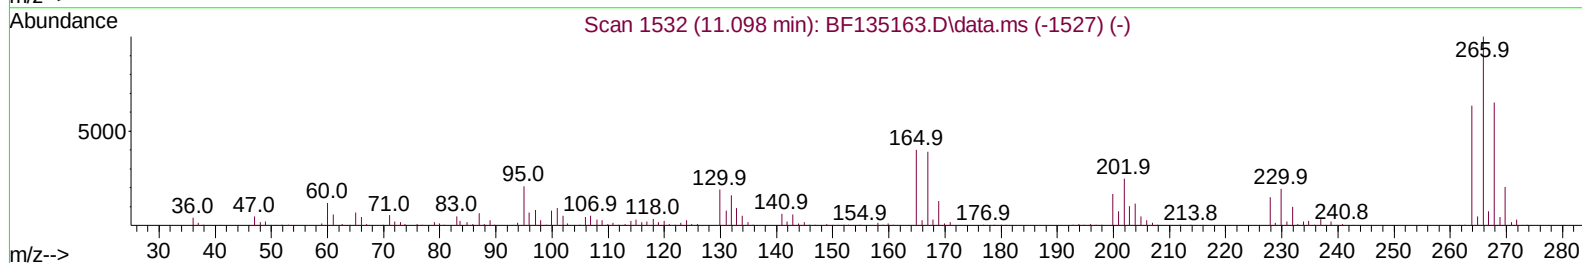
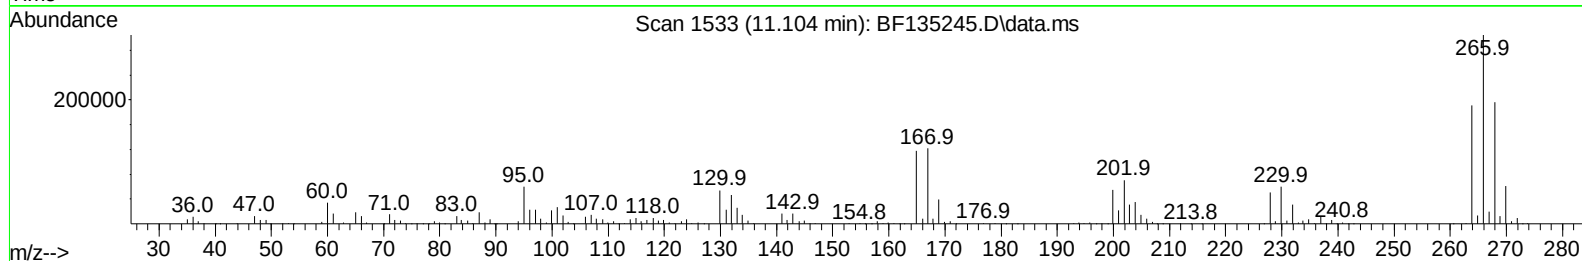


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091423\
Data File : BF135245.D
Acq On : 14 Sep 2023 10:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 15 05:18:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

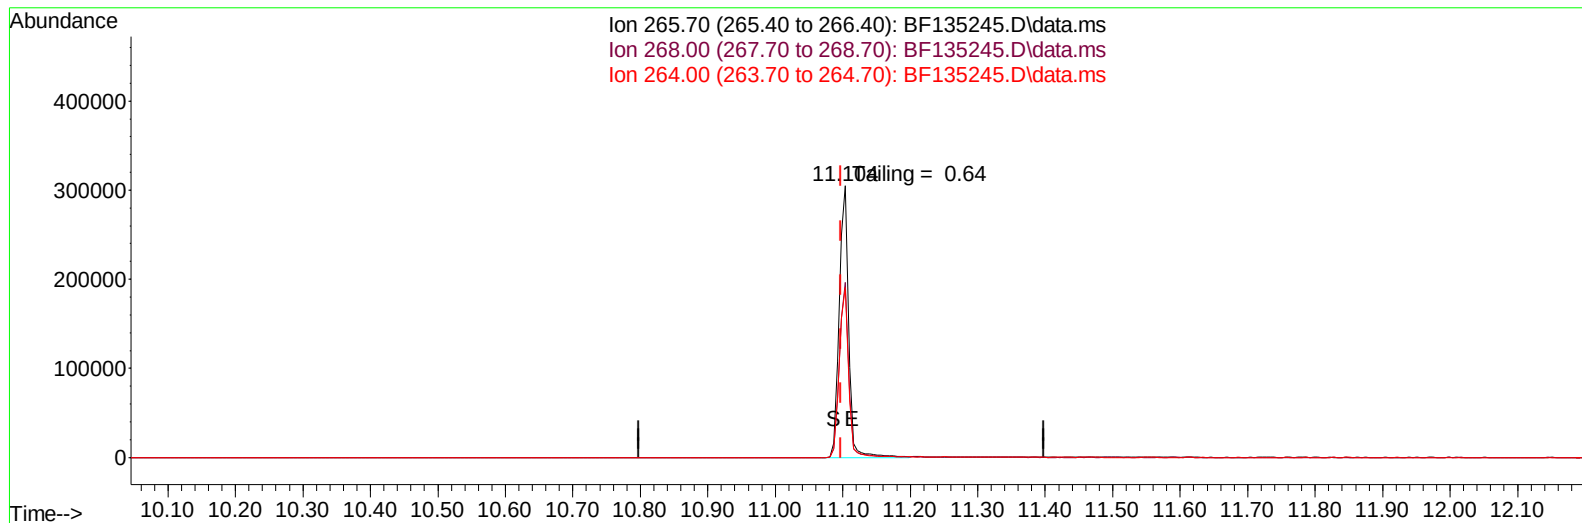




TIC: BF135245.D\data.ms

(70) Pentachlorophenol (C)**11.104min (+ 0.006) 685985.23 ng****response 295260**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	64.52
264.00	63.50	62.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091423\
Data File : BF135245.D
Acq On : 14 Sep 2023 10:25
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 15 05:18:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

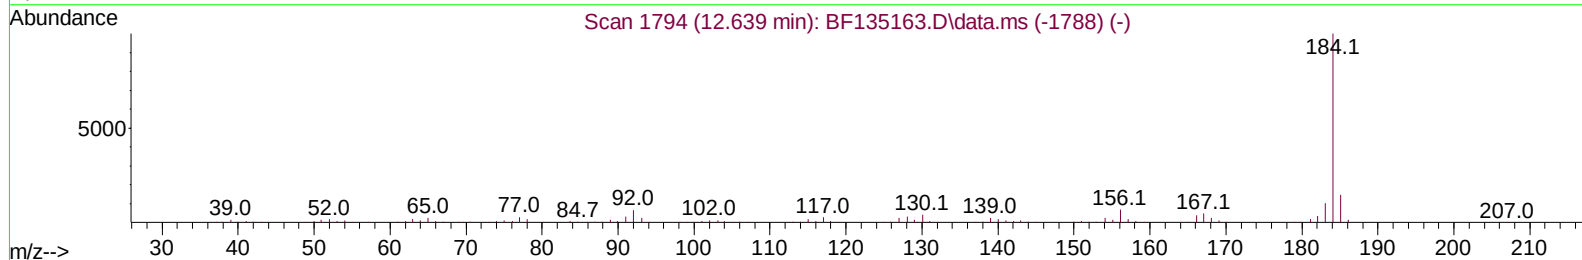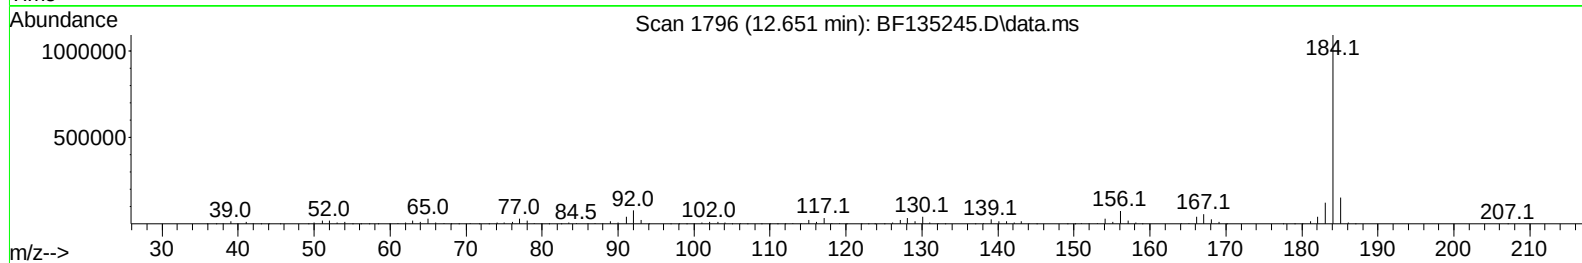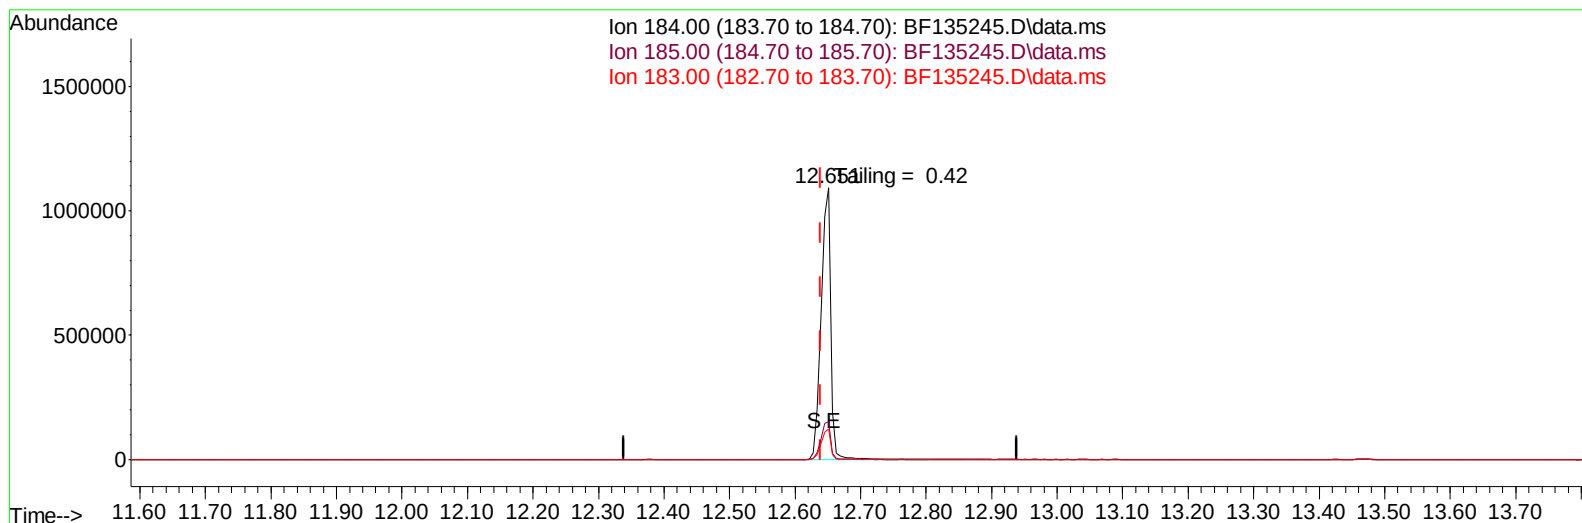

TIC: BF135245.D\data.ms

(77) Benzidine

12.651min (+ 0.012) 167154.35 ng

response 1116375

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.86
183.00	10.30	11.27
0.00	0.00	0.00