
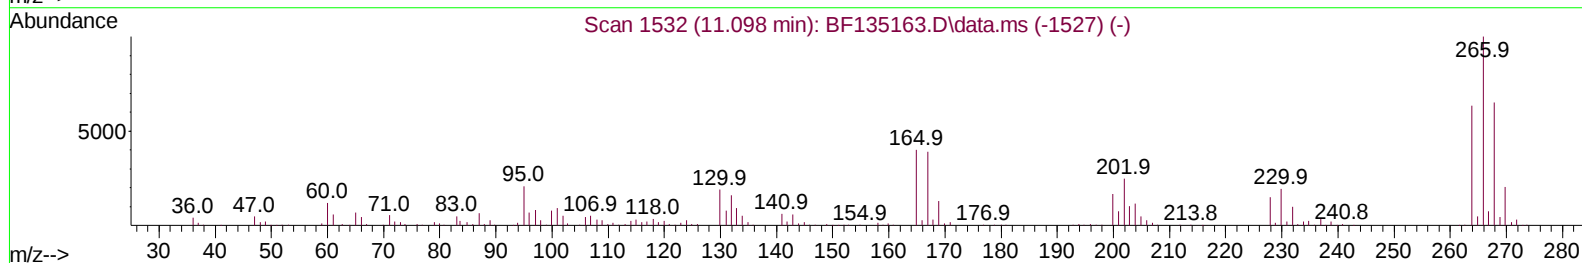
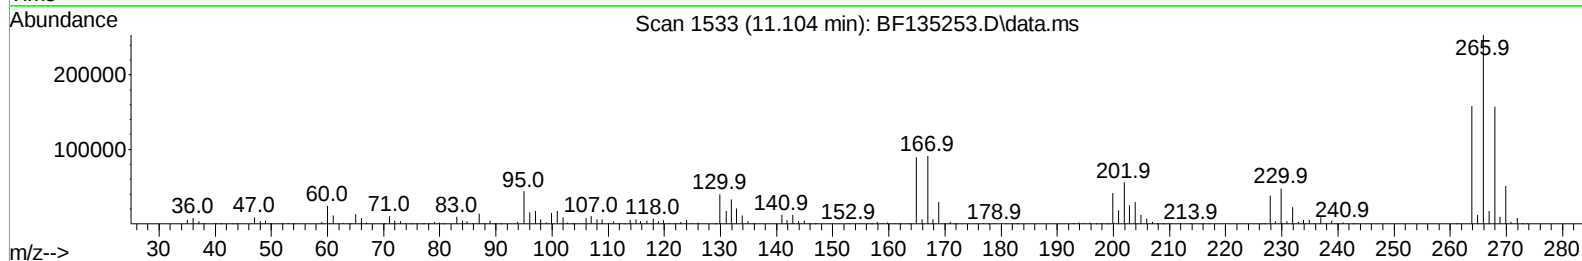


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091423\
Data File : BF135253.D
Acq On : 14 Sep 2023 14:37
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 15 05:23:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

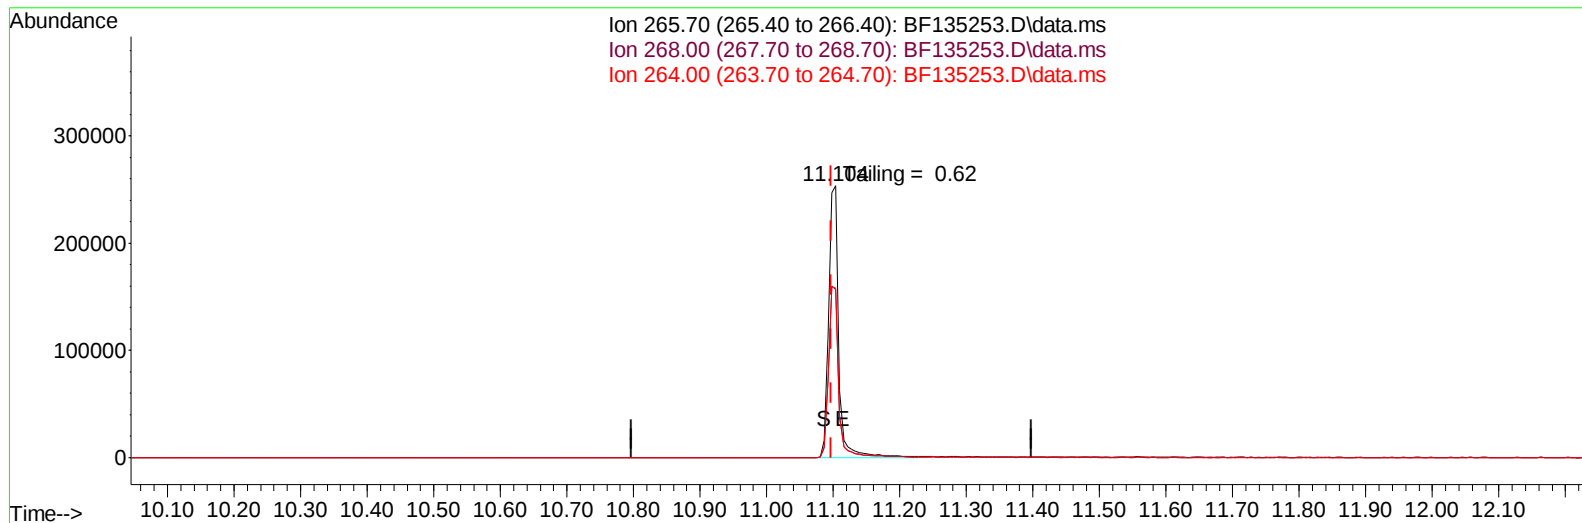

TIC: BF135253.D\data.ms

(70) Pentachlorophenol (C)




11.104min (+ 0.006) 255226.03 ng

response 269219

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	61.92
264.00	63.50	62.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091423\
Data File : BF135253.D
Acq On : 14 Sep 2023 14:37
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 15 05:23:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

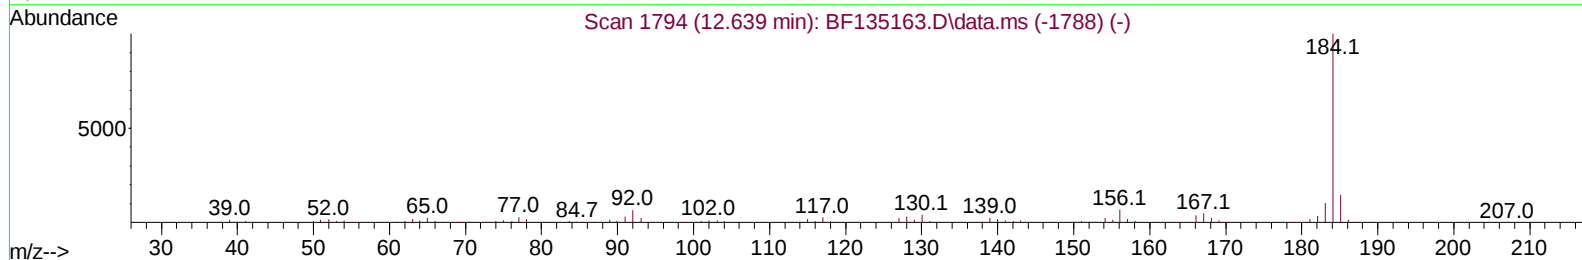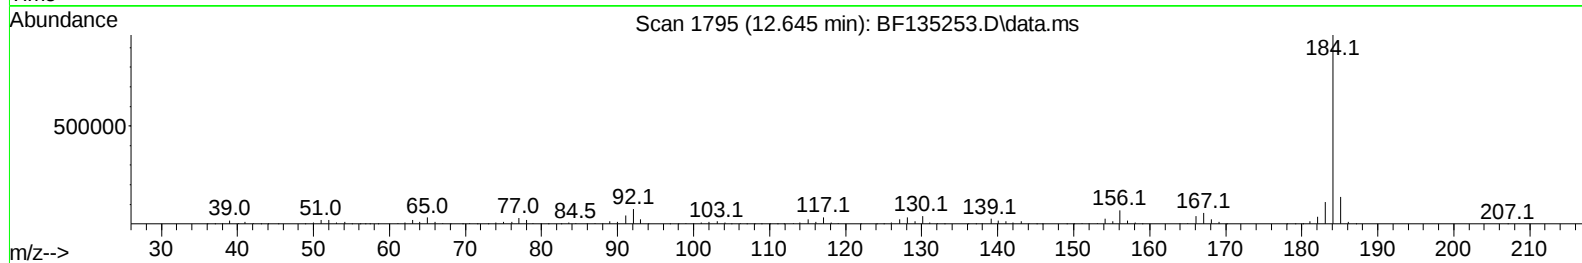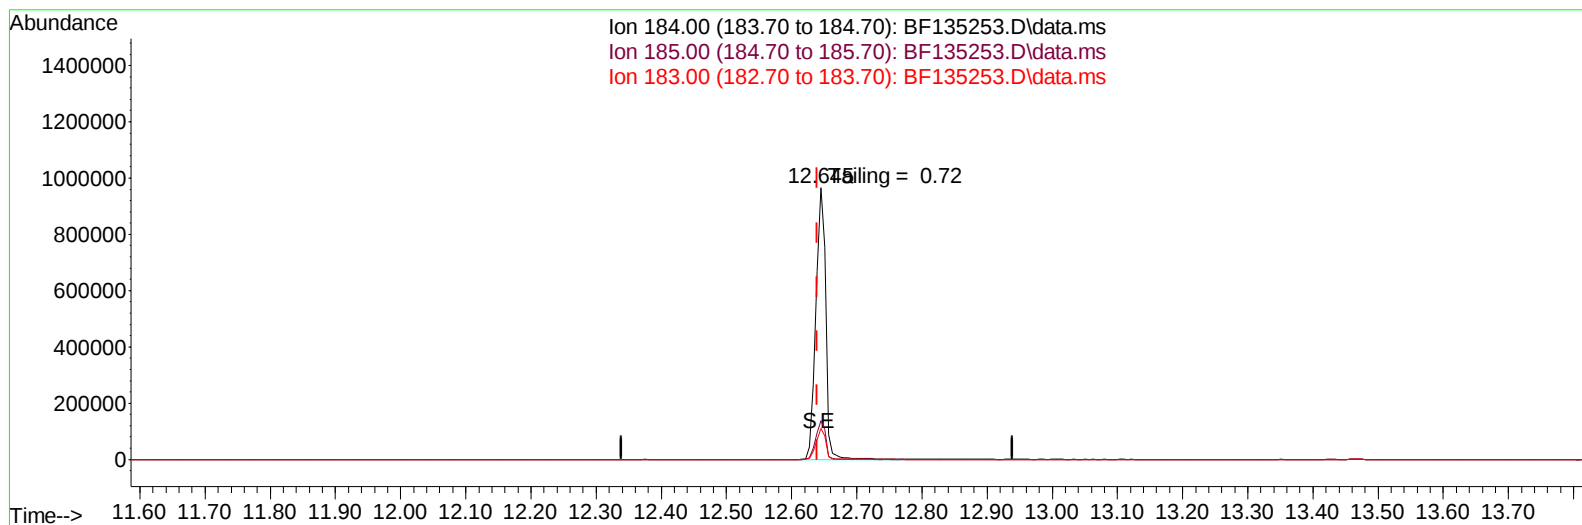

TIC: BF135253.D\data.ms

(77) Benzidine

12.645min (+ 0.006) 223139.49 ng

response 1019427

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.37
183.00	10.30	11.39
0.00	0.00	0.00