

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091423\
 Data File : BF135251.D
 Acq On : 14 Sep 2023 13:33
 Operator : CG\JU
 Sample : PB155300TB
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB155300TB

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135251.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.199	14	19	25	rVB	57740	71867	1.79%	0.280%
2	5.028	497	500	512	rVB	53678	78624	1.96%	0.306%
3	5.404	559	564	567	rBV	3279377	3509315	87.44%	13.671%
4	6.410	729	735	738	rBV	3100528	3526709	87.87%	13.739%
5	6.763	791	795	798	rBV	954981	747134	18.62%	2.911%
6	7.328	885	891	894	rBV	2206130	2363267	58.88%	9.207%
7	8.040	1007	1012	1016	rBV	1114679	990135	24.67%	3.857%
8	9.122	1190	1196	1199	rBV	3972651	4004078	99.76%	15.599%
9	9.798	1306	1311	1315	rBV	1379252	1132531	28.22%	4.412%
10	10.592	1441	1446	1450	rBV	2364627	2545015	63.41%	9.915%
11	11.292	1561	1565	1568	rBV	1441676	1241124	30.92%	4.835%
12	12.892	1832	1837	1840	rBV	3699156	4013558	100.00%	15.635%
13	13.945	2012	2016	2026	rBV	860066	779742	19.43%	3.038%
14	15.416	2261	2266	2271	rBV	511364	666443	16.60%	2.596%




Sum of corrected areas: 25669542

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091423\
Data File : BF135251.D
Acq On : 14 Sep 2023 13:33
Operator : CG\JU
Sample : PB155300TB
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155300TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

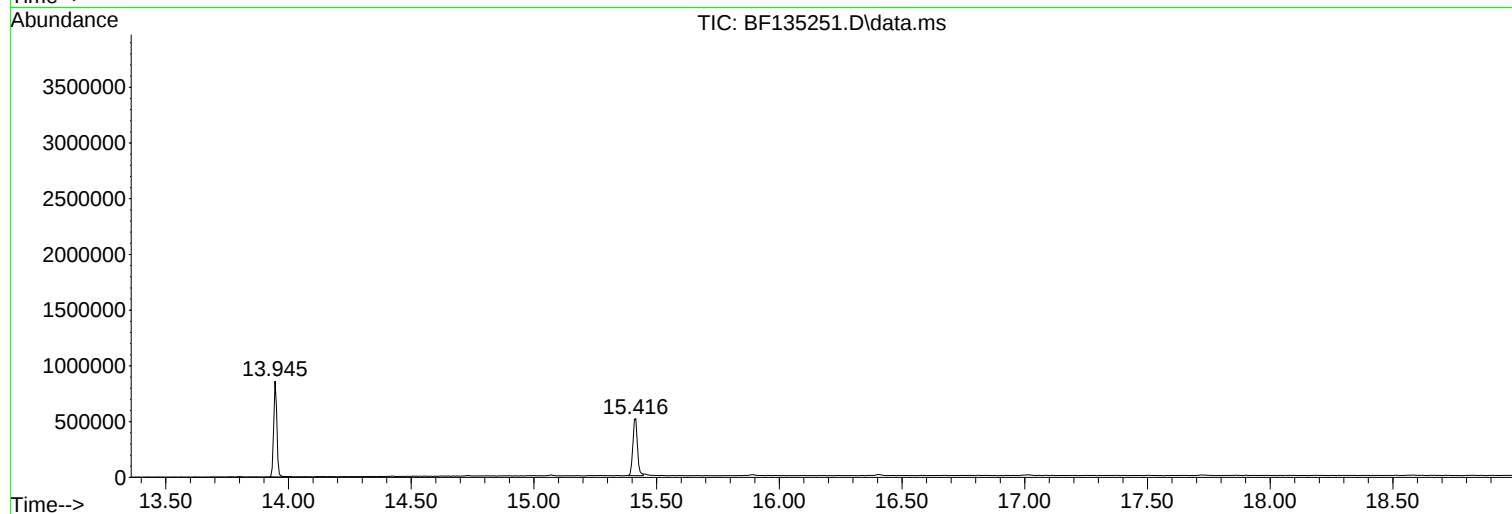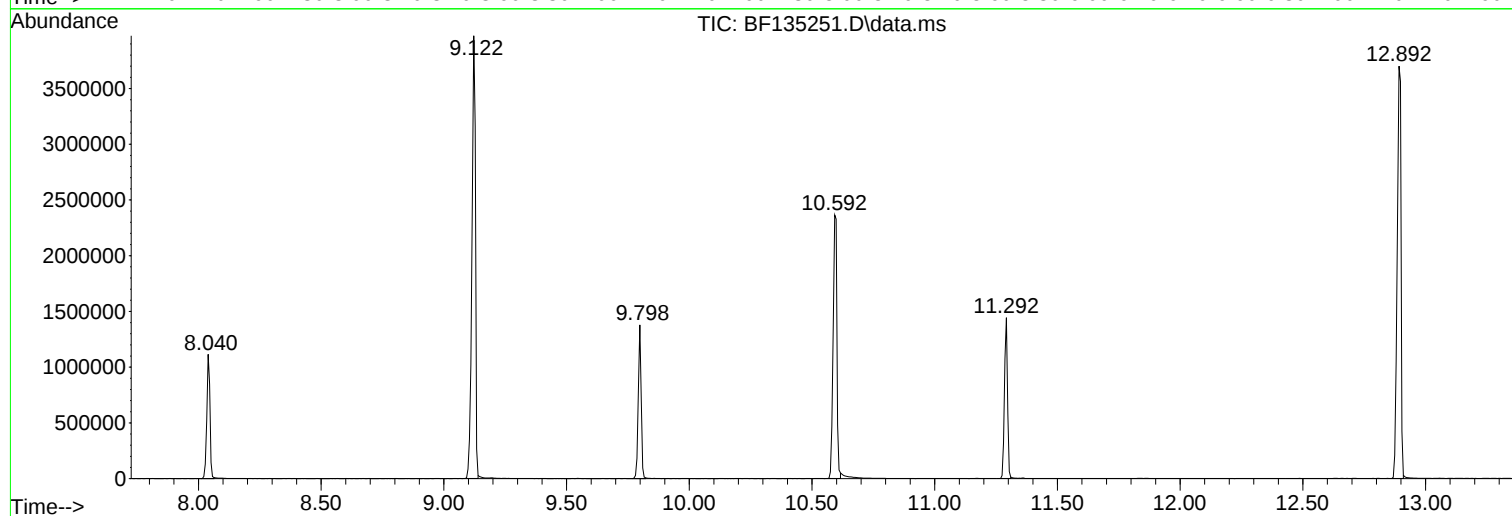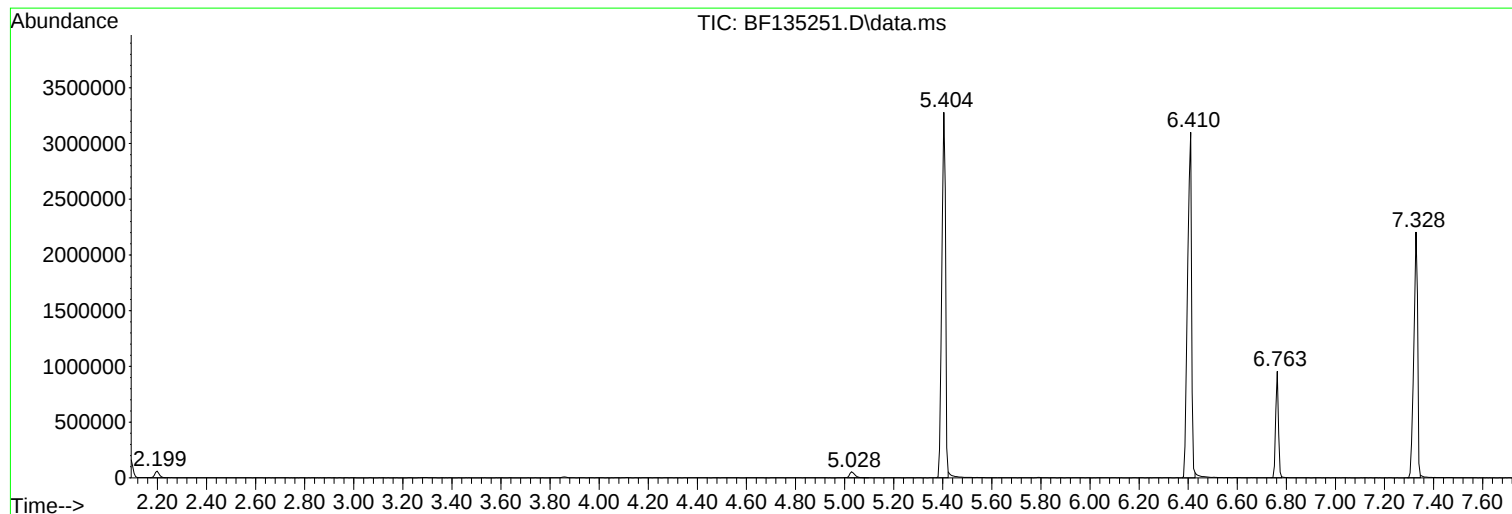

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091423\
Data File : BF135251.D
Acq On : 14 Sep 2023 13:33
Operator : CG\JU
Sample : PB155300TB
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155300TB










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.028	2.10 ng	78624	1,4-Dichlorobenzene-d4	6.763

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59		
2	Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	36		
3	2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	28		
4	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23		
5	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	12		

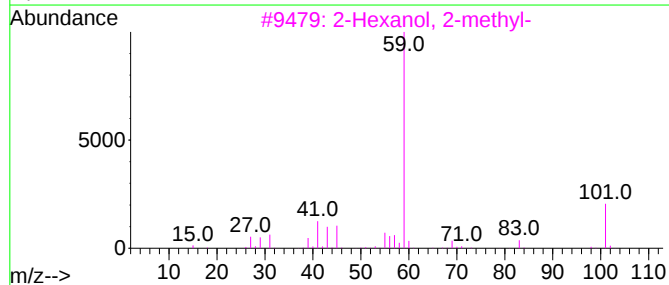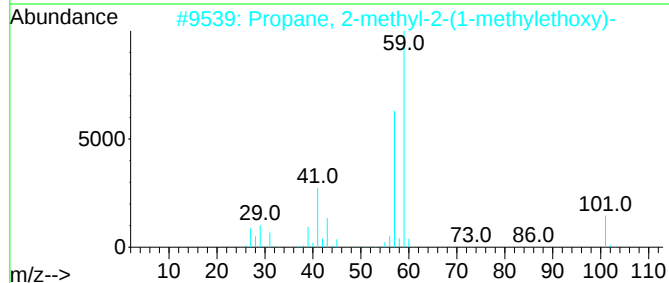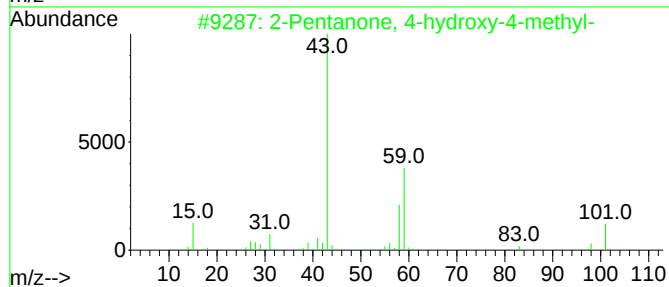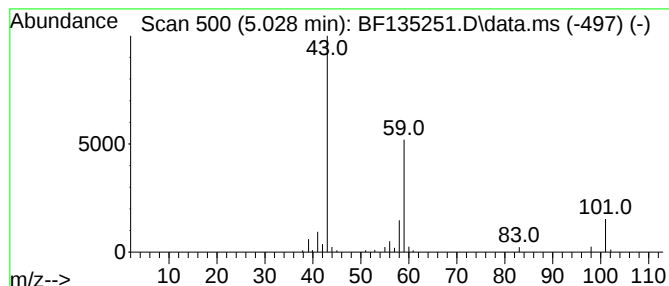

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091423\
Data File : BF135251.D
Acq On : 14 Sep 2023 13:33
Operator : CG\JU
Sample : PB155300TB
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155300TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.028	2.1	ng	78624	1	6.763	747134	20.0