

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091423\
 Data File : BF135263.D
 Acq On : 14 Sep 2023 20:05
 Operator : CG\JU
 Sample : 04361-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SP-303-20230907

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135263.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.987	490	493	499	rBV	53163	60033	1.74%	0.349%
2	5.392	558	562	573	rBV	1582022	1463904	42.38%	8.503%
3	6.404	730	734	748	rBV	958699	909169	26.32%	5.281%
4	6.763	791	795	798	rBV	931569	771866	22.35%	4.483%
5	7.328	886	891	894	rBV	2145170	2146838	62.15%	12.469%
6	8.039	1008	1012	1015	rBV	1116778	908495	26.30%	5.277%
7	9.122	1190	1196	1199	rBV	3819461	3454308	100.00%	20.064%
8	9.798	1307	1311	1314	rBV	1209734	986898	28.57%	5.732%
9	10.592	1442	1446	1449	rBV	1780148	1601457	46.36%	9.302%
10	11.292	1561	1565	1568	rBV	1007157	871348	25.22%	5.061%
11	12.892	1832	1837	1840	rBV	2937728	2762300	79.97%	16.044%
12	13.945	2012	2016	2026	rVB	711895	658080	19.05%	3.822%
13	15.415	2261	2266	2271	rBV	488856	622056	18.01%	3.613%




Sum of corrected areas: 17216752

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091423\
Data File : BF135263.D
Acq On : 14 Sep 2023 20:05
Operator : CG\JU
Sample : 04361-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-303-20230907

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

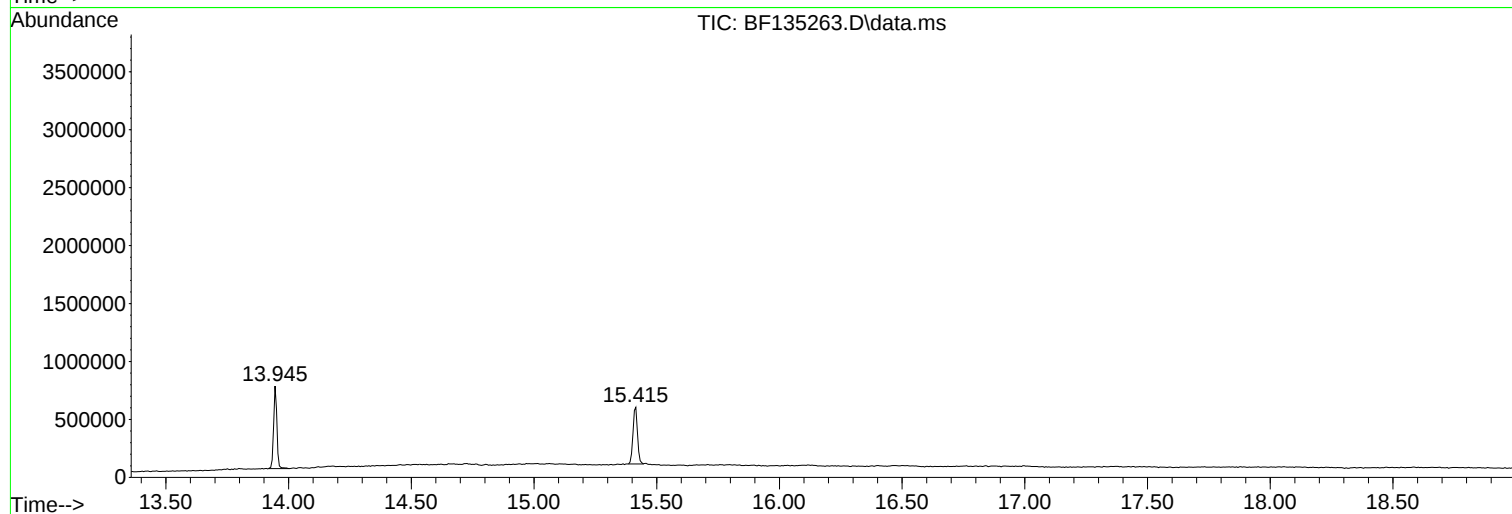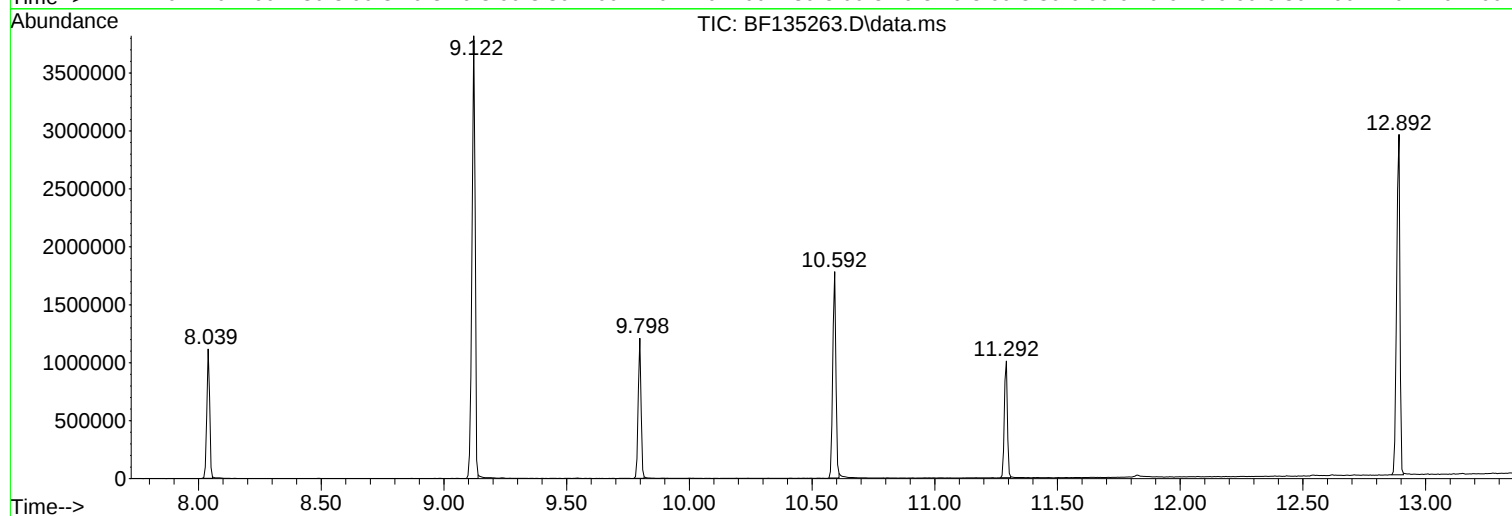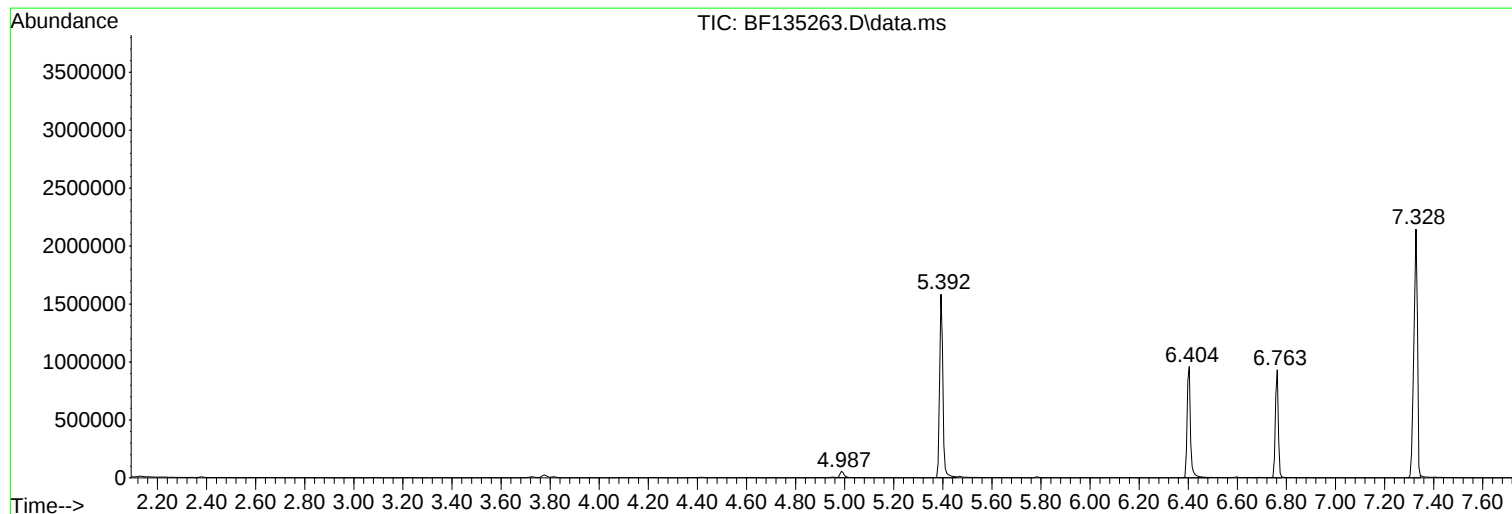

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091423\
Data File : BF135263.D
Acq On : 14 Sep 2023 20:05
Operator : CG\JU
Sample : 04361-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-303-20230907

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091423\
Data File : BF135263.D
Acq On : 14 Sep 2023 20:05
Operator : CG\JU
Sample : 04361-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-303-20230907

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------