
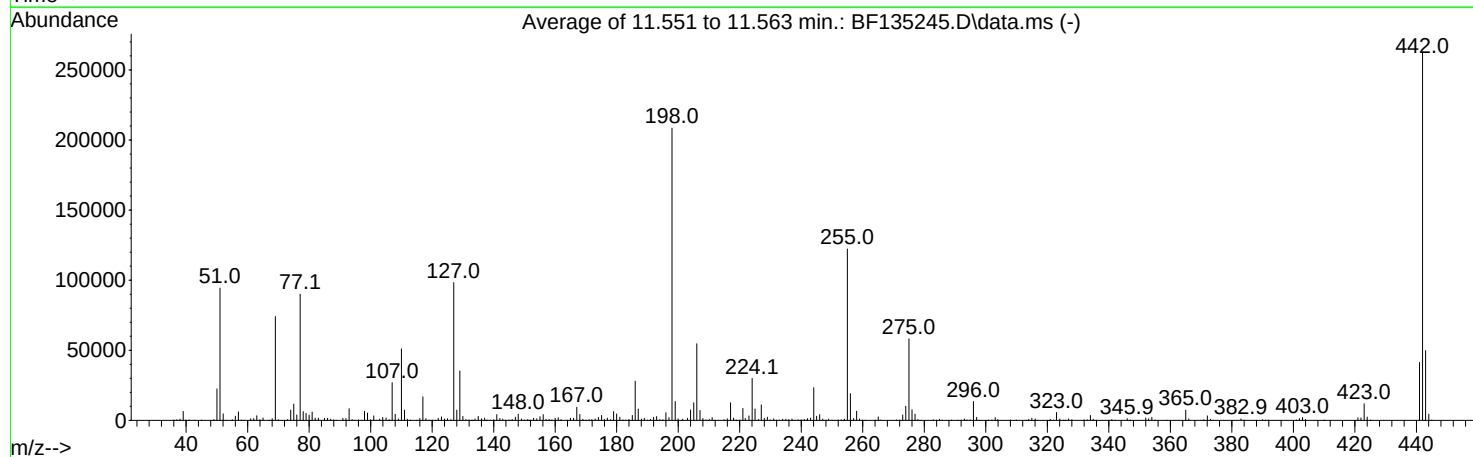


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091423\
Data File : BF135245.D
Acq On : 14 Sep 2023 10:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 12 00:19:07 2023

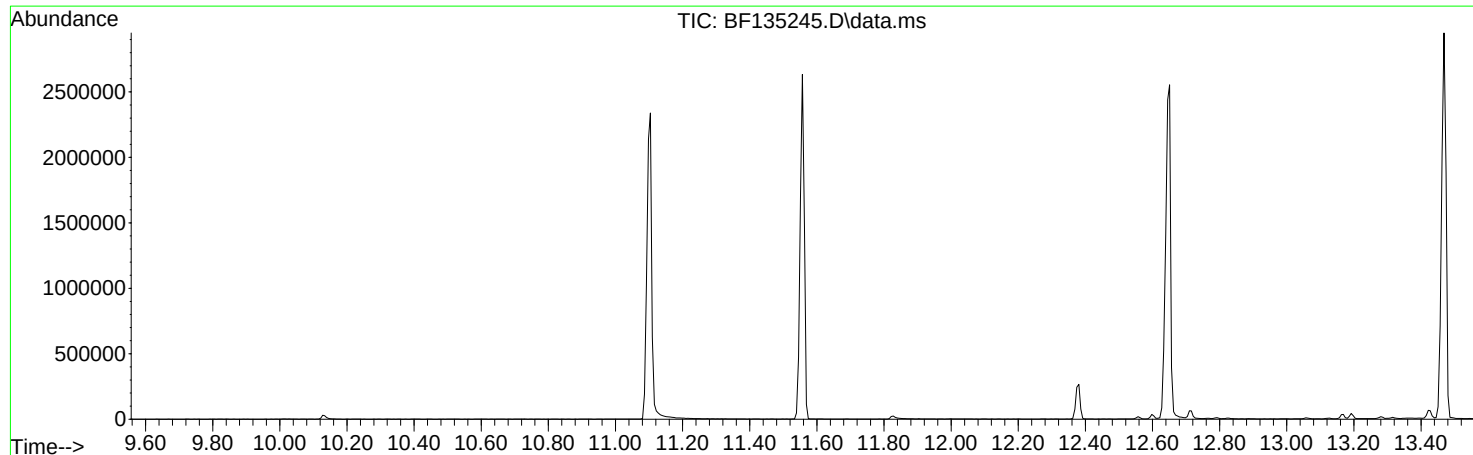




AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1604

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.3	94373	PASS
68	69	0.00	2	1.7	1225	PASS
69	198	0.00	100	35.5	74077	PASS
70	69	0.00	2	0.6	437	PASS
127	198	10	80	47.2	98323	PASS
197	198	0.00	2	1.0	2010	PASS
198	198	100	100	100.0	208491	PASS
199	198	5	9	6.5	13477	PASS
275	198	10	60	27.9	58203	PASS
365	198	1	100	3.5	7279	PASS
441	198	0.01	100	19.8	41299	PASS
442	442	50	100	100.0	262443	PASS
443	442	15	24	19.0	49752	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091423\
Data File : BF135245.D
Acq On : 14 Sep 2023 10:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 15 05:18:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

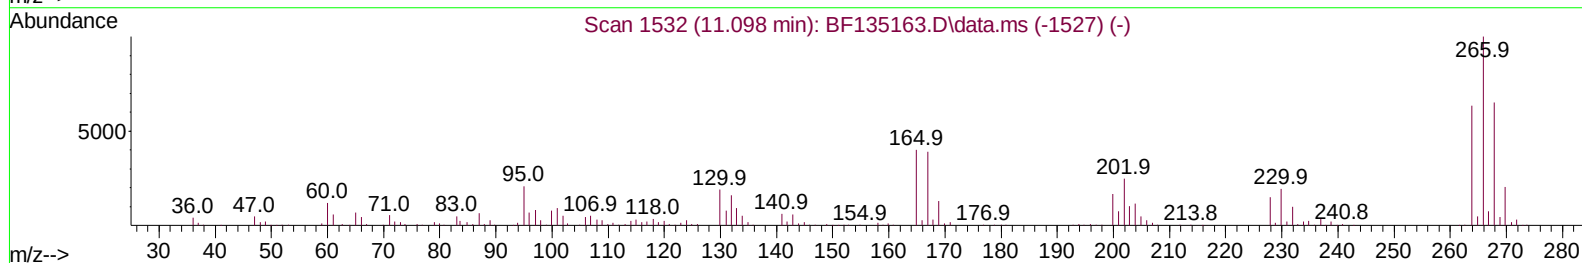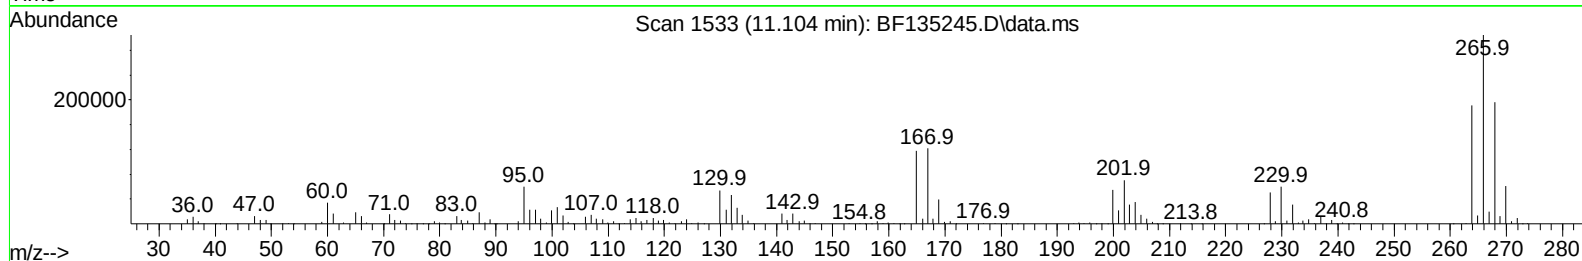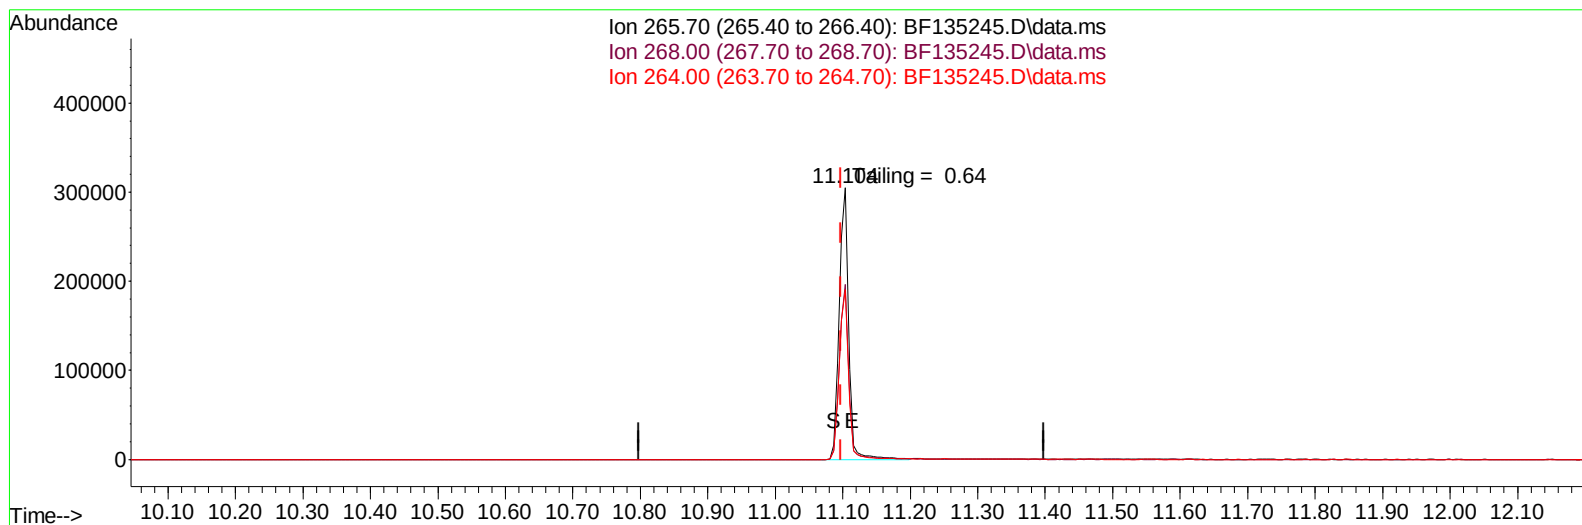

TIC: BF135245.D\data.ms

(70) Pentachlorophenol (C)

11.104min (+ 0.006) 685985.23 ng




response 295260

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	64.52
264.00	63.50	62.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091423\
Data File : BF135245.D
Acq On : 14 Sep 2023 10:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 15 05:18:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

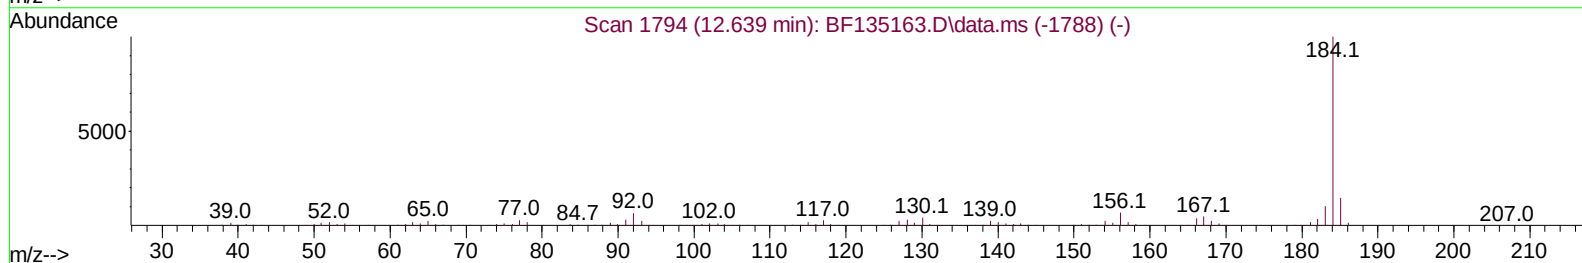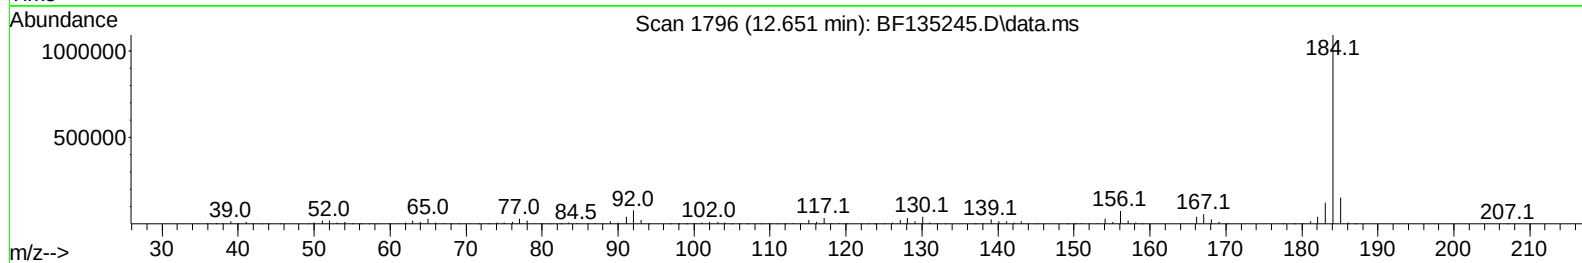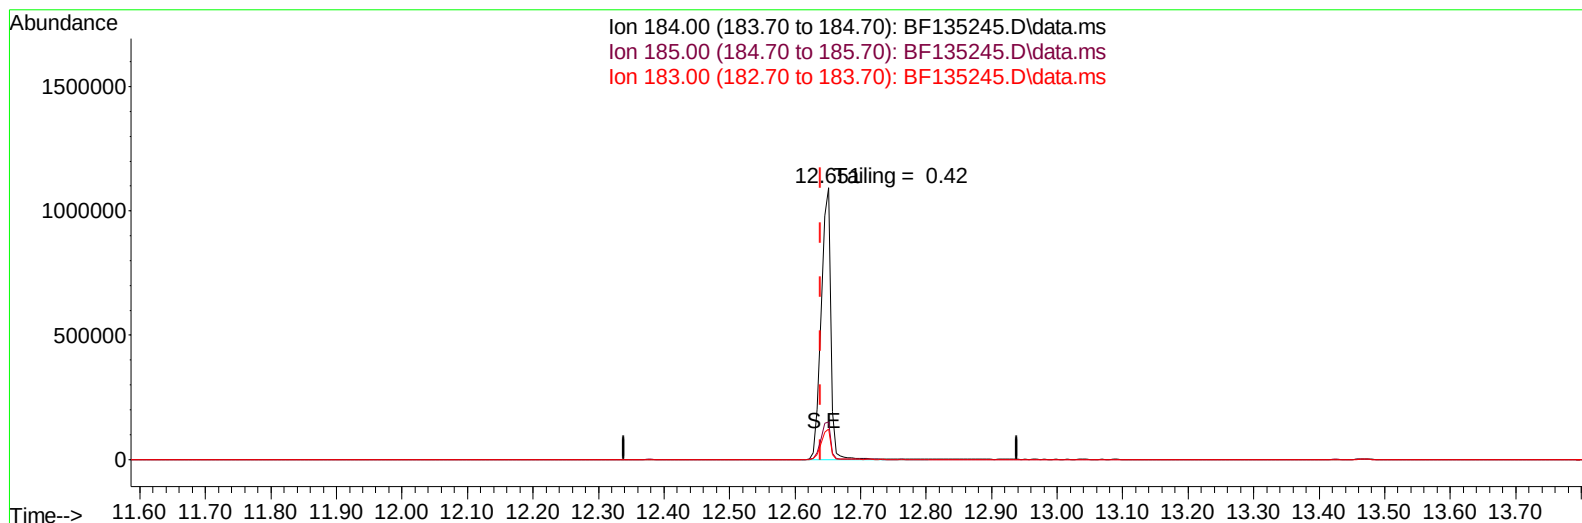

TIC: BF135245.D\data.ms

(77) Benzidine

12.651min (+ 0.012) 167154.35 ng

response 1116375

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.86
183.00	10.30	11.27
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/14/2023	BNA_F	<u>BF135245.D</u>
Compound Name	Response	Retention Time
DDT	558529	13.469
DDD	13613	13.169
DDE	964	12.827
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14577	573106	2.54

Instrument :
BNA_F
ClientSampleId :
DFTPP