
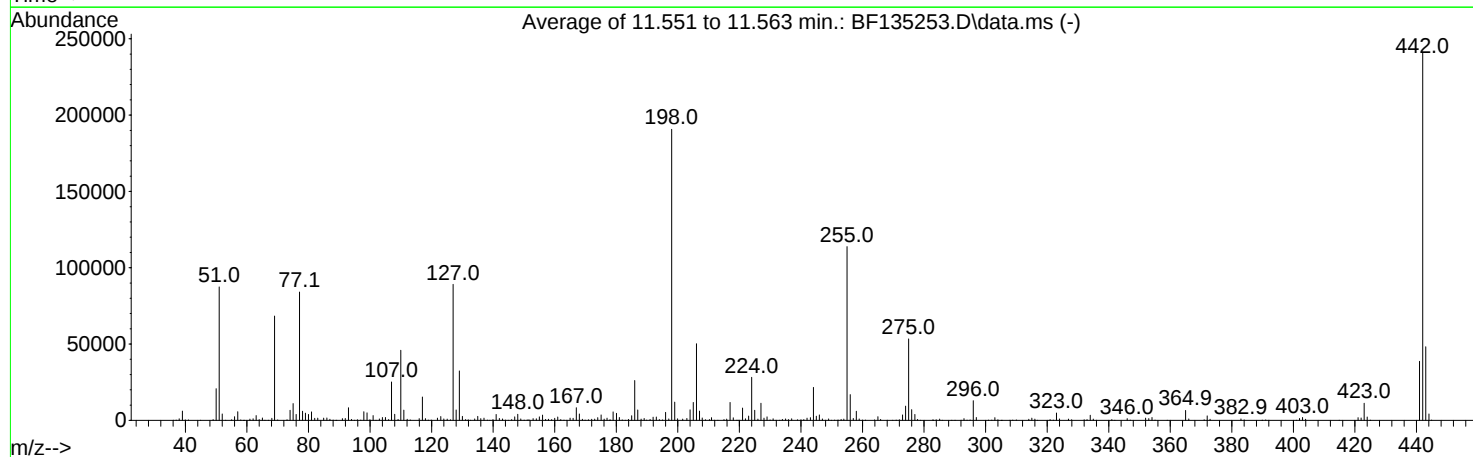


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091423\
 Data File : BF135253.D
 Acq On : 14 Sep 2023 14:37
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 12 00:19:07 2023

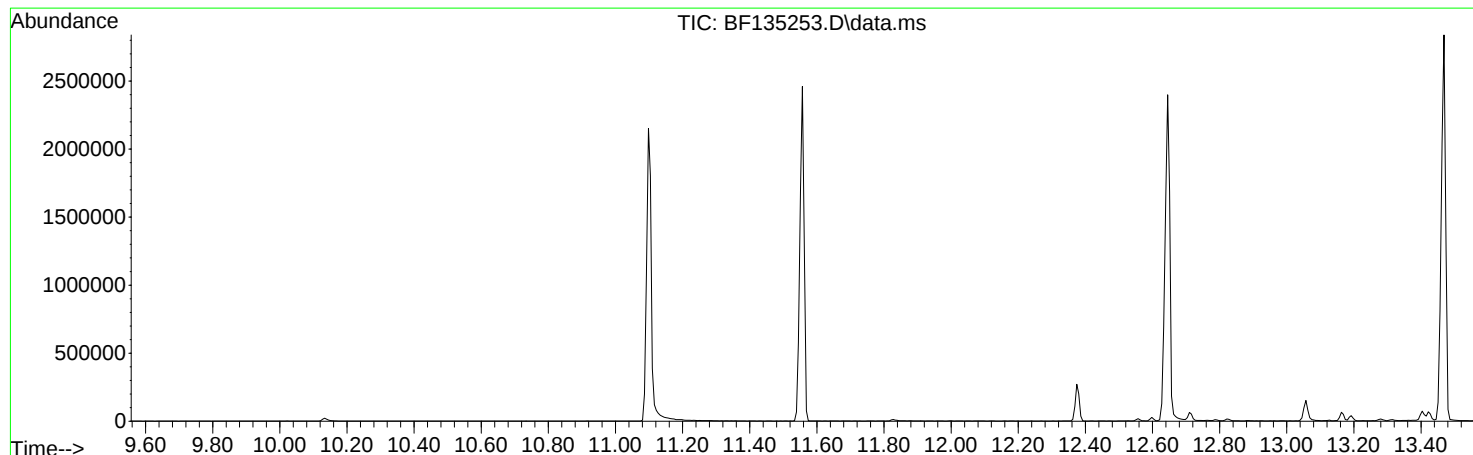




AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.9	87480	PASS
68	69	0.00	2	1.9	1322	PASS
69	198	0.00	100	35.9	68371	PASS
70	69	0.00	2	0.4	297	PASS
127	198	10	80	46.7	89099	PASS
197	198	0.00	2	0.5	909	PASS
198	198	100	100	100.0	190709	PASS
199	198	5	9	6.2	11904	PASS
275	198	10	60	28.0	53395	PASS
365	198	1	100	3.4	6547	PASS
441	198	0.01	100	20.3	38728	PASS
442	442	50	100	100.0	241024	PASS
443	442	15	24	20.0	48197	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091423\
Data File : BF135253.D
Acq On : 14 Sep 2023 14:37
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 15 05:23:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

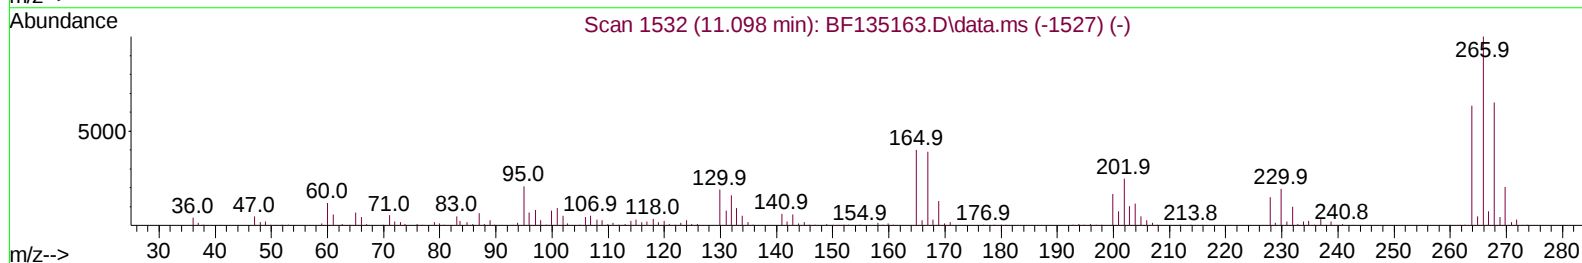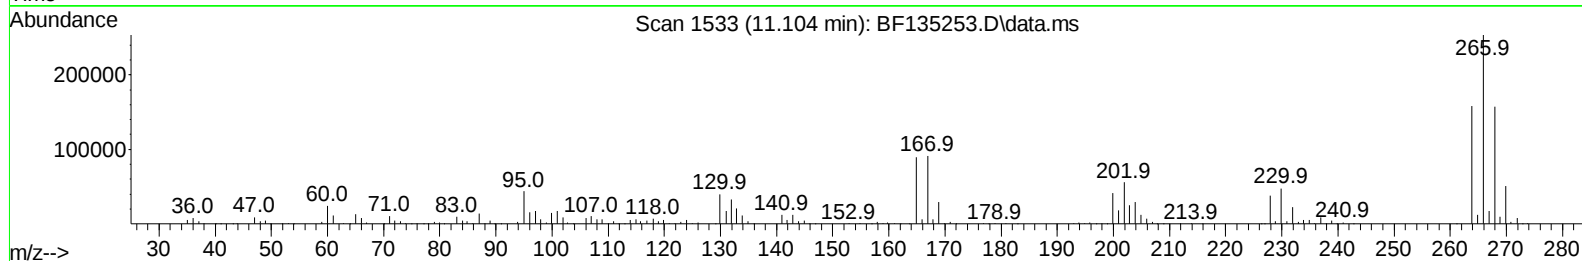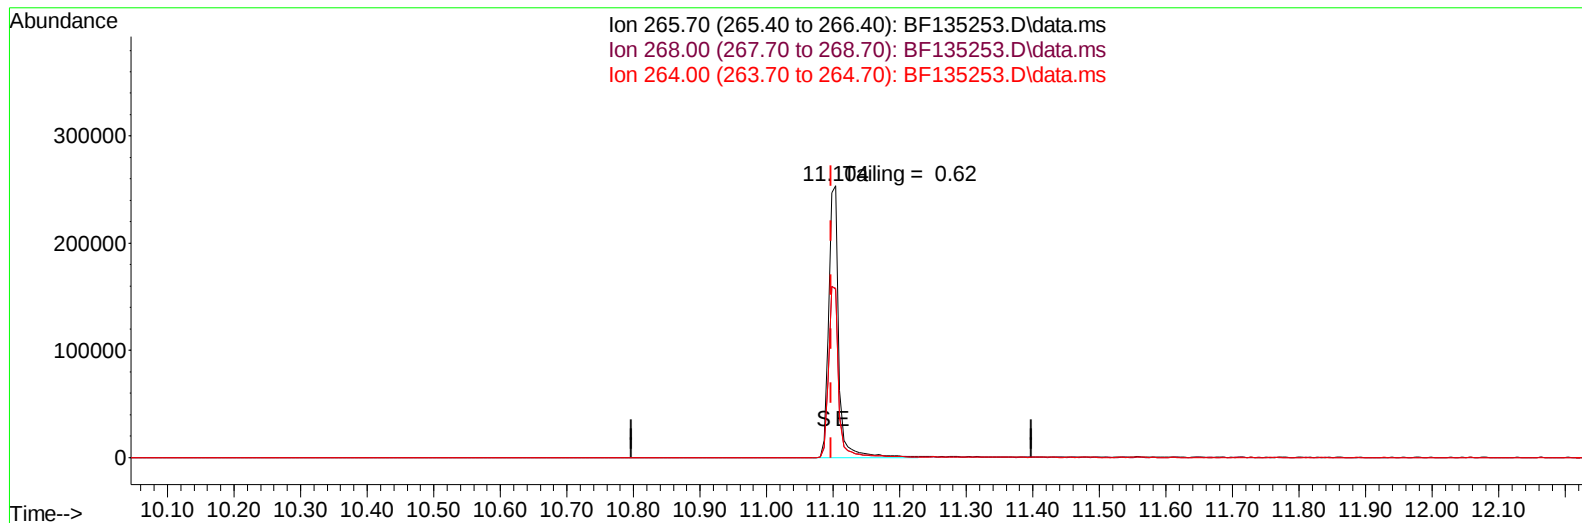

TIC: BF135253.D\data.ms

(70) Pentachlorophenol (C)

11.104min (+ 0.006) 255226.03 ng




response 269219

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	61.92
264.00	63.50	62.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091423\
Data File : BF135253.D
Acq On : 14 Sep 2023 14:37
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 15 05:23:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

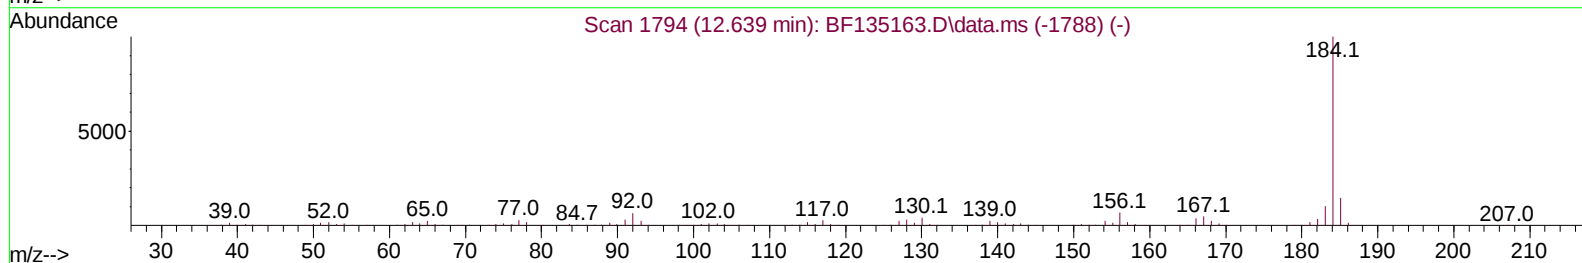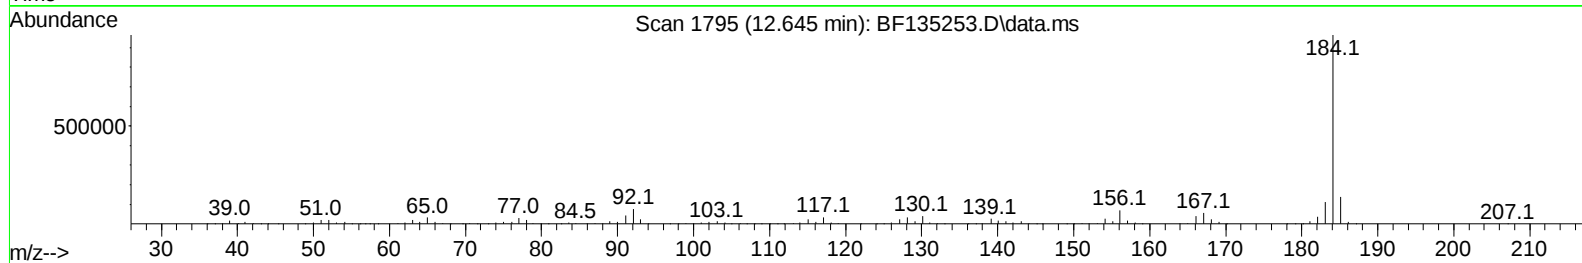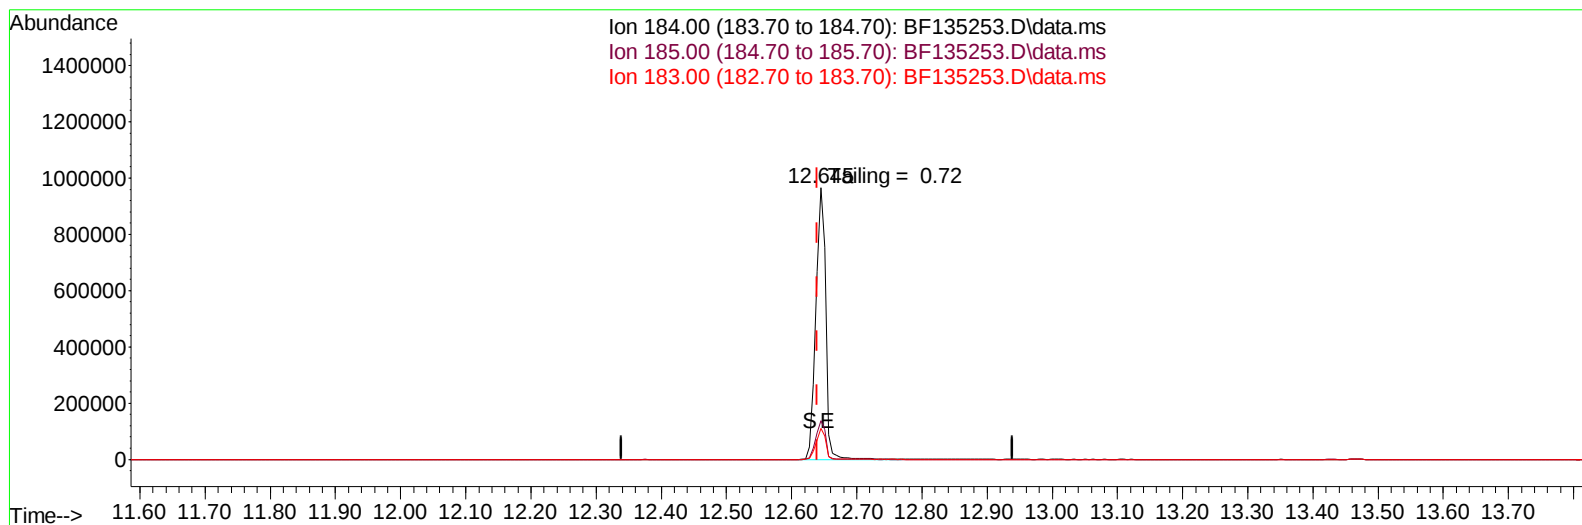

TIC: BF135253.D\data.ms

(77) Benzidine

12.645min (+ 0.006) 223139.49 ng

response 1019427

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.37
183.00	10.30	11.39
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/14/2023	BNA_F	<u>BF135253.D</u>
Compound Name	Response	Retention Time
DDT	511831	13.468
DDD	17937	13.163
DDE	2005	12.821
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19942	531773	3.75

Instrument :
BNA_F
ClientSampleId :
DFTPP