

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091424\
 Data File : BF139358.D
 Acq On : 14 Sep 2024 09:58
 Operator : RC/JU
 Sample : PB163293BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB163293BL

Quant Time: Sep 16 01:50:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 14 02:58:23 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.875	152	79463	20.000	ng	0.00
21) Naphthalene-d8	8.157	136	299670	20.000	ng	0.00
39) Acenaphthene-d10	9.910	164	168574	20.000	ng	0.00
64) Phenanthrene-d10	11.398	188	326160	20.000	ng	0.00
76) Chrysene-d12	14.027	240	219748	20.000	ng	0.00
86) Perylene-d12	15.498	264	181316	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.504	112	588588	120.835	ng	0.01
7) Phenol-d6	6.504	99	767084	119.978	ng	0.00
23) Nitrobenzene-d5	7.440	82	521097	81.748	ng	0.00
42) 2,4,6-Tribromophenol	10.704	330	212756	118.549	ng	0.00
45) 2-Fluorobiphenyl	9.234	172	992284	82.557	ng	0.00
79) Terphenyl-d14	12.986	244	1143742	85.431	ng	0.00
Target Compounds						
						Qvalue
19) n-Nitroso-di-n-propyla...	7.440	70	74983	19.791	ng	# 75
25) Isophorone	7.440	82	519619	51.543	ng	# 66
51) 2,6-Dinitrotoluene	9.910	165	21739	8.869	ng	# 15
57) 2,4-Dinitrotoluene	9.910	165	21739	6.569	ng	# 16
67) 4-Bromophenyl-phenylether	10.698	248	15011	4.644	ng	# 1
77) Benzidine	12.980	184	17247	5.478	ng	# 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091424\
Data File : BF139358.D
Acq On : 14 Sep 2024 09:58
Operator : RC/JU
Sample : PB163293BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB163293BL


Quant Time: Sep 16 01:50:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 14 02:58:23 2024
Response via : Initial Calibration

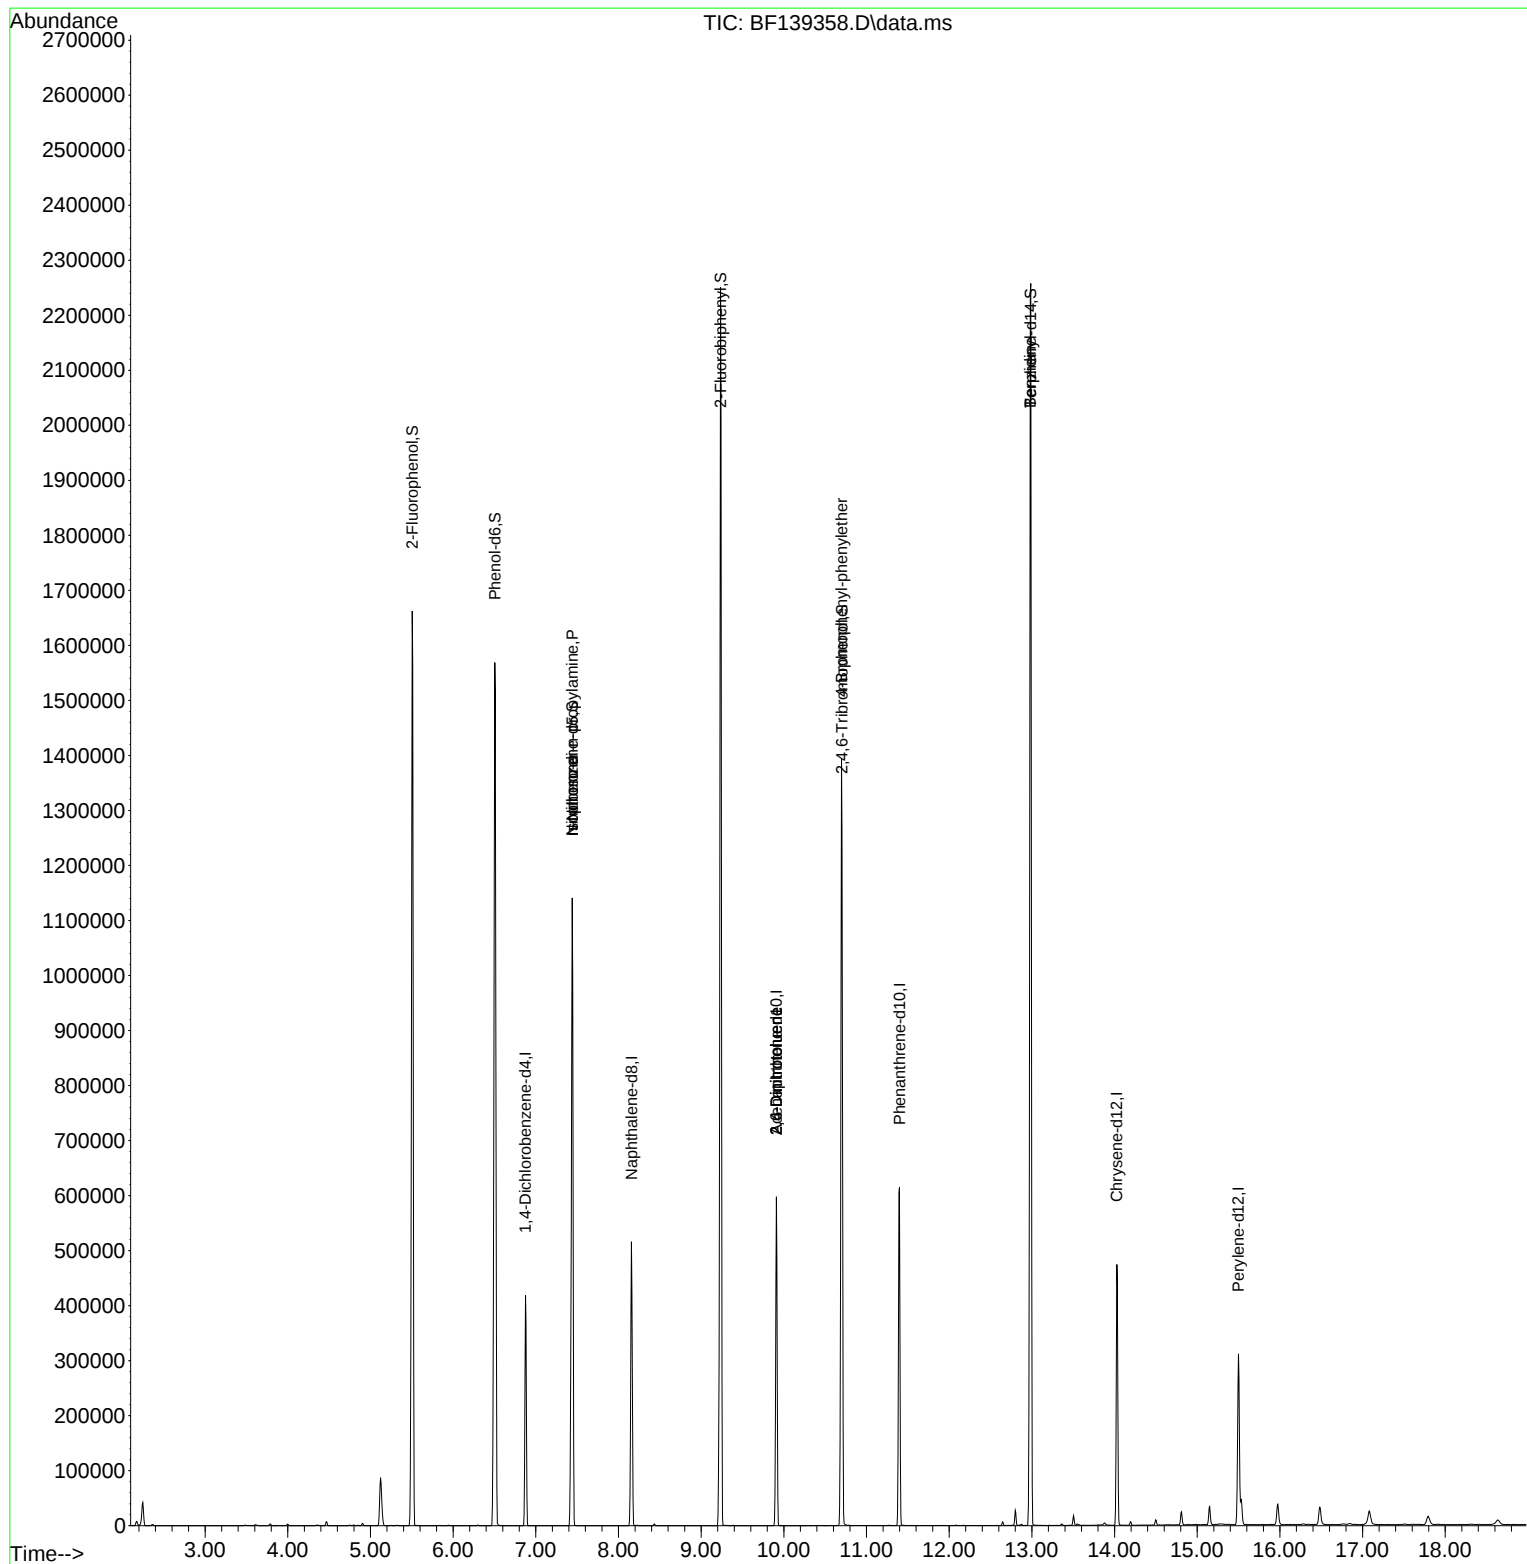


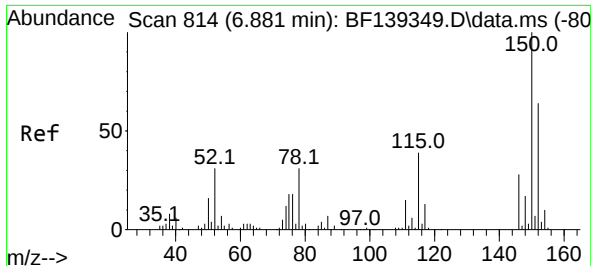


#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.875 min Scan# 814
Delta R.T. -0.006 min
Lab File: BF139358.D
Acq: 14 Sep 2024 09:58

Instrument :
BNA_F
ClientSampleId :
PB163293BL



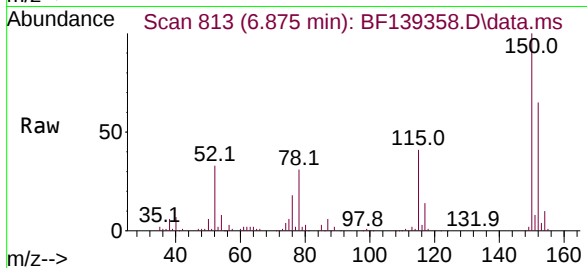


Tgt Ion:152 Resp: 79463
Ion Ratio Lower Upper
152 100
150 154.2 124.1 186.1
115 63.9 48.1 72.1

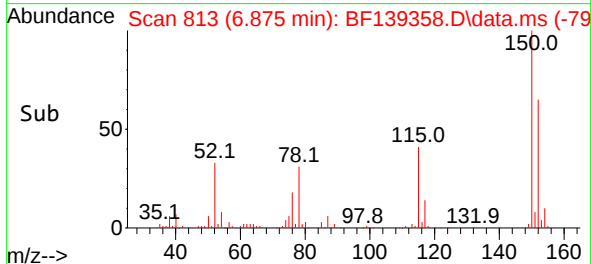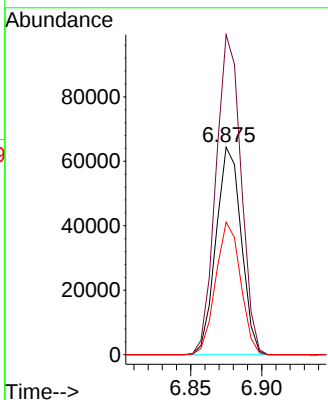

#5
2-Fluorophenol
Concen: 120.835 ng
RT: 5.504 min Scan# 580
Delta R.T. 0.011 min
Lab File: BF139358.D
Acq: 14 Sep 2024 09:58


Tgt Ion:112 Resp: 588588
Ion Ratio Lower Upper
112 100
64 70.4 54.8 82.2
63 41.1 33.0 49.4

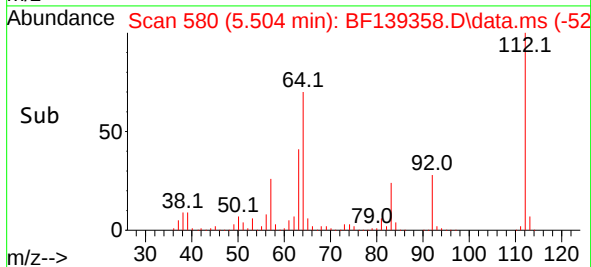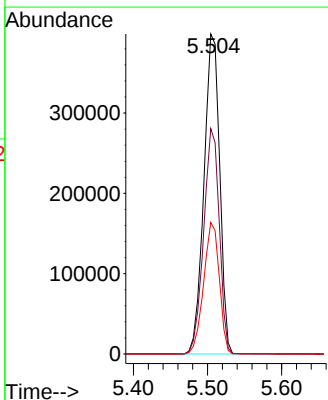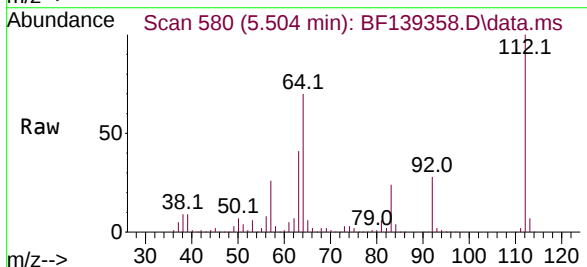






#7
Phenol-d6
Concen: 119.978 ng
RT: 6.504 min Scan# 71
Delta R.T. -0.000 min
Lab File: BF139358.D
Acq: 14 Sep 2024 09:58

Instrument :
BNA_F
ClientSampleId :
PB163293BL







Tgt Ion:	99	Resp:	767084
Ion	Ratio	Lower	Upper
99	100		
42	26.5	21.9	32.9
71	42.6	34.6	52.0

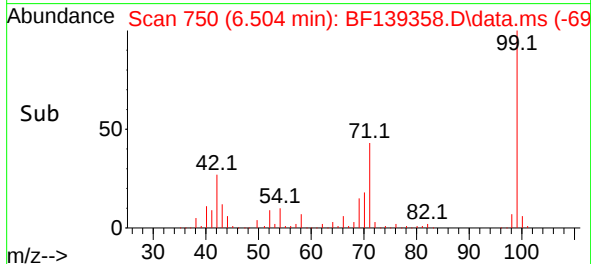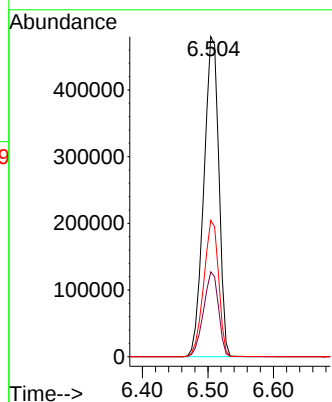

#19
n-Nitroso-di-n-propylamine
Concen: 19.791 ng
RT: 7.440 min Scan# 909
Delta R.T. 0.147 min
Lab File: BF139358.D
Acq: 14 Sep 2024 09:58

Tgt Ion:	70	Resp:	74983
Ion	Ratio	Lower	Upper
70	100		
42	58.4	61.2	91.8#
101	0.0	7.5	11.3#
130	1.8	15.8	23.8#

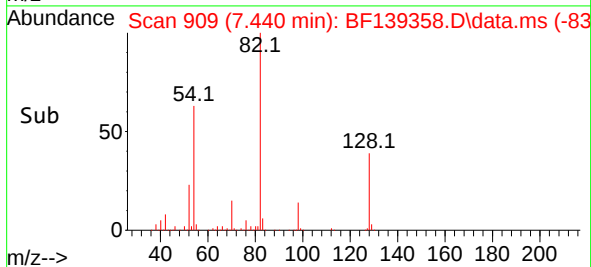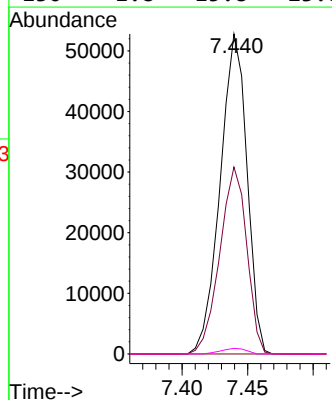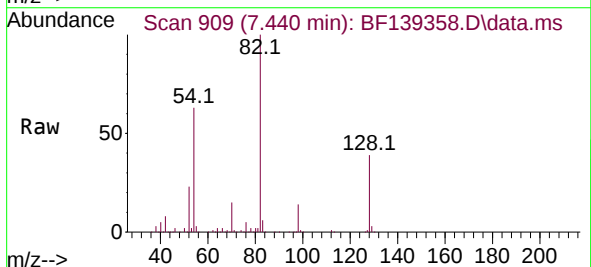



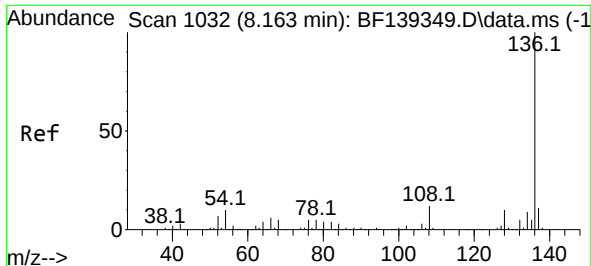


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.157 min Scan# 1031
Delta R.T. -0.006 min
Lab File: BF139358.D
Acq: 14 Sep 2024 09:58

Instrument :
BNA_F
ClientSampleId :
PB163293BL

Tgt Ion:136 Resp: 299670




Ion	Ratio	Lower	Upper
136	100		
137	10.8	8.6	12.8
54	9.6	7.8	11.8
68	4.7	3.6	5.4

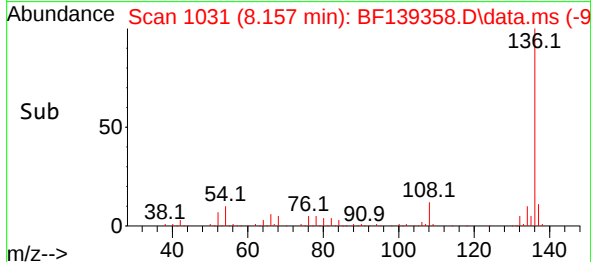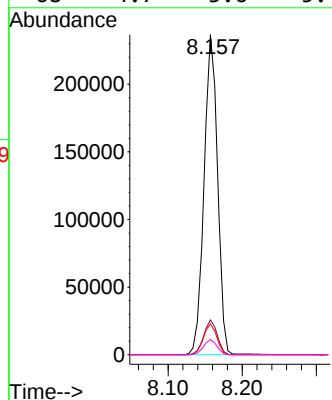


#23
Nitrobenzene-d5
Concen: 81.748 ng
RT: 7.440 min Scan# 909
Delta R.T. -0.006 min
Lab File: BF139358.D
Acq: 14 Sep 2024 09:58

Tgt Ion: 82 Resp: 521097

Ion	Ratio	Lower	Upper
82	100		
128	38.9	31.8	47.6
54	63.5	50.6	75.8


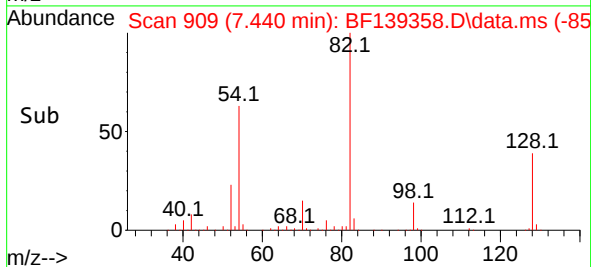
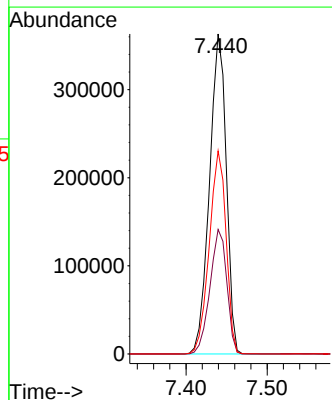
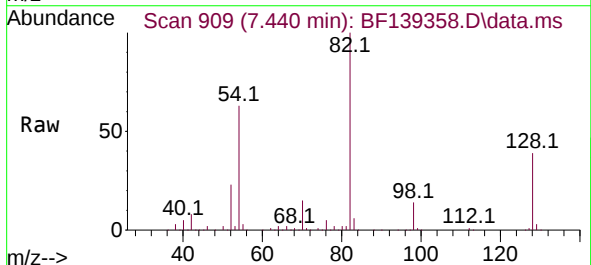


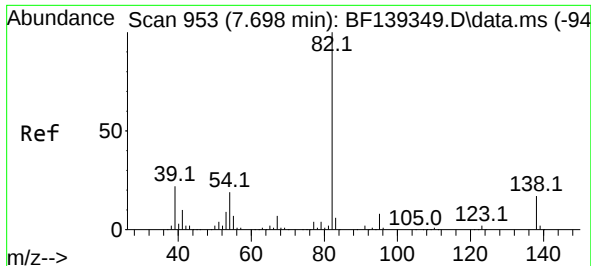

#25
Isophorone
Concen: 51.543 ng
RT: 7.440 min Scan# 90
Delta R.T. -0.259 min
Lab File: BF139358.D
Acq: 14 Sep 2024 09:58




Instrument :
BNA_F
ClientSampleId :
PB163293BL


Tgt Ion: 82 Resp: 519619
Ion Ratio Lower Upper
82 100
95 0.0 6.7 10.1#
138 0.0 13.3 19.9#

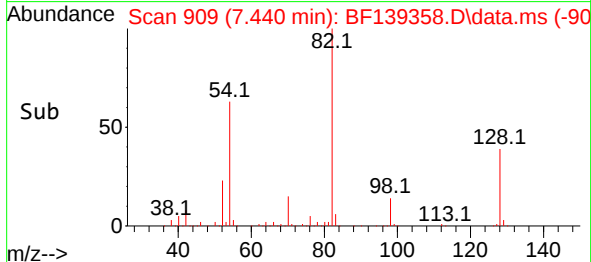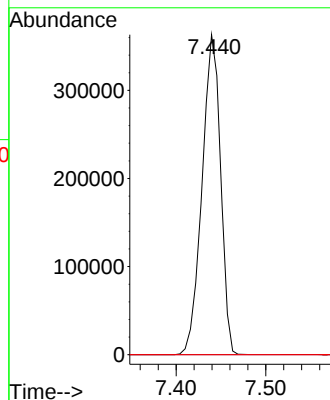

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.910 min Scan# 1329
Delta R.T. -0.006 min
Lab File: BF139358.D
Acq: 14 Sep 2024 09:58


Tgt Ion:164 Resp: 168574
Ion Ratio Lower Upper
164 100
162 100.9 81.3 121.9
160 45.1 36.4 54.6

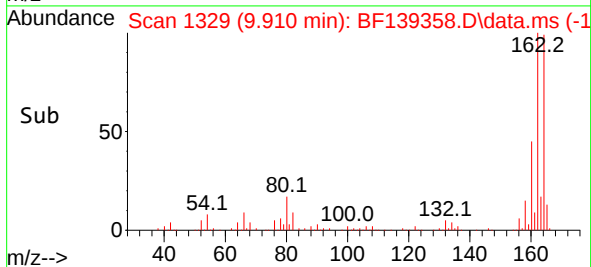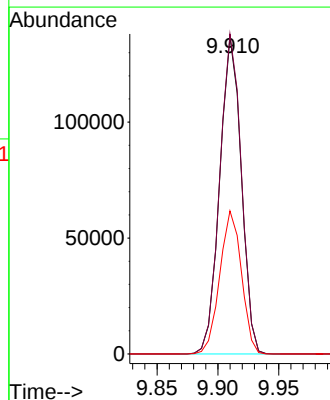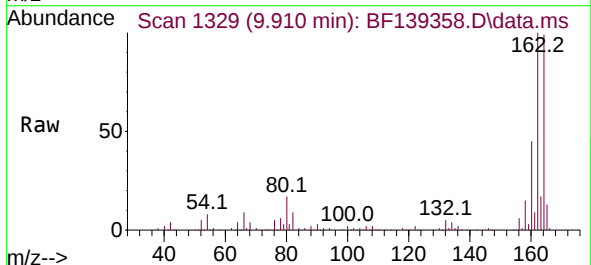






#42
2,4,6-Tribromophenol
Concen: 118.549 ng
RT: 10.704 min Scan# 1464
Delta R.T. 0.006 min
Lab File: BF139358.D
Acq: 14 Sep 2024 09:58

Instrument :
BNA_F
ClientSampleId :
PB163293BL



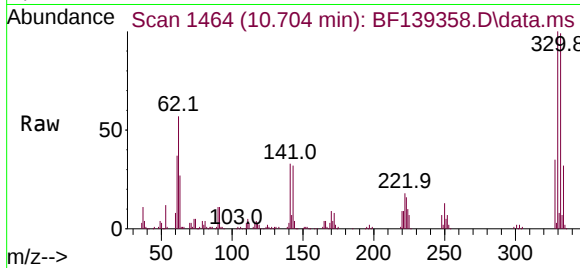



Tgt Ion:330 Resp: 212756
Ion Ratio Lower Upper
330 100
332 97.6 75.2 112.8
141 37.7 31.2 46.8

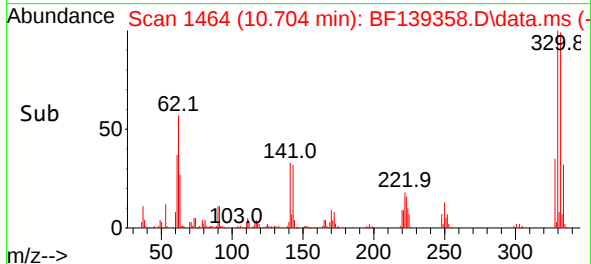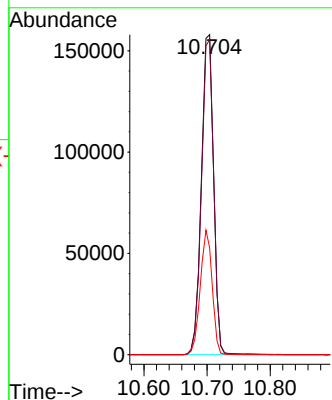

#45
2-Fluorobiphenyl
Concen: 82.557 ng
RT: 9.234 min Scan# 1214
Delta R.T. -0.000 min
Lab File: BF139358.D
Acq: 14 Sep 2024 09:58

Tgt Ion:172 Resp: 992284
Ion Ratio Lower Upper
172 100
171 35.5 28.3 42.5
170 23.3 19.0 28.6

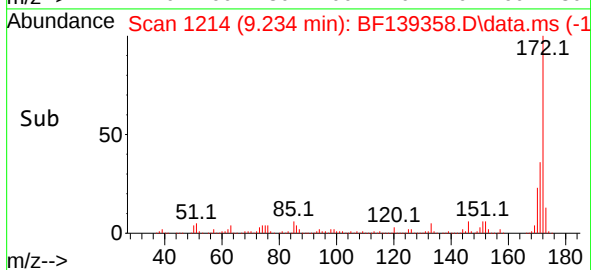
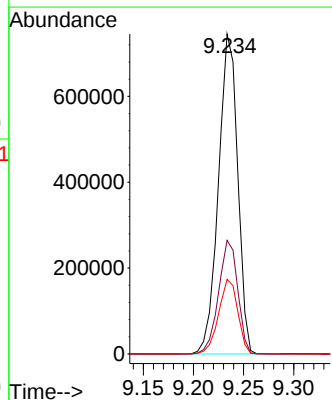
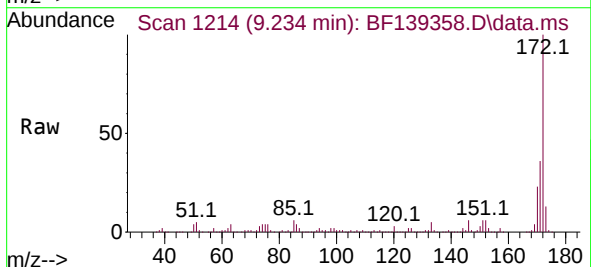




#51
2,6-Dinitrotoluene
Concen: 8.869 ng
RT: 9.910 min Scan# 11
Delta R.T. 0.212 min
Lab File: BF139358.D
Acq: 14 Sep 2024 09:58




Instrument :
BNA_F
ClientSampleId :
PB163293BL

Tgt Ion:165 Resp: 21739
Ion Ratio Lower Upper
165 100
63 1.1 60.9 91.3#
89 1.2 54.7 82.1#

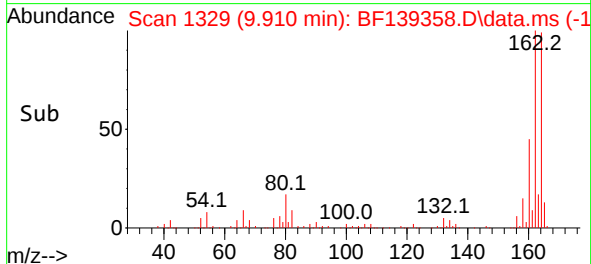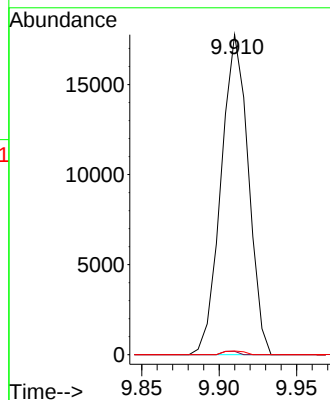

#57
2,4-Dinitrotoluene
Concen: 6.569 ng
RT: 9.910 min Scan# 1329
Delta R.T. -0.188 min
Lab File: BF139358.D
Acq: 14 Sep 2024 09:58

Tgt Ion:165 Resp: 21739
Ion Ratio Lower Upper
165 100
63 1.1 47.8 71.6#
89 1.2 66.7 100.1#
182 0.0 2.2 3.4#

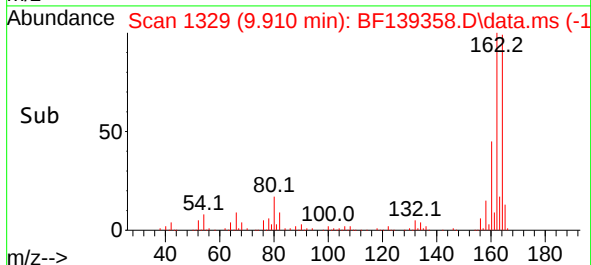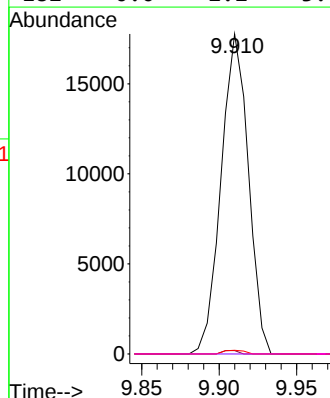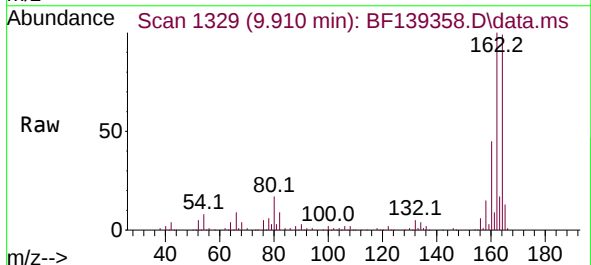



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.398 min Scan# 11

Delta R.T. -0.000 min

Lab File: BF139358.D

Acq: 14 Sep 2024 09:58

Instrument :

BNA_F

ClientSampleId :

PB163293BL





Tgt Ion:188 Resp: 326160

Ion Ratio Lower Upper

188 100

94 7.4 5.5 8.3

80 8.0 6.6 9.8

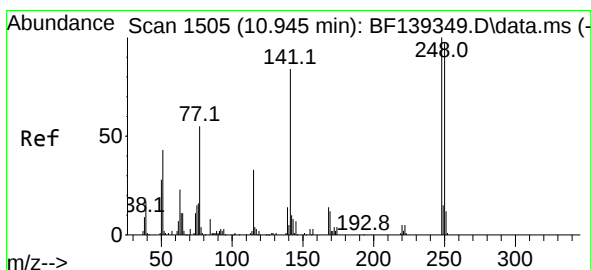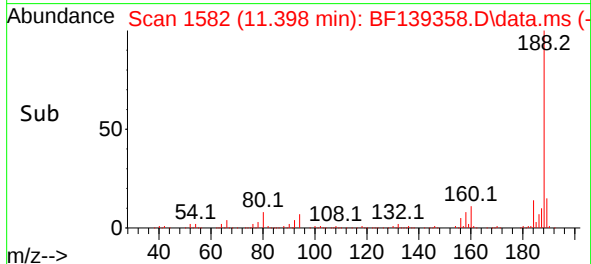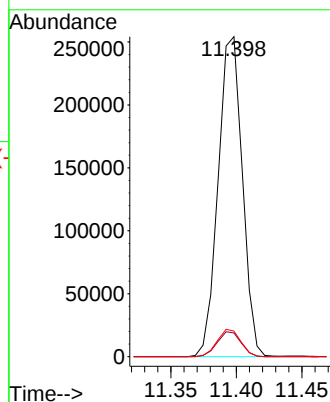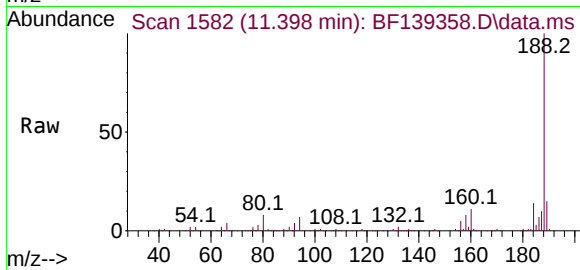

#67

4-Bromophenyl-phenylether

Concen: 4.644 ng

RT: 10.698 min Scan# 1463

Delta R.T. -0.247 min

Lab File: BF139358.D

Acq: 14 Sep 2024 09:58




Tgt Ion:248 Resp: 15011


Ion Ratio Lower Upper

248 100

250 191.6 77.6 116.4#

141 542.8 66.9 100.3#



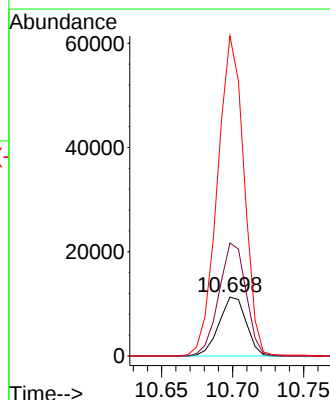
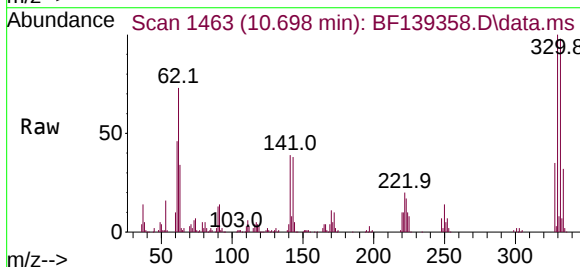


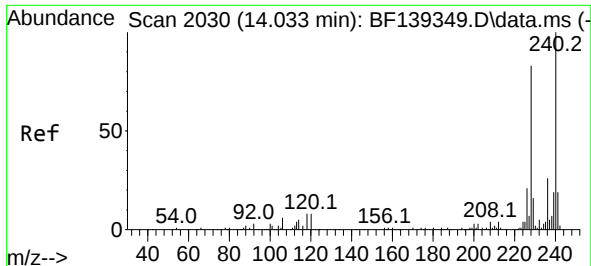

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.027 min Scan# 2030
Delta R.T. -0.006 min
Lab File: BF139358.D
Acq: 14 Sep 2024 09:58




Instrument :
BNA_F
ClientSampleId :
PB163293BL


Tgt Ion:240 Resp: 219748
Ion Ratio Lower Upper
240 100
120 8.7 6.2 9.2
236 25.8 20.9 31.3

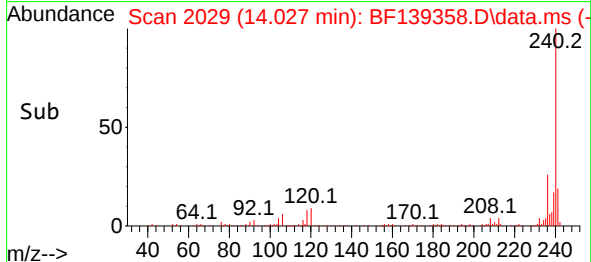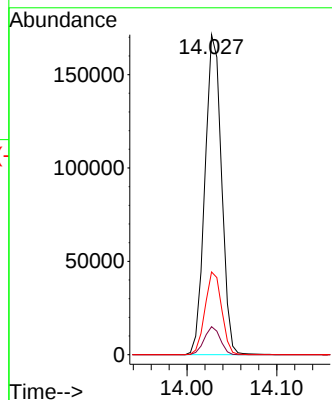

#77
Benzidine
Concen: 5.478 ng
RT: 12.980 min Scan# 1851
Delta R.T. 0.253 min
Lab File: BF139358.D
Acq: 14 Sep 2024 09:58

Tgt Ion:184 Resp: 17247
Ion Ratio Lower Upper
184 100
185 16.3 11.5 17.3
183 6.1 8.9 13.3#

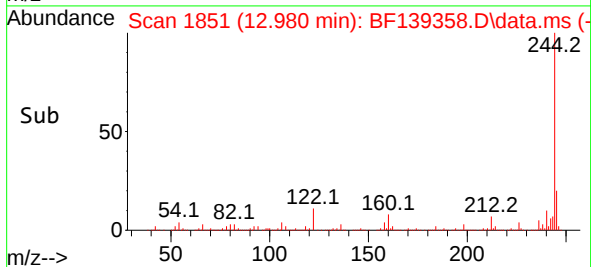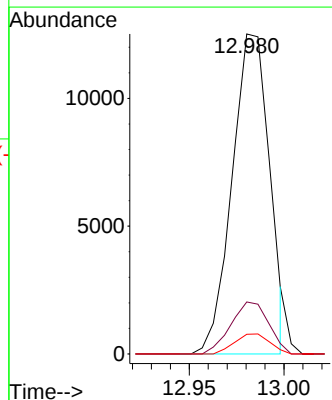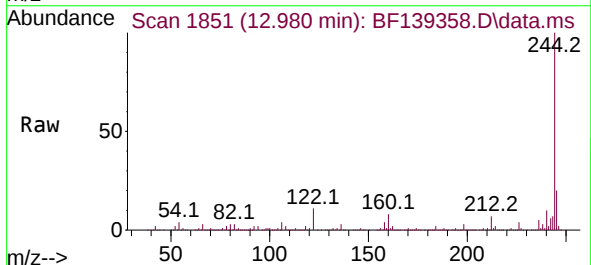



#79

Terphenyl-d14

Concen: 85.431 ng

RT: 12.986 min Scan# 11

Delta R.T. 0.006 min

Lab File: BF139358.D


Acq: 14 Sep 2024 09:58

Instrument :

BNA_F

ClientSampleId :

PB163293BL

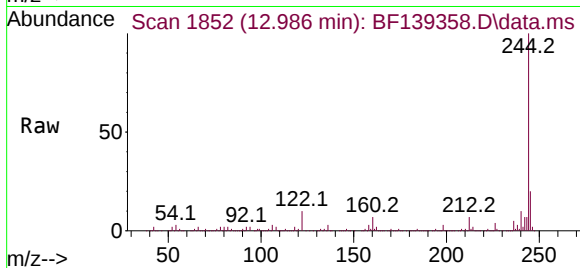




Tgt Ion:244 Resp: 1143742

Ion Ratio Lower Upper

244 100

212 7.3 6.0 9.0

122 10.2 7.6 11.4

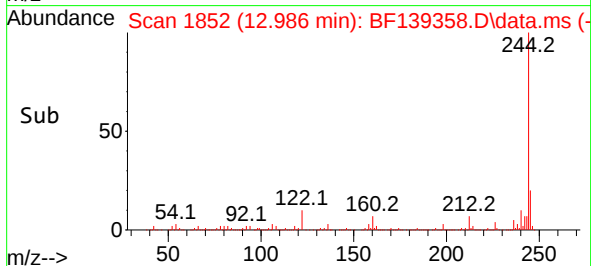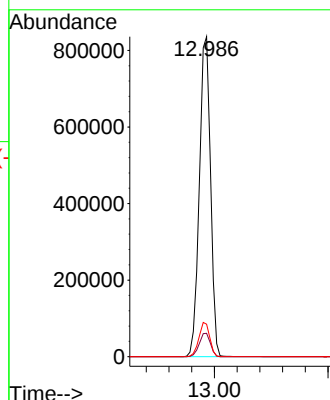

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.498 min Scan# 2279

Delta R.T. -0.000 min

Lab File: BF139358.D

Acq: 14 Sep 2024 09:58

Tgt Ion:264 Resp: 181316

Ion Ratio Lower Upper

264 100

260 23.8 19.5 29.3

265 21.0 16.6 25.0

