


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091424\
Data File : BF139356.D
Acq On : 14 Sep 2024 09:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Sep 14 02:58:23 2024

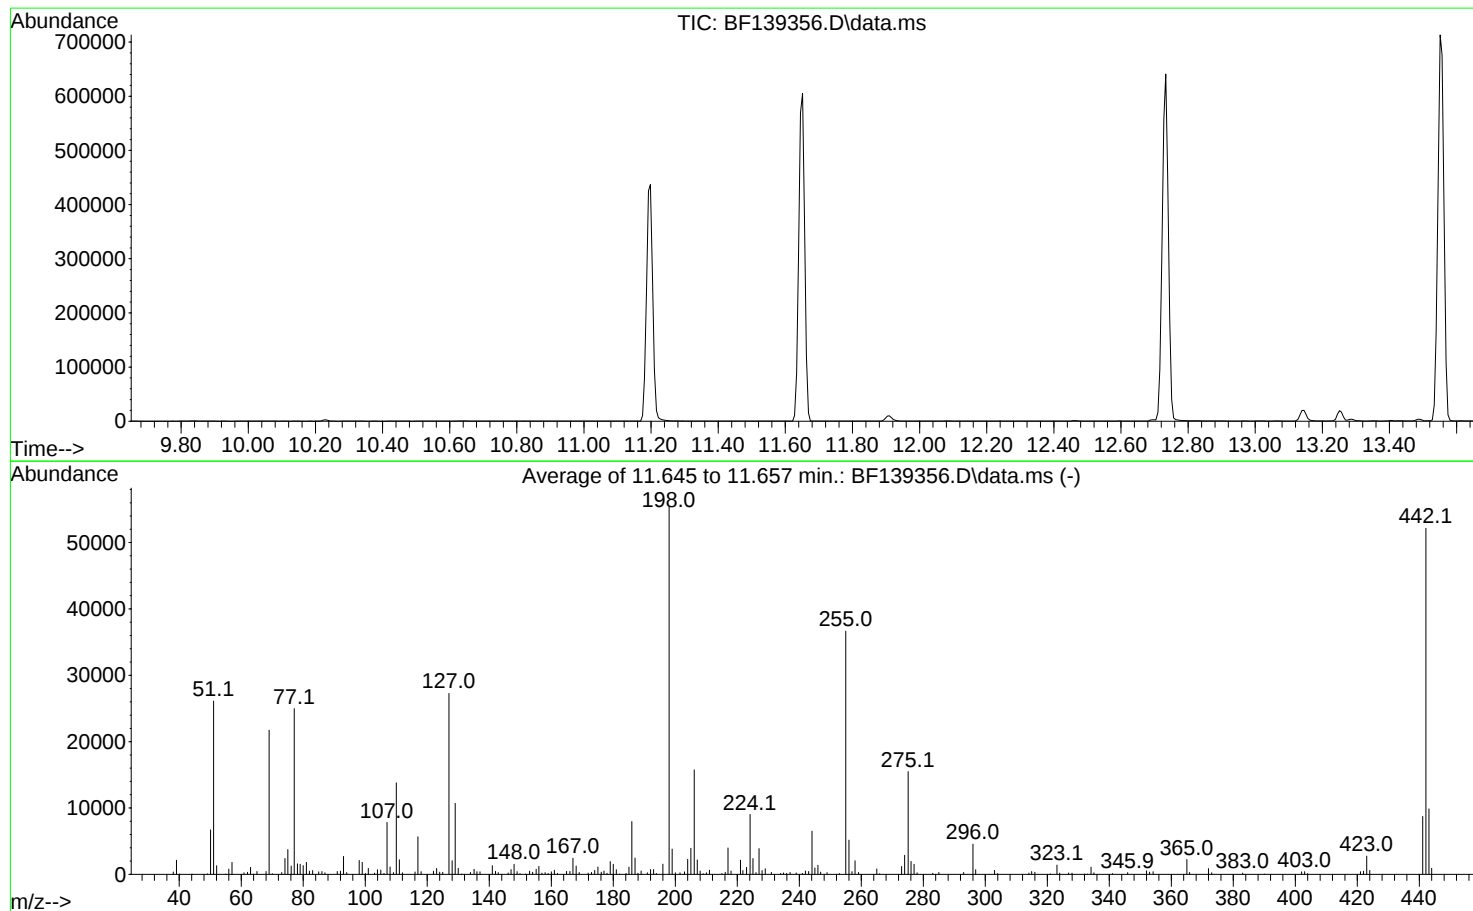




AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.1	26103	PASS
68	69	0.00	2	2.0	426	PASS
69	198	0.00	100	39.2	21725	PASS
70	69	0.00	2	0.5	108	PASS
127	198	10	80	49.2	27277	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55435	PASS
199	198	5	9	6.9	3823	PASS
275	198	10	60	27.9	15485	PASS
365	198	1	100	4.1	2250	PASS
441	198	0.01	100	15.7	8720	PASS
442	442	50	100	100.0	52155	PASS
443	442	15	24	18.9	9858	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091424\
Data File : BF139356.D
Acq On : 14 Sep 2024 09:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 16 02:01:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 14 02:58:23 2024
Response via : Initial Calibration

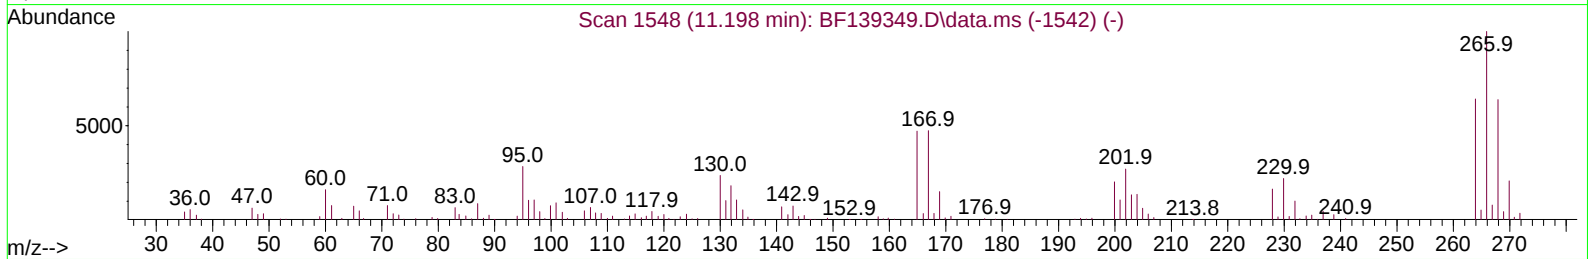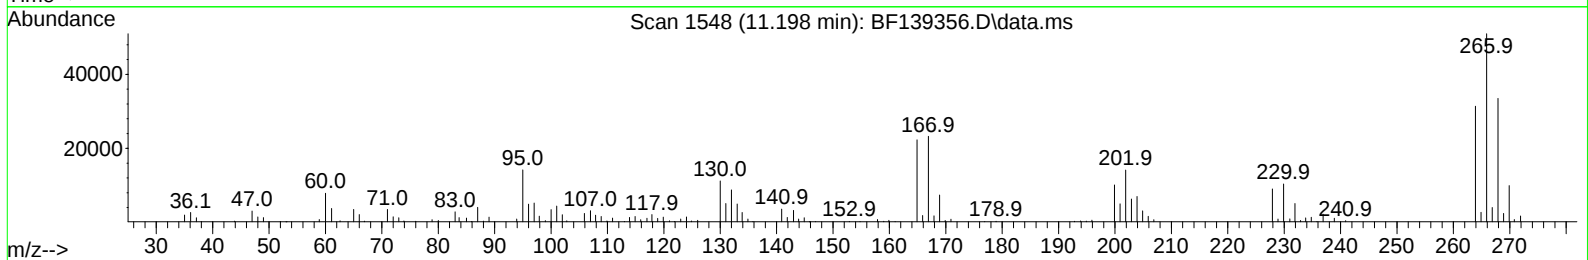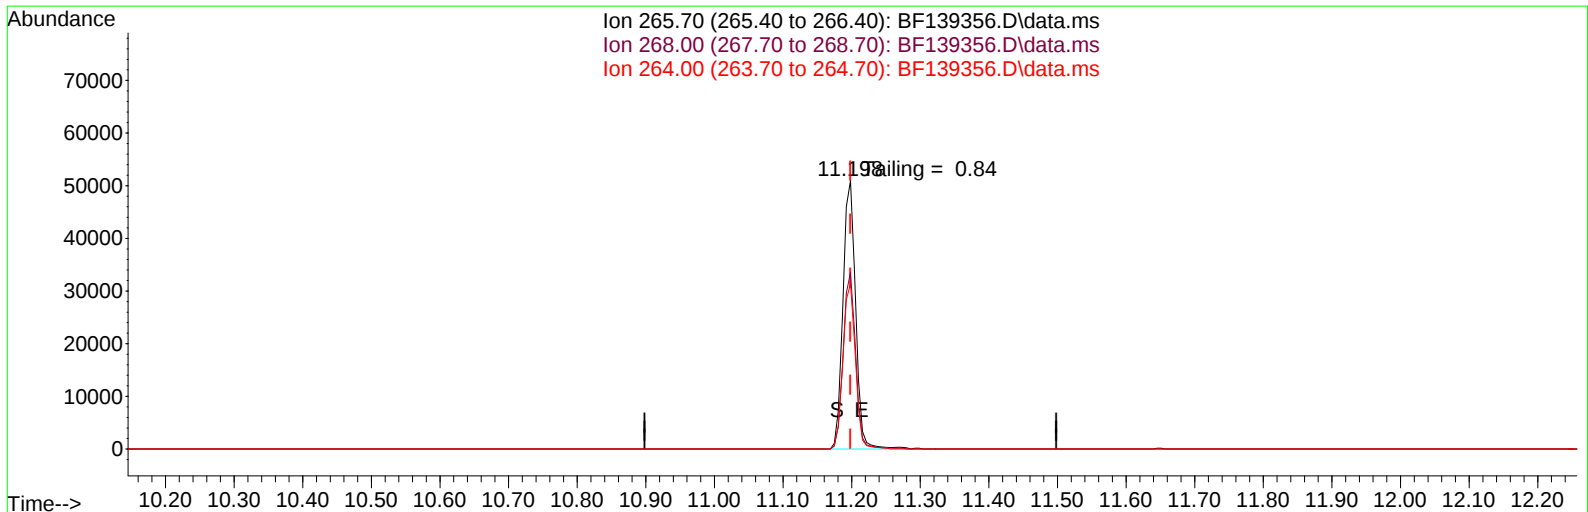

TIC: BF139356.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.000) 52901.37 ng




response 64976

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	65.69
264.00	64.20	61.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091424\
Data File : BF139356.D
Acq On : 14 Sep 2024 09:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 16 02:01:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 14 02:58:23 2024
Response via : Initial Calibration

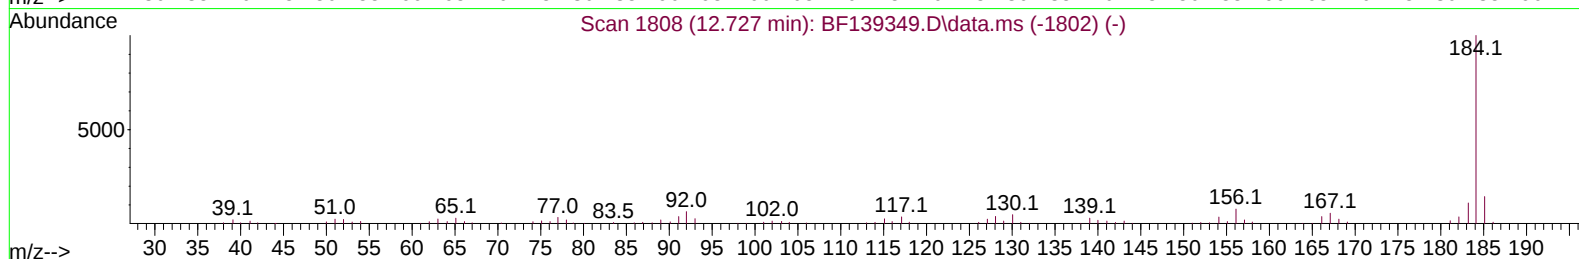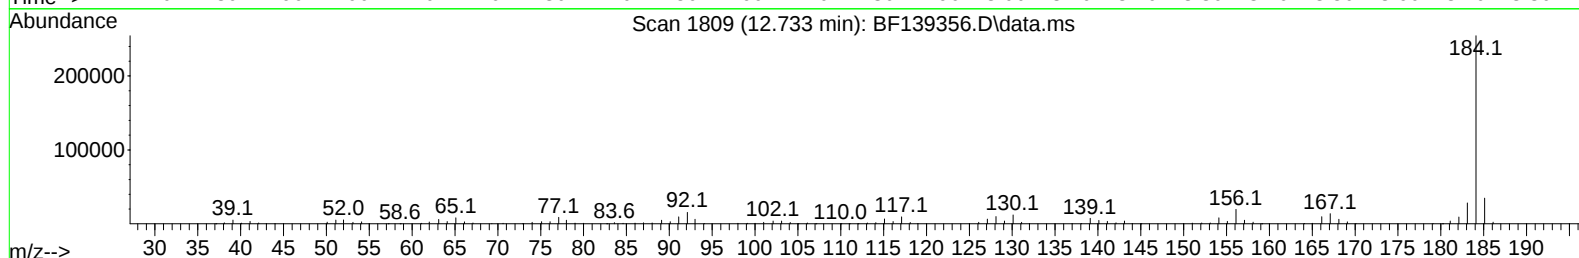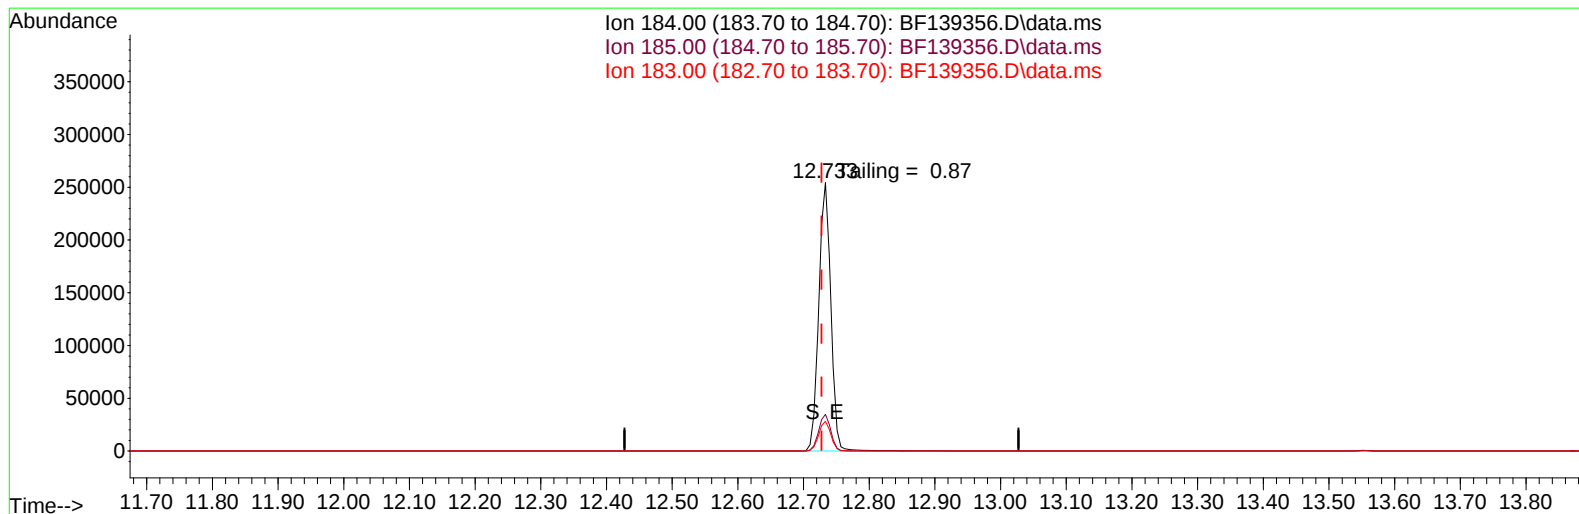

TIC: BF139356.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 0.00 ng

response 325485

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.69
183.00	11.10	11.12
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/14/2024	BNA_F	<u>BF139356.D</u>
Compound Name	Response	Retention Time
DDT	169327	13.551
DDD	6908	13.251
DDE	0	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6908	176235	3.92

Instrument :
BNA_F
ClientSampleId :
DFTPP