
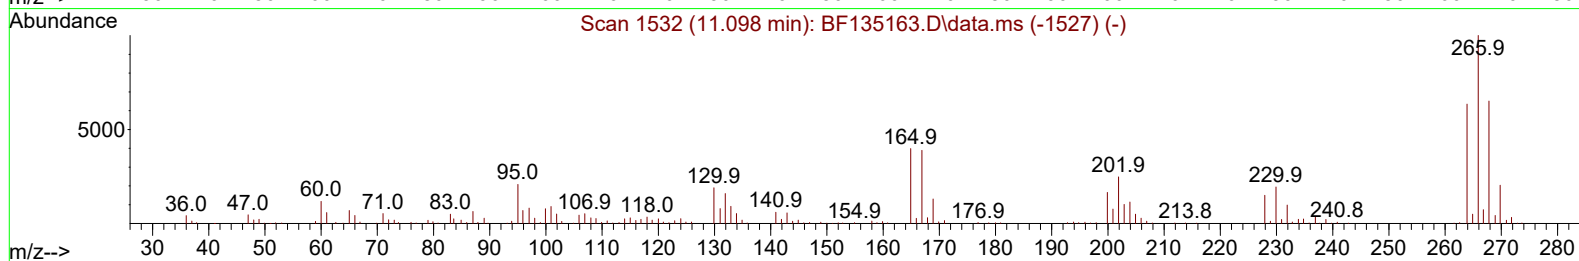
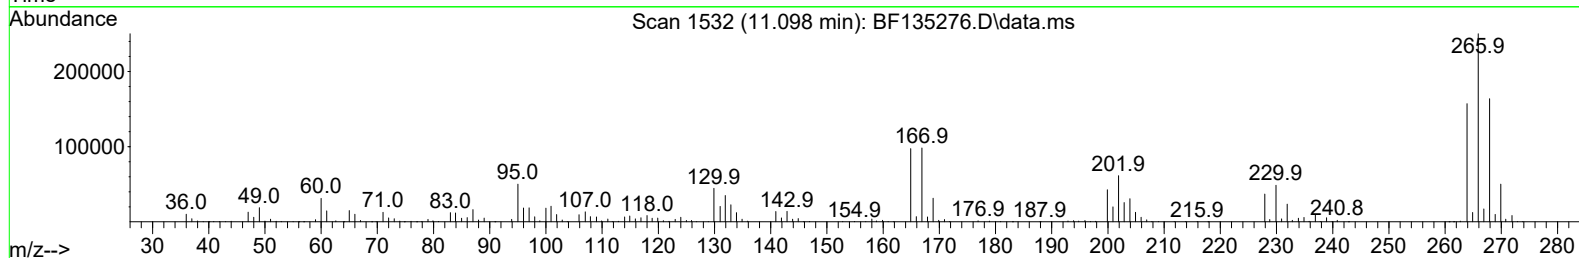


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091523\  
Data File : BF135276.D  
Acq On    : 15 Sep 2023  12:59  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Sep 16 07:27:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

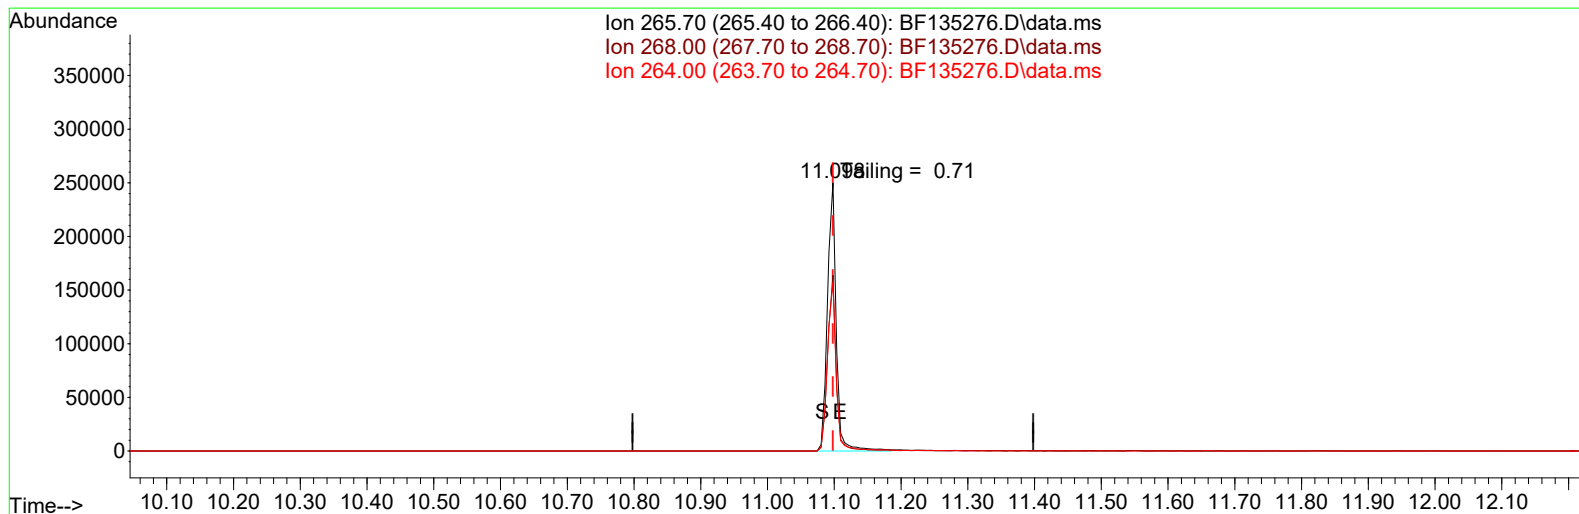

TIC: BF135276.D\data.ms

(70) **Pentachlorophenol (C)**




11.098min (-0.000) 35625.43 ng

response **230439**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	65.46
264.00	63.50	62.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091523\
Data File : BF135276.D
Acq On : 15 Sep 2023 12:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 16 07:27:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

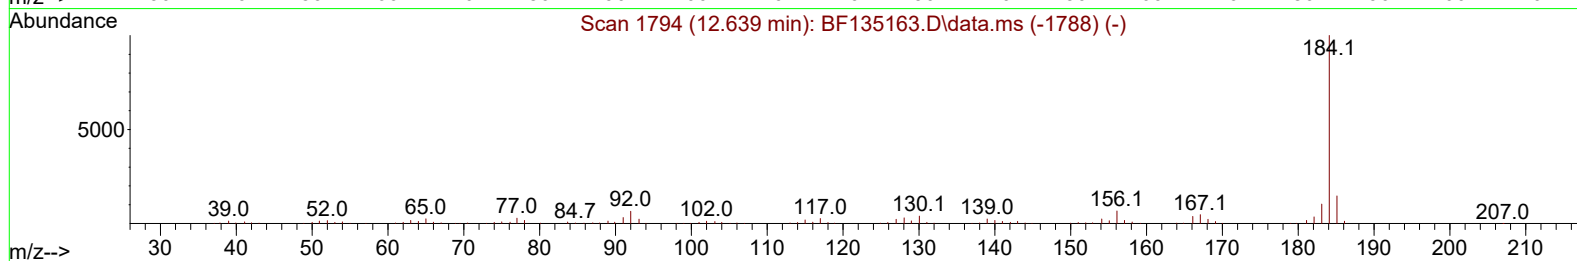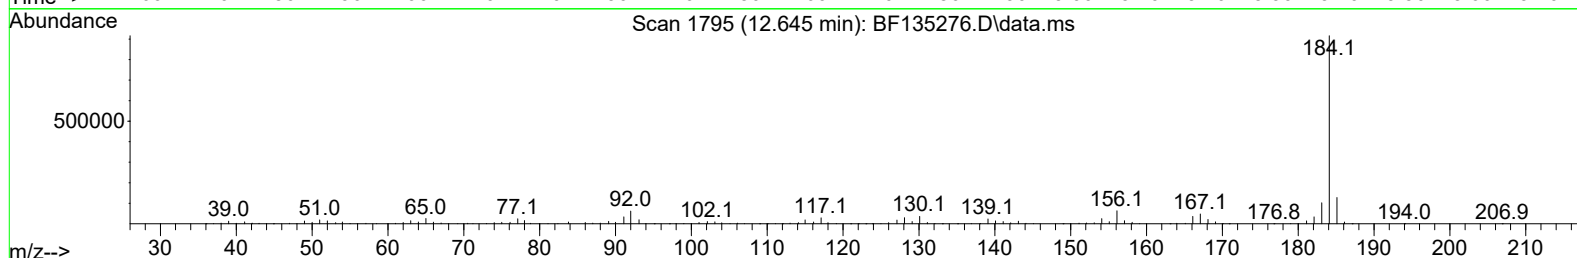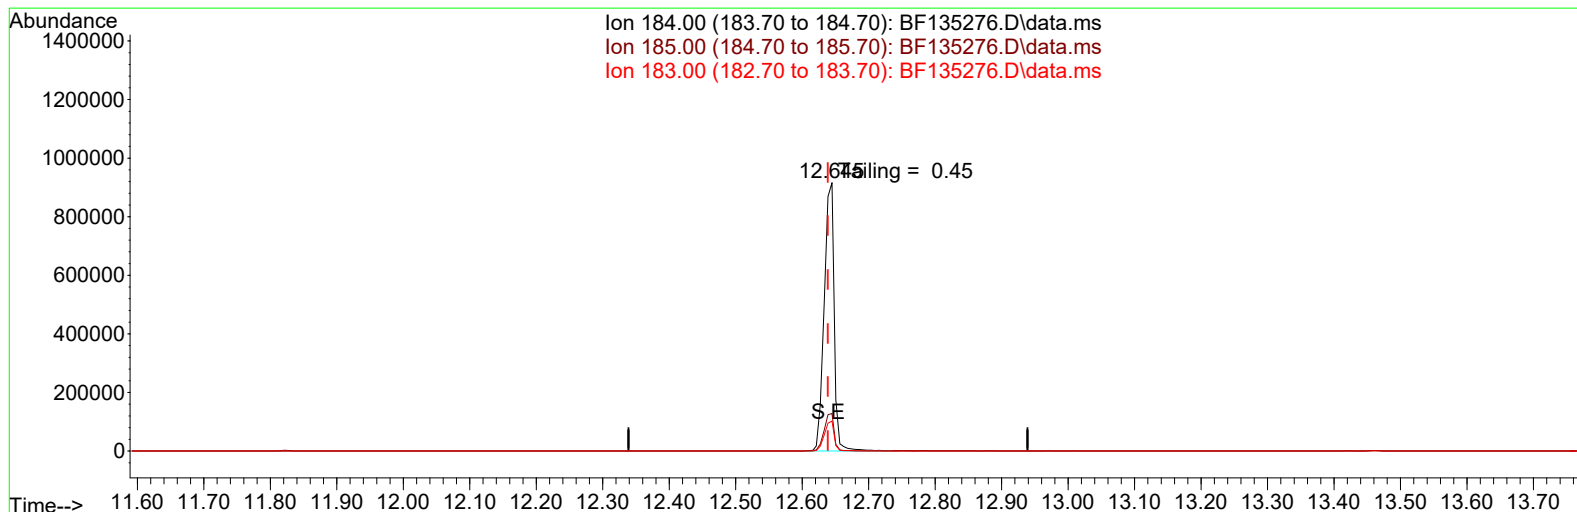

TIC: BF135276.D\data.ms

(77) Benzidine

12.645min (+ 0.006) 25632.04 ng

response 964119

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.99
183.00	10.30	11.14
0.00	0.00	0.00