


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091523\
Data File : BF135276.D
Acq On : 15 Sep 2023 12:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 12 00:19:07 2023

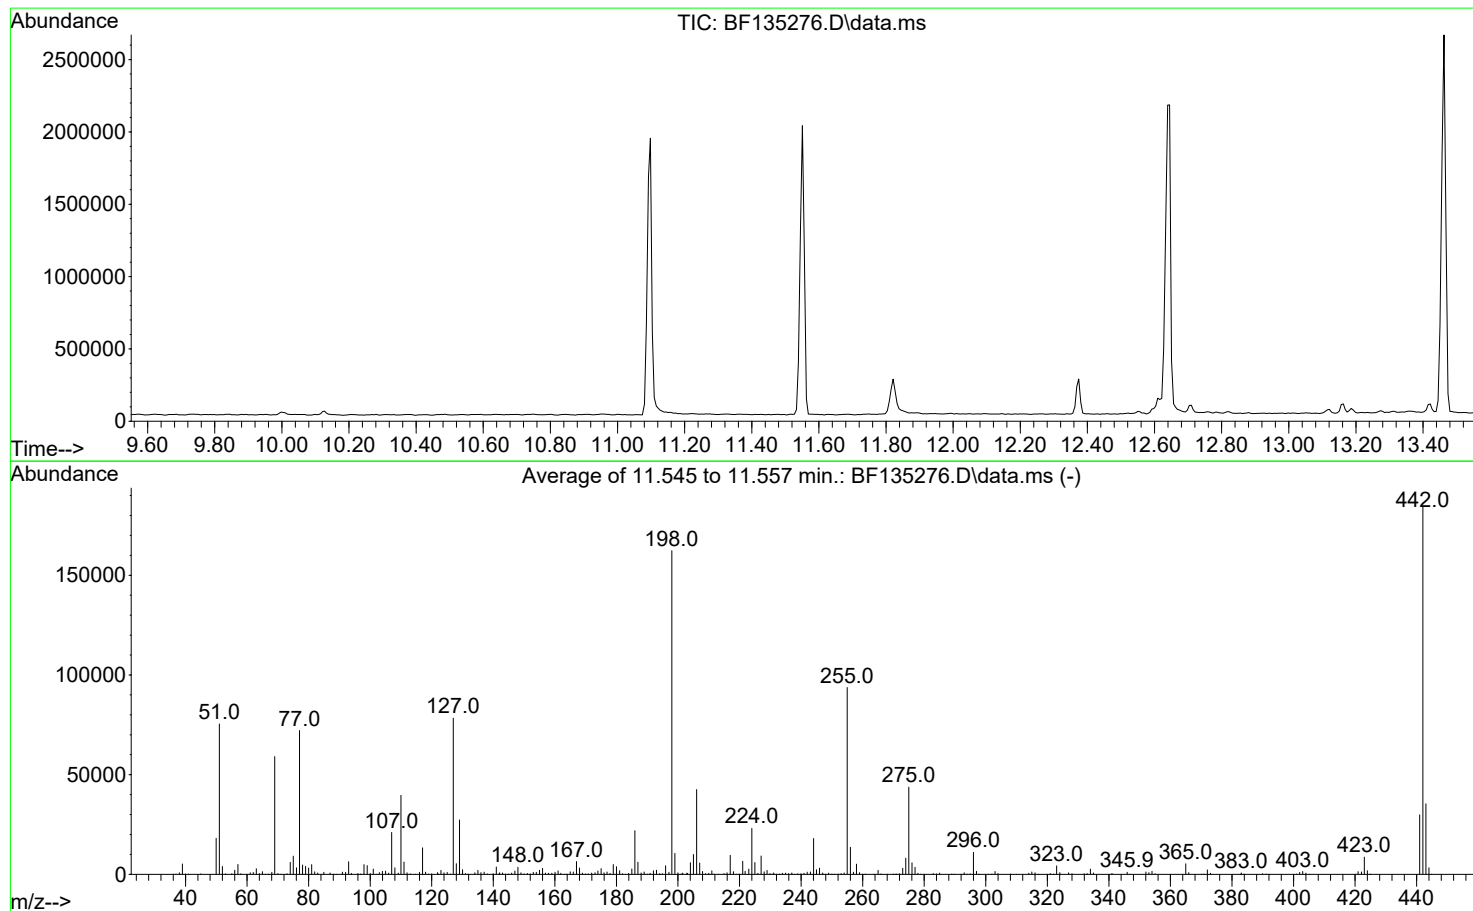

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.5	75468	PASS
68	69	0.00	2	1.8	1070	PASS
69	198	0.00	100	36.4	59024	PASS
70	69	0.00	2	0.7	391	PASS
127	198	10	80	48.3	78347	PASS
197	198	0.00	2	0.6	1038	PASS
198	198	100	100	100.0	162352	PASS
199	198	5	9	6.5	10510	PASS
275	198	10	60	26.9	43709	PASS
365	198	1	100	3.3	5307	PASS
441	198	0.01	100	18.4	29877	PASS
442	442	50	100	100.0	184480	PASS
443	442	15	24	19.2	35419	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/14/2023	BNA_F	<u>BF135276.D</u>
Compound Name	Response	Retention Time
DDT	450569	13.462
DDD	18104	13.162
DDE	1765	12.821
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19869	470438	4.22

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091523\
Data File : BF135276.D
Acq On : 15 Sep 2023 12:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 16 07:27:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

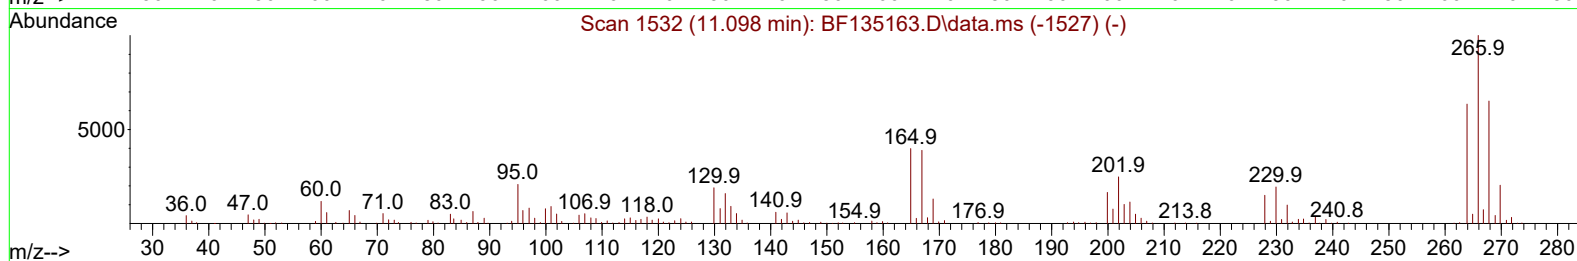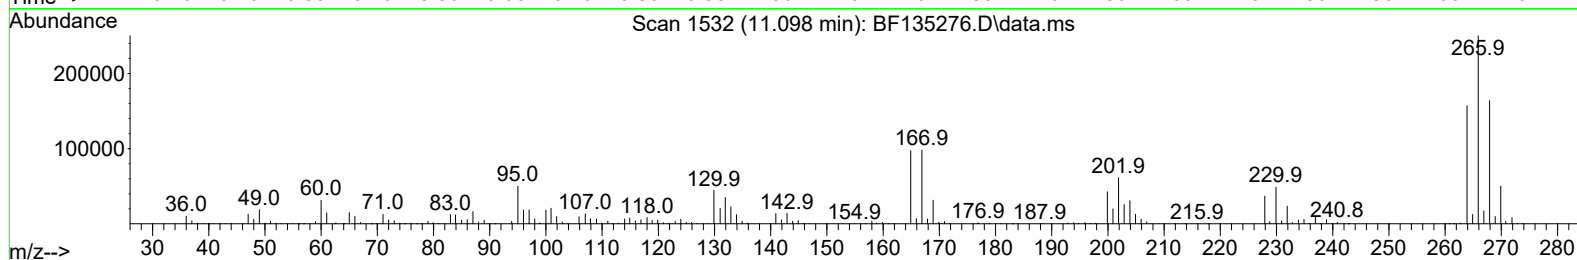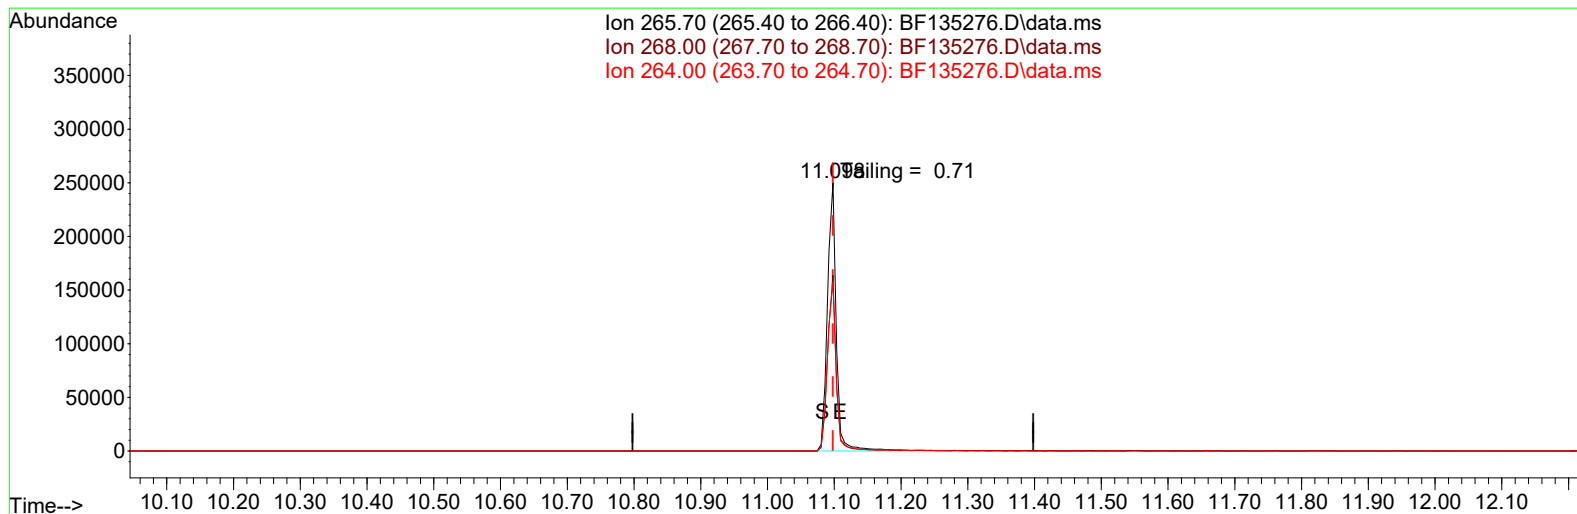

TIC: BF135276.D\data.ms

(70) Pentachlorophenol (C)

11.098min (-0.000) 35625.43 ng




response 230439

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	65.46
264.00	63.50	62.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091523\
Data File : BF135276.D
Acq On : 15 Sep 2023 12:59
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 16 07:27:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

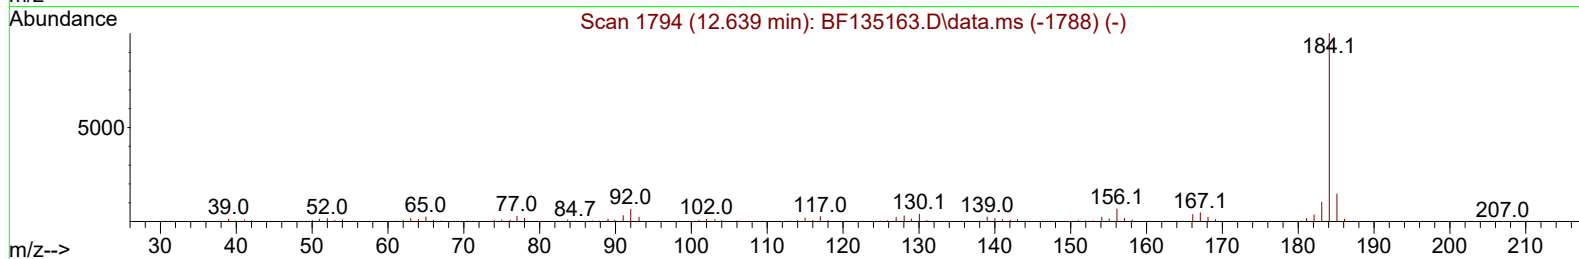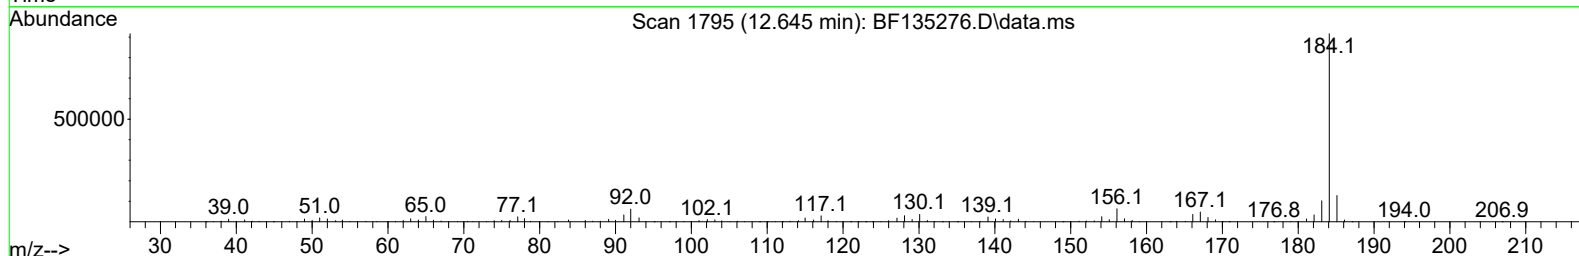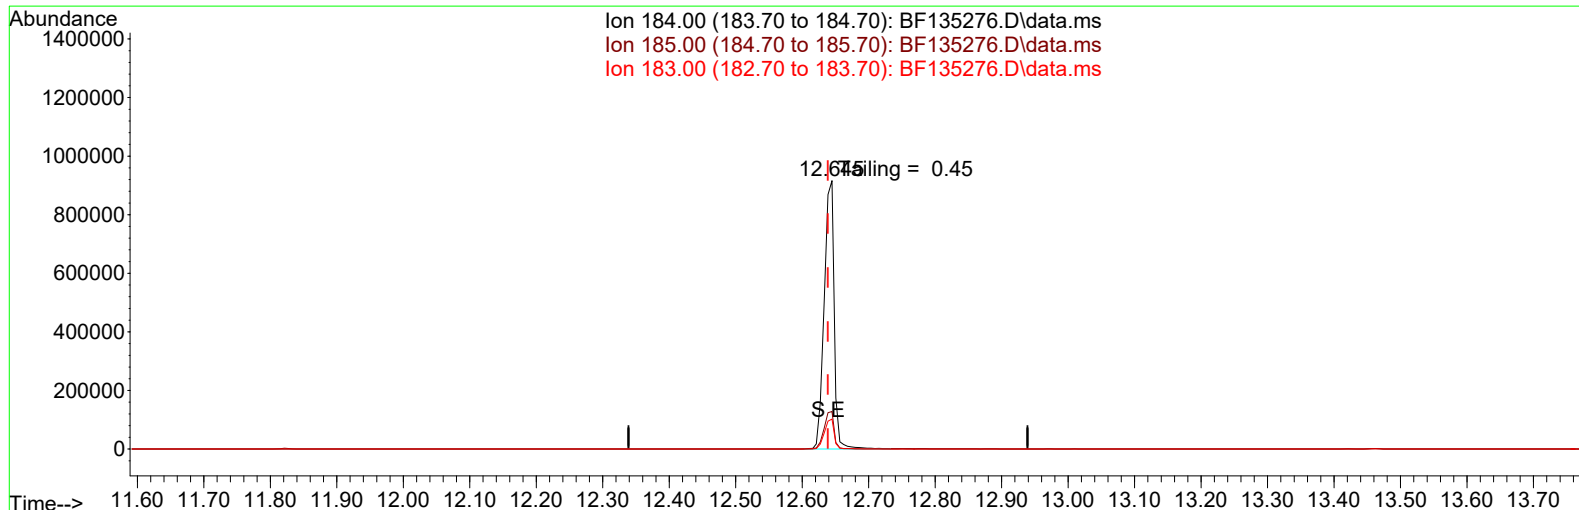

TIC: BF135276.D\data.ms

(77) Benzidine

12.645min (+ 0.006) 25632.04 ng

response 964119

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.99
183.00	10.30	11.14
0.00	0.00	0.00