

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091619\
 Data File : BF117052.D
 Acq On : 16 Sep 2019 10:22
 Operator : HP/JU
 Sample : PB123054BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB123054BL

Quant Time: Sep 16 11:53:36 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 13 16:23:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.82	152	79736	20.00	ng	0.00
21) Naphthalene-d8	8.10	136	315082	20.00	ng	0.00
39) Acenaphthene-d10	9.85	164	162786	20.00	ng	0.00
64) Phenanthrene-d10	11.33	188	274876	20.00	ng	0.00
76) Chrysene-d12	13.96	240	182079	20.00	ng	-0.01
87) Perylene-d12	15.41	264	142715	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.46	112	611049	119.64	ng	0.02
7) Phenol-d6	6.46	99	818584	124.02	ng	0.00
23) Nitrobenzene-d5	7.39	82	533305	88.93	ng	0.00
42) 2,4,6-Tribromophenol	10.64	330	178381	131.11	ng	0.00
45) 2-Fluorobiphenyl	9.17	172	946120	90.88	ng	0.00
79) Terphenyl-d14	12.92	244	952370	97.77	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091619\
Data File : BF117052.D
Acq On : 16 Sep 2019 10:22
Operator : HP/JU
Sample : PB123054BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB123054BL

Quant Time: Sep 16 11:53:36 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 13 16:23:17 2019
Response via : Initial Calibration

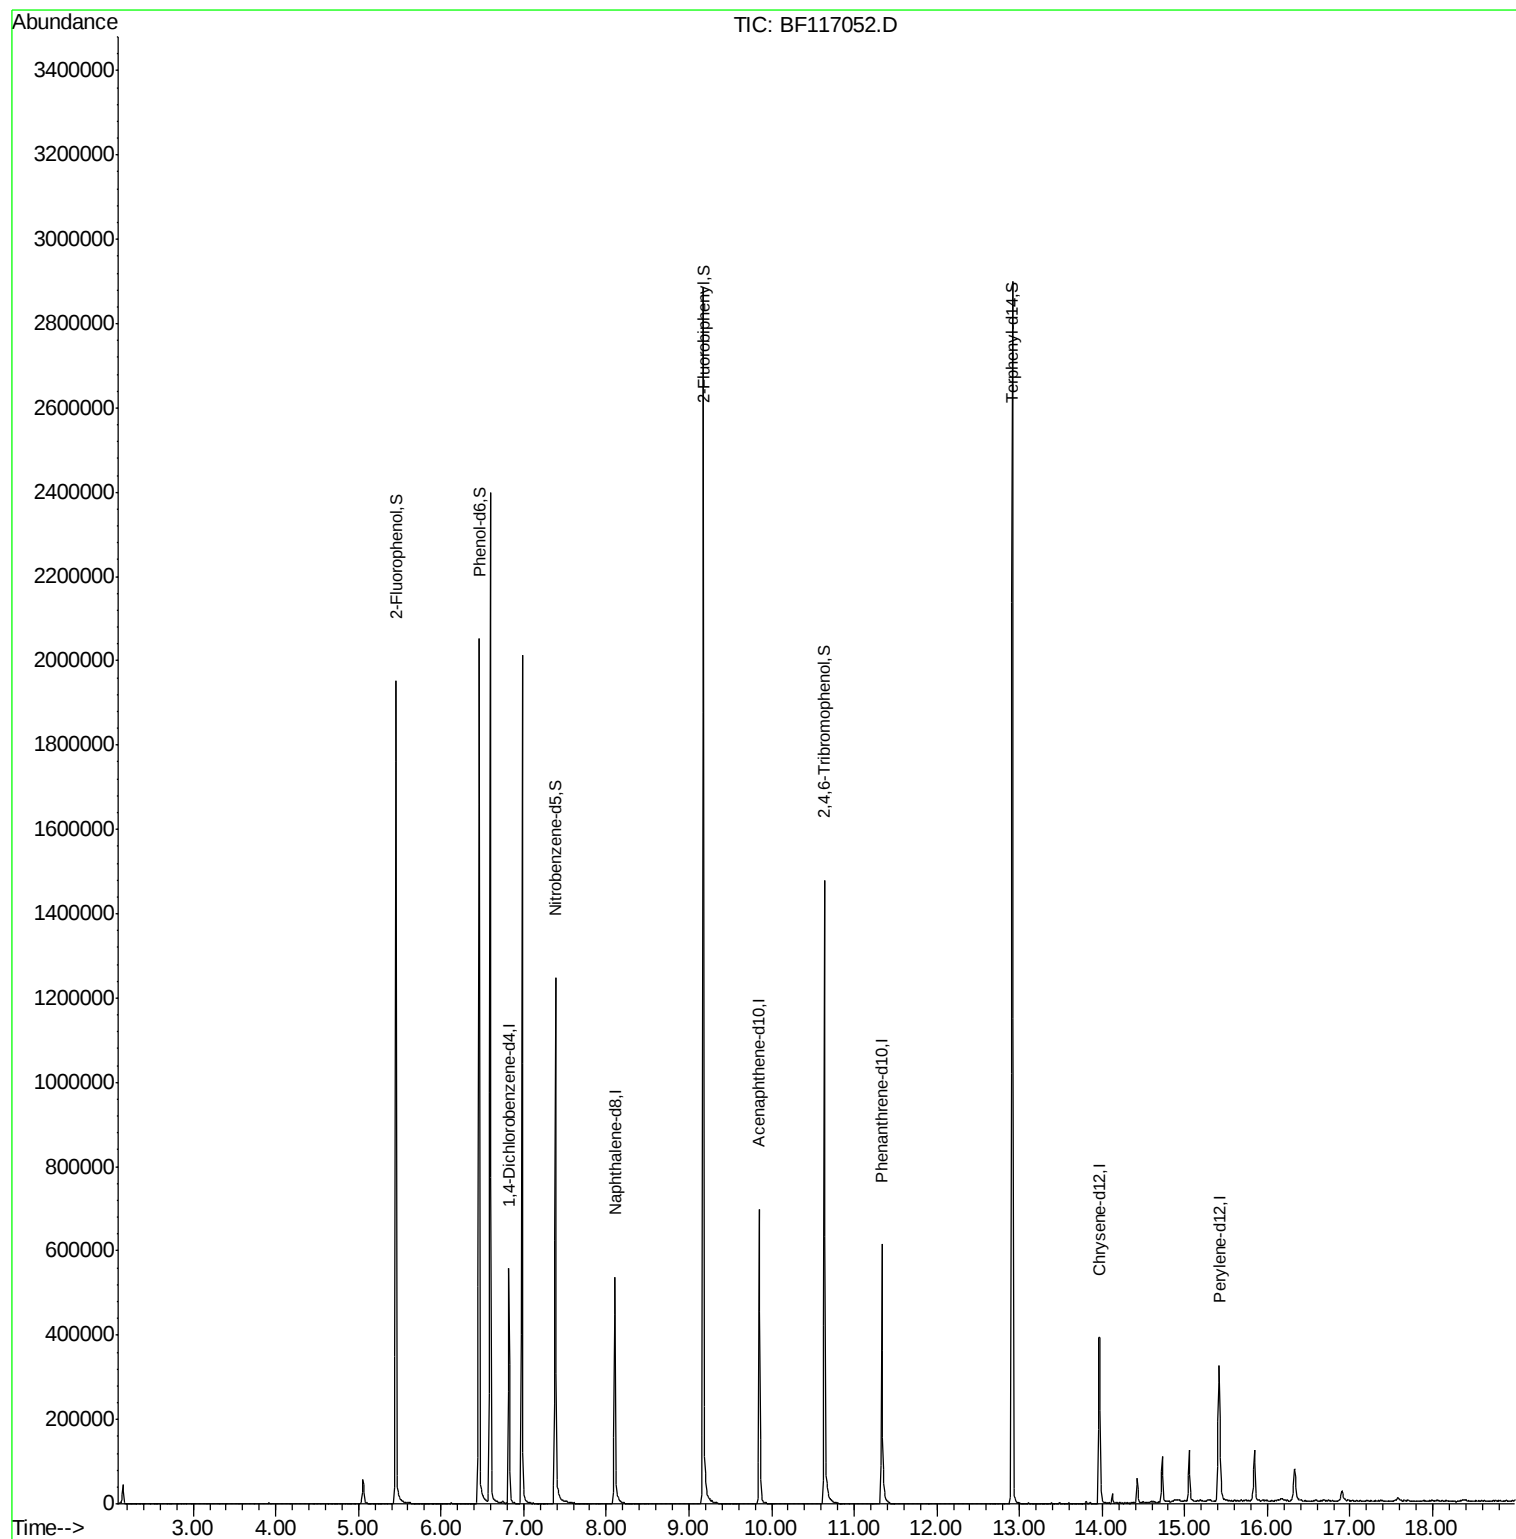




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.82 min Scan# 805
Delta R.T. 0.00 min
Lab File: BF117052.D
Acq: 16 Sep 2019 10:22

Instrument :
BNA_F
ClientSampleId :
PB123054BL

Tot Ion:152 Resp: 79736
Ion Ratio Lower Upper
152 100
150 161.7 127.5 191.3
115 66.5 55.0 82.4

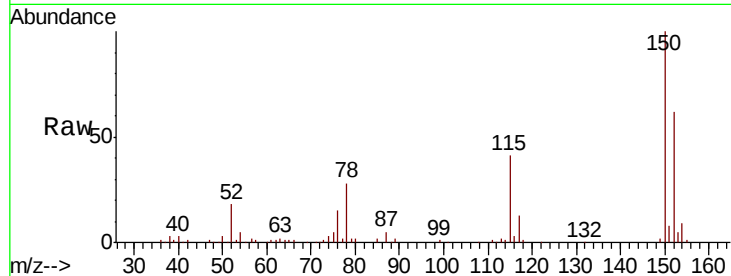


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

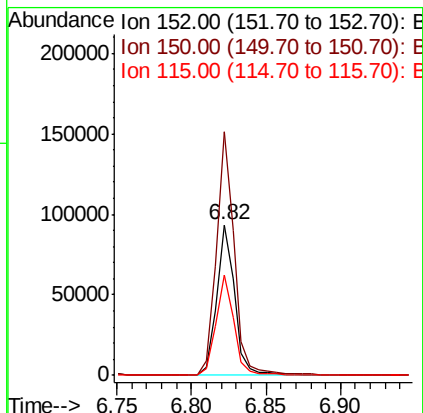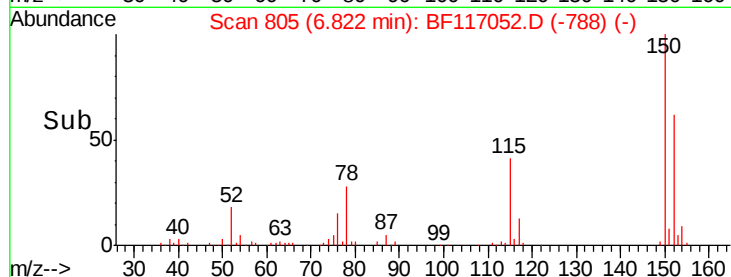



#5

2-Fluorophenol
Concen: 119.645 ng
RT: 5.46 min Scan# 573
Delta R.T. 0.02 min
Lab File: BF117052.D
Acq: 16 Sep 2019 10:22

Tgt Ion:112 Resp: 611049
Ion Ratio Lower Upper
112 100
64 54.0 45.7 68.5
63 29.2 24.9 37.3

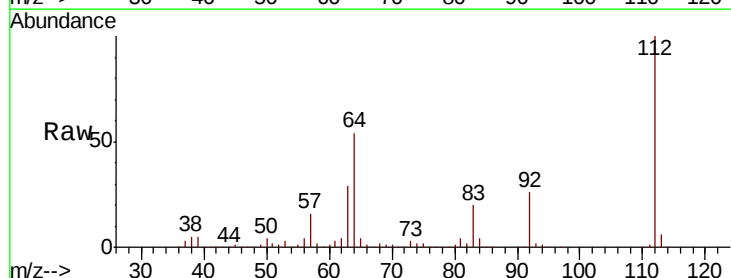

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

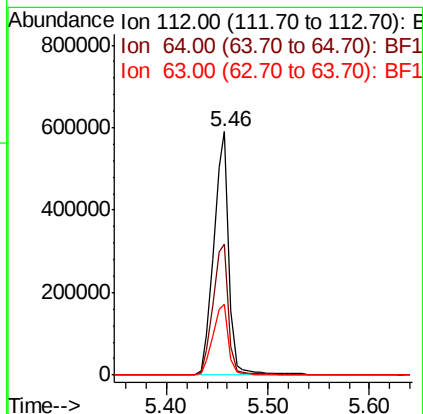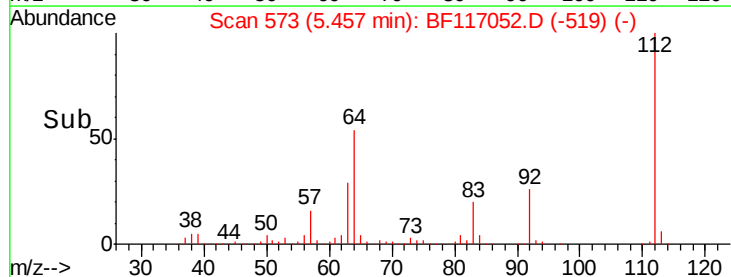



#7

Phenol-d6

Concen: 124.022 ng

RT: 6.46 min Scan# 744

Delta R.T. 0.01 min

Lab File: BF117052.D

Acq: 16 Sep 2019 10:22

Instrument :

BNA_F

ClientSampleId :

PB123054BL


Tot Ion: 99 Resp: 818584

Ion Ratio Lower Upper




99 100

42 15.5 12.2 18.2

71 37.5 29.8 44.8

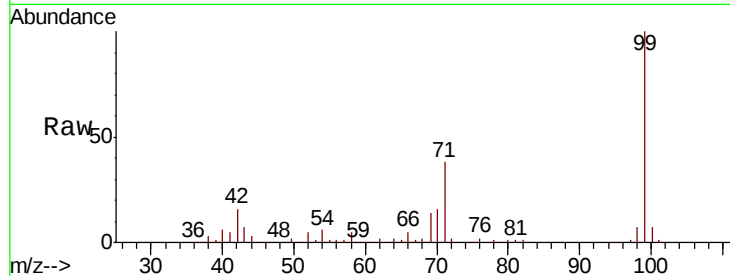

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

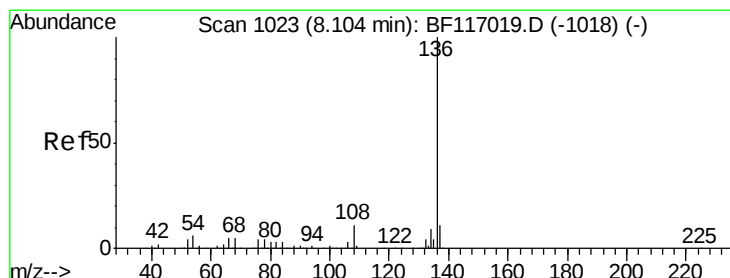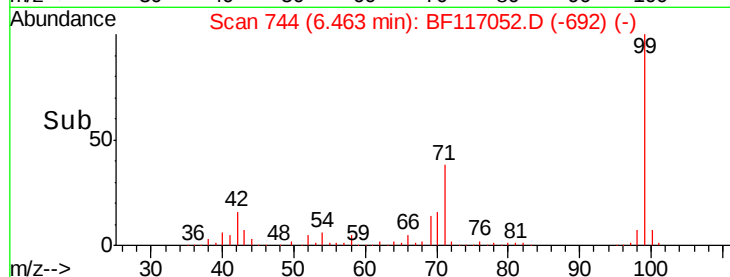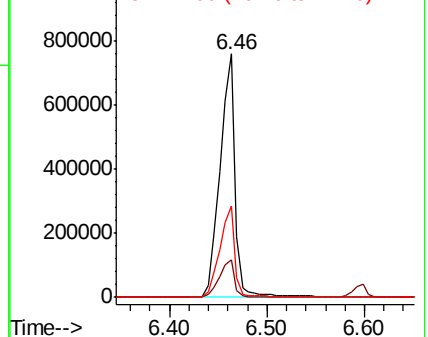

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.10 min Scan# 1023

Delta R.T. 0.00 min

Lab File: BF117052.D

Acq: 16 Sep 2019 10:22

Tgt Ion: 136 Resp: 315082


Ion Ratio Lower Upper

136 100



137 10.3 9.0 13.4

54 4.7 4.5 6.7

68 4.3 4.0 6.0

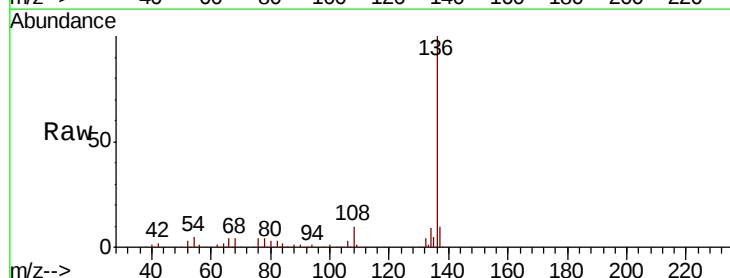

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1



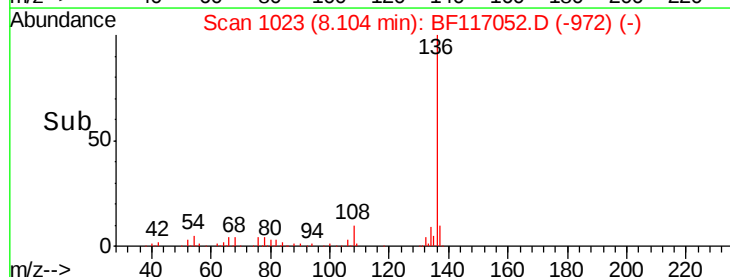
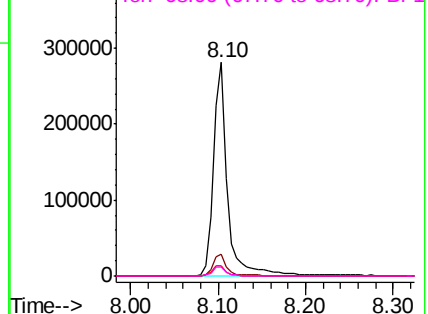




#23
 Nitrobenzene-d5
 Concen: 88.933 ng
 RT: 7.39 min Scan# 901
 Delta R.T. 0.00 min
 Lab File: BF117052.D
 Acq: 16 Sep 2019 10:22




Instrument :
 BNA_F
 ClientSampleId :
 PB123054BL

Tot Ion	82	Resp	533305
Ion Ratio	100	Lower	Upper
128	43.3	32.3	48.5
54	40.5	33.3	49.9

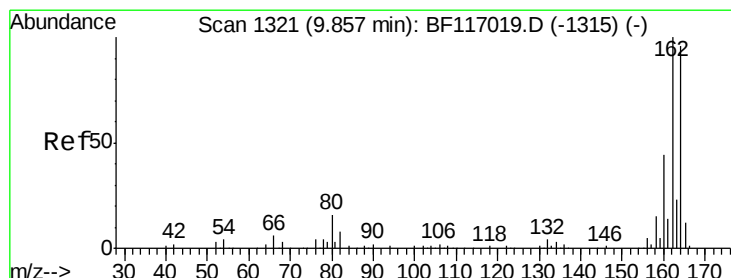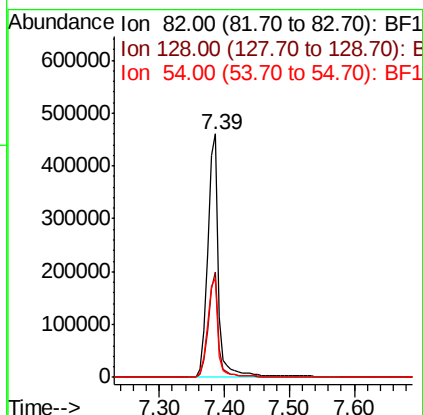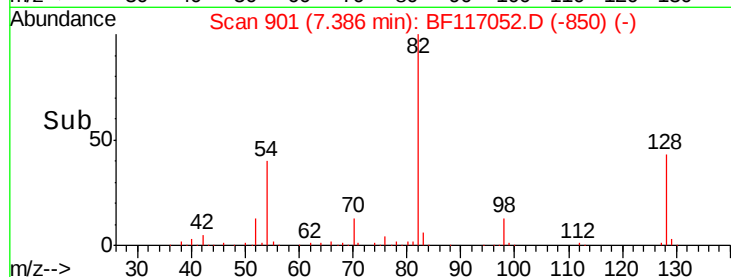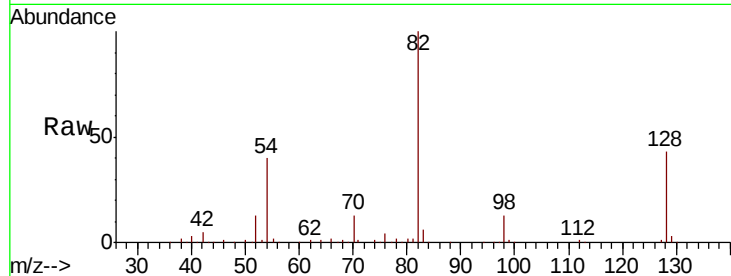

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.85 min Scan# 1320
 Delta R.T. -0.01 min
 Lab File: BF117052.D
 Acq: 16 Sep 2019 10:22

Tgt Ion	164	Resp	162786
Ion Ratio <td>100</td> <td>Lower</td> <td>Upper</td>	100	Lower	Upper
162	105.6	83.4	125.2
160	45.2	36.4	54.6

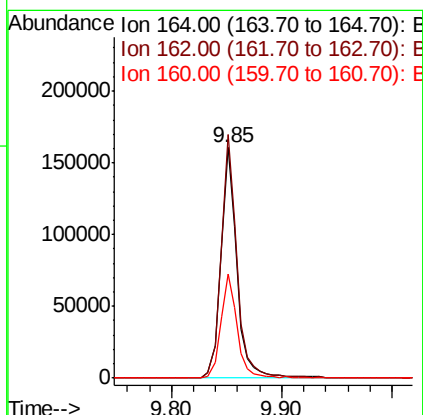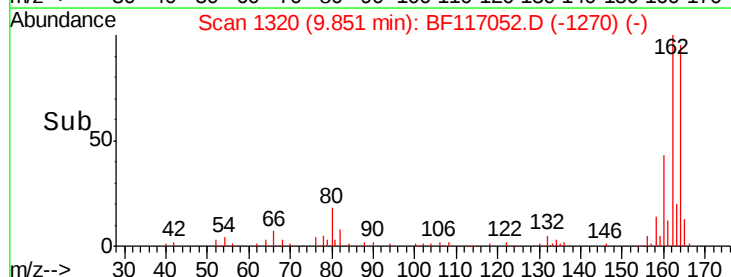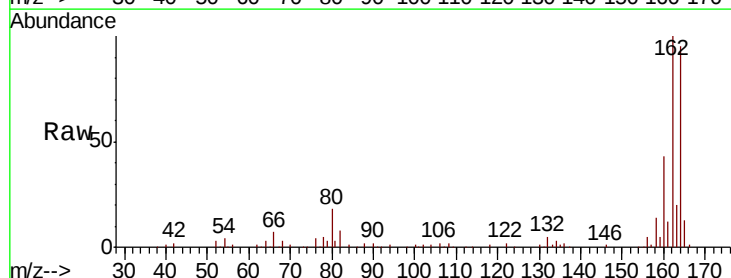




#42
 2,4,6-Tribromophenol
 Concen: 131.113 ng
 RT: 10.64 min Scan# 1454
 Delta R.T. -0.01 min
 Lab File: BF117052.D
 Acq: 16 Sep 2019 10:22

Instrument :
 BNA_F
 ClientSampleId :
 PB123054BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.0	78.0	117.0
141	44.3	35.8	53.6



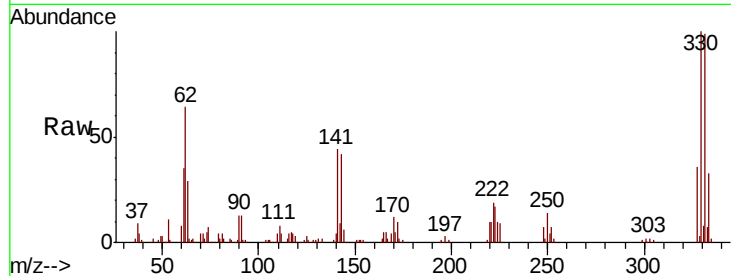


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

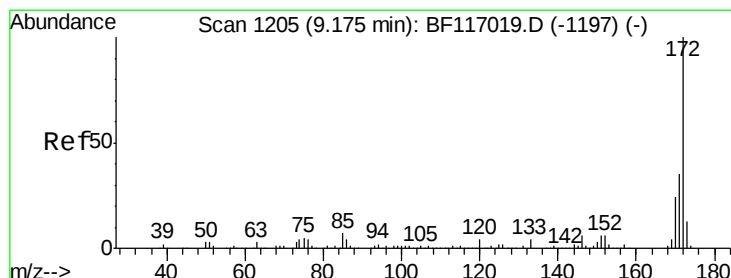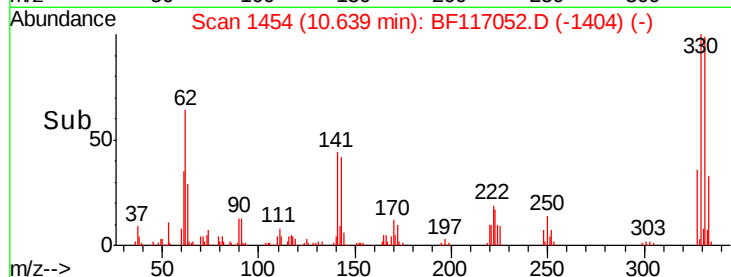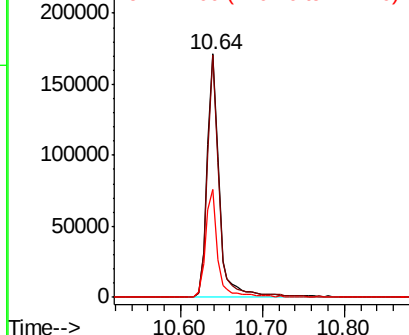

#45
 2-Fluorobiphenyl
 Concen: 90.876 ng
 RT: 9.17 min Scan# 1205
 Delta R.T. 0.00 min
 Lab File: BF117052.D
 Acq: 16 Sep 2019 10:22

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.1	28.2	42.2
170	23.7	18.9	28.3


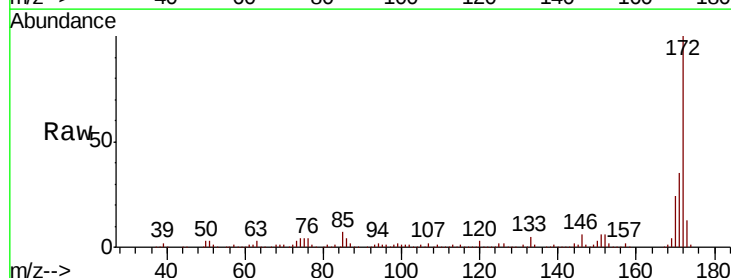



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

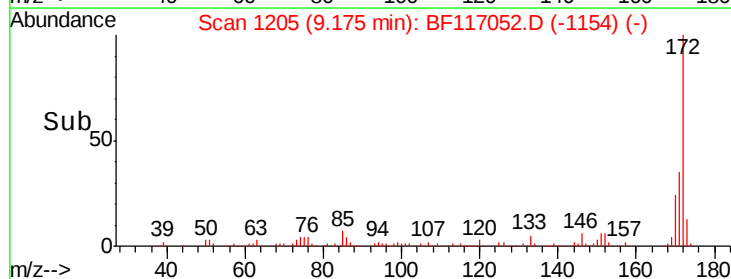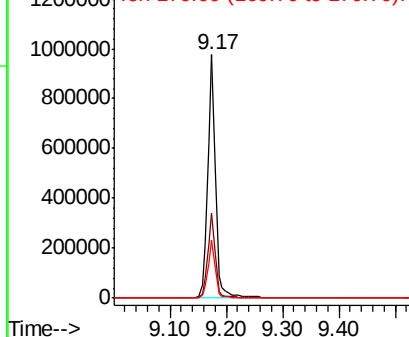

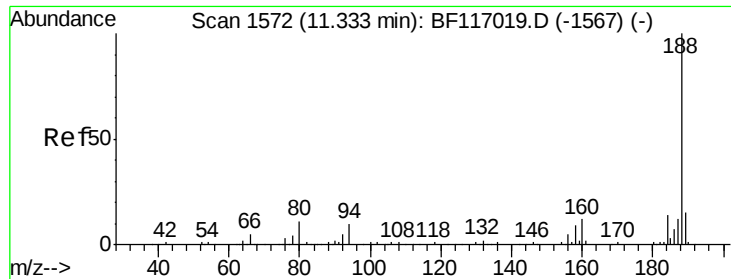

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.33 min Scan# 1572

Delta R.T. 0.00 min

Lab File: BF117052.D

Acq: 16 Sep 2019 10:22

Instrument :

BNA_F

ClientSampleId :

PB123054BL



Tot Ion:188 Resp: 274876

Ion Ratio Lower Upper

188 100

94 8.6 8.2 12.2



80 10.0 9.0 13.6

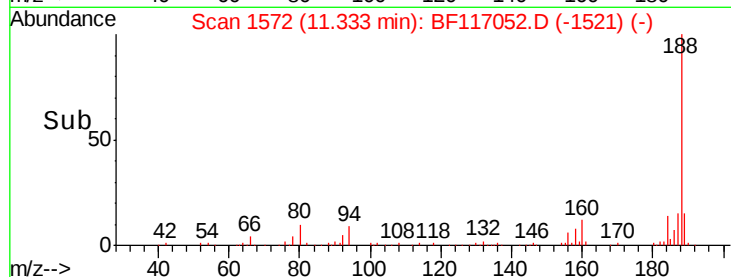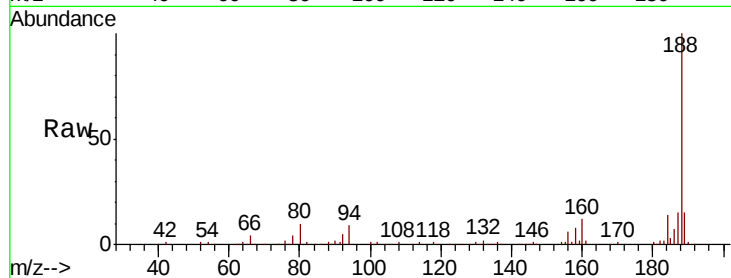

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

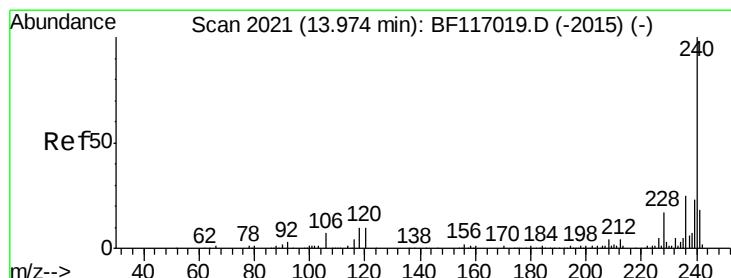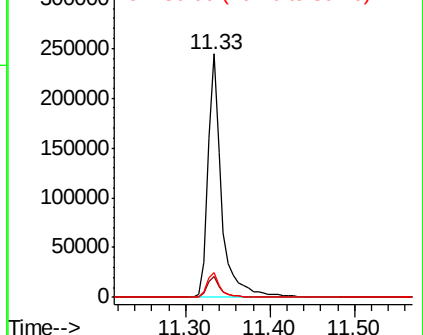

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.96 min Scan# 2019

Delta R.T. -0.01 min

Lab File: BF117052.D

Acq: 16 Sep 2019 10:22



Tgt Ion:240 Resp: 182079

Ion Ratio Lower Upper

240 100

120 12.2 8.3 12.5


236 24.7 20.3 30.5

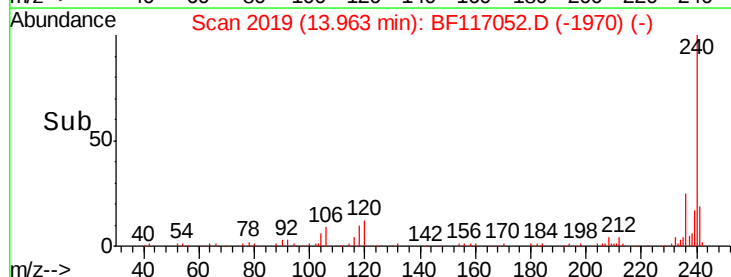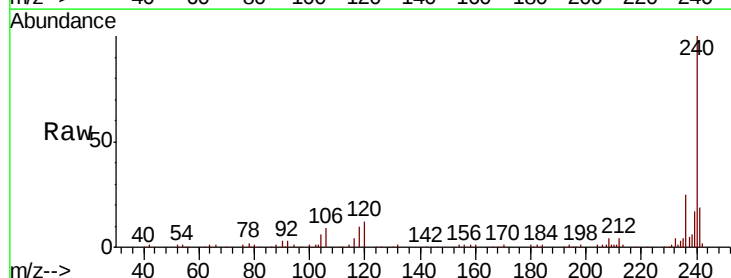


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E




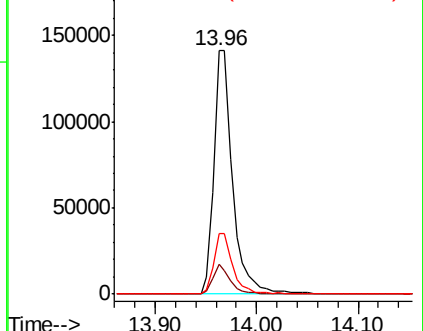


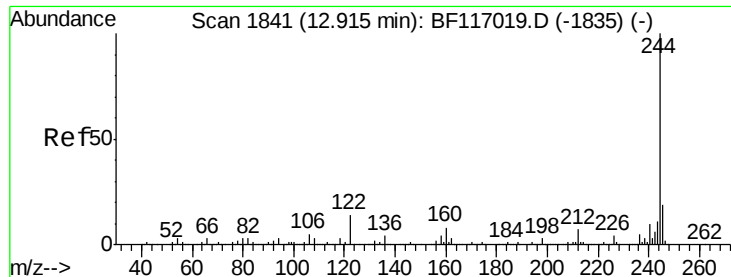

#79
 Terphenyl-d14
 Concen: 97.770 ng
 RT: 12.92 min Scan# 1841
 Delta R.T. 0.00 min
 Lab File: BF117052.D
 Acq: 16 Sep 2019 10:22

Instrument :
 BNA_F
 ClientSampleId :
 PB123054BL

Tot Ion:244 Resp: 952370
 Ion Ratio Lower Upper
 244 100
 212 7.1 5.8 8.8
 122 13.5 11.3 16.9

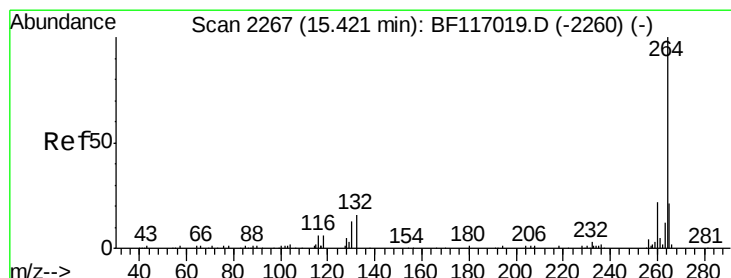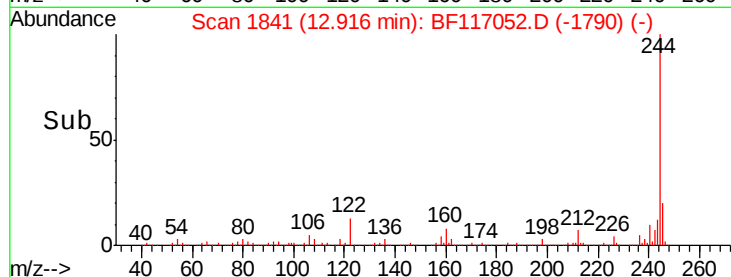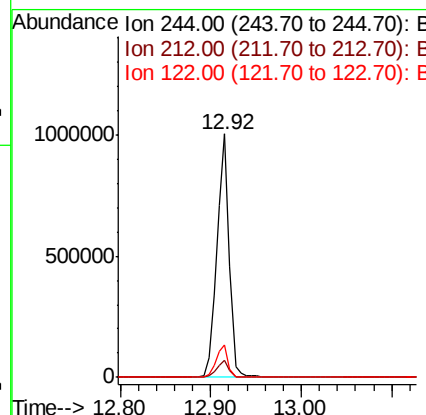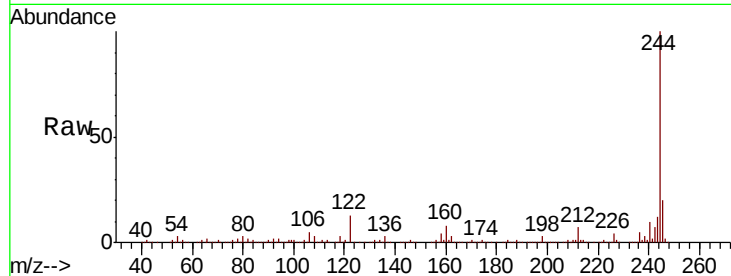

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.41 min Scan# 2265
 Delta R.T. -0.01 min
 Lab File: BF117052.D
 Acq: 16 Sep 2019 10:22

Tgt Ion:264 Resp: 142715
 Ion Ratio Lower Upper
 264 100
 260 23.9 17.6 26.4
 265 21.6 16.6 24.8

