


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091619\
 Data File : BF117048.D
 Acq On : 16 Sep 2019 8:05
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 13 16:23:17 2019

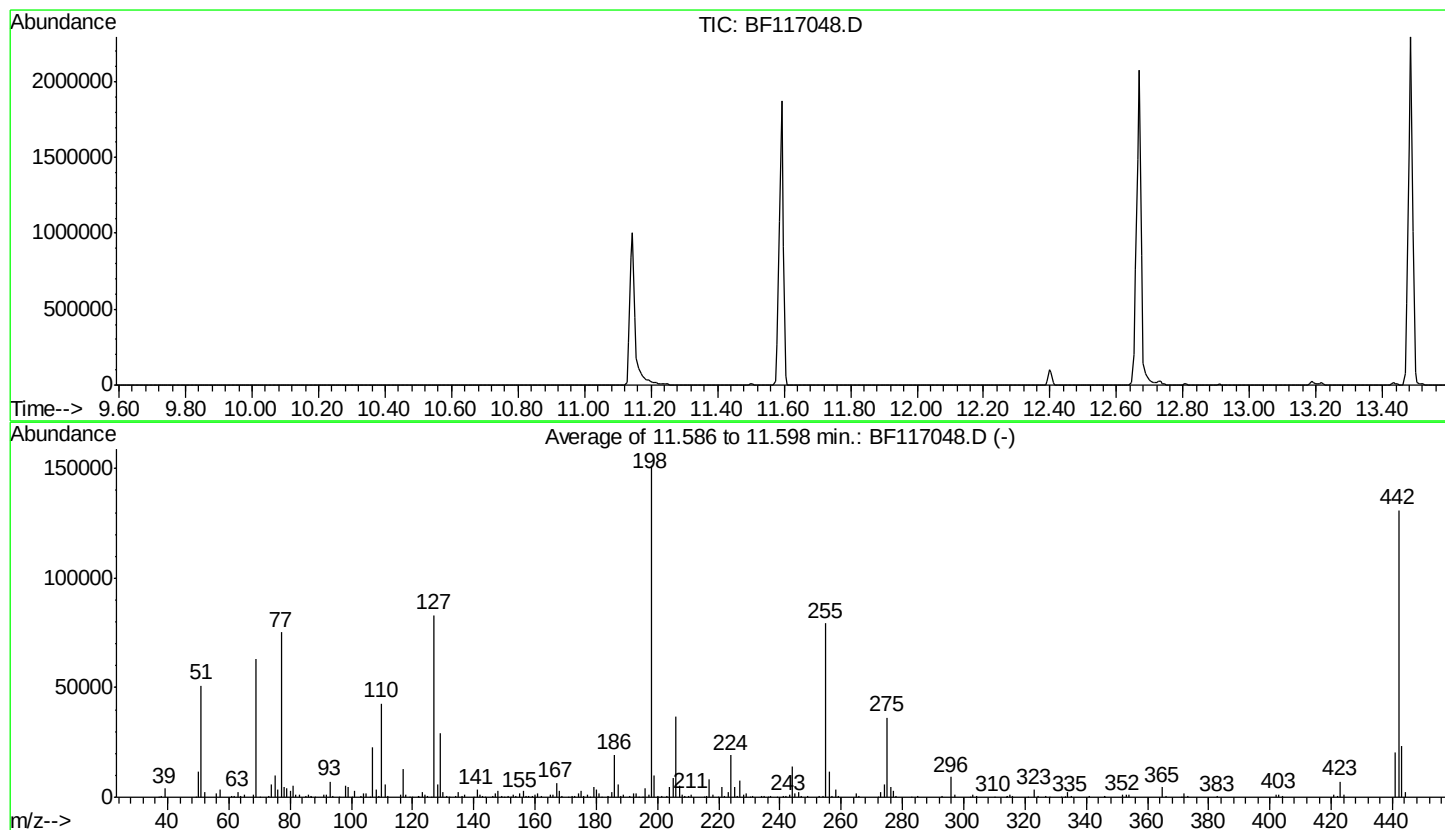

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	51074	PASS
68	69	0.00	2	1.5	929	PASS
69	198	0.00	100	41.8	63242	PASS
70	69	0.00	2	0.5	294	PASS
127	198	10	80	54.8	83042	PASS
197	198	0.00	2	0.9	1291	PASS
198	198	100	100	100.0	151410	PASS
199	198	5	9	6.6	9988	PASS
275	198	10	60	24.1	36544	PASS
365	198	1	100	3.0	4598	PASS
441	198	0.01	100	13.6	20520	PASS
442	198	50	100	86.6	131138	PASS
443	442	15	24	17.9	23468	PASS