
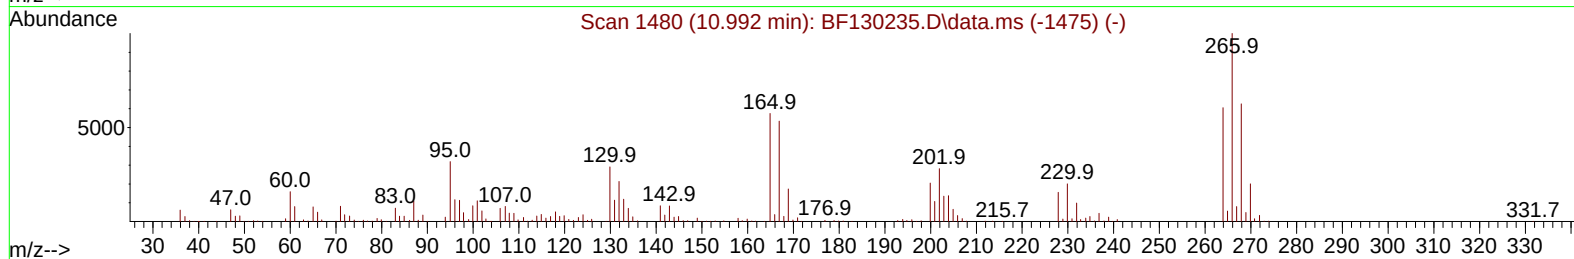
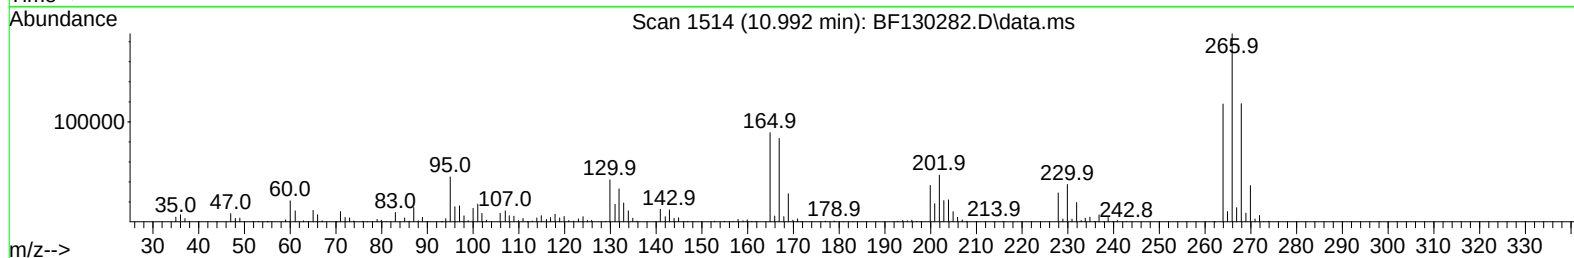


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091622\
 Data File : BF130282.D
 Acq On : 16 Sep 2022 09:42
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 17 06:03:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 17 03:22:32 2022
 Response via : Initial Calibration

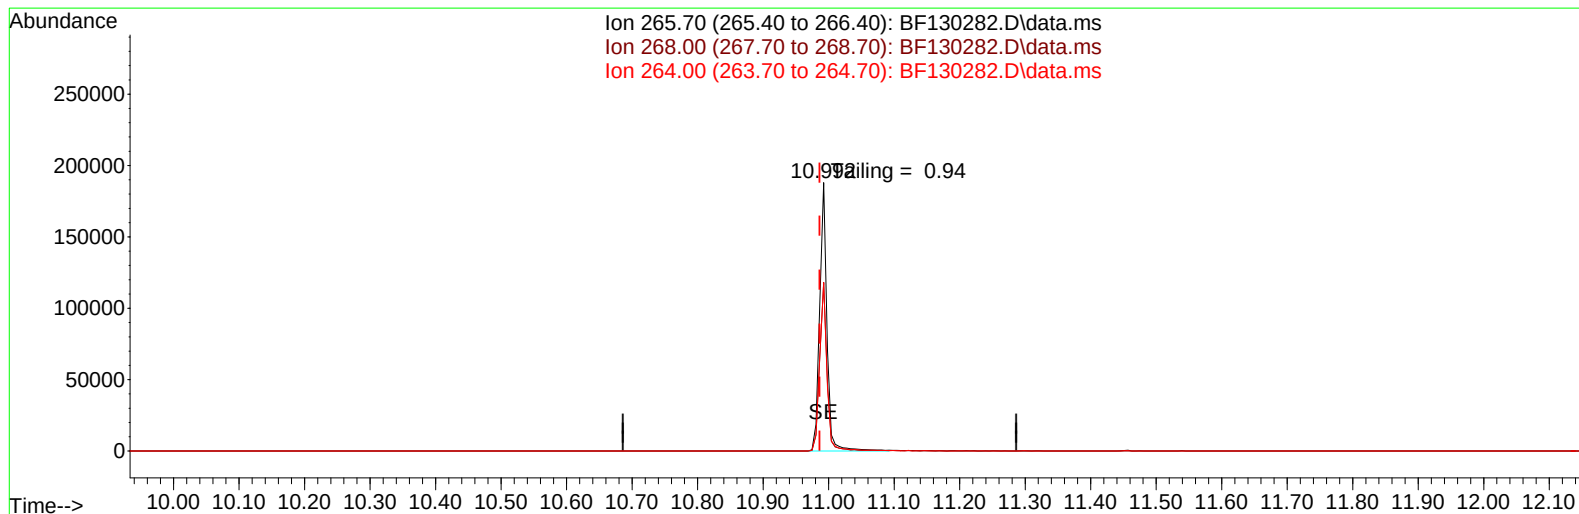

TIC: BF130282.D\data.ms




(70) Pentachlorophenol (C)

10.992min (+ 0.006) 32178.05 ng

response 147931

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.84
264.00	63.10	62.71
0.00	0.00	0.00

Quant Time: Sep 17 06:03:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 17 03:22:32 2022
Response via : Initial Calibration

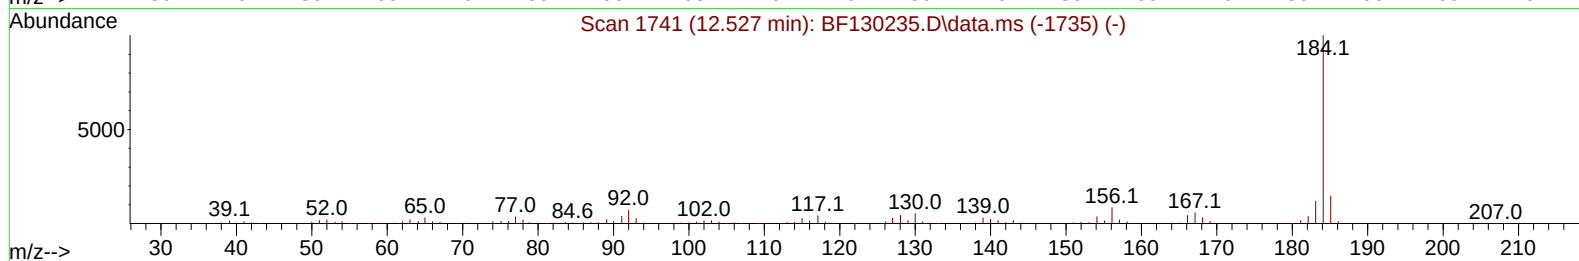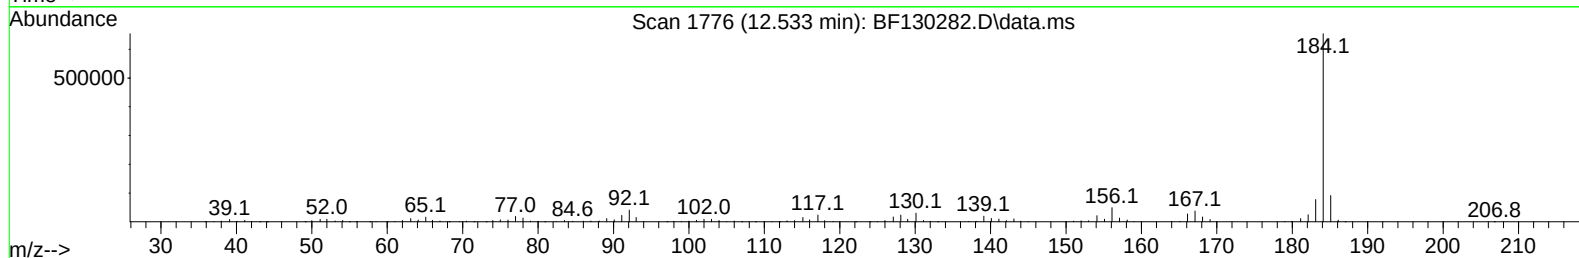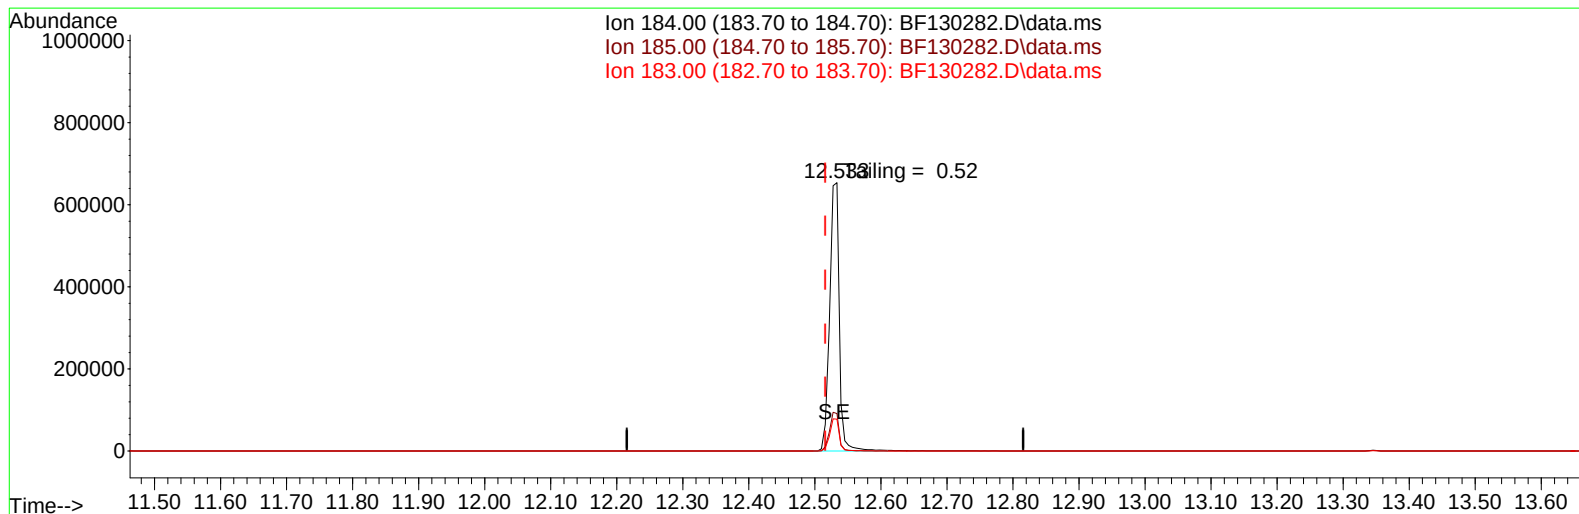

TIC: BF130282.D\data.ms

(77) Benzidine

12.533min (+ 0.018) 0.00 ng

response **659978**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.95
183.00	11.40	11.87
0.00	0.00	0.00