
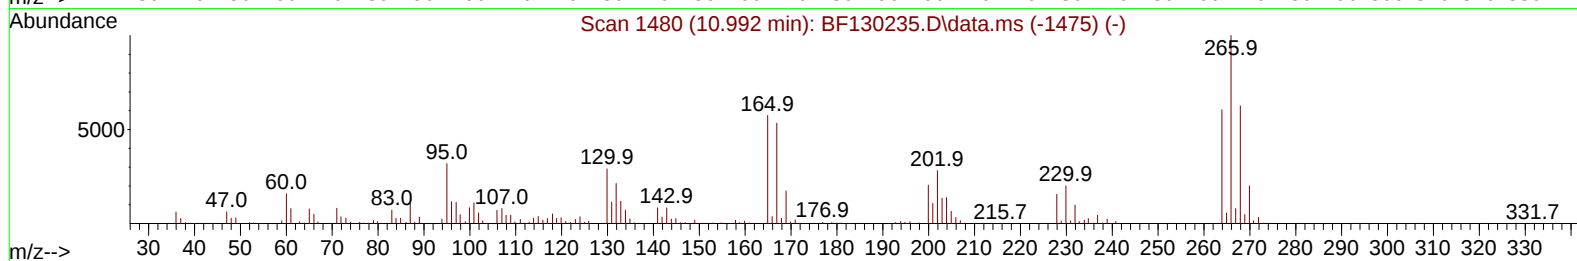
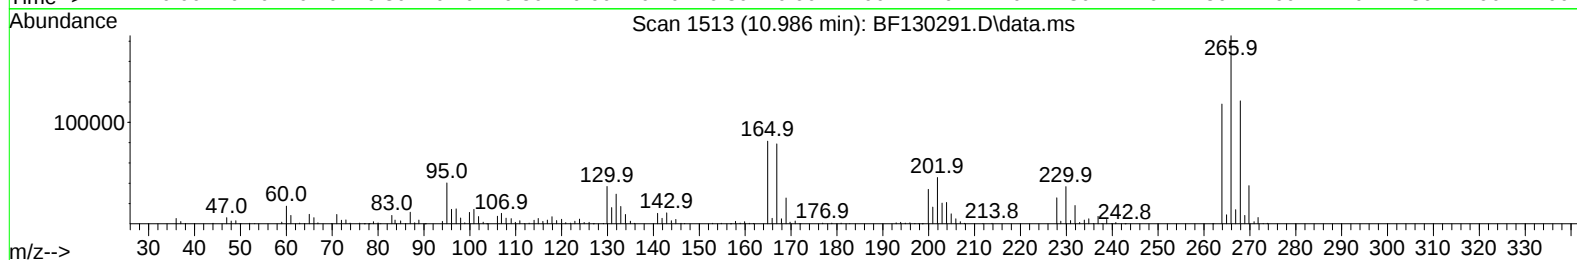


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091622\
Data File : BF130291.D
Acq On : 16 Sep 2022 15:38
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 17 06:05:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 17 03:22:32 2022
Response via : Initial Calibration



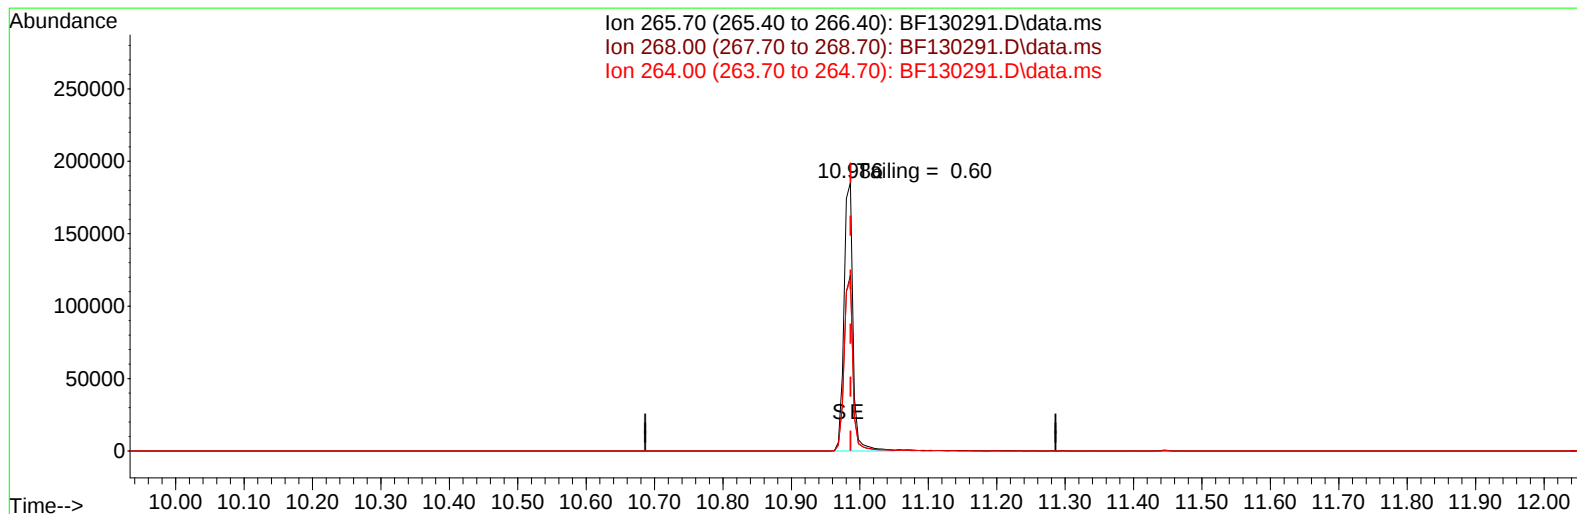


TIC: BF130291.D\data.ms

(70) Pentachlorophenol (C)**10.986min (-0.000) 30575.43 ng****response 169702**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	65.42
264.00	63.10	63.73
0.00	0.00	0.00

Quant Time: Sep 17 06:05:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 17 03:22:32 2022
Response via : Initial Calibration

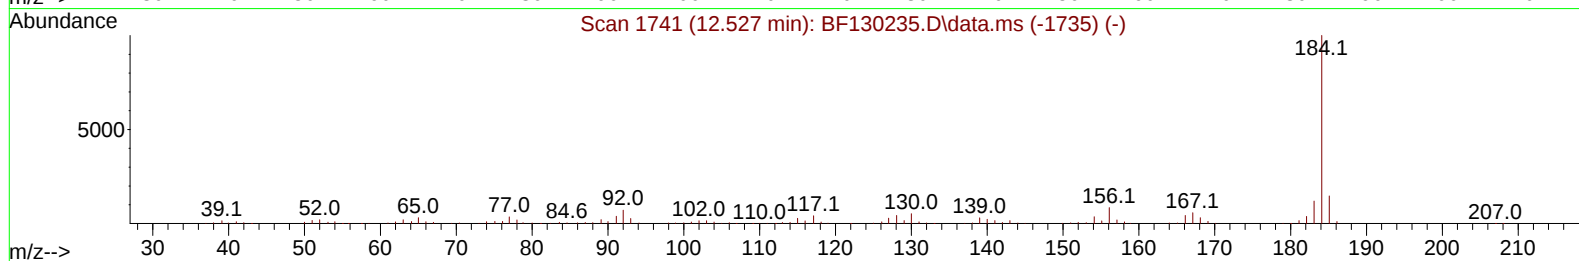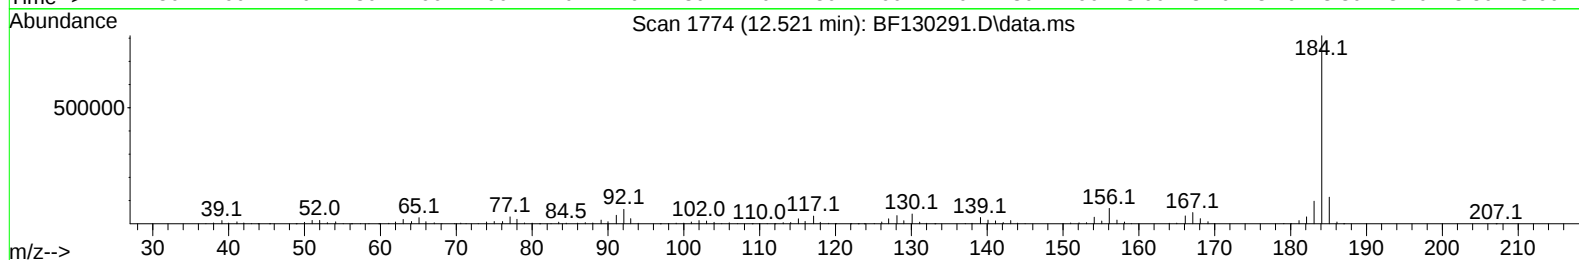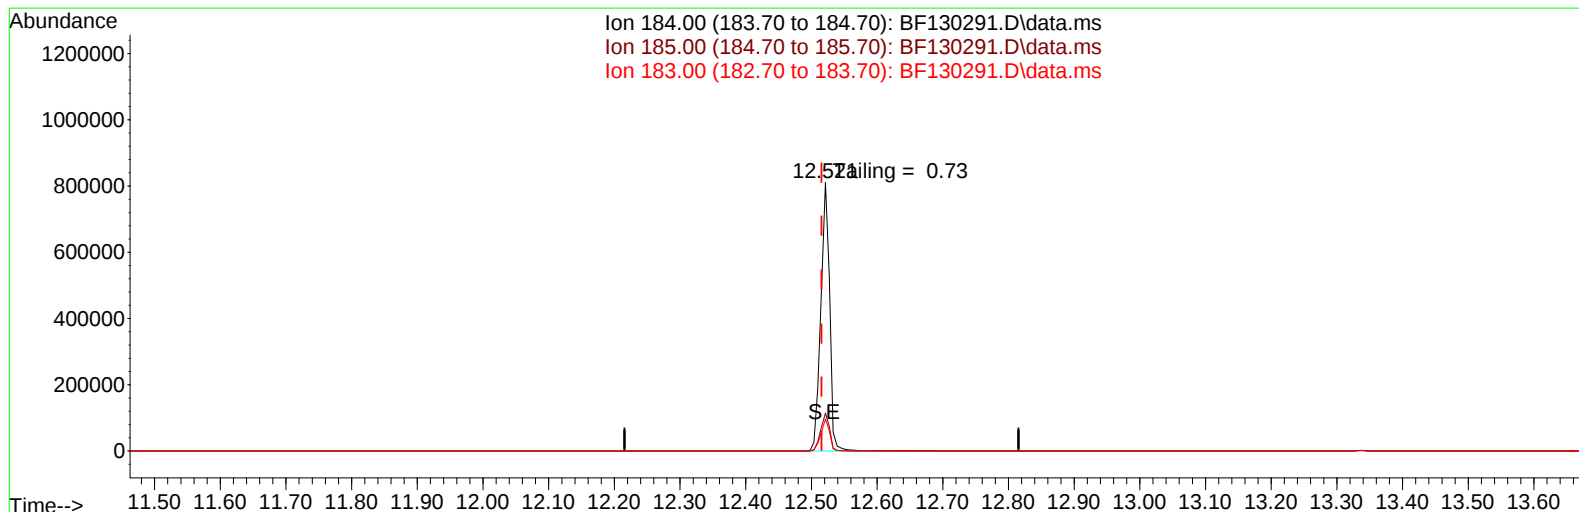

TIC: BF130291.D\data.ms

(77) Benzidine

12.521min (+ 0.006) 0.00 ng

response 762931

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.12
183.00	11.40	12.01
0.00	0.00	0.00