
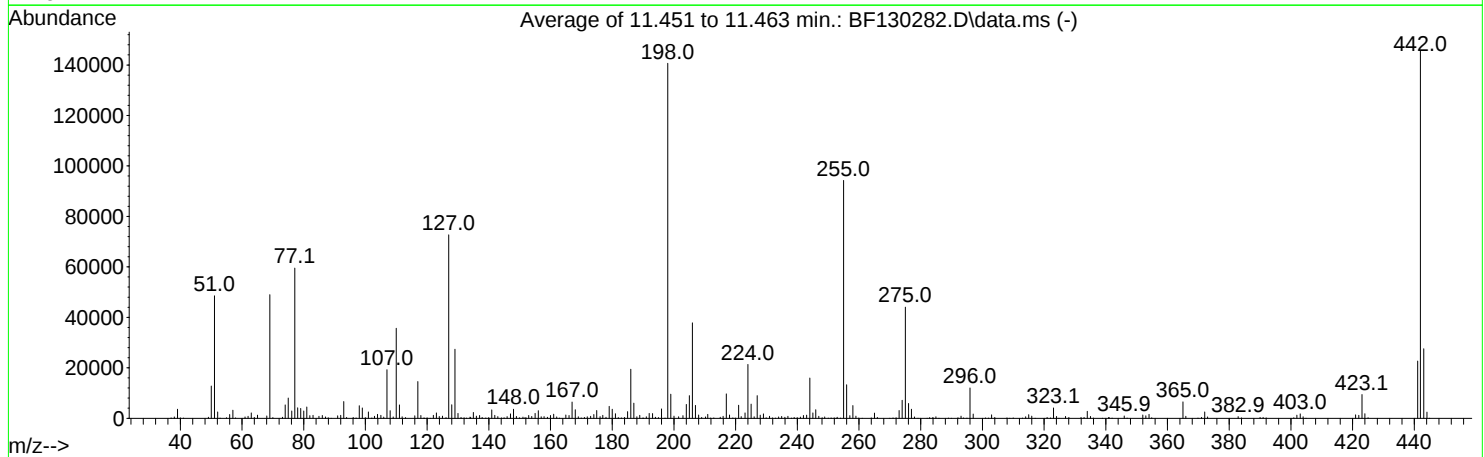


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091622\
 Data File : BF130282.D
 Acq On : 16 Sep 2022 09:42
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 19 15:06:14 2022

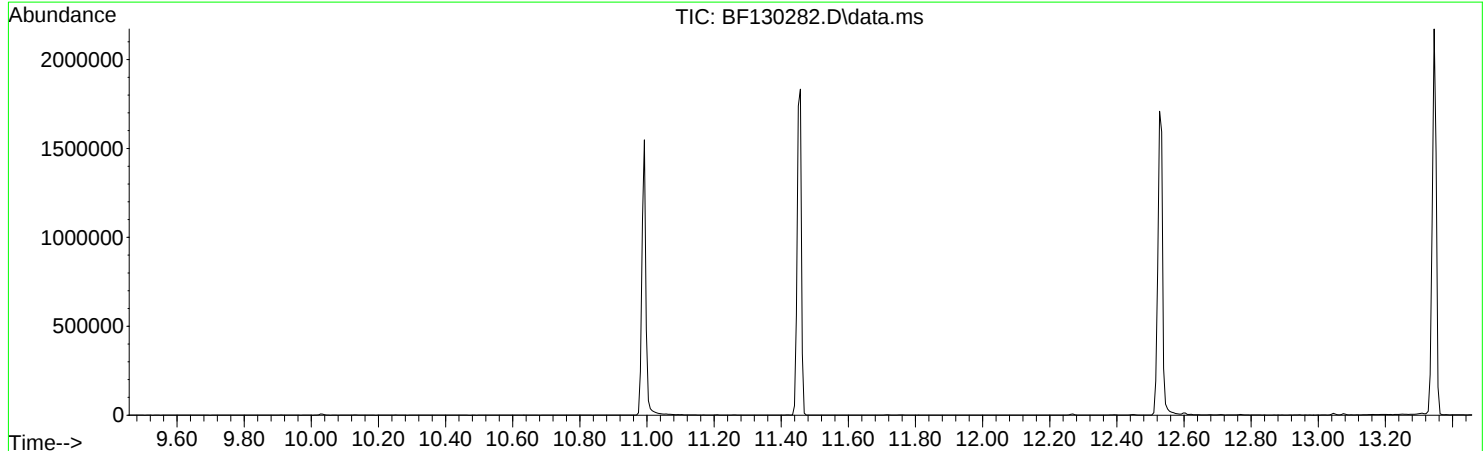




AutoFind: Scans 1592, 1593, 1594; Background Corrected with Scan 1586

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	48542	PASS
68	69	0.00	2	1.9	937	PASS
69	198	0.00	100	34.8	48966	PASS
70	69	0.00	2	0.6	307	PASS
127	198	10	80	51.7	72721	PASS
197	198	0.00	2	0.1	100	PASS
198	198	100	100	100.0	140691	PASS
199	198	5	9	6.8	9578	PASS
275	198	10	60	31.3	44028	PASS
365	198	1	100	4.6	6515	PASS
441	198	0.01	100	16.1	22641	PASS
442	442	50	100	100.0	145781	PASS
443	442	15	24	18.9	27550	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091622\
 Data File : BF130282.D
 Acq On : 16 Sep 2022 09:42
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 17 06:03:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 17 03:22:32 2022
 Response via : Initial Calibration

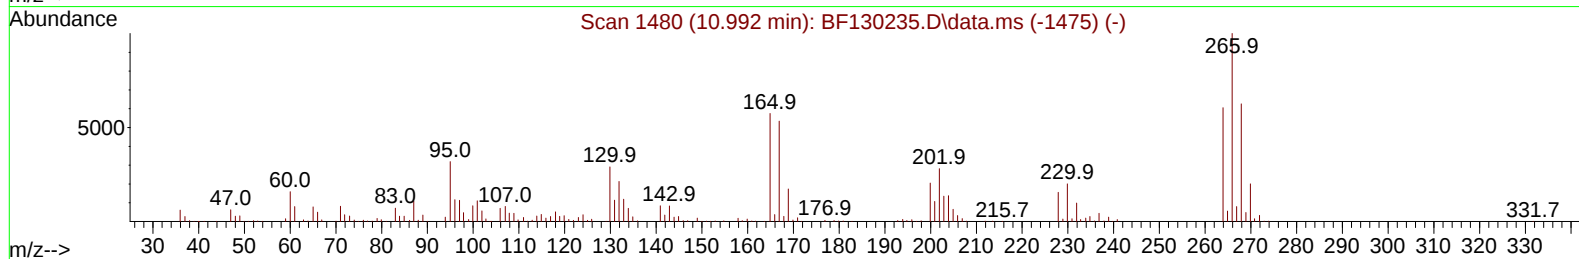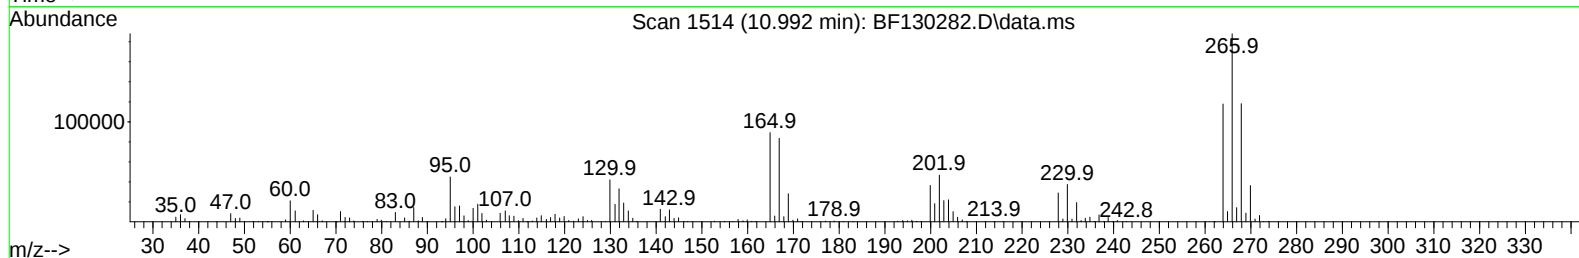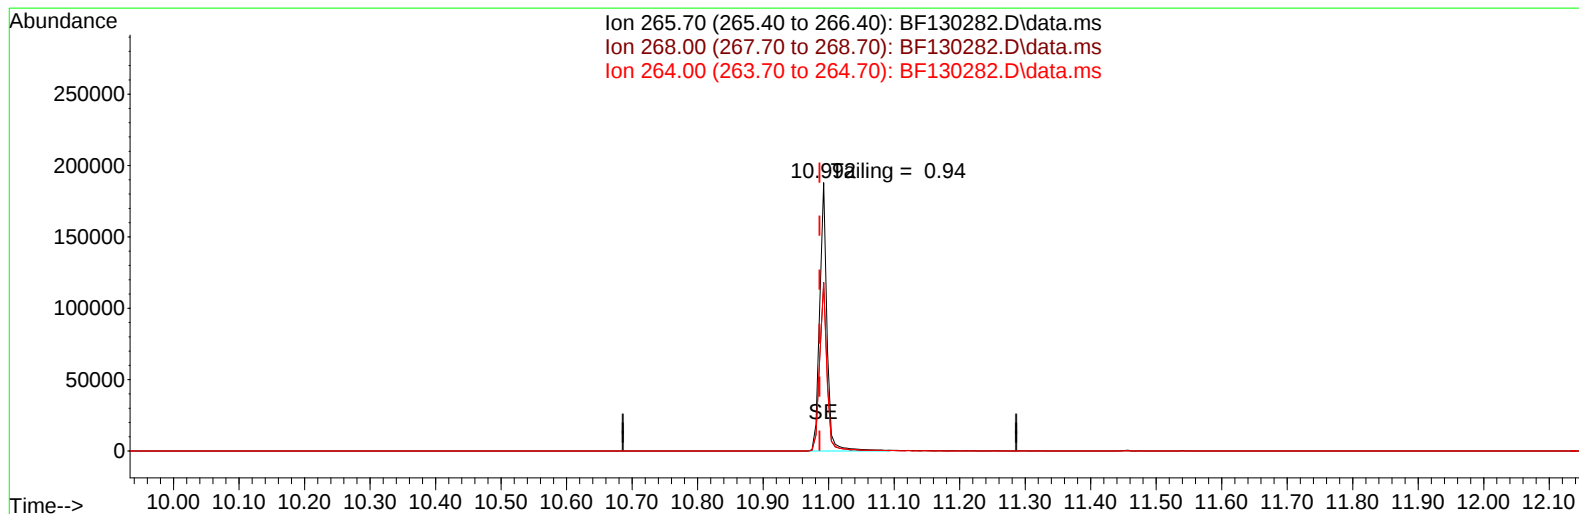

TIC: BF130282.D\data.ms

(70) Pentachlorophenol (C)

10.992min (+ 0.006) 32178.05 ng




response 147931

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.84
264.00	63.10	62.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091622\
Data File : BF130282.D
Acq On : 16 Sep 2022 09:42
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 17 06:03:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 17 03:22:32 2022
Response via : Initial Calibration

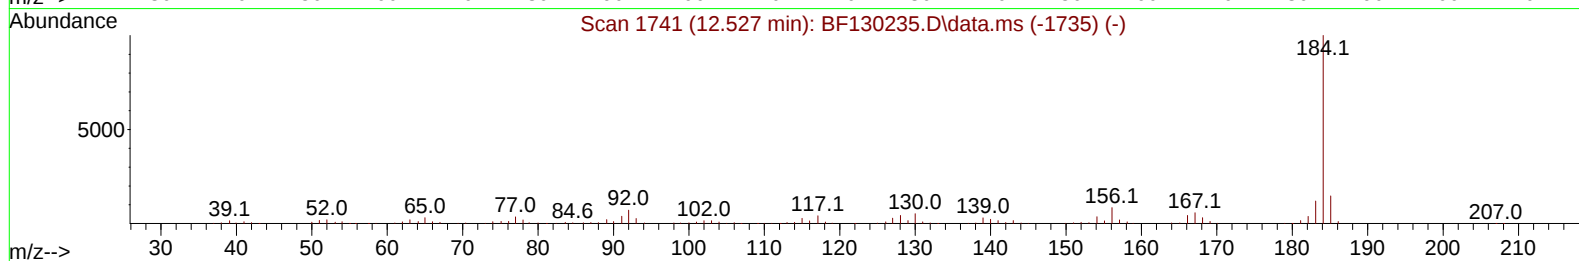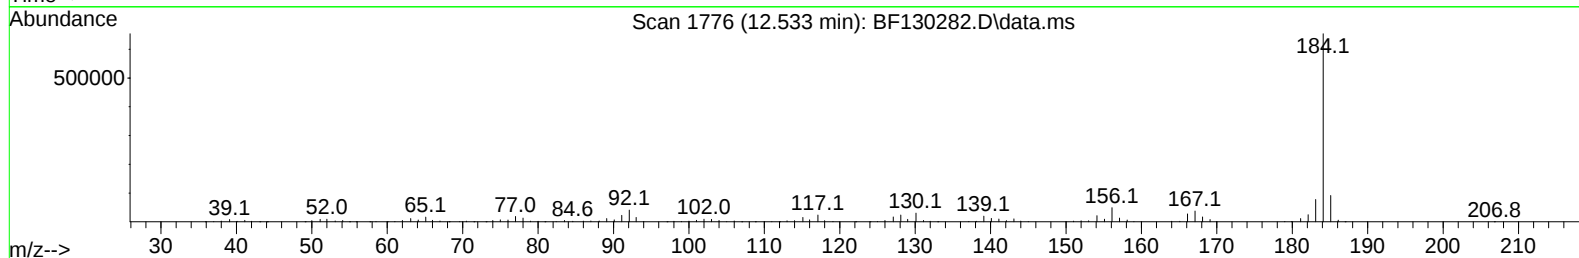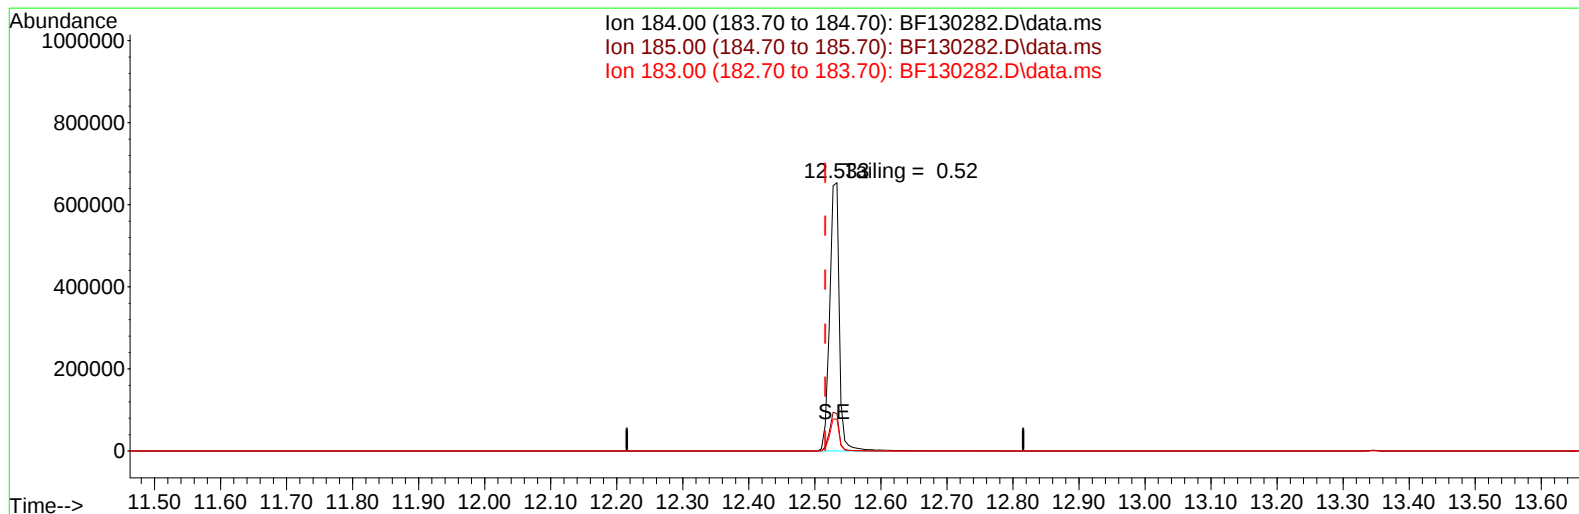

TIC: BF130282.D\data.ms

(77) Benzidine

12.533min (+ 0.018) 0.00 ng

response 659978

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.95
183.00	11.40	11.87
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/16/2022	BNA_F	<u>BF130282.D</u>
Compound Name	Response	Retention Time
DDT	334316	13.345
DDD	3532	13.045
DDE	393	12.704
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3925	338241	1.16

Instrument :
BNA_F
ClientSampleId :
DFTPP