


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091622\
Data File : BF130291.D
Acq On : 16 Sep 2022 15:38
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Sep 19 15:06:14 2022

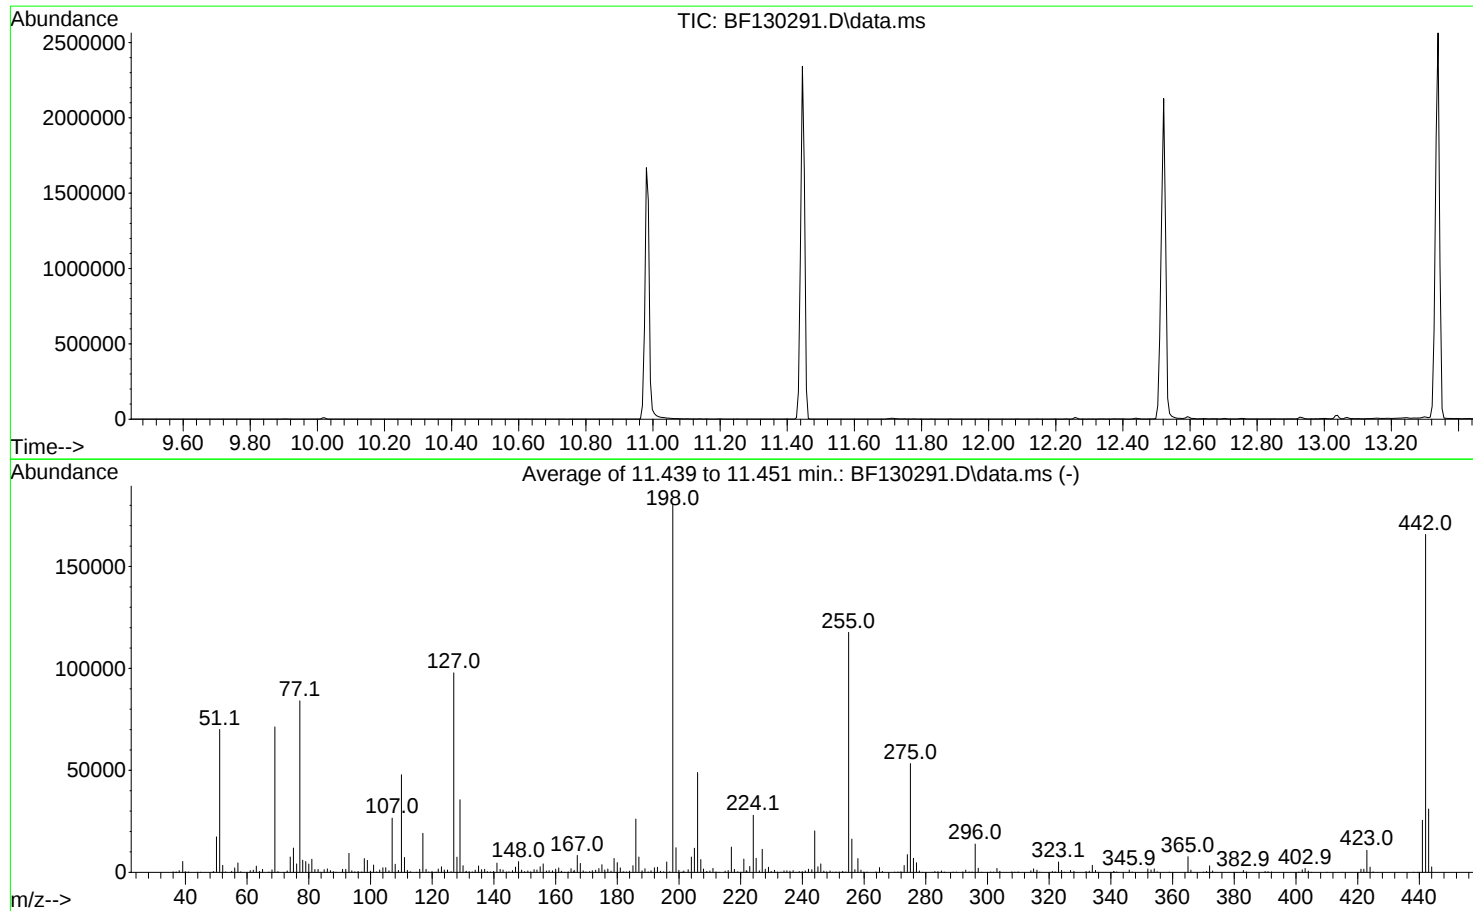




AutoFind: Scans 1590, 1591, 1592; Background Corrected with Scan 1585

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	70045	PASS
68	69	0.00	2	1.7	1242	PASS
69	198	0.00	100	39.5	71299	PASS
70	69	0.00	2	0.6	396	PASS
127	198	10	80	54.2	97821	PASS
197	198	0.00	2	0.2	315	PASS
198	198	100	100	100.0	180440	PASS
199	198	5	9	6.7	12023	PASS
275	198	10	60	29.5	53320	PASS
365	198	1	100	4.2	7654	PASS
441	198	0.01	100	14.2	25585	PASS
442	442	50	100	100.0	165712	PASS
443	442	15	24	18.7	31017	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091622\
Data File : BF130291.D
Acq On : 16 Sep 2022 15:38
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 17 06:05:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 17 03:22:32 2022
Response via : Initial Calibration

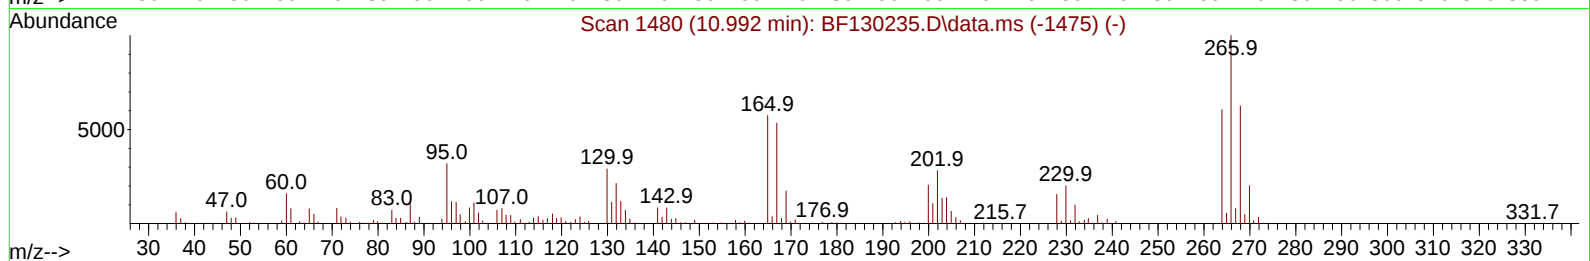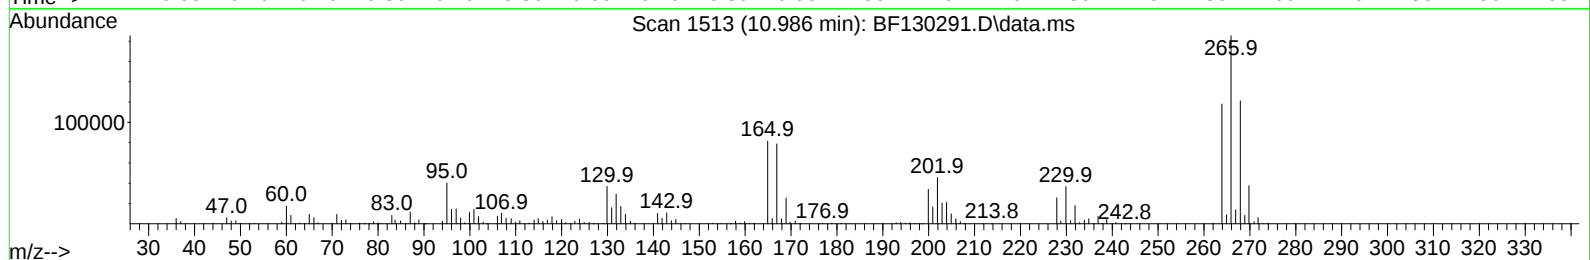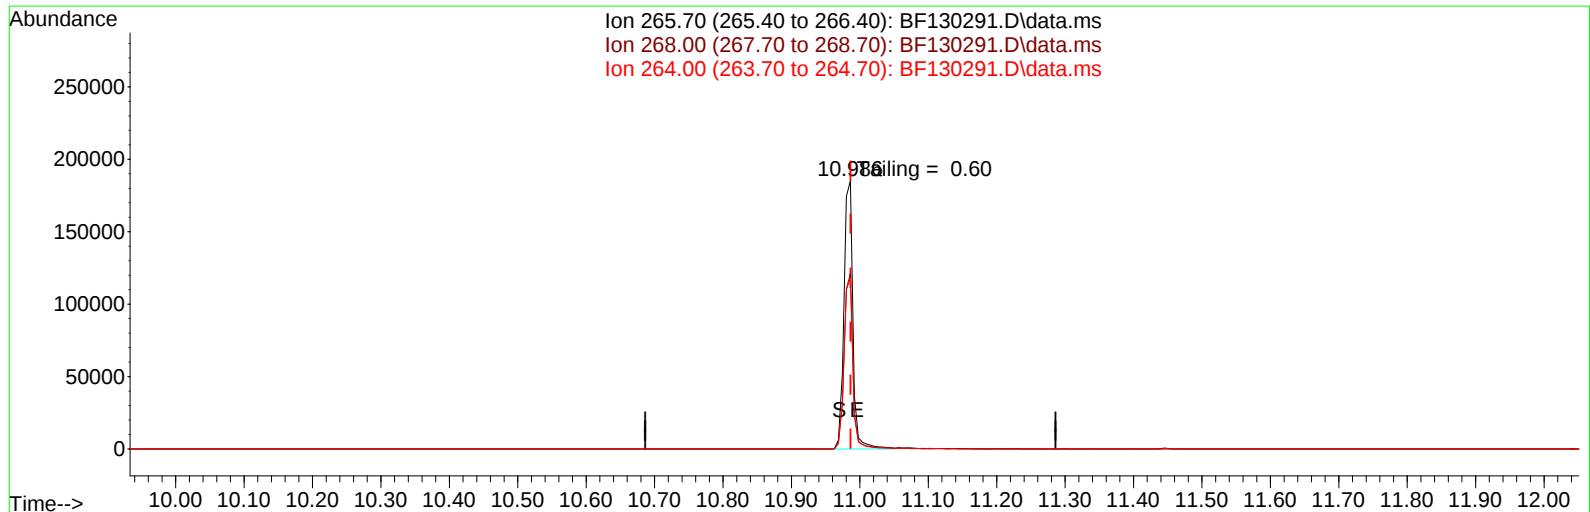

TIC: BF130291.D\data.ms

(70) Pentachlorophenol (C)

10.986min (-0.000) 30575.43 ng

response 169702

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	65.42
264.00	63.10	63.73
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/16/2022	BNA_F	<u>BF130291.D</u>
Compound Name	Response	Retention Time
DDT	399502	13.339
DDD	5936	13.039
DDE	458	12.704
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6394	405896	1.58

Instrument :
BNA_F
ClientSampleId :
DFTPP