

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091718\
 Data File : BF109082.D
 Acq On : 18 Sep 2018 7:39
 Operator : JU/SJ
 Sample : J4930-01
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 091318-JETT-E-D-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.901	432	436	450	rVB	126926	138359	3.55%	0.552%
2	5.325	504	508	511	rBV	1478787	1273101	32.66%	5.082%
3	6.348	678	682	693	rBV	1099437	869239	22.30%	3.470%
4	6.489	701	706	709	rBV	2471136	2233994	57.30%	8.918%
5	6.719	741	745	749	rBV	1046993	845679	21.69%	3.376%
6	6.878	768	772	775	rBV	3361134	2889425	74.12%	11.534%
7	7.284	835	841	844	rBV	2610199	2419704	62.07%	9.659%
8	8.001	959	963	966	rBV	1245038	977781	25.08%	3.903%
9	9.078	1142	1146	1149	rBV	4263672	3898467	100.00%	15.563%
10	9.472	1209	1213	1216	rBV	313280	267851	6.87%	1.069%
11	9.748	1257	1260	1264	rBV	1153990	1002137	25.71%	4.001%
12	10.430	1373	1376	1379	rVB	70858	49948	1.28%	0.199%
13	10.530	1389	1393	1408	rBV	1593656	1560320	40.02%	6.229%
14	11.224	1508	1511	1515	rBV	1033699	919531	23.59%	3.671%
15	12.813	1776	1781	1784	rBV	3851760	3480581	89.28%	13.894%
16	13.718	1931	1935	1944	rBV	83253	130035	3.34%	0.519%
17	13.854	1954	1958	1961	rBV	926055	889144	22.81%	3.549%
18	14.707	2099	2103	2107	rBV	427094	384358	9.86%	1.534%
19	15.254	2191	2196	2201	rBV	611391	723449	18.56%	2.888%
20	15.307	2202	2205	2212	rVB	37195	50779	1.30%	0.203%
21	17.671	2598	2607	2613	rBV	13160	46408	1.19%	0.185%


Sum of corrected areas: 25050290

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091718\
Data File : BF109082.D
Acq On : 18 Sep 2018 7:39
Operator : JU/SJ
Sample : J4930-01
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
091318-JETT-E-D-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

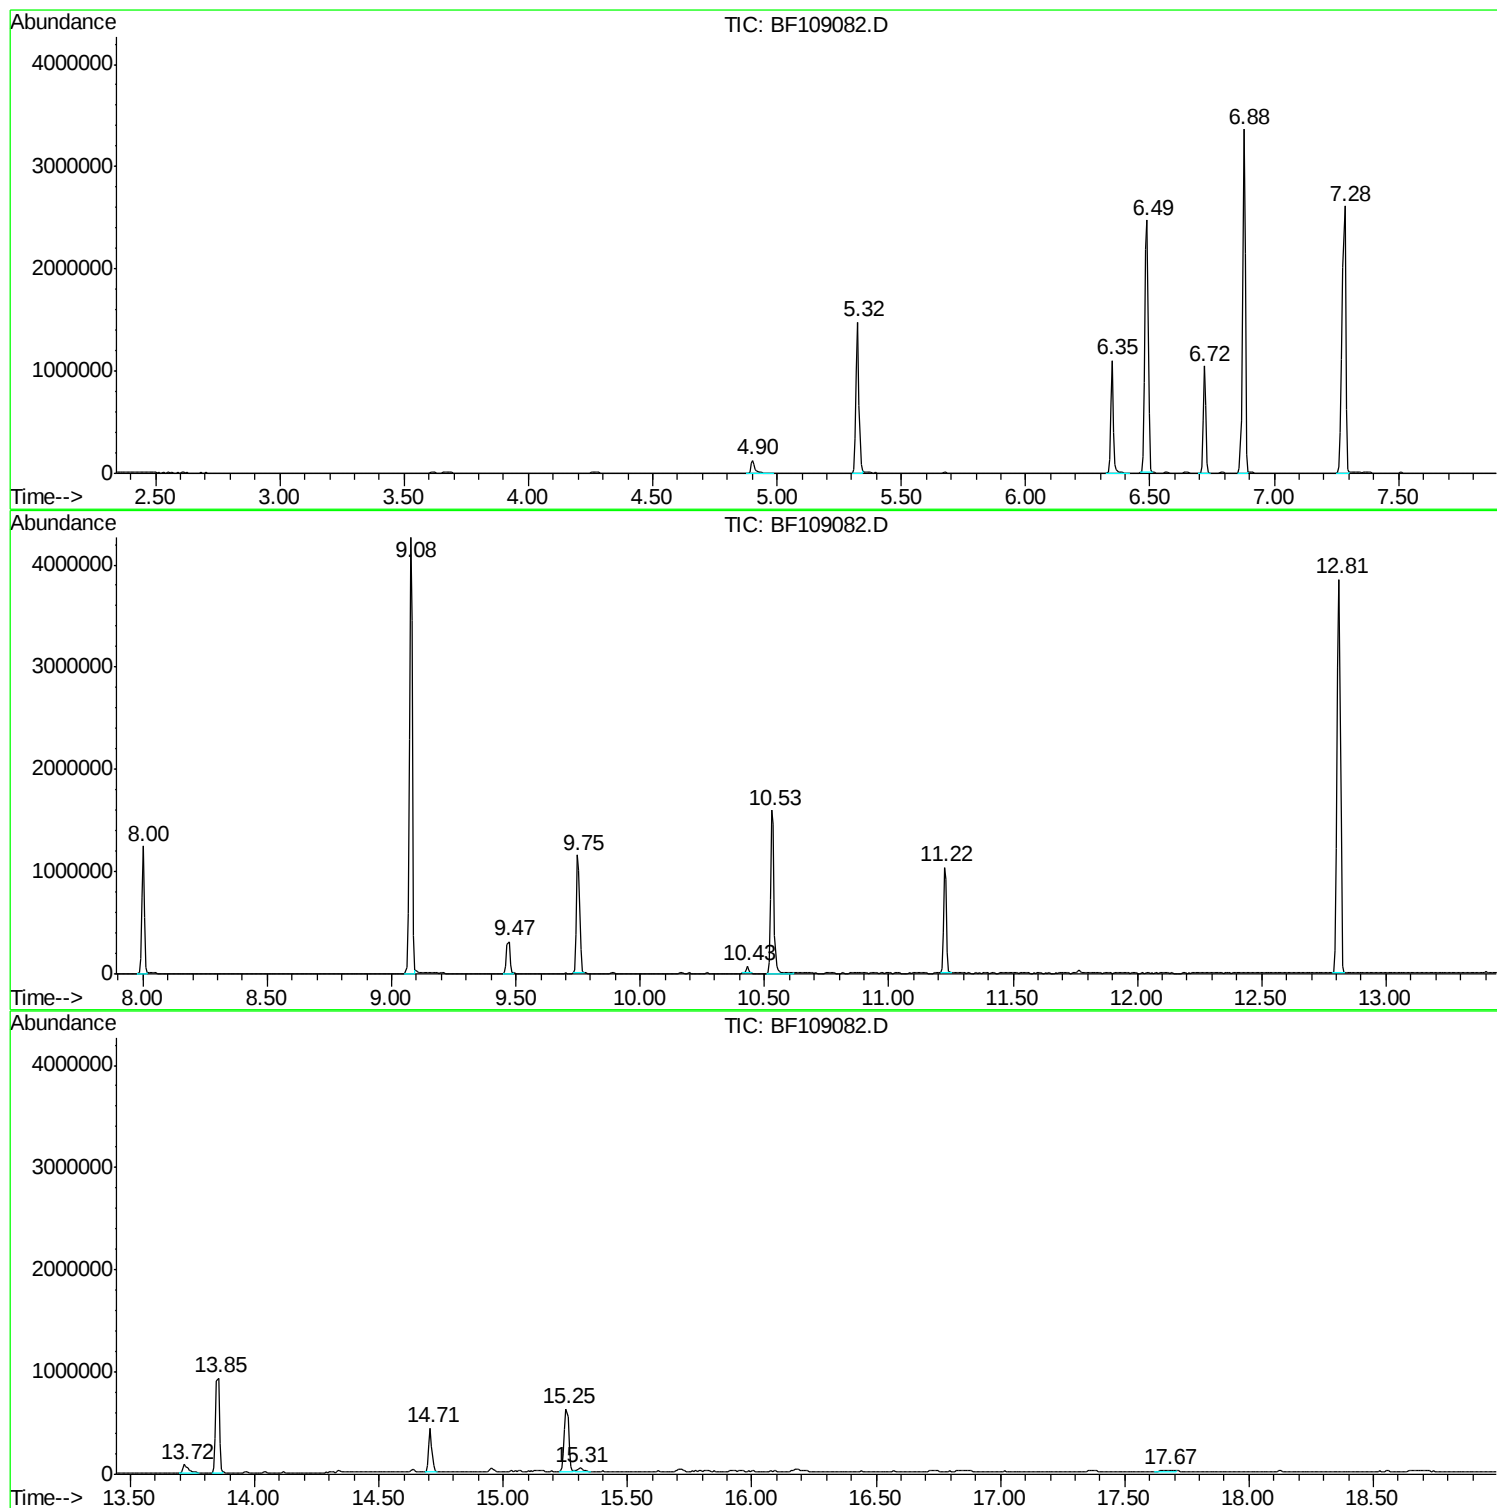

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091718\
Data_File : BF109082.D
Acq_On : 18-Sep-2018 7:399
Operator : JU/SJJ
Sample : J4930-011
Misc :
ALS_Vial : 44 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
091318-JETT-E-D-B

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091418.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
