

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091718\
 Data File : BF109083.D
 Acq On : 18 Sep 2018 8:06
 Operator : JU/SJ
 Sample : J4930-02
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 091318-JETT-E-D-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.901	432	436	446	rVB	142589	154522	3.75%	0.611%
2	5.325	504	508	511	rBV	1489161	1290013	31.29%	5.097%
3	6.348	678	682	690	rBV	1115724	872759	21.17%	3.448%
4	6.489	701	706	709	rBV	2580954	2308520	56.00%	9.121%
5	6.719	742	745	749	rBV	1063428	807681	19.59%	3.191%
6	6.878	768	772	775	rBV	3473856	3009144	72.99%	11.889%
7	7.283	835	841	844	rBV	2655327	2553356	61.94%	10.088%
8	8.001	959	963	966	rBV	1196149	930321	22.57%	3.676%
9	9.077	1142	1146	1150	rBV	4296413	4122535	100.00%	16.288%
10	9.472	1209	1213	1216	rBV	219594	195986	4.75%	0.774%
11	9.748	1257	1260	1264	rBV2	1101391	931189	22.59%	3.679%
12	10.530	1389	1393	1405	rBV	1593649	1593097	38.64%	6.294%
13	11.224	1508	1511	1515	rBV	1001682	863437	20.94%	3.411%
14	12.648	1749	1753	1756	rVB	48935	43572	1.06%	0.172%
15	12.813	1776	1781	1784	rBV	3936618	3745129	90.85%	14.797%
16	13.724	1931	1936	1944	rBV2	33785	55022	1.33%	0.217%
17	13.848	1953	1957	1961	rBV	886370	862137	20.91%	3.406%
18	14.707	2099	2103	2107	rVB	189134	172147	4.18%	0.680%
19	14.954	2141	2145	2150	rBV	41260	45772	1.11%	0.181%
20	15.254	2191	2196	2202	rBV	569516	650595	15.78%	2.570%
21	15.306	2202	2205	2214	rVB	40560	57174	1.39%	0.226%
22	15.712	2269	2274	2278	rBV2	34414	46272	1.12%	0.183%


Sum of corrected areas: 25310380

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091718\
Data File : BF109083.D
Acq On : 18 Sep 2018 8:06
Operator : JU/SJ
Sample : J4930-02
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
091318-JETT-E-D-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

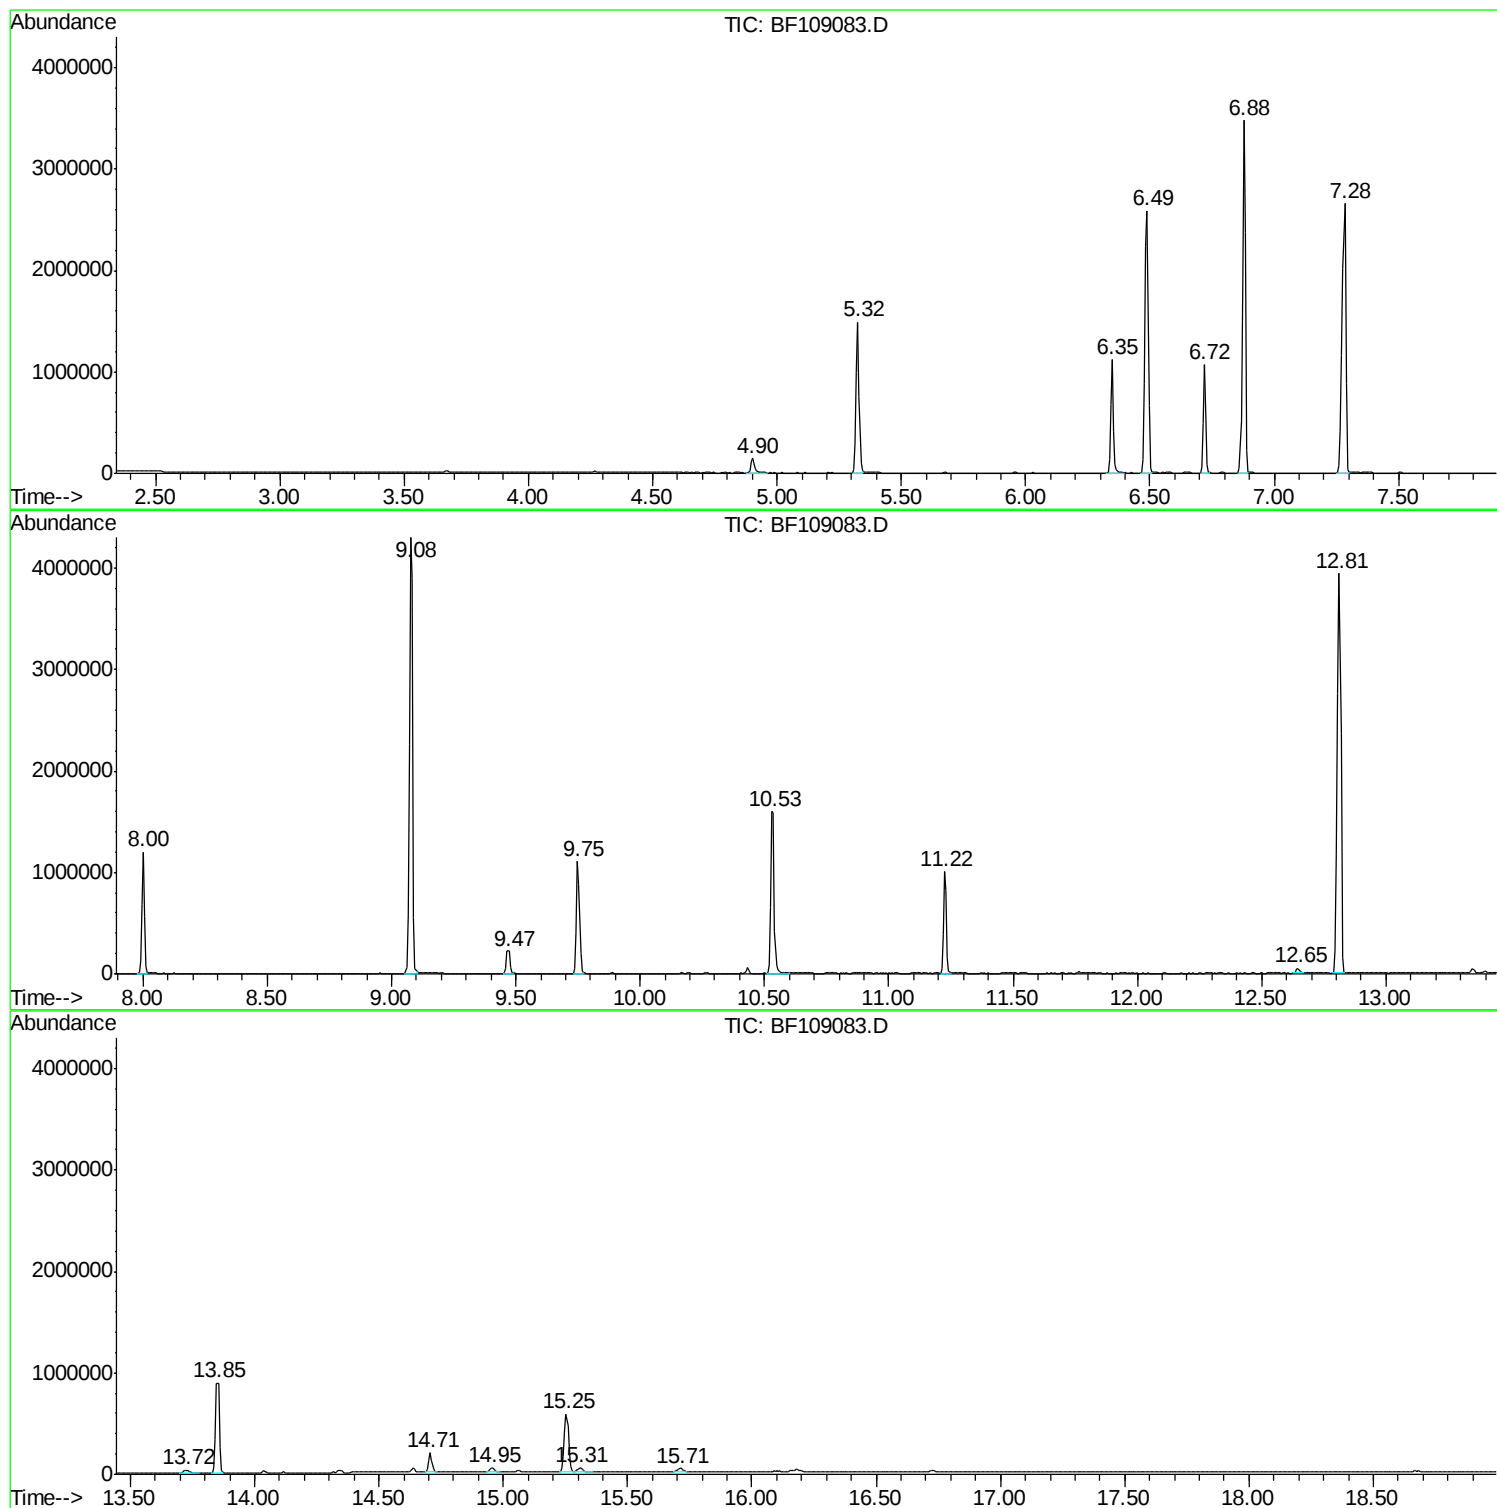

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091718\
Data_File : BF109083.D
Acq_On : 18-Sep-2018 8:066
Operator : JU/SJJ
Sample : J4930-022
Misc :
ALS_Vial : 45 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
091318-JETT-E-D-S

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091418.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
