

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091718\
 Data File : BF109084.D
 Acq On : 18 Sep 2018 8:33
 Operator : JU/SJ
 Sample : J4930-03
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 091318-JETT-E-U-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.901	433	436	445	rVB	179955	197331	4.34%	0.707%
2	5.325	504	508	512	rBV	1676148	1481086	32.55%	5.303%
3	6.348	678	682	689	rBV	1299706	1025778	22.54%	3.673%
4	6.490	701	706	709	rBV	2805571	2528831	55.57%	9.055%
5	6.719	741	745	749	rBV	1134285	880548	19.35%	3.153%
6	6.878	768	772	775	rBV	3594542	3245233	71.32%	11.620%
7	7.284	835	841	844	rBV	2916174	2766955	60.80%	9.908%
8	8.001	959	963	966	rBV	1359333	1053158	23.14%	3.771%
9	9.083	1141	1147	1149	rBV	4655549	4550561	100.00%	16.294%
10	9.472	1209	1213	1216	rBV	394867	334289	7.35%	1.197%
11	9.748	1257	1260	1264	rBV	1260378	1094235	24.05%	3.918%
12	10.430	1373	1376	1379	rVB	66251	47172	1.04%	0.169%
13	10.530	1389	1393	1408	rBV	1777476	1759373	38.66%	6.300%
14	11.225	1508	1511	1515	rBV	1181579	967679	21.27%	3.465%
15	12.642	1749	1752	1756	rBV	81569	75788	1.67%	0.271%
16	12.813	1776	1781	1784	rBV	4084824	3875437	85.16%	13.877%
17	13.348	1869	1872	1875	rBV	67403	53585	1.18%	0.192%
18	13.718	1931	1935	1947	rBV	83302	148626	3.27%	0.532%
19	13.848	1954	1957	1961	rBV	919620	864295	18.99%	3.095%
20	14.636	2087	2091	2096	rBV	52503	48820	1.07%	0.175%
21	14.707	2099	2103	2108	rVB	47178	46905	1.03%	0.168%
22	14.954	2141	2145	2150	rVB	55745	56613	1.24%	0.203%
23	15.254	2191	2196	2201	rBV	622749	704067	15.47%	2.521%
24	15.307	2201	2205	2210	rVB	54265	66759	1.47%	0.239%
25	15.712	2270	2274	2278	rBV2	40193	54291	1.19%	0.194%


Sum of corrected areas: 27927415

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091718\
Data File : BF109084.D
Acq On : 18 Sep 2018 8:33
Operator : JU/SJ
Sample : J4930-03
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
091318-JETT-E-U-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

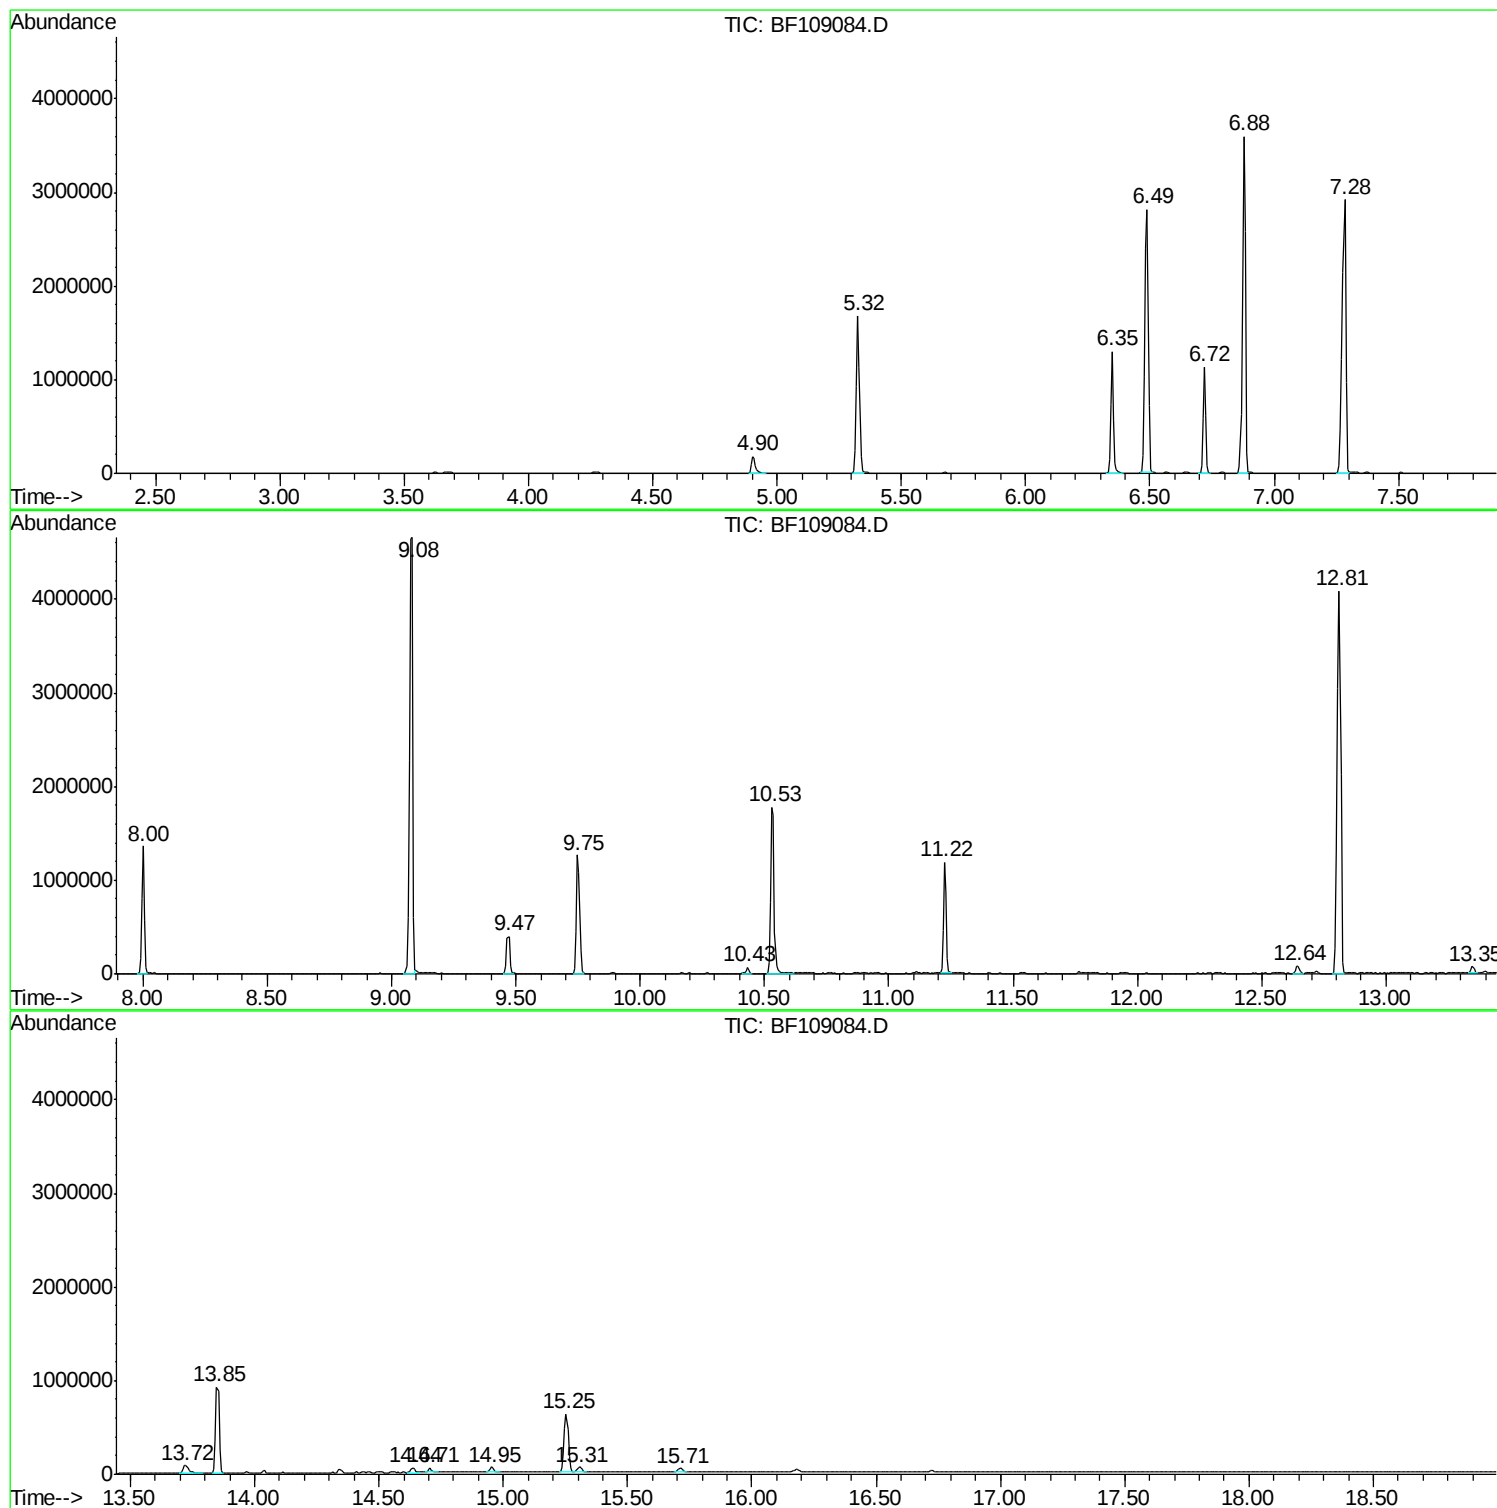

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091718\
Data_File : BF109084.D
Acq_On : 18-Sep-2018 8:333
Operator : JU/SJJ
Sample : J4930-033
Misc :
ALS_Vial : 46 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
091318-JETT-E-U-B

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091418.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
