

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091718\
 Data File : BF109085.D
 Acq On : 18 Sep 2018 9:00
 Operator : JU/SJ
 Sample : J4930-04
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 091318-JETT-E-U-S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.901	432	436	443	rBV	171389	180386	4.78%	0.765%
2	5.325	504	508	512	rBV	1540995	1329152	35.26%	5.634%
3	6.348	678	682	695	rBV	1127880	883495	23.43%	3.745%
4	6.489	701	706	709	rBV	2448228	2209098	58.60%	9.364%
5	6.719	742	745	749	rBV	966990	737433	19.56%	3.126%
6	6.878	768	772	775	rBV	3309983	2850412	75.61%	12.082%
7	7.284	835	841	844	rBV	2461406	2324710	61.66%	9.854%
8	8.001	959	963	966	rBV	1015104	811443	21.52%	3.439%
9	9.078	1142	1146	1149	rBV	4007057	3640211	96.56%	15.430%
10	9.472	1209	1213	1216	rBV	140556	122791	3.26%	0.520%
11	9.748	1257	1260	1264	rBV2	952023	789947	20.95%	3.348%
12	10.530	1390	1393	1405	rBV	1563629	1491790	39.57%	6.323%
13	11.224	1508	1511	1515	rBV	952317	812726	21.56%	3.445%
14	12.813	1776	1781	1784	rBV	4095499	3770017	100.00%	15.980%
15	13.848	1954	1957	1961	rBV	888715	857983	22.76%	3.637%
16	14.707	2100	2103	2107	rBV	172440	157264	4.17%	0.667%
17	15.254	2191	2196	2202	rBV	545047	623099	16.53%	2.641%


Sum of corrected areas: 23591957

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091718\
Data File : BF109085.D
Acq On : 18 Sep 2018 9:00
Operator : JU/SJ
Sample : J4930-04
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
091318-JETT-E-U-S

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

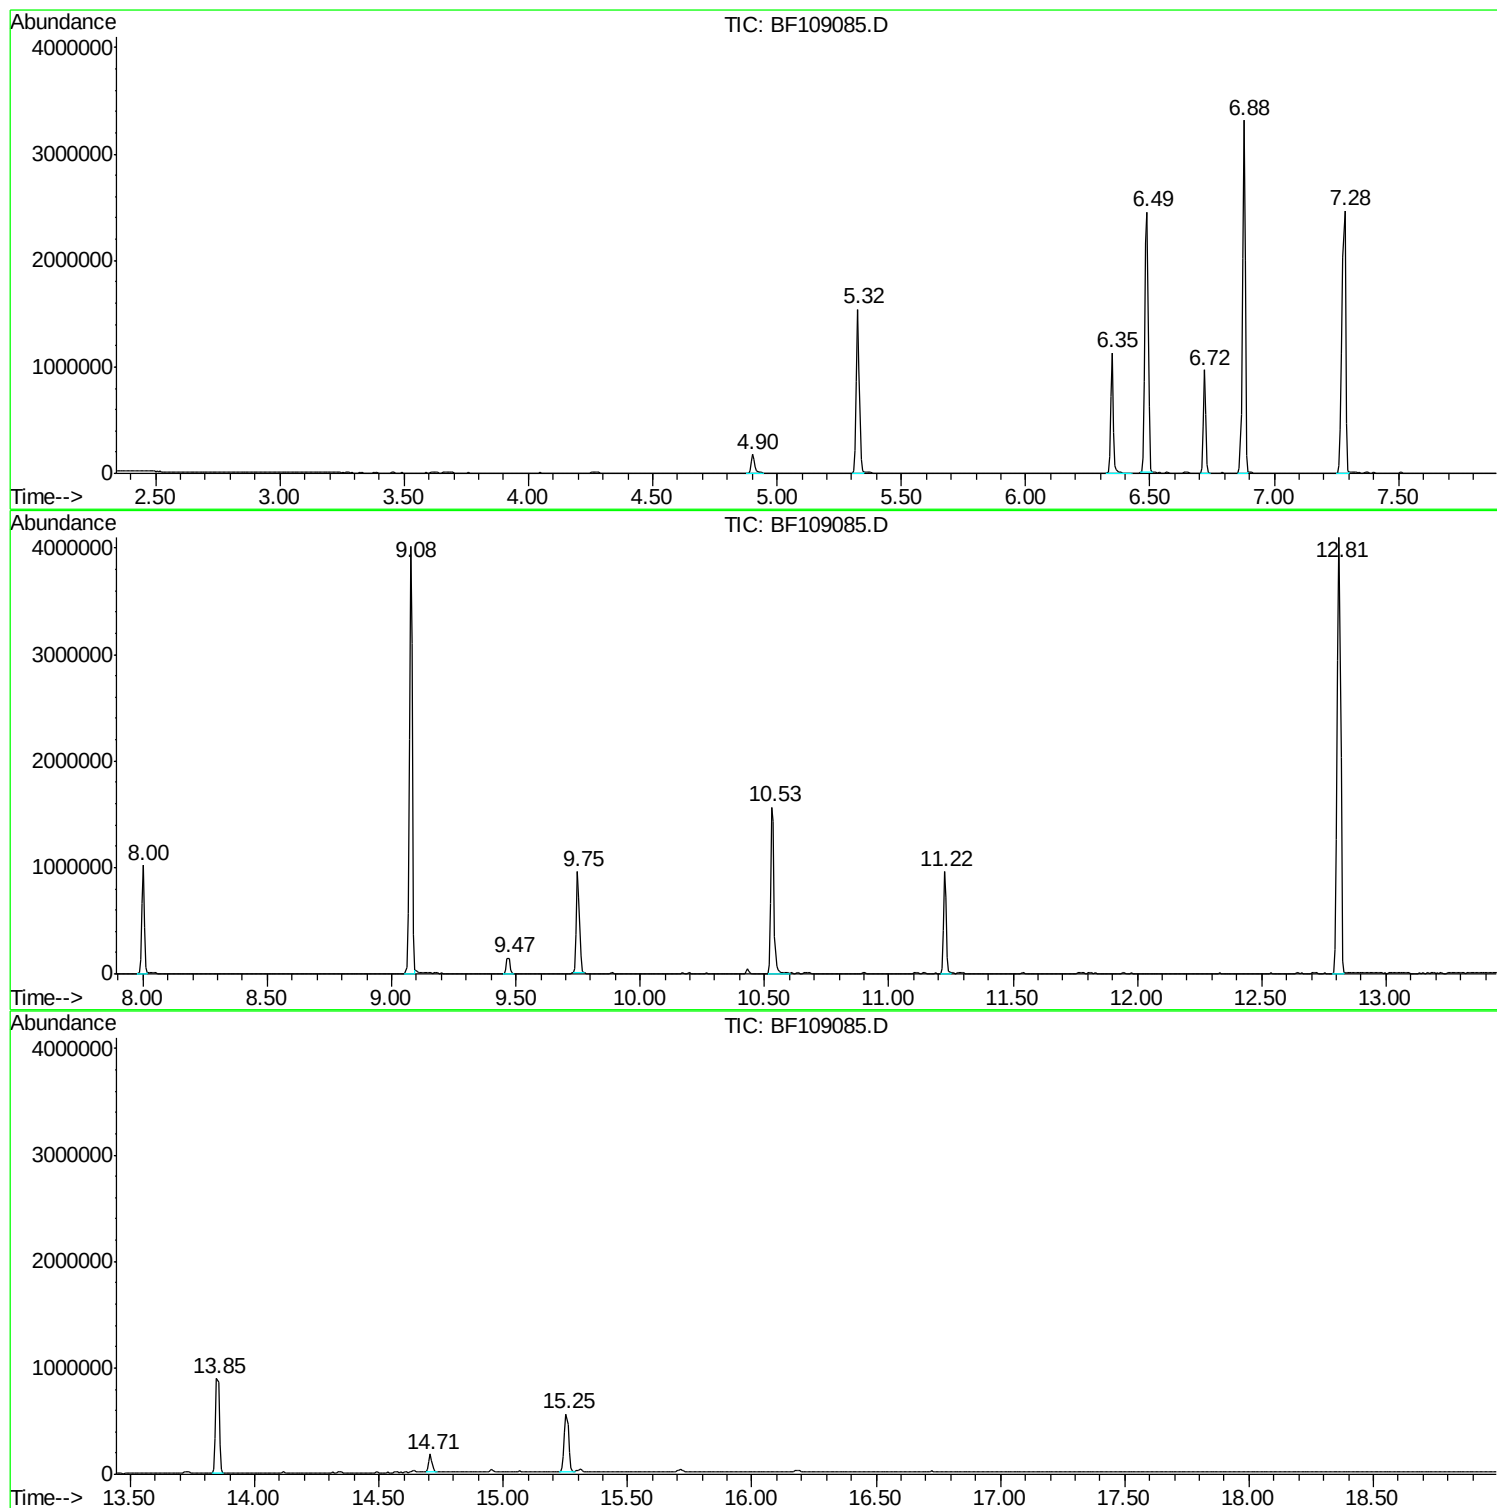

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091718\
Data_File : BF109085.D
Acq_On : 18-Sep-2018 9:000
Operator : JU/SJJ
Sample : J4930-044
Misc :
ALS_Vial : 47 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
091318-JETT-E-U-S

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091418.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
