

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091718\
 Data File : BF109086.D
 Acq On : 18 Sep 2018 9:28
 Operator : JU/SJ
 Sample : J4930-05
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 091318-DBRI-E-D-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.901	432	436	444	rBV	151402	169302	4.03%	0.653%
2	5.325	504	508	511	rBV	1611919	1406068	33.47%	5.427%
3	6.348	678	682	691	rBV	1260561	964196	22.95%	3.721%
4	6.489	701	706	709	rBV	2604185	2403662	57.22%	9.277%
5	6.719	741	745	748	rBV	1078728	821818	19.56%	3.172%
6	6.878	768	772	775	rBV	3519391	3069887	73.08%	11.848%
7	7.283	835	841	844	rBV	2724365	2605058	62.01%	10.054%
8	8.001	959	963	966	rBV	1263725	968792	23.06%	3.739%
9	9.077	1142	1146	1149	rBV	4390647	4200801	100.00%	16.213%
10	9.466	1209	1212	1216	rBV	257398	219089	5.22%	0.846%
11	9.748	1257	1260	1264	rBV	1144903	1005560	23.94%	3.881%
12	10.530	1389	1393	1410	rBV	1680963	1624458	38.67%	6.269%
13	11.224	1508	1511	1515	rBV	1106394	891707	21.23%	3.441%
14	12.813	1776	1781	1784	rBV	4067025	3693971	87.93%	14.256%
15	13.724	1932	1936	1941	rBV	34471	45458	1.08%	0.175%
16	13.848	1953	1957	1961	rBV	887440	852649	20.30%	3.291%
17	14.636	2087	2091	2098	rBV	47219	48014	1.14%	0.185%
18	14.707	2099	2103	2106	rVB	61964	57039	1.36%	0.220%
19	14.954	2141	2145	2150	rBV	52159	58755	1.40%	0.227%
20	15.254	2191	2196	2201	rBV	608840	682218	16.24%	2.633%
21	15.306	2201	2205	2212	rVB	49831	67635	1.61%	0.261%
22	15.712	2270	2274	2280	rVB2	39995	54707	1.30%	0.211%


Sum of corrected areas: 25910844

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091718\
Data File : BF109086.D
Acq On : 18 Sep 2018 9:28
Operator : JU/SJ
Sample : J4930-05
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
091318-DBRI-E-D-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

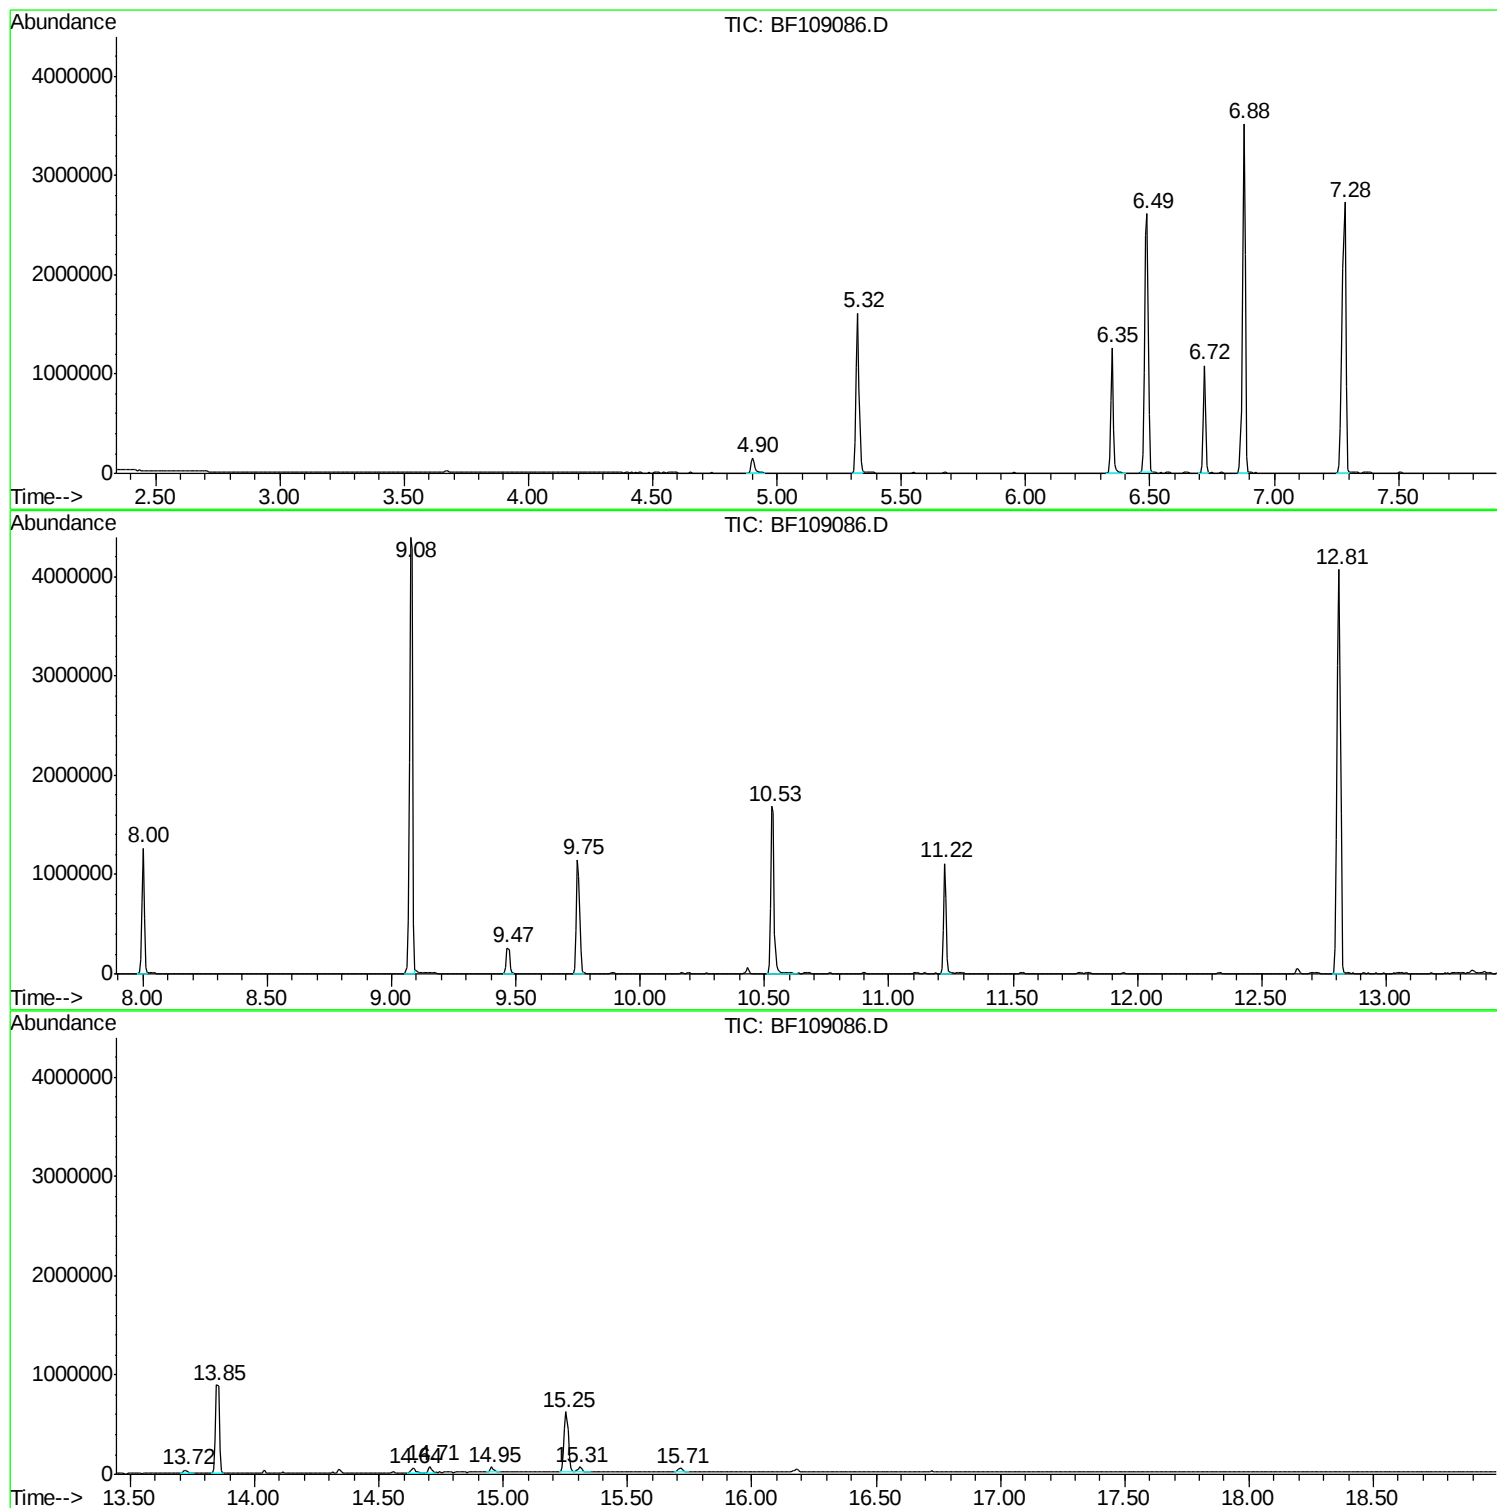

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091718\
Data_File : BF109086.D
Acq_On : 18-Sep-2018 9:288
Operator : JU/SJJ
Sample : J4930-055
Misc :
ALS_Vial : 48 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
091318-DBRI-E-D-B

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091418.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
