

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091718\
 Data File : BF109089.D
 Acq On : 18 Sep 2018 10:50
 Operator : JU/SJ
 Sample : J4930-11
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 091318-TIPC-F-D-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.901	433	436	446	rVB	134022	154337	3.52%	0.586%
2	5.325	504	508	511	rBV	1374732	1252169	28.54%	4.754%
3	6.348	678	682	693	rBV	1027904	889503	20.27%	3.377%
4	6.489	701	706	709	rBV	2476788	2359249	53.77%	8.957%
5	6.719	741	745	748	rBV	1178574	889059	20.26%	3.375%
6	6.878	768	772	775	rBV	3542889	3171686	72.29%	12.042%
7	7.283	835	841	844	rBV	2780098	2664212	60.72%	10.115%
8	8.001	959	963	966	rBV	1385051	1053349	24.01%	3.999%
9	9.077	1142	1146	1150	rBV	4477283	4387603	100.00%	16.658%
10	9.466	1209	1212	1216	rBV	120828	98302	2.24%	0.373%
11	9.748	1257	1260	1264	rBV	1321217	1113471	25.38%	4.227%
12	10.430	1373	1376	1380	rVB	71686	51218	1.17%	0.194%
13	10.530	1389	1393	1410	rBV	1731731	1648965	37.58%	6.261%
14	11.224	1508	1511	1515	rBV	1137933	963335	21.96%	3.657%
15	12.813	1776	1781	1784	rBV	3907997	3529690	80.45%	13.401%
16	13.724	1932	1936	1946	rBV2	34938	63826	1.45%	0.242%
17	13.848	1954	1957	1961	rBV	908066	857155	19.54%	3.254%
18	14.636	2088	2091	2097	rVB	54608	49548	1.13%	0.188%
19	14.707	2099	2103	2108	rVB	77258	70975	1.62%	0.269%
20	14.954	2141	2145	2149	rBV	68392	70245	1.60%	0.267%
21	15.254	2191	2196	2201	rBV	663882	762845	17.39%	2.896%
22	15.306	2201	2205	2212	rVB	74494	96373	2.20%	0.366%
23	15.712	2269	2274	2280	rBV	60425	84942	1.94%	0.322%
24	16.177	2348	2353	2361	rVB3	34111	56832	1.30%	0.216%


Sum of corrected areas: 26338889

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091718\
Data File : BF109089.D
Acq On : 18 Sep 2018 10:50
Operator : JU/SJ
Sample : J4930-11
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
091318-TIPC-F-D-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

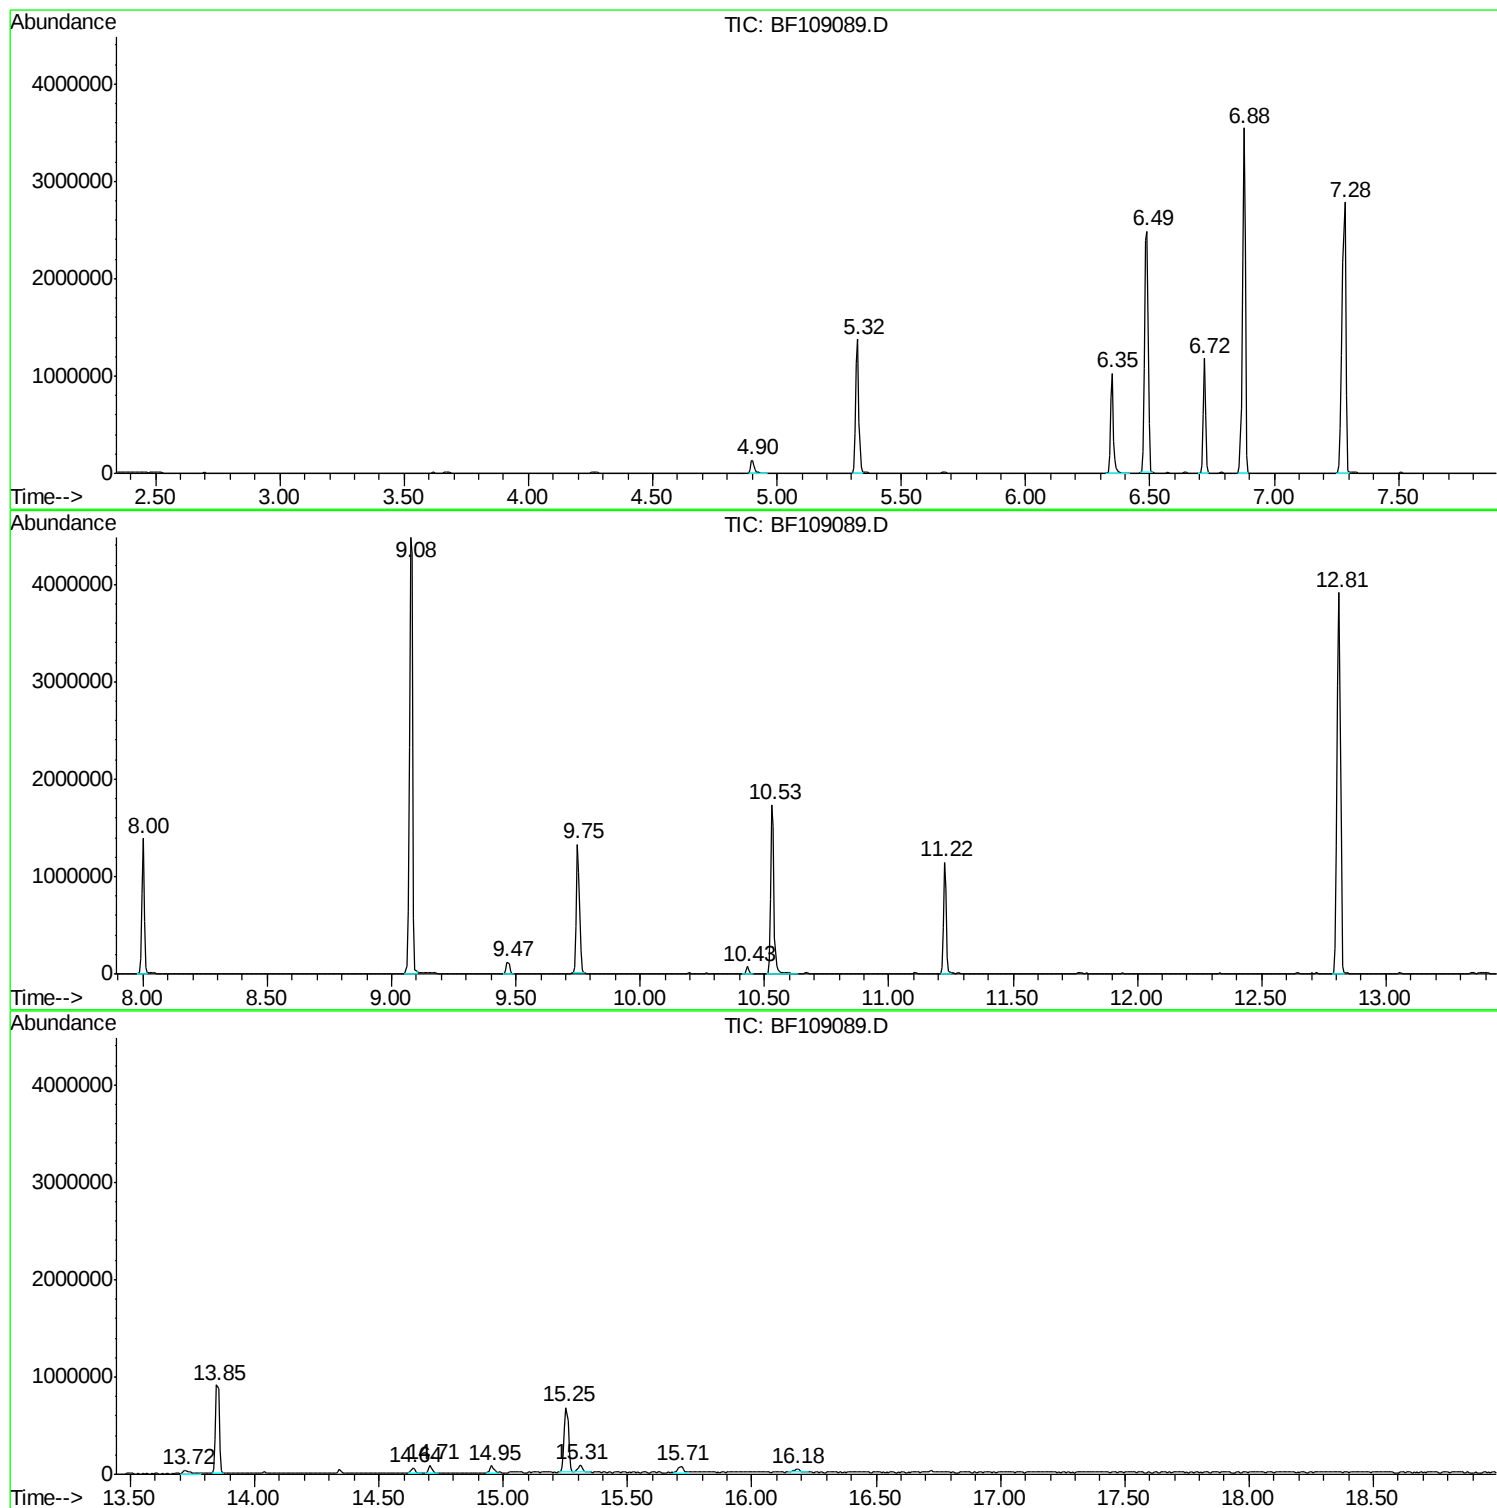

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091718\
Data_File : BF109089.D
Acq_On : 18-Sep-2018 10:500
Operator : JU/SJJ
Sample : J4930-111
Misc :
ALS_Vial : 51 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
091318-TIPC-F-D-B

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091418.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
