


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091718\
Data File : BF109037.D
Acq On : 17 Sep 2018 10:12
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091418.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Sep 14 13:26:52 2018

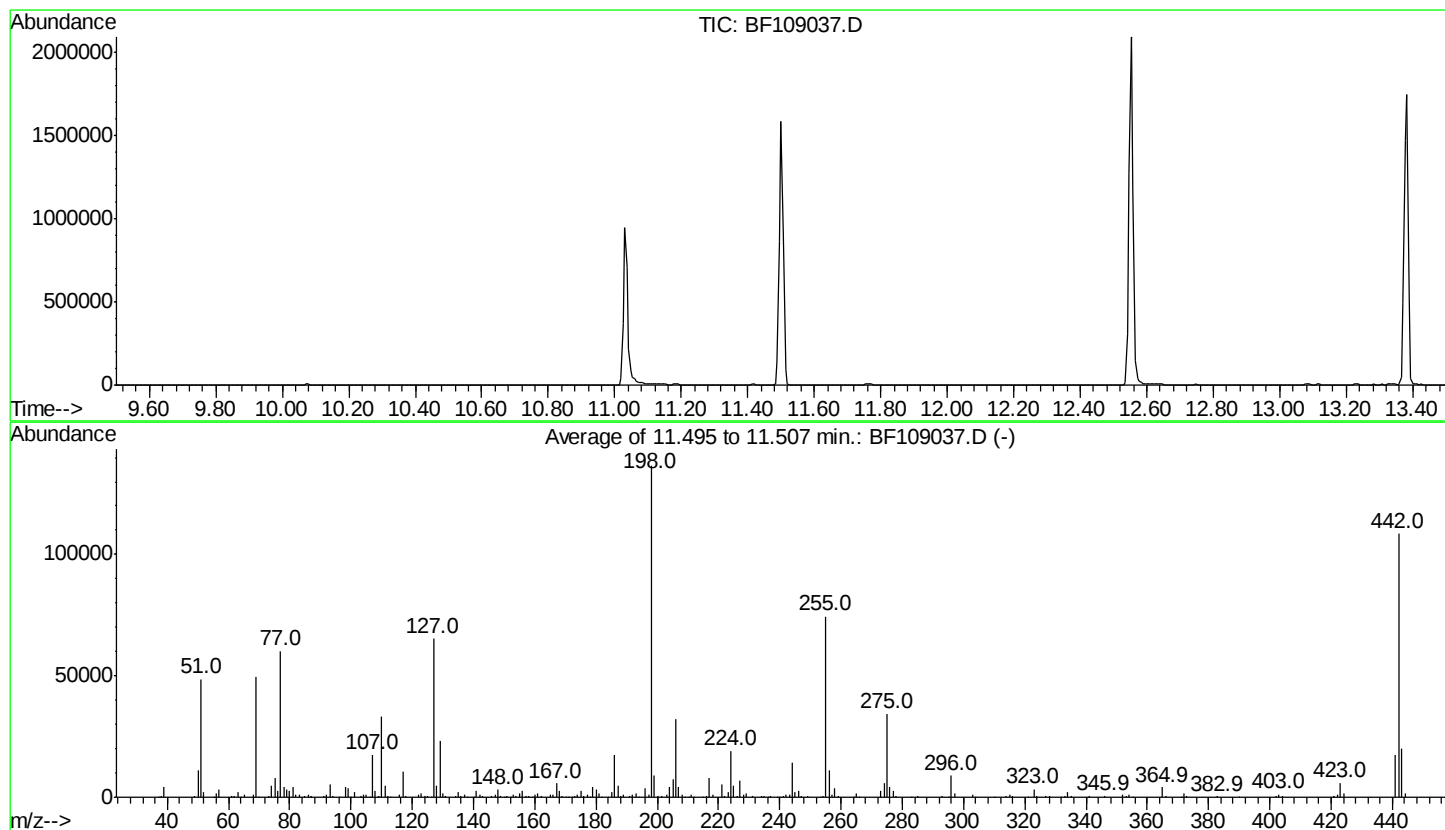

AutoFind: Scans 1557, 1558, 1559; Background Corrected with Scan 1552

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	48584	PASS
68	69	0.00	2	1.9	945	PASS
69	198	0.00	100	36.1	49330	PASS
70	69	0.00	2	0.5	240	PASS
127	198	10	80	47.8	65352	PASS
197	198	0.00	2	0.7	954	PASS
198	198	100	100	100.0	136610	PASS
199	198	5	9	6.6	9069	PASS
275	198	10	60	25.2	34429	PASS
365	198	1	100	3.1	4167	PASS
441	198	0.01	100	12.8	17483	PASS
442	198	50	100	79.4	108402	PASS
443	442	15	24	18.5	20043	PASS