


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091718\
 Data File : BF109064.D
 Acq On : 17 Sep 2018 23:26
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 14 13:26:52 2018

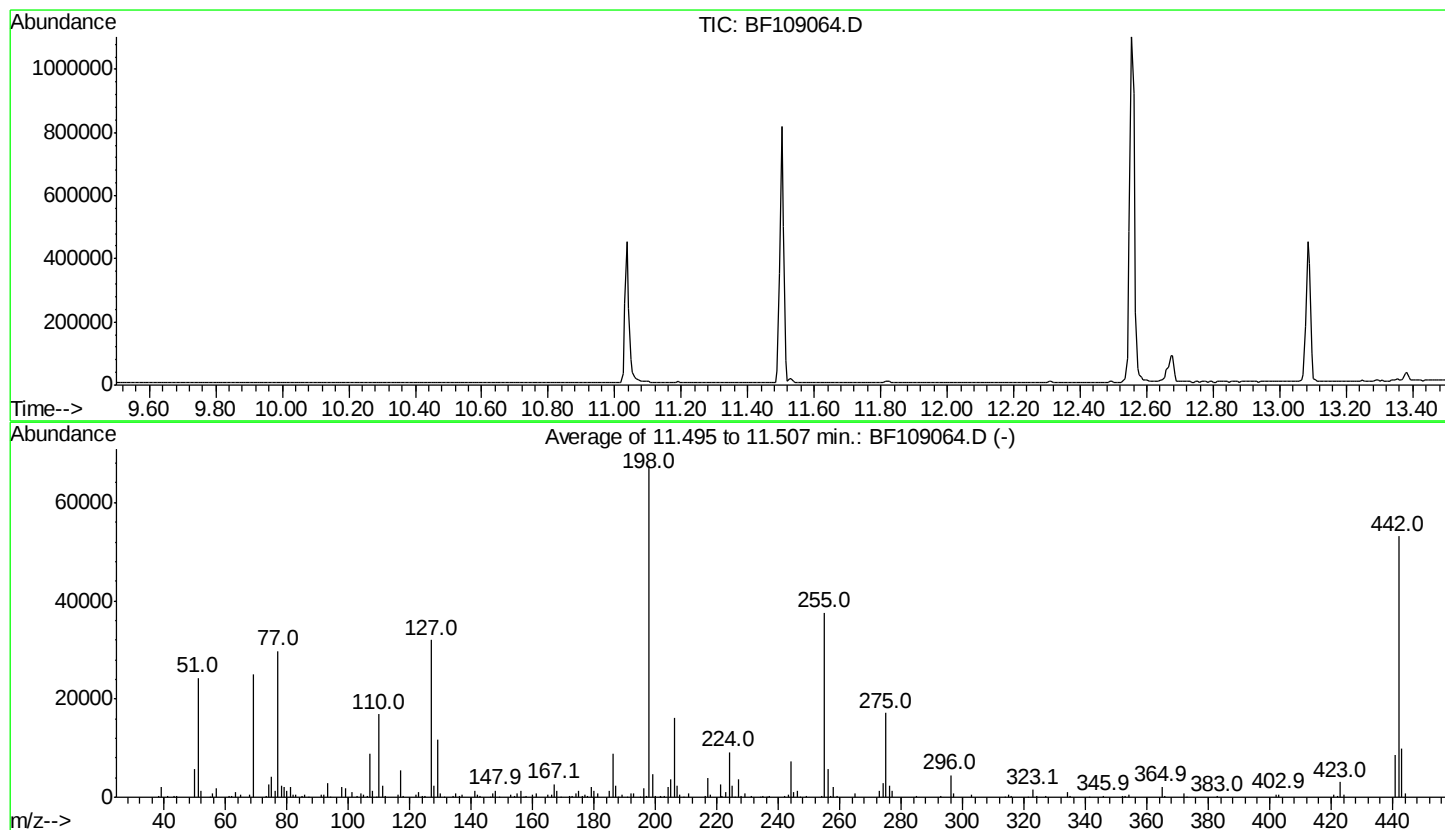

AutoFind: Scans 1557, 1558, 1559; Background Corrected with Scan 1553

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	24356	PASS
68	69	0.00	2	1.9	480	PASS
69	198	0.00	100	37.2	25125	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.4	31968	PASS
197	198	0.00	2	0.4	287	PASS
198	198	100	100	100.0	67514	PASS
199	198	5	9	6.9	4655	PASS
275	198	10	60	25.3	17108	PASS
365	198	1	100	3.2	2157	PASS
441	198	0.01	100	12.7	8549	PASS
442	198	50	100	78.7	53139	PASS
443	442	15	24	18.5	9808	PASS