

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091719\
 Data File : BF117096.D
 Acq On : 17 Sep 2019 10:24
 Operator : HP/JU
 Sample : PB123116BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB123116BL

Quant Time: Sep 17 17:51:17 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 13 16:23:17 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.82	152	77110	20.00	ng	0.00
21) Naphthalene-d8	8.10	136	303578	20.00	ng	0.00
39) Acenaphthene-d10	9.85	164	165868	20.00	ng	0.00
64) Phenanthrene-d10	11.34	188	264954	20.00	ng	0.00
76) Chrysene-d12	13.97	240	158319	20.00	ng	0.00
87) Perylene-d12	15.42	264	123493	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.46	112	598353	121.15	ng	0.02
7) Phenol-d6	6.47	99	811390	127.12	ng	0.01
23) Nitrobenzene-d5	7.39	82	530815	91.87	ng	0.00
42) 2,4,6-Tribromophenol	10.65	330	176449	127.28	ng	0.00
45) 2-Fluorobiphenyl	9.17	172	955300	90.05	ng	0.00
79) Terphenyl-d14	12.92	244	871259	102.87	ng	0.00
Target Compounds						
9) Benzaldehyde	6.47	77	1112	Below Cal		Qvalue
19) n-Nitroso-di-n-propylamine	7.39	70	69459	17.871	ng	# 1
25) Isophorone	7.39	82	530812	51.888	ng	# 79
51) 2,6-Dinitrotoluene	9.85	165	20347	8.507	ng	# 66
57) 2,4-Dinitrotoluene	9.85	165	20347	6.553	ng	# 24
65) 4,6-Dinitro-2-methylphenol	10.64	198	307	7.120	ng	# 18
67) 4-Bromophenyl-phenylether	10.64	248	11731	4.335	ng	# 1
77) Benzidine	12.92	184	12133	2.379	ng	# 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091719\
Data File : BF117096.D
Acq On : 17 Sep 2019 10:24
Operator : HP/JU
Sample : PB123116BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB123116BL

Quant Time: Sep 17 17:51:17 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 13 16:23:17 2019
Response via : Initial Calibration

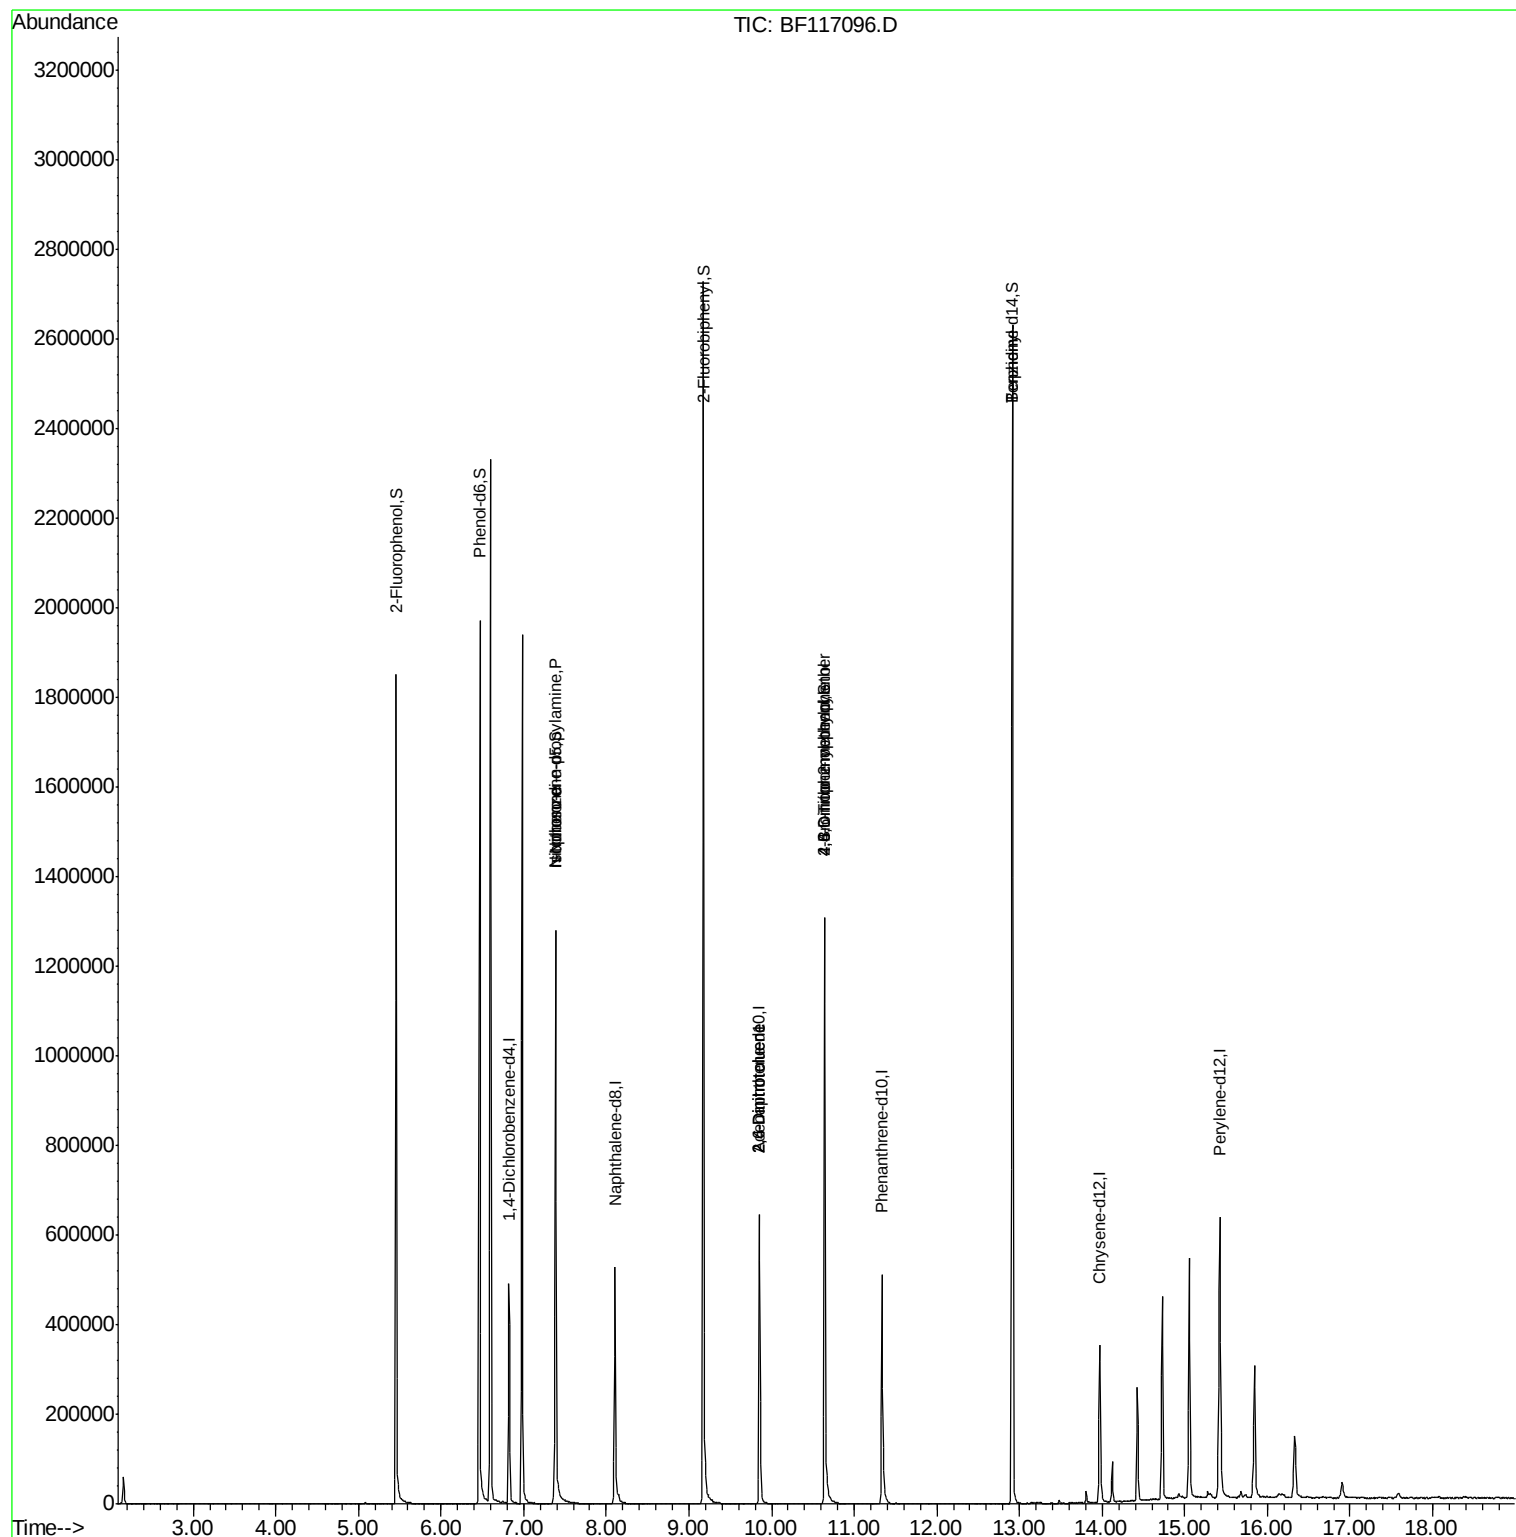

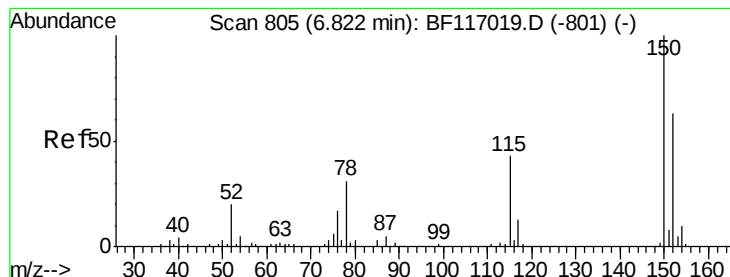


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.82 min Scan# 805
Delta R.T. 0.00 min
Lab File: BF117096.D
Acq: 17 Sep 2019 10:24

Instrument :
BNA_F
ClientSampleId :
PB123116BL

Tot Ion:152 Resp: 77110
Ion Ratio Lower Upper
152 100
150 159.3 127.5 191.3
115 67.6 55.0 82.4




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

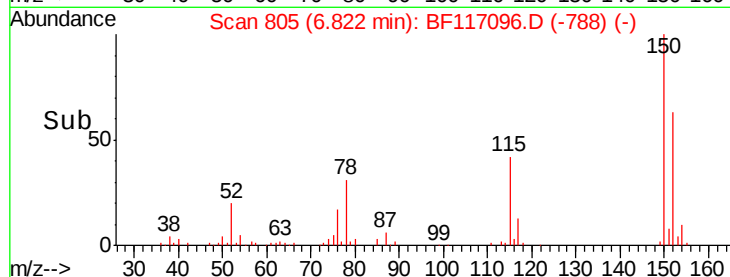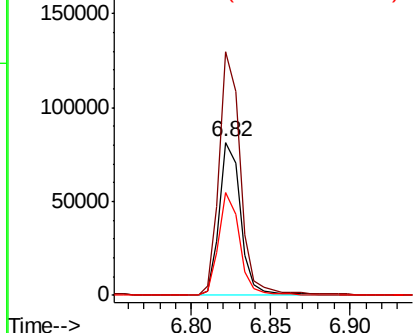



#5


2-Fluorophenol
Concen: 121.149 ng
RT: 5.46 min Scan# 573
Delta R.T. 0.02 min
Lab File: BF117096.D
Acq: 17 Sep 2019 10:24

Tgt Ion:112 Resp: 598353
Ion Ratio Lower Upper
112 100
64 59.7 45.7 68.5
63 31.7 24.9 37.3



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

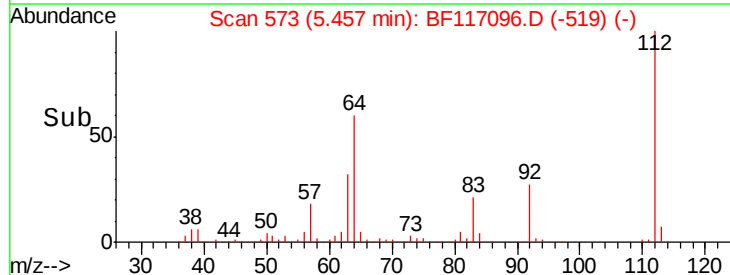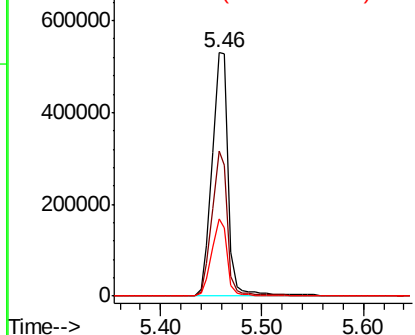

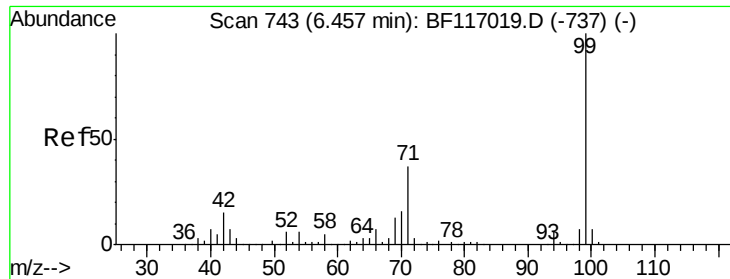

#7

Phenol-d6

Concen: 127.118 ng

RT: 6.47 min Scan# 745

Delta R.T. 0.01 min

Lab File: BF117096.D

Acq: 17 Sep 2019 10:24

Instrument :

BNA_F

ClientSampleId :

PB123116BL


Tot Ion: 99 Resp: 811390

Ion Ratio Lower Upper




99 100

42 15.3 12.2 18.2

71 36.7 29.8 44.8

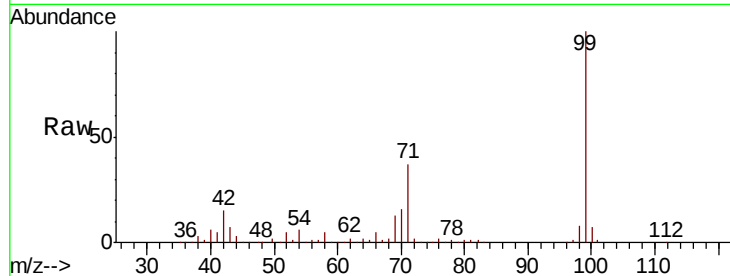

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

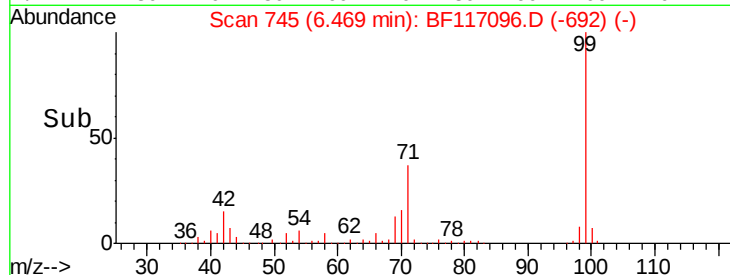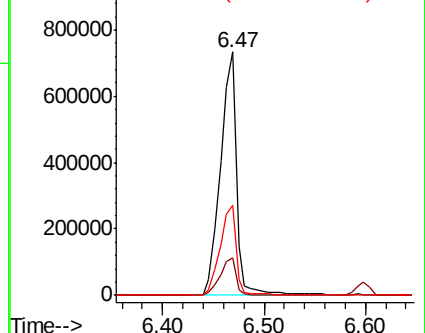

#9

Benzaldehyde

Concen: Below Cal

RT: 6.47 min Scan# 745

Delta R.T. 0.09 min

Lab File: BF117096.D

Acq: 17 Sep 2019 10:24


Tgt Ion: 77 Resp: 1112

Ion Ratio Lower Upper



77 100

105 0.0 81.8 121.8#

106 0.0 77.3 117.3#



Abundance Ion 77.00 (76.70 to 77.70): BF1
Ion 105.00 (104.70 to 105.70): E
Ion 106.00 (105.70 to 106.70): E

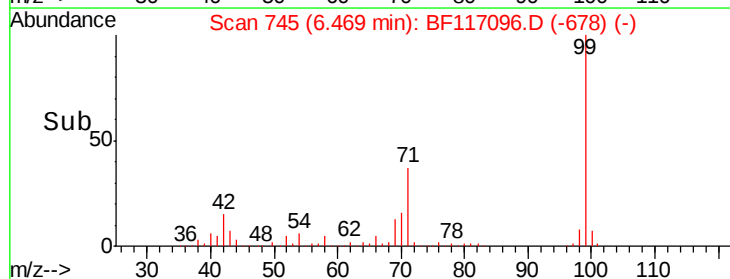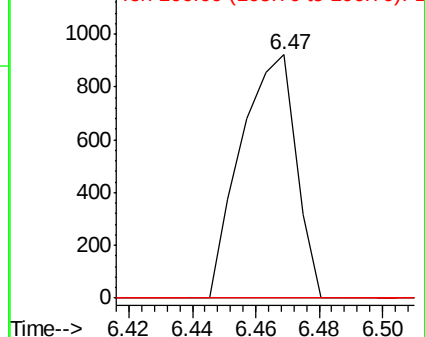



#19

n-Nitroso-di-n-propylamine

Concen: 17.871 ng

RT: 7.39 min Scan# 901

Delta R.T. 0.15 min

Lab File: BF117096.D

Acq: 17 Sep 2019 10:24

Instrument :

BNA_F

ClientSampleId :

PB123116BL

Tot Ion: 70 Resp: 69459





Ion Ratio Lower Upper

70 100

42 36.9 34.0 51.0

101 0.0 7.8 11.6#

130 2.0 17.8 26.8#

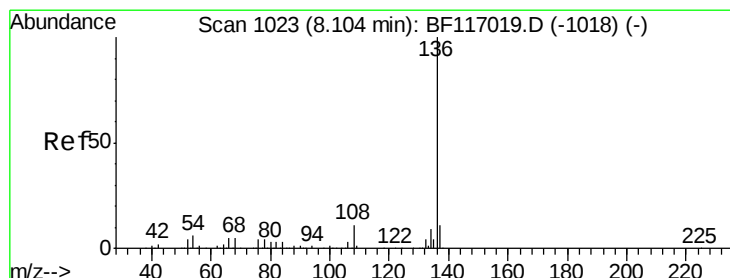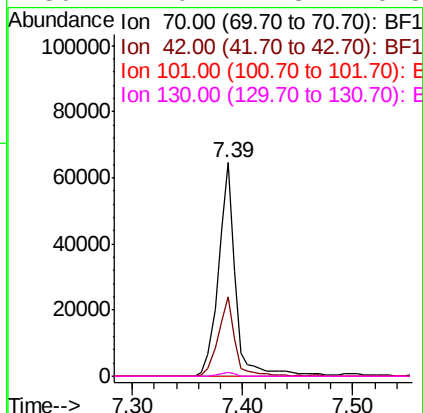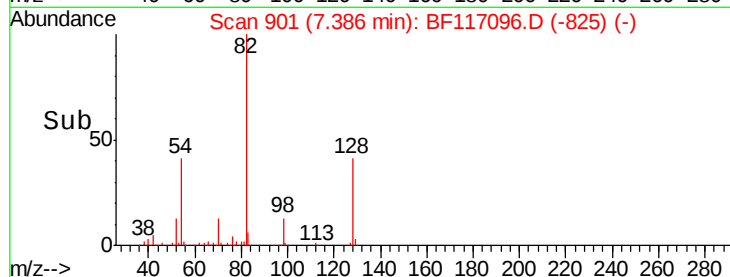

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.10 min Scan# 1023

Delta R.T. 0.00 min

Lab File: BF117096.D

Acq: 17 Sep 2019 10:24

Tgt Ion: 136 Resp: 303578




Ion Ratio Lower Upper


136 100

137 11.2 9.0 13.4

54 5.5 4.5 6.7

68 4.1 4.0 6.0

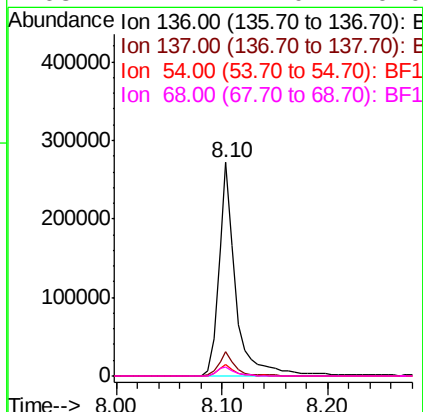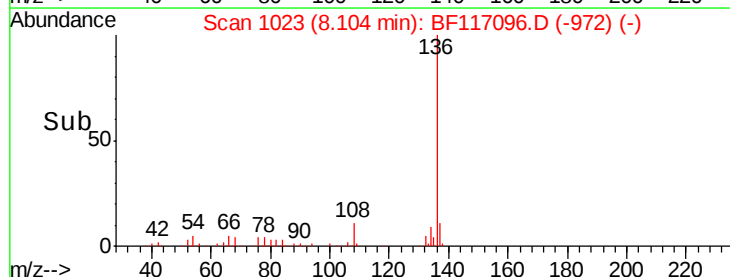

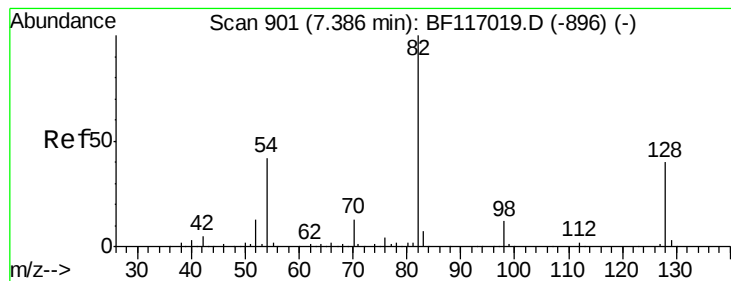

#23

Nitrobenzene-d5

Concen: 91.872 ng

RT: 7.39 min Scan# 901

Delta R.T. 0.00 min

Lab File: BF117096.D

Acq: 17 Sep 2019 10:24

Instrument :

BNA_F

ClientSampleId :

PB123116BL


Tot Ion: 82 Resp: 530815

Ion Ratio Lower Upper

82 100

128 40.9 32.3 48.5




54 40.8 33.3 49.9

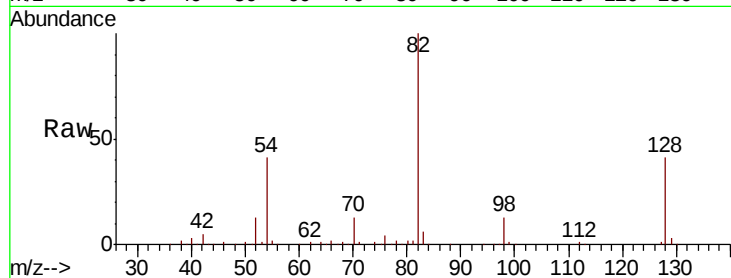

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): BF1

Ion 54.00 (53.70 to 54.70): BF1

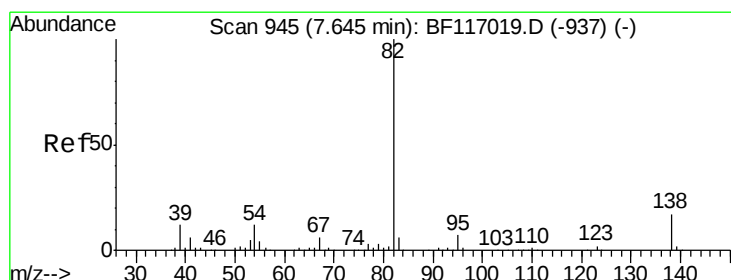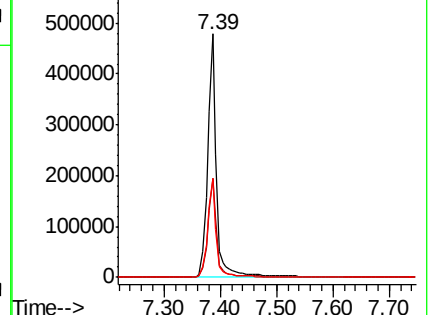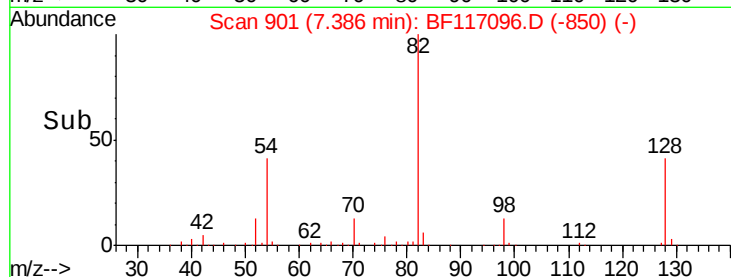

#25

Isophorone

Concen: 51.888 ng

RT: 7.39 min Scan# 901

Delta R.T. -0.26 min

Lab File: BF117096.D

Acq: 17 Sep 2019 10:24


Tgt Ion: 82 Resp: 530812

Ion Ratio Lower Upper

82 100

95 0.0 5.8 8.6#



138 0.0 13.5 20.3#

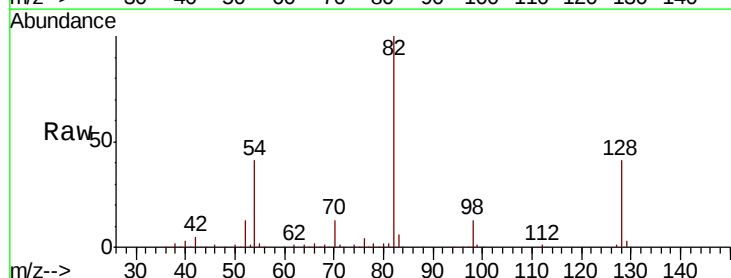


Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

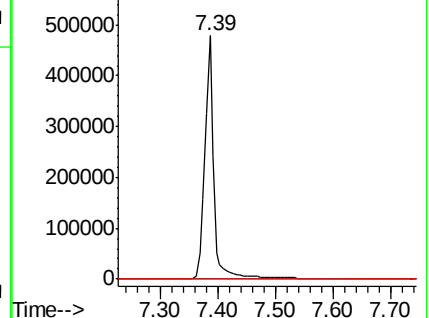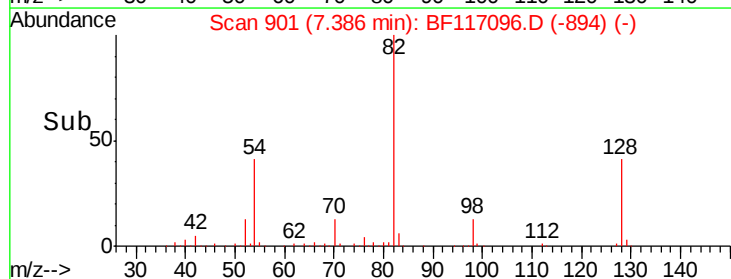

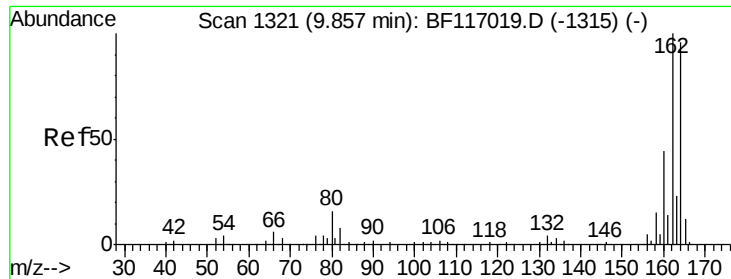

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.85 min Scan# 1320

Delta R.T. -0.01 min

Lab File: BF117096.D

Acq: 17 Sep 2019 10:24

Instrument :

BNA_F

ClientSampleId :

PB123116BL


Tot Ion:164 Resp: 165868

Ion Ratio Lower Upper

164 100

162 102.0 83.4 125.2




160 44.7 36.4 54.6

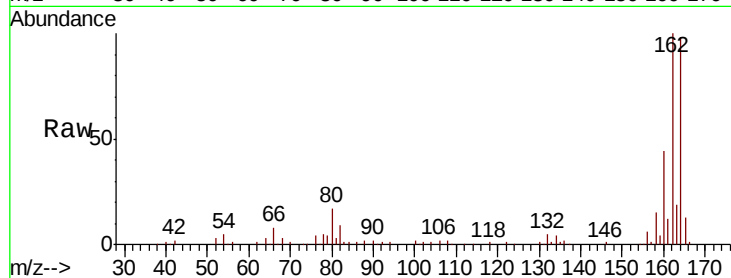

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

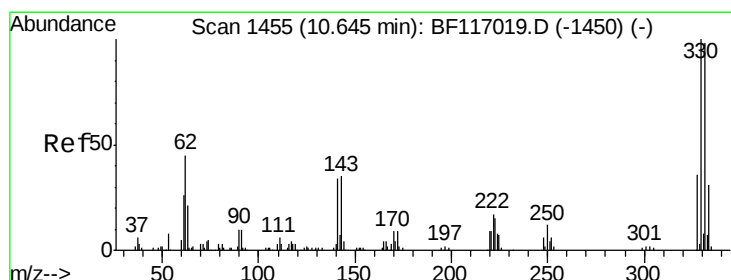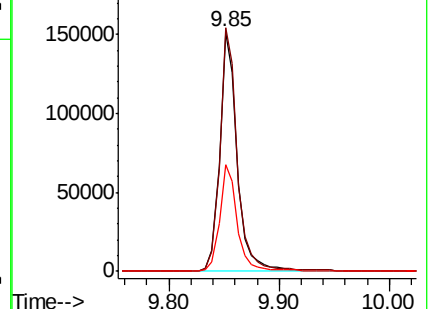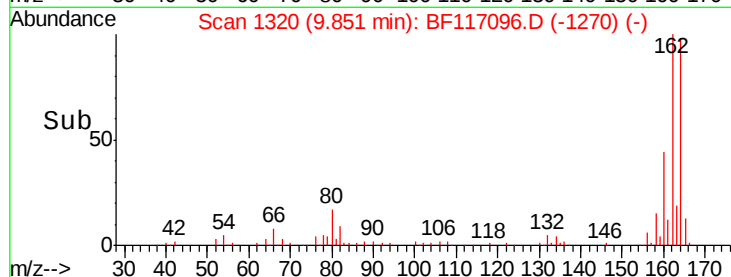

#42

2,4,6-Tribromophenol

Concen: 127.283 ng

RT: 10.65 min Scan# 1455

Delta R.T. 0.00 min

Lab File: BF117096.D

Acq: 17 Sep 2019 10:24


Tgt Ion:330 Resp: 176449

Ion Ratio Lower Upper

330 100

332 97.0 78.0 117.0



141 45.1 35.8 53.6

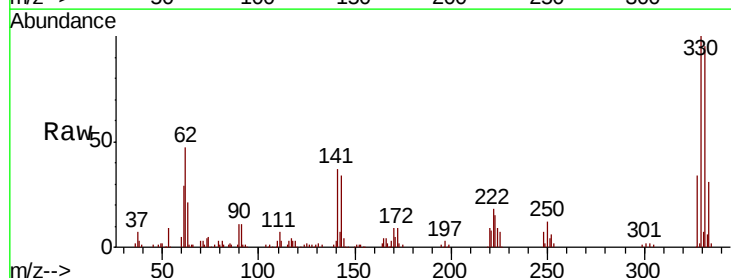

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



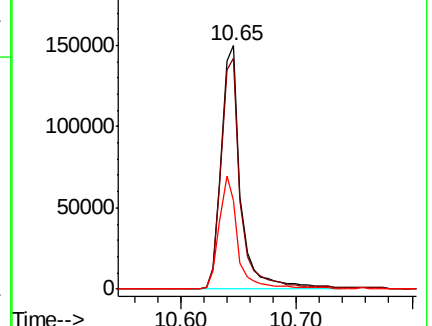
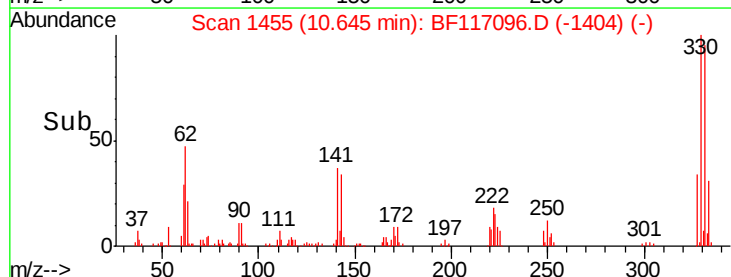




#45
 2-Fluorobiphenyl
 Concen: 90.053 ng
 RT: 9.17 min Scan# 1205
 Delta R.T. 0.00 min
 Lab File: BF117096.D
 Acq: 17 Sep 2019 10:24




Instrument :
 BNA_F
 ClientSampleId :
 PB123116BL


Tot Ion:172 Resp: 955300
 Ion Ratio Lower Upper
 172 100
 171 35.4 28.2 42.2
 170 23.5 18.9 28.3

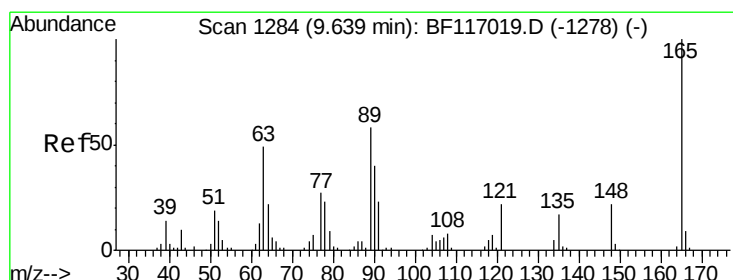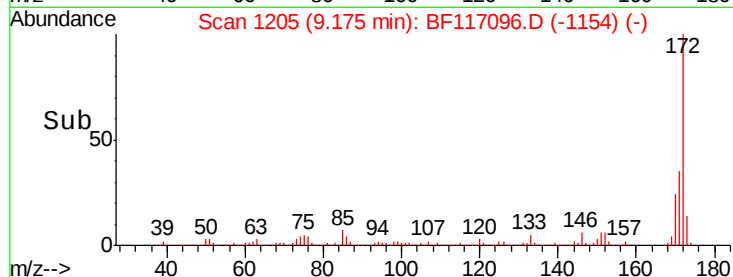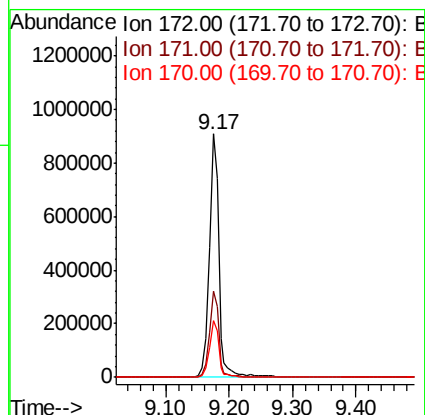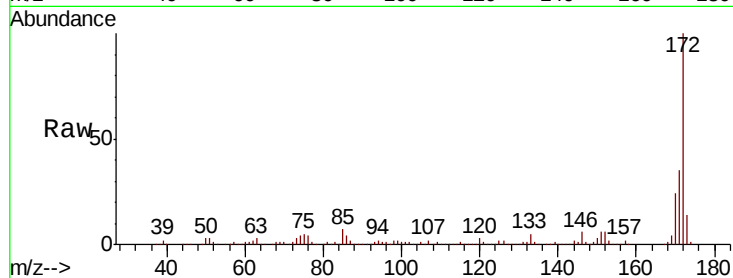

#51
 2,6-Dinitrotoluene
 Concen: 8.507 ng
 RT: 9.85 min Scan# 1320
 Delta R.T. 0.21 min
 Lab File: BF117096.D
 Acq: 17 Sep 2019 10:24

Tgt Ion:165 Resp: 20347
 Ion Ratio Lower Upper
 165 100
 63 0.0 41.8 62.8#
 89 0.0 46.5 69.7#


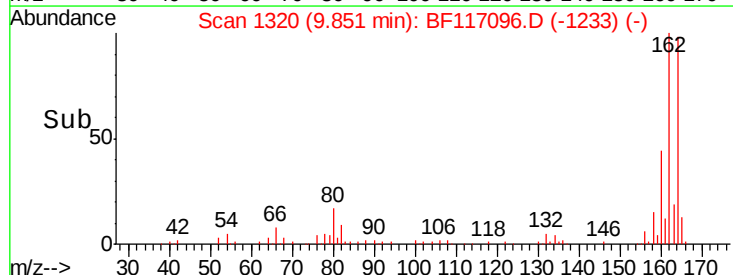
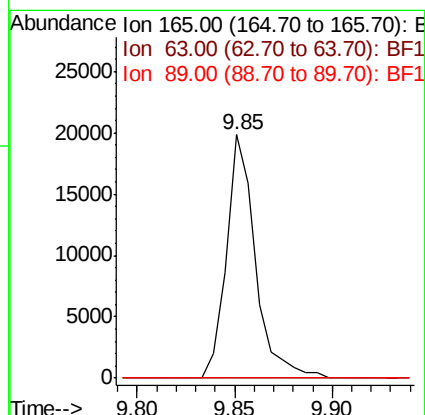
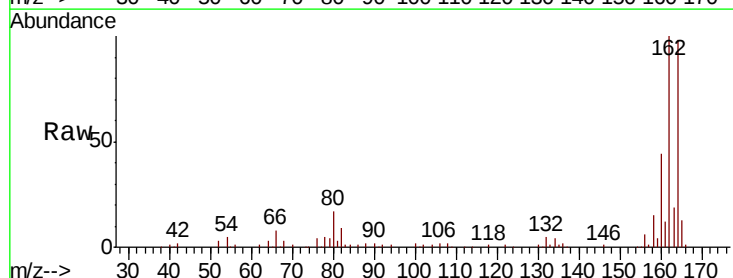


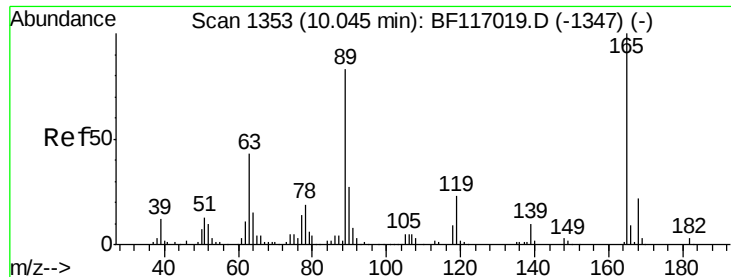

#57
 2,4-Dinitrotoluene
 Concen: 6.553 ng
 RT: 9.85 min Scan# 1320
 Delta R.T. -0.19 min
 Lab File: BF117096.D
 Acq: 17 Sep 2019 10:24




Instrument :
 BNA_F
 ClientSampleId :
 PB123116BL


Tot Ion:165	Resp:	20347
Ion Ratio	Lower	Upper
165	100	
63	0.0	35.0 52.4#
89	0.0	66.1 99.1#
182	0.0	2.0 3.0#

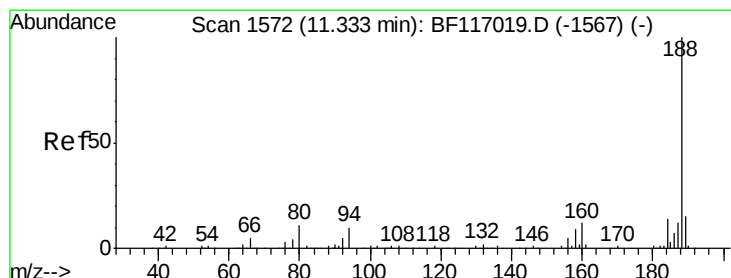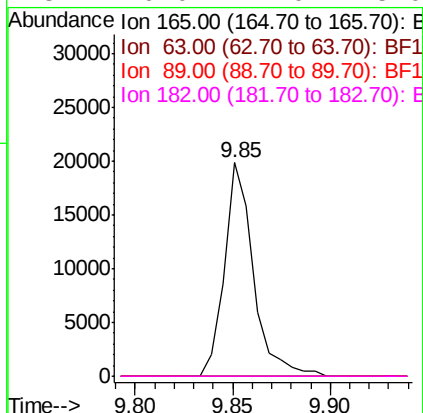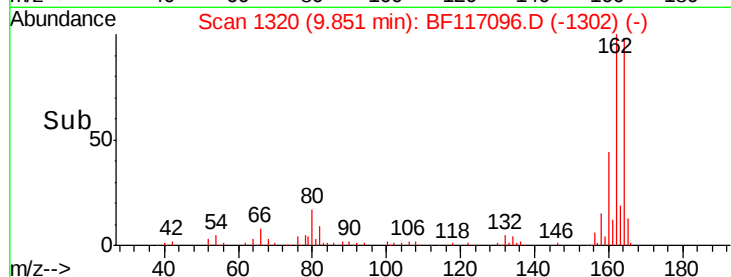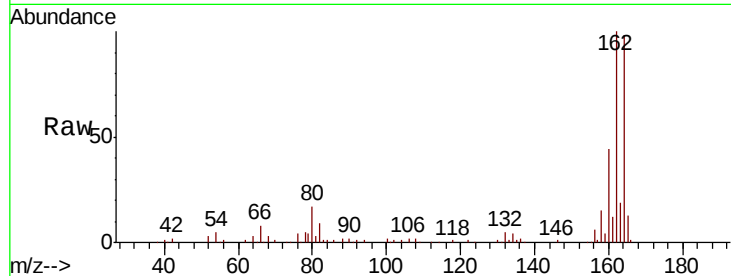

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.34 min Scan# 1573
 Delta R.T. 0.01 min
 Lab File: BF117096.D
 Acq: 17 Sep 2019 10:24

Tgt Ion:188	Resp:	264954
Ion Ratio	Lower	Upper
188	100	
94	8.3	8.2 12.2
80	9.7	9.0 13.6

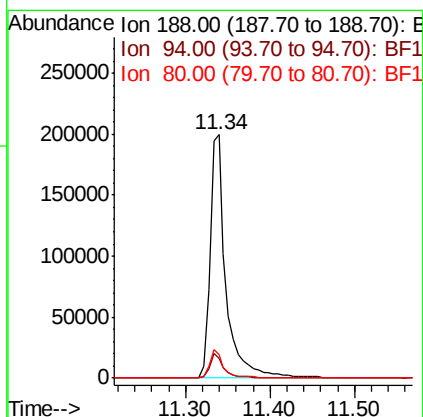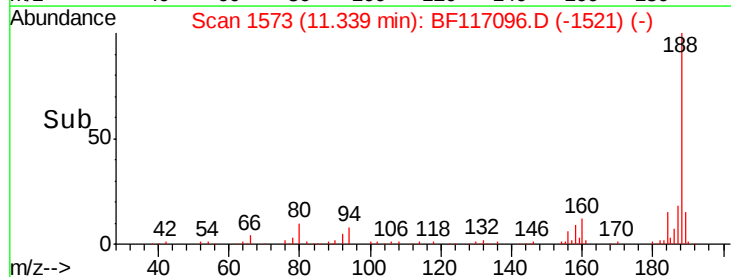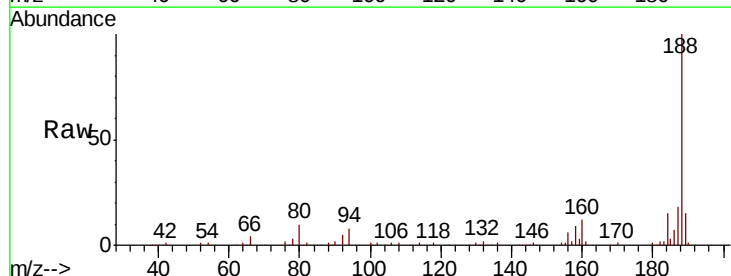


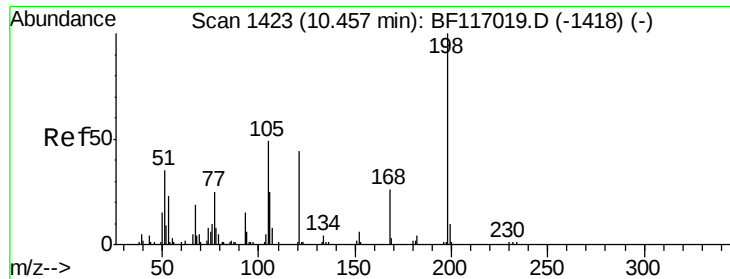




#65
 4,6-Dinitro-2-methylphenol
 Concen: 7.120 ng
 RT: 10.64 min Scan# 1454
 Delta R.T. 0.18 min
 Lab File: BF117096.D
 Acq: 17 Sep 2019 10:24

Instrument :
 BNA_F
 ClientSampleId :
 PB123116BL

Tot Ion:198 Resp: 307
 Ion Ratio Lower Upper
 198 100
 51 176.9 18.7 58.7#
 105 226.5 30.2 70.2#

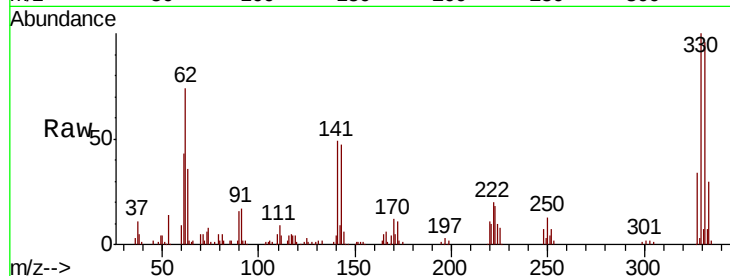


Abundance Ion 198.00 (197.70 to 198.70): E
 Ion 51.00 (50.70 to 51.70): BF1
 Ion 105.00 (104.70 to 105.70): E

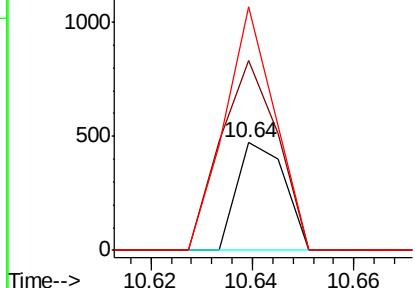
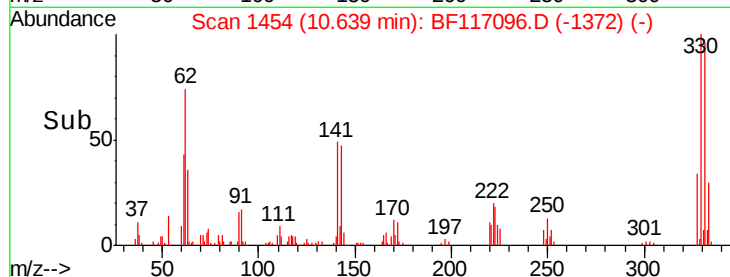



#67
 4-Bromophenyl-phenylether
 Concen: 4.335 ng
 RT: 10.64 min Scan# 1454
 Delta R.T. -0.24 min
 Lab File: BF117096.D
 Acq: 17 Sep 2019 10:24

Tgt Ion:248 Resp: 11731
 Ion Ratio Lower Upper
 248 100
 250 180.8 76.2 114.4#
 141 678.7 75.0 112.4#



Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E



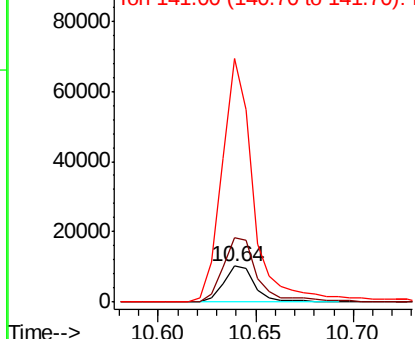
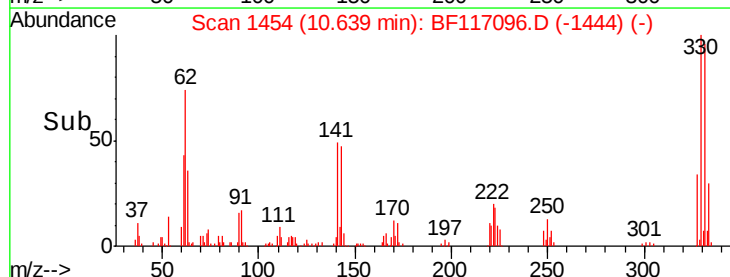


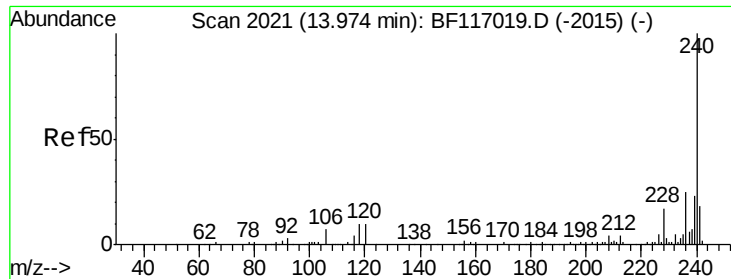

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.97 min Scan# 2020
Delta R.T. -0.01 min
Lab File: BF117096.D
Acq: 17 Sep 2019 10:24




Instrument :
BNA_F
ClientSampleId :
PB123116BL


Tot Ion:240 Resp: 158319
Ion Ratio Lower Upper
240 100
120 12.4 8.3 12.5
236 25.8 20.3 30.5

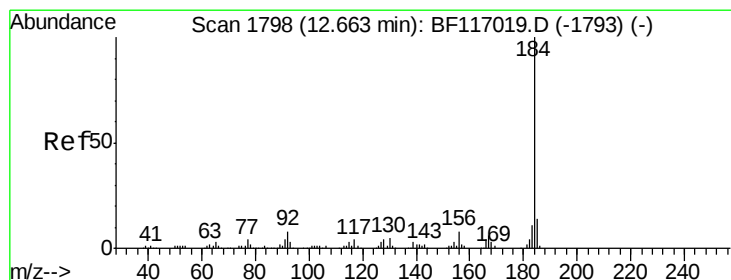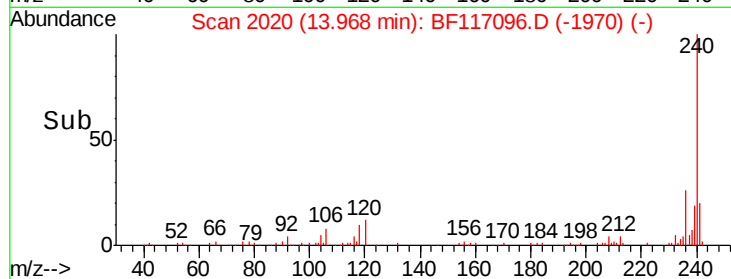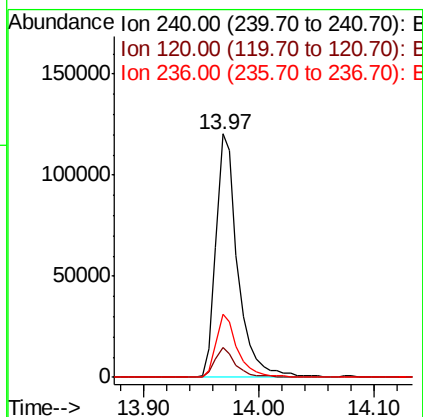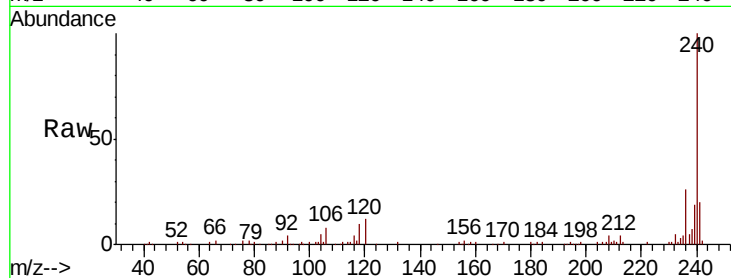

#77
Benzidine
Concen: 2.379 ng
RT: 12.92 min Scan# 1841
Delta R.T. 0.25 min
Lab File: BF117096.D
Acq: 17 Sep 2019 10:24

Tgt Ion:184 Resp: 12133
Ion Ratio Lower Upper
184 100
185 17.3 11.6 17.4
183 8.0 9.0 13.4#

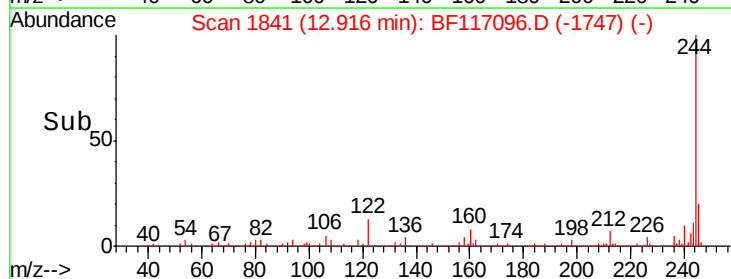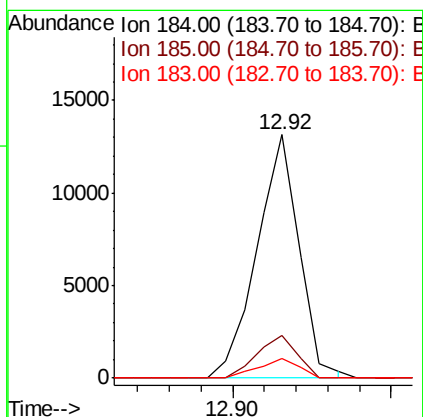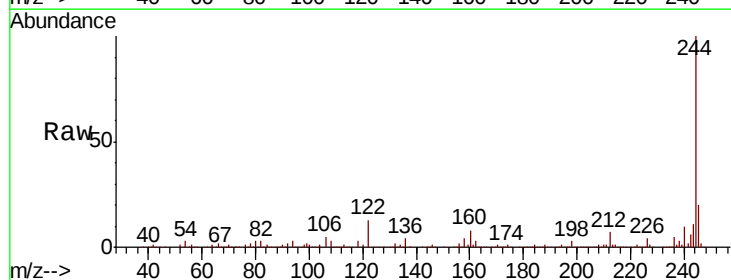

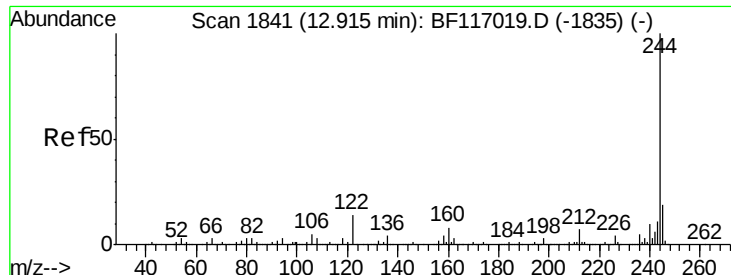

#79

Terphenyl-d14

Concen: 102.867 ng

RT: 12.92 min Scan# 1841

Delta R.T. 0.00 min

Lab File: BF117096.D

Acq: 17 Sep 2019 10:24

Instrument :

BNA_F

ClientSampleId :

PB123116BL


Tot Ion:244 Resp: 871259

Ion Ratio Lower Upper

244 100

212 7.4 5.8 8.8




122 13.4 11.3 16.9

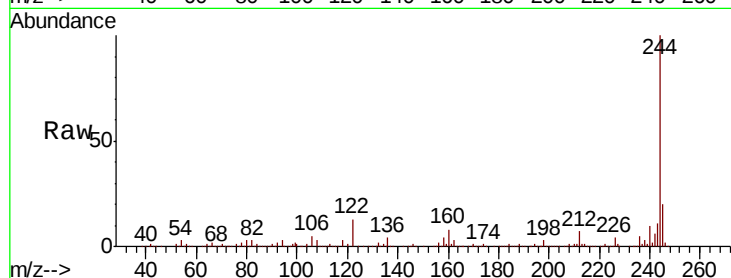

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

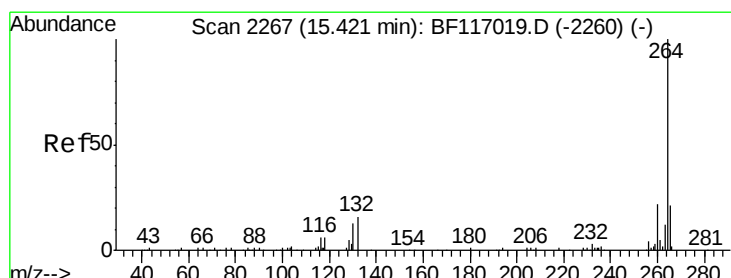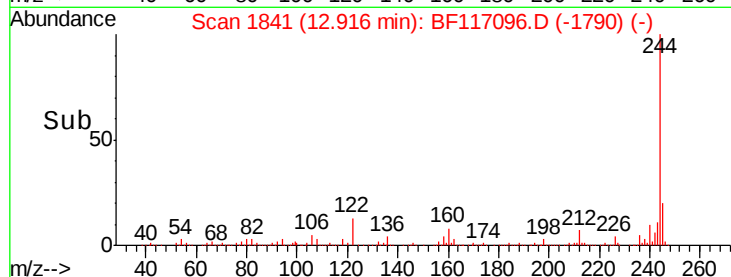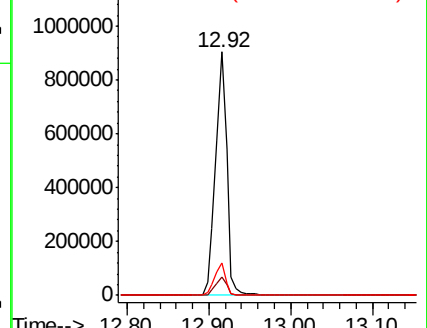

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.42 min Scan# 2267

Delta R.T. 0.00 min

Lab File: BF117096.D

Acq: 17 Sep 2019 10:24


Tgt Ion:264 Resp: 123493

Ion Ratio Lower Upper

264 100

260 22.2 17.6 26.4

265 22.3 16.6 24.8

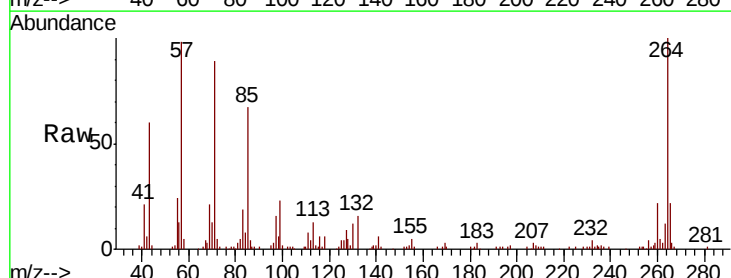

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

