
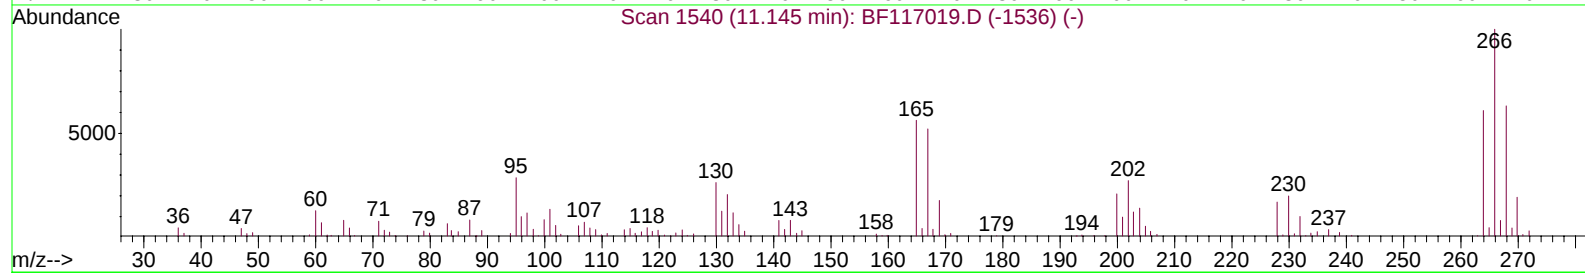
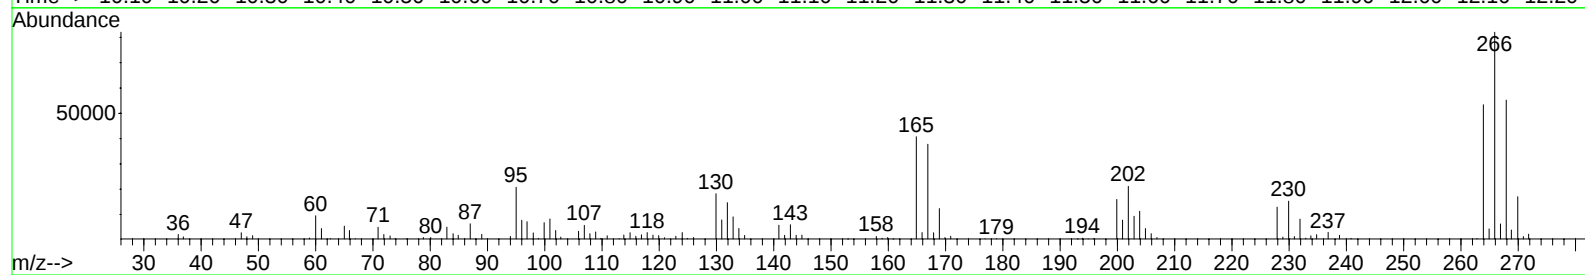


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF091719\
Data File : BF117093.D
Acq On : 17 Sep 2019 8:05
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 17 19:10:48 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 13 16:23:17 2019
Response via : Initial Calibration

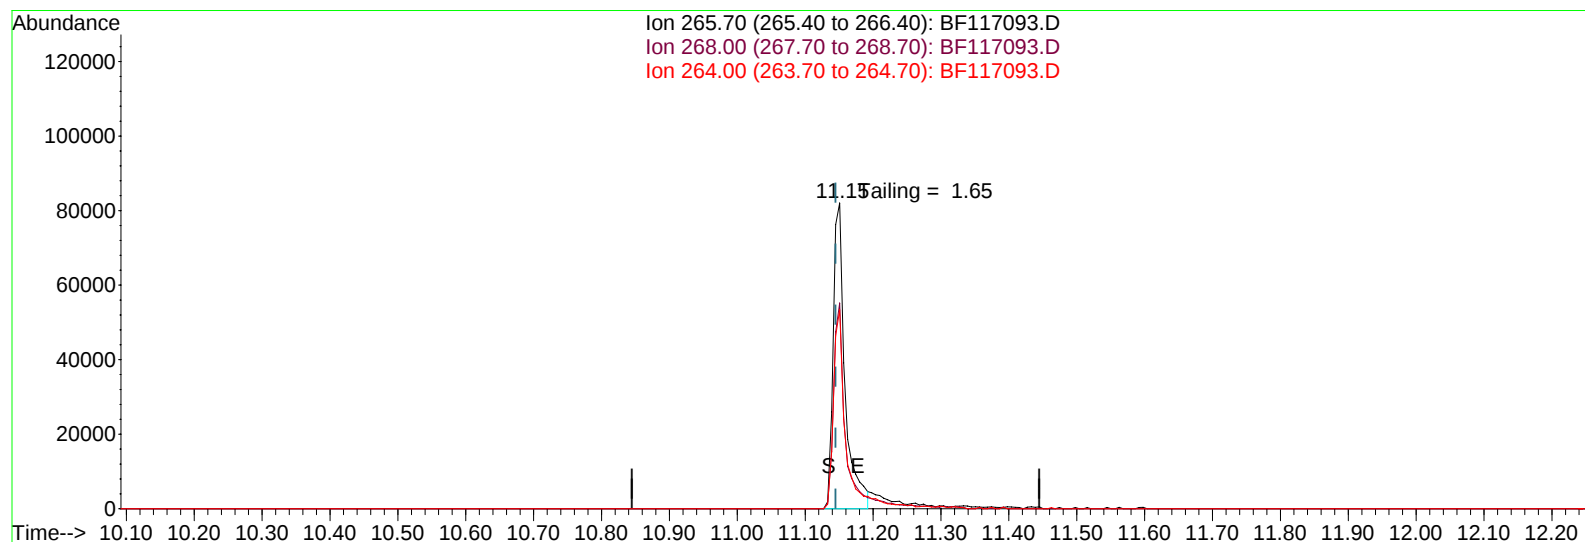

TIC: BF117093.D

(70) Pentachlorophenol (C)




11.151min (+0.006) 34170.99ng

response 108959

Ion	Exp%	Act%
265.70	100	100
268.00	63.10	67.30
264.00	61.00	65.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF091719\
 Data File : BF117093.D
 Acq On : 17 Sep 2019 8:05
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 17 19:10:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 13 16:23:17 2019
 Response via : Initial Calibration

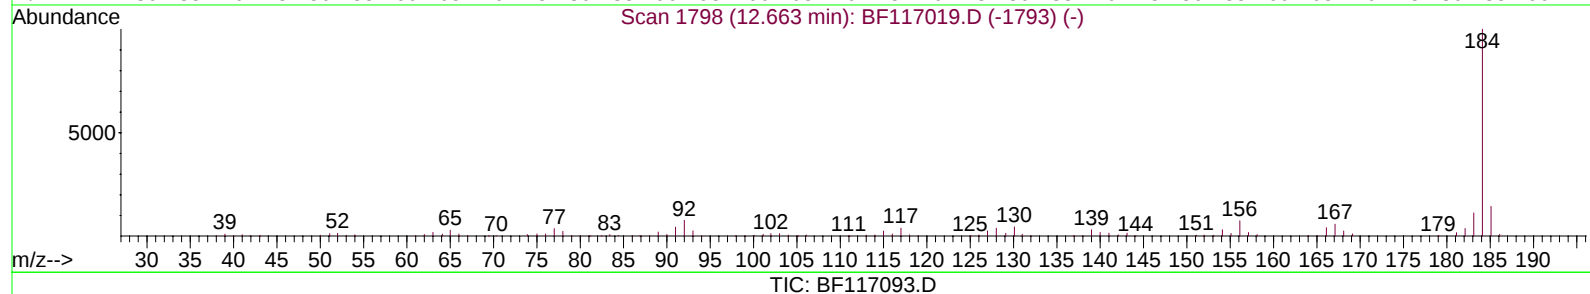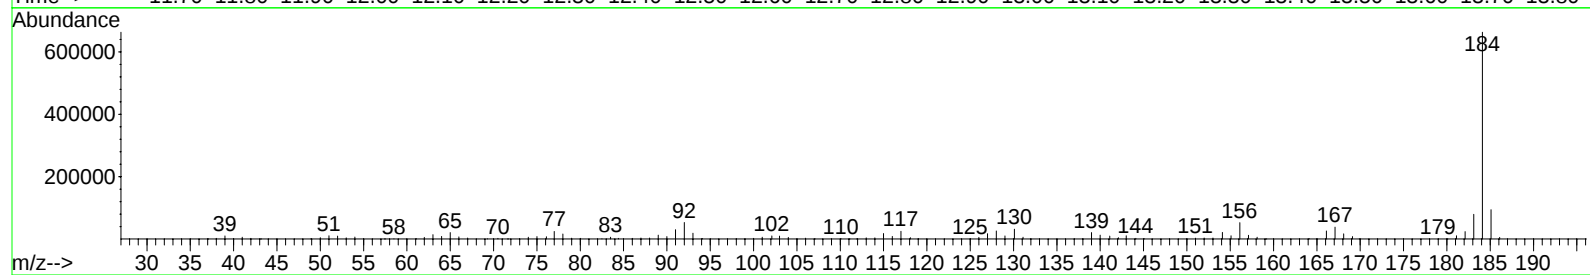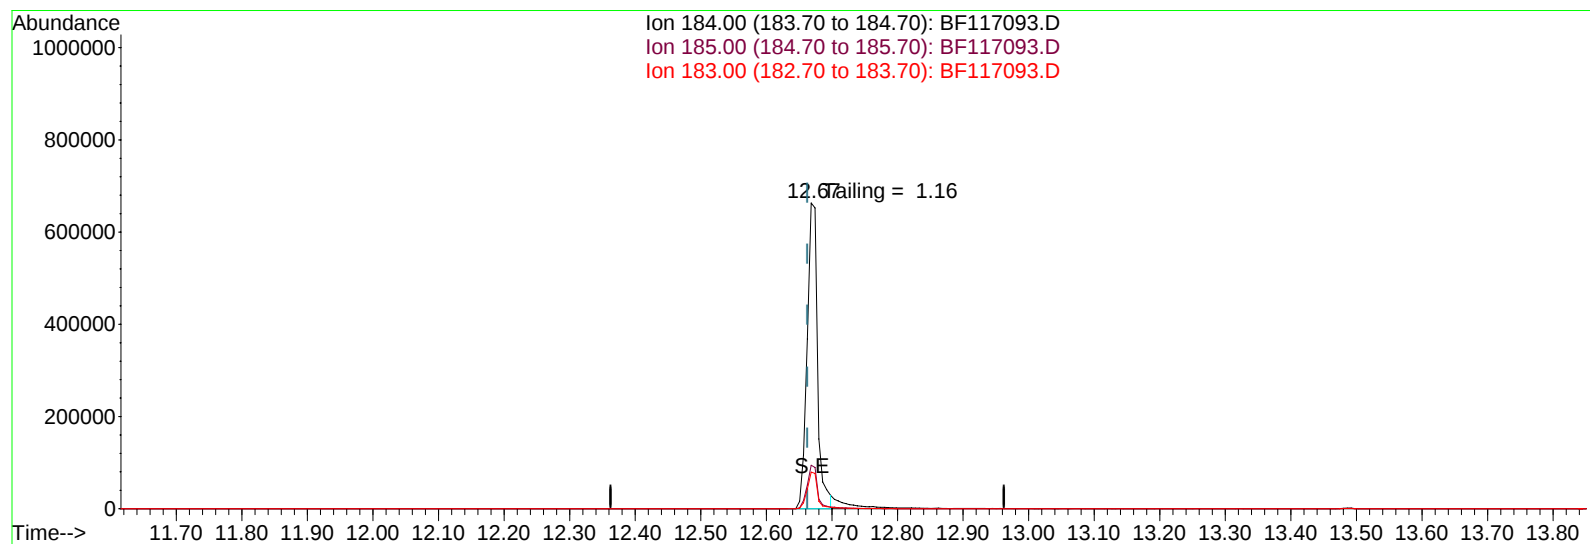

(77) Benzidine

12.668min (+0.006) 0.00ng

response 786692

Ion	Exp%	Act%
184.00	100	100
185.00	14.50	14.23
183.00	11.20	12.00
0.00	0.00	0.00