

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091719\
 Data File : BF117106.D
 Acq On : 17 Sep 2019 15:04
 Operator : HP/JU
 Sample : K4883-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW6-R2-1

Quant Time: Sep 26 07:52:29 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 13 16:23:17 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.82	152	64912	20.00	ng	0.00
21) Naphthalene-d8	8.10	136	249673	20.00	ng	0.00
39) Acenaphthene-d10	9.85	164	129886	20.00	ng	0.00
64) Phenanthrene-d10	11.33	188	214016	20.00	ng	0.00
76) Chrysene-d12	13.97	240	145934	20.00	ng	0.00
87) Perylene-d12	15.42	264	121492	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.45	112	217400	52.29	ng	0.00
7) Phenol-d6	6.46	99	174156	32.41	ng	0.00
23) Nitrobenzene-d5	7.39	82	423338	89.09	ng	0.00
42) 2,4,6-Tribromophenol	10.64	330	141219	130.09	ng	0.00
45) 2-Fluorobiphenyl	9.17	172	734227	88.39	ng	0.00
79) Terphenyl-d14	12.92	244	621674	79.63	ng	0.00
Target Compounds						
10) Phenol	6.47	94	25146	4.245	ng	94
50) Dimethylphthalate	9.57	163	37091	4.033	ng	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091719\
Data File : BF117106.D
Acq On : 17 Sep 2019 15:04
Operator : HP/JU
Sample : K4883-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW6-R2-1

Quant Time: Sep 26 07:52:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 13 16:23:17 2019
Response via : Initial Calibration

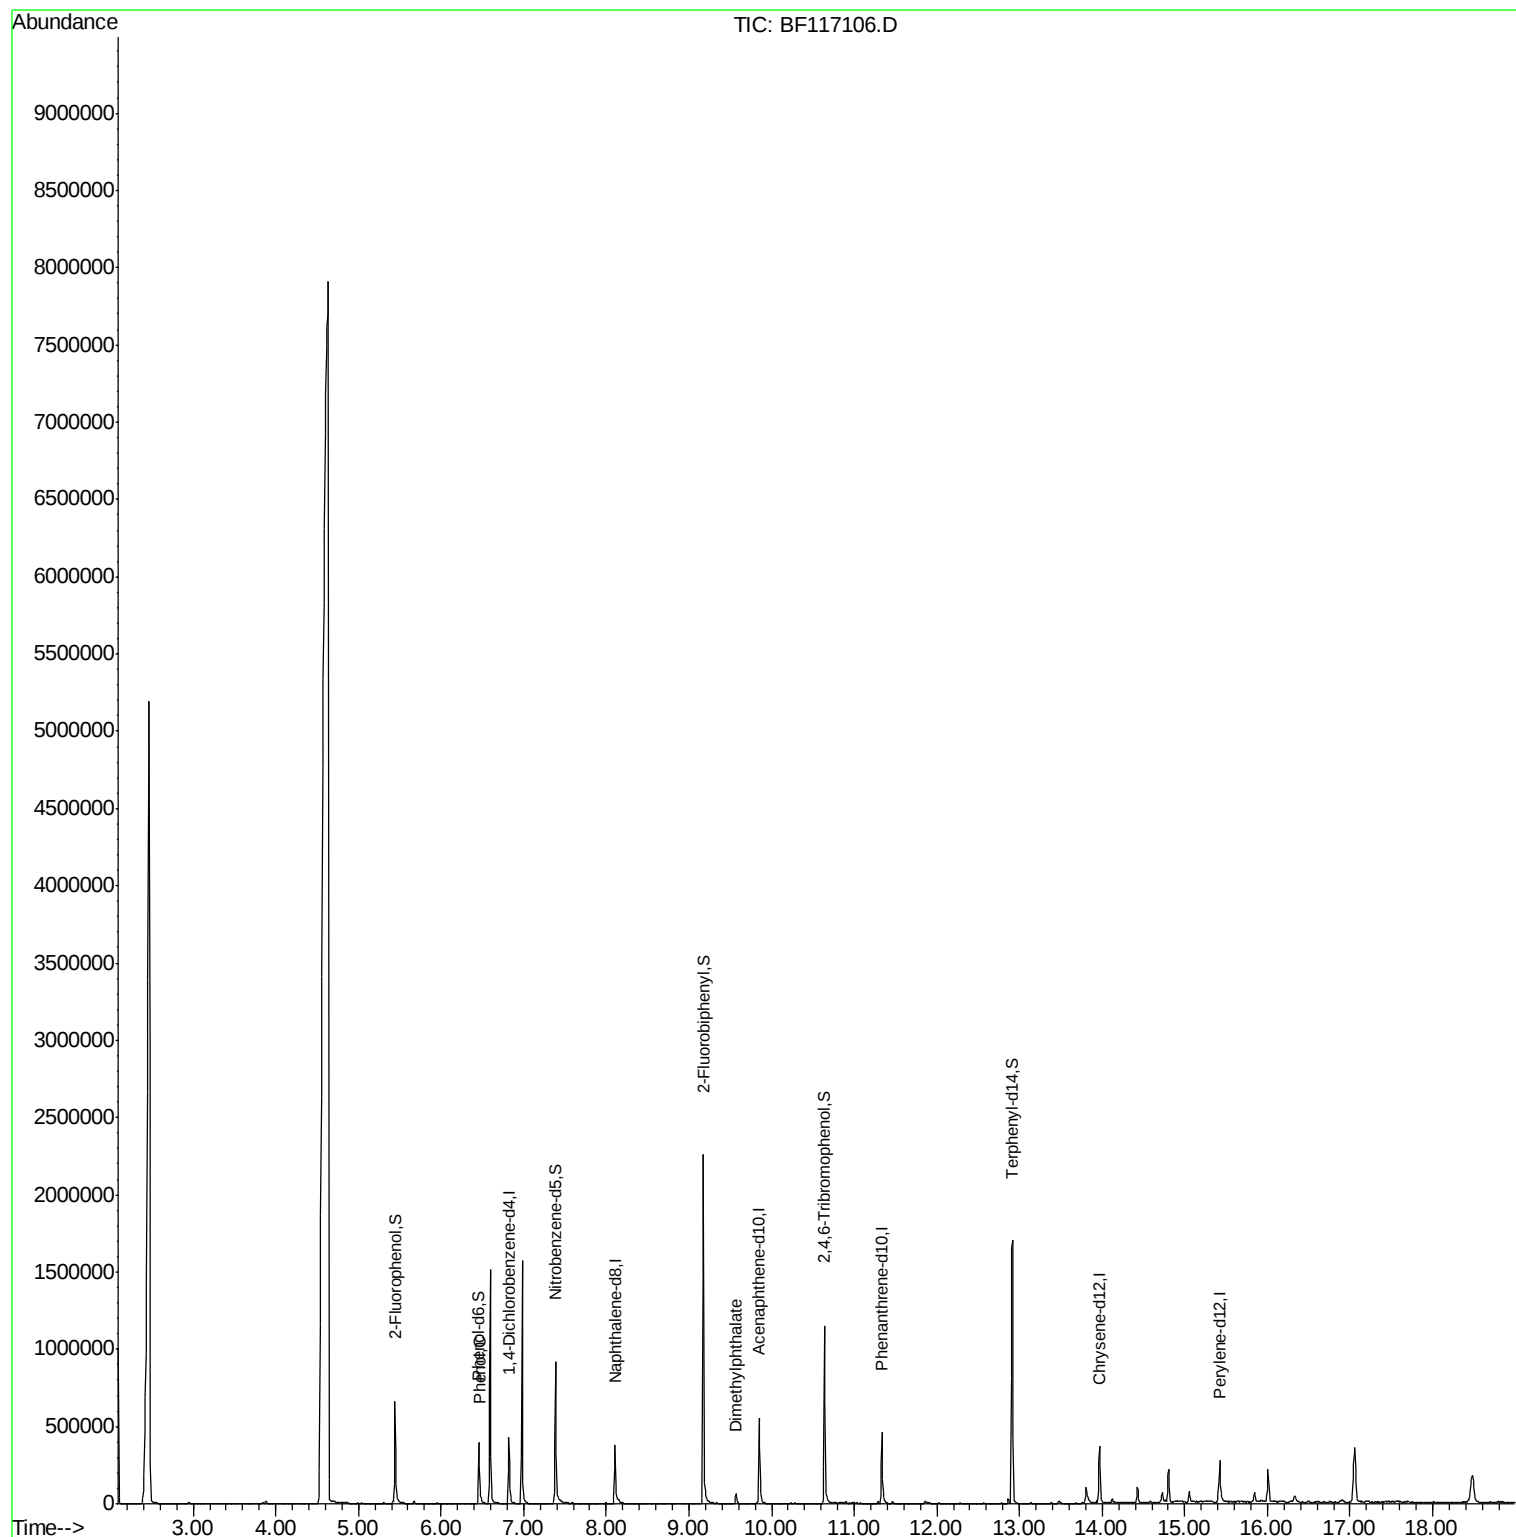




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.82 min Scan# 805
Delta R.T. 0.00 min
Lab File: BF117106.D
Acq: 17 Sep 2019 15:04

Instrument :
BNA_F
ClientSampleId :
MW6-R2-1

Tot Ion:152 Resp: 64912
Ion Ratio Lower Upper
152 100
150 152.4 127.5 191.3
115 65.2 55.0 82.4

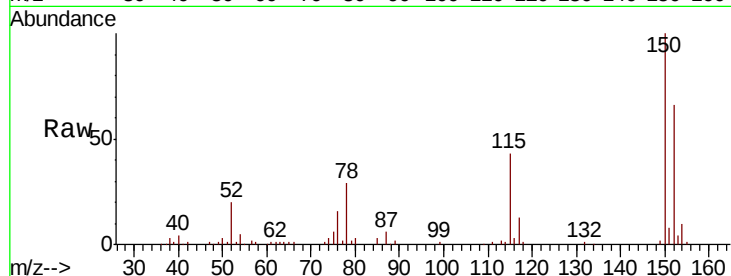


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

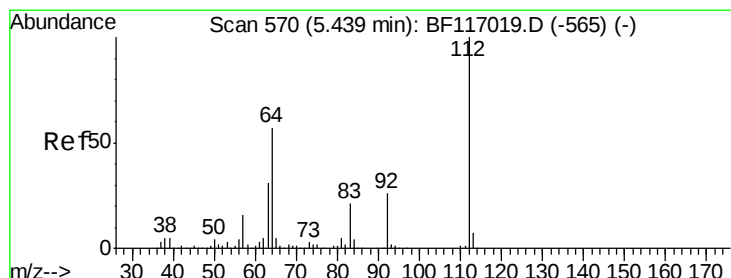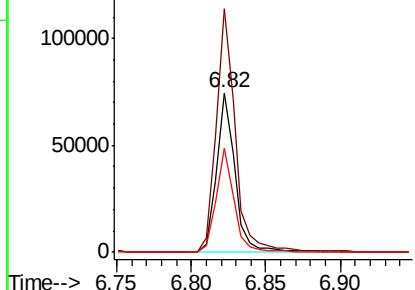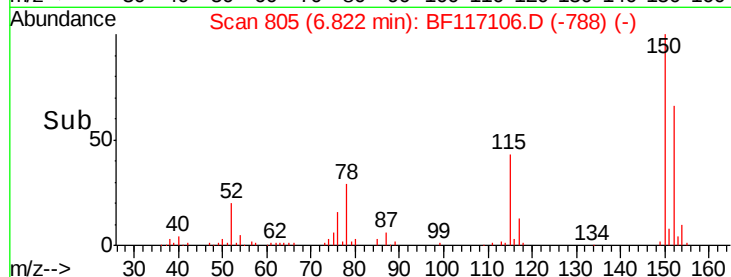



#5




2-Fluorophenol
Concen: 52.289 ng
RT: 5.45 min Scan# 571
Delta R.T. 0.01 min
Lab File: BF117106.D
Acq: 17 Sep 2019 15:04

Tgt Ion:112 Resp: 217400
Ion Ratio Lower Upper
112 100
64 54.5 45.7 68.5
63 29.2 24.9 37.3

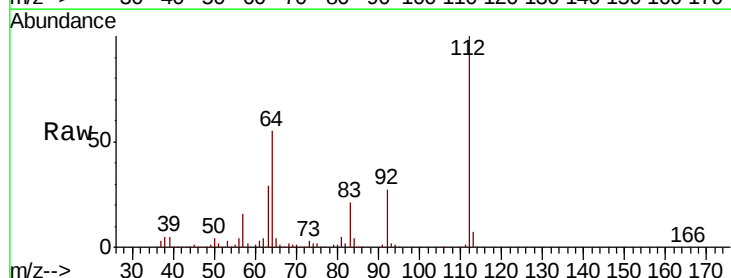

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

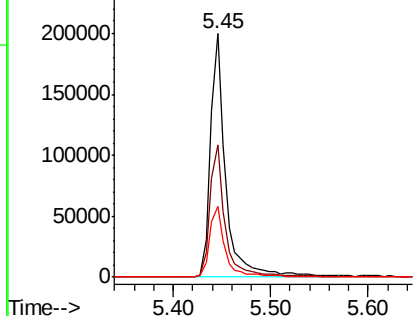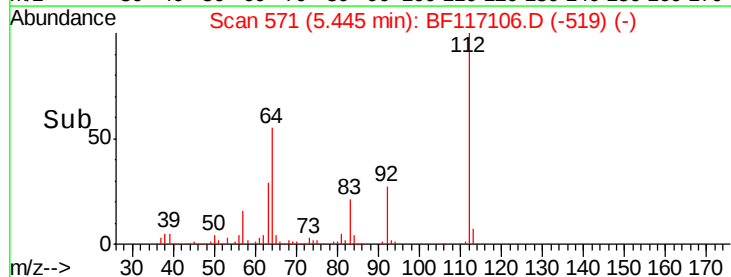

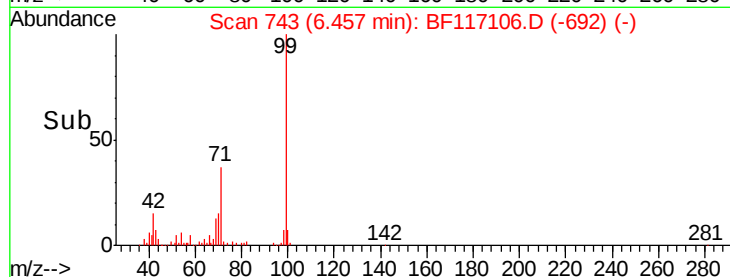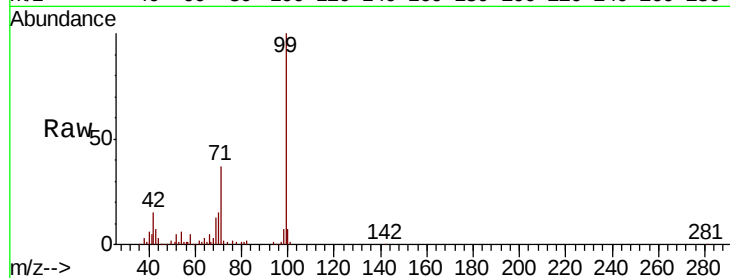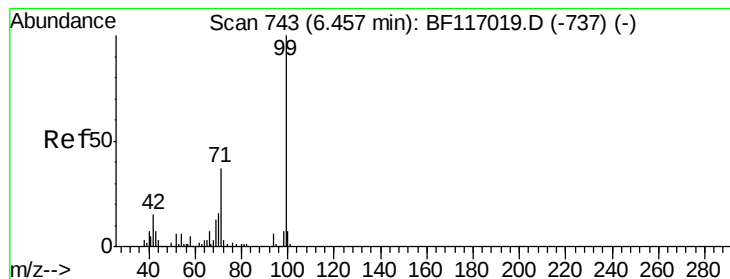

#7

Phenol-d6

Concen: 32.412 ng

RT: 6.46 min Scan# 743

Delta R.T. 0.00 min

Lab File: BF117106.D

Acq: 17 Sep 2019 15:04

Instrument :

BNA_F

ClientSampleId :

MW6-R2-1





Tot Ion: 99 Resp: 174156

Ion Ratio Lower Upper

99 100

42 14.6 12.2 18.2

71 37.1 29.8 44.8

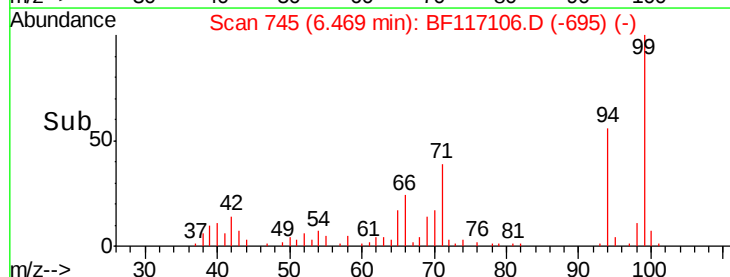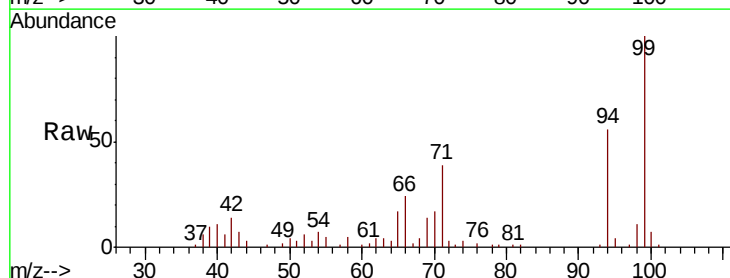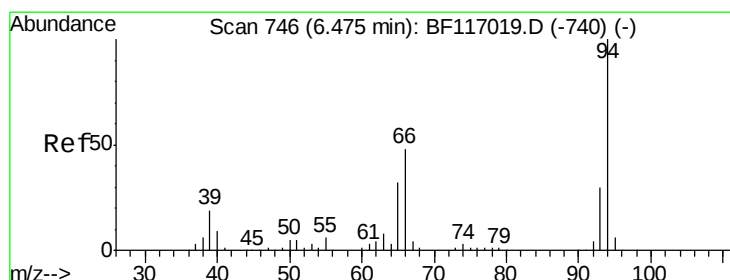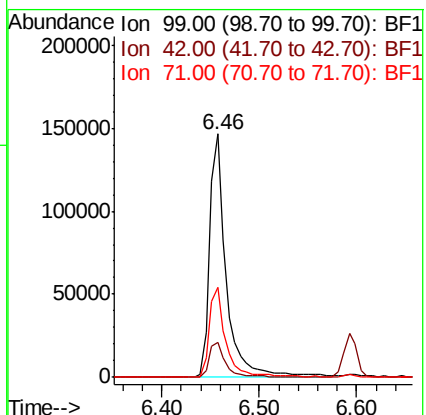

#10

Phenol

Concen: 4.245 ng

RT: 6.47 min Scan# 745

Delta R.T. -0.01 min

Lab File: BF117106.D

Acq: 17 Sep 2019 15:04


Tgt Ion: 94 Resp: 25146


Ion Ratio Lower Upper

94 100

65 30.9 12.5 52.5

66 43.5 28.9 68.9

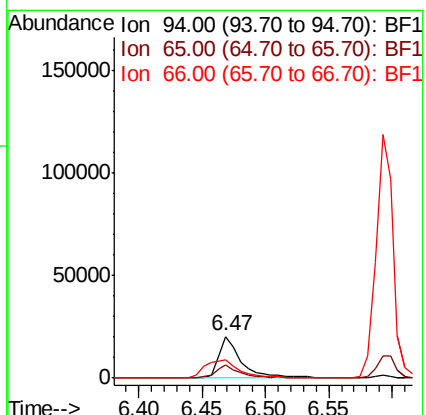

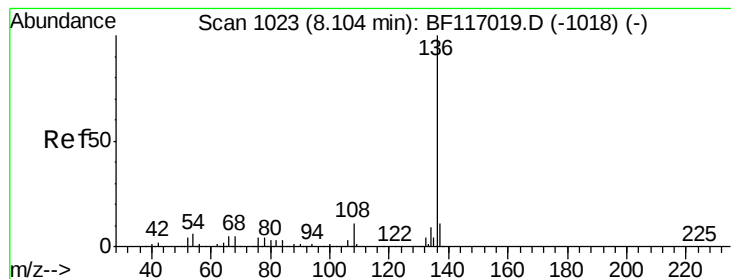

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.10 min Scan# 1023

Delta R.T. 0.00 min

Lab File: BF117106.D

Acq: 17 Sep 2019 15:04

Instrument :

BNA_F

ClientSampleId :

MW6-R2-1

Tot Ion:136 Resp: 249673



Ion Ratio Lower Upper

136 100

137 11.2 9.0 13.4

54 5.3 4.5 6.7

68 4.8 4.0 6.0

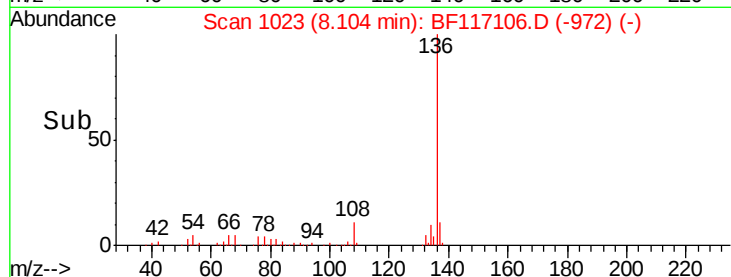
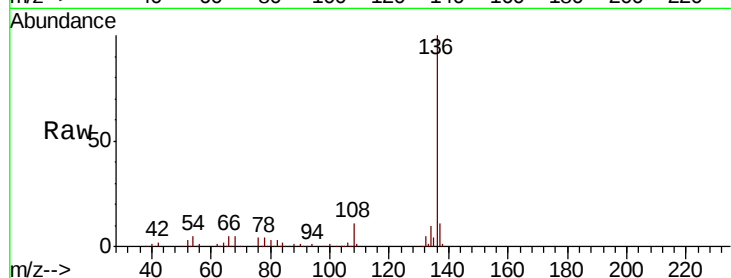


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

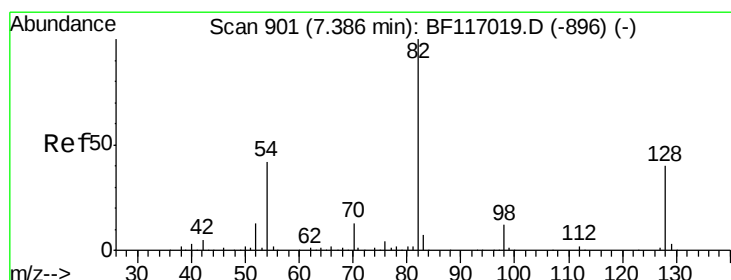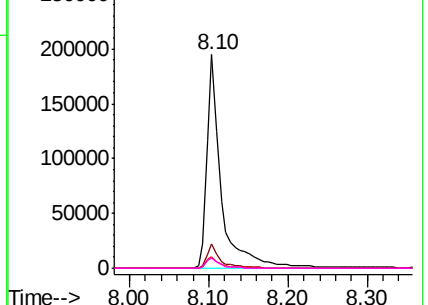

#23

Nitrobenzene-d5

Concen: 89.089 ng

RT: 7.39 min Scan# 901

Delta R.T. 0.00 min

Lab File: BF117106.D

Acq: 17 Sep 2019 15:04



Tgt Ion: 82 Resp: 423338

Ion Ratio Lower Upper

82 100

128 43.2 32.3 48.5


54 39.9 33.3 49.9

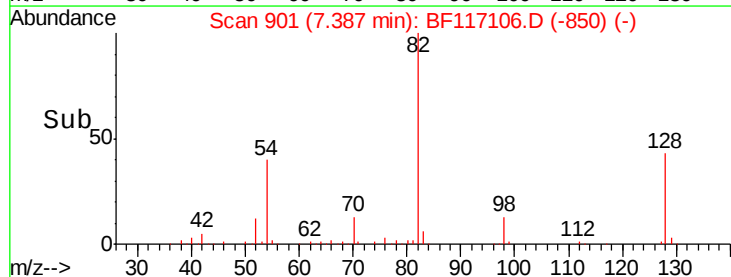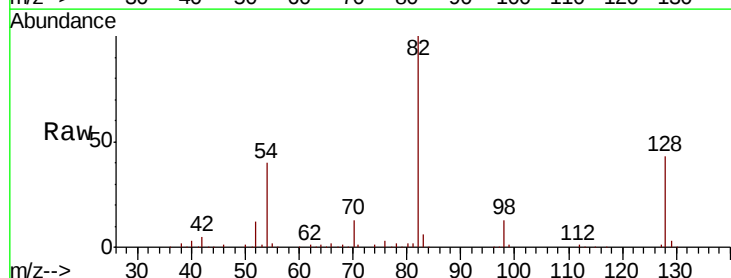


Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

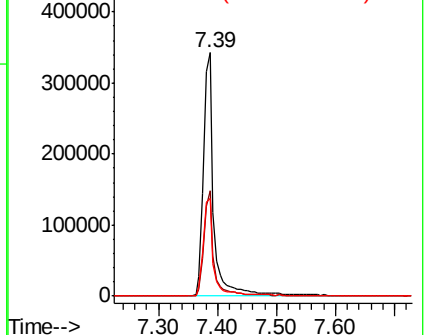


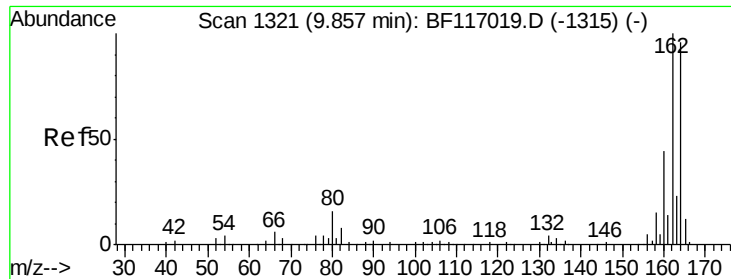




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.85 min Scan# 1320
Delta R.T. -0.01 min
Lab File: BF117106.D
Acq: 17 Sep 2019 15:04

Instrument :
BNA_F
ClientSampleId :
MW6-R2-1

Tot Ion:164 Resp: 129886
Ion Ratio Lower Upper
164 100
162 101.6 83.4 125.2
160 43.6 36.4 54.6

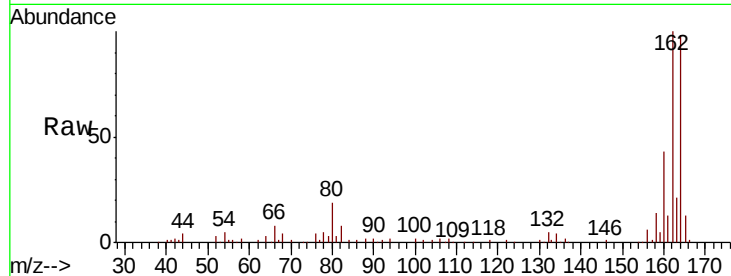


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

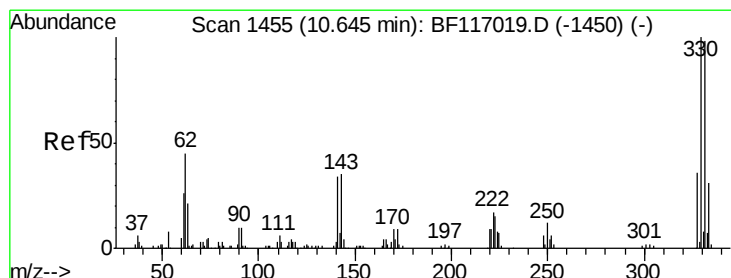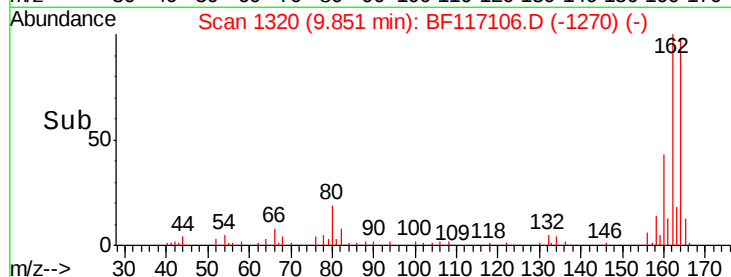
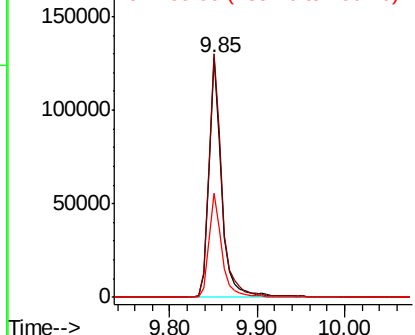



#42
2,4,6-Tribromophenol
Concen: 130.090 ng
RT: 10.64 min Scan# 1454
Delta R.T. -0.01 min
Lab File: BF117106.D
Acq: 17 Sep 2019 15:04

Tgt Ion:330 Resp: 141219
Ion Ratio Lower Upper
330 100
332 96.9 78.0 117.0
141 45.5 35.8 53.6

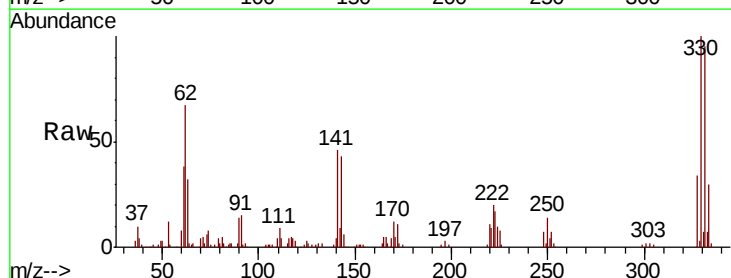

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

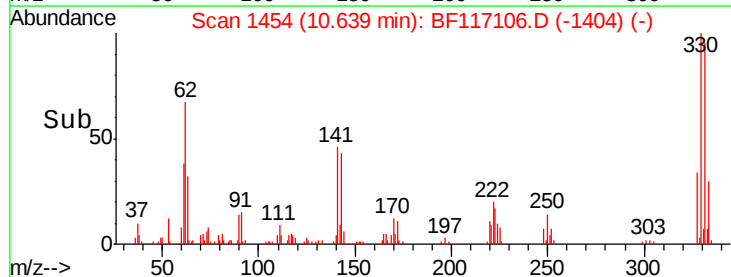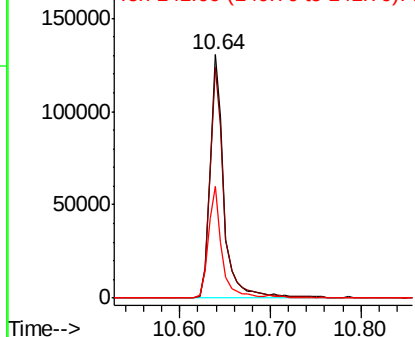

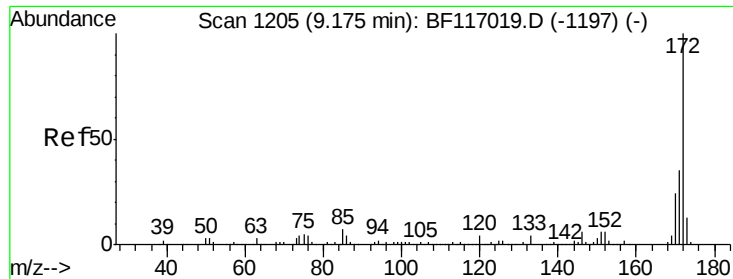

#45

2-Fluorobiphenyl

Concen: 88.387 ng

RT: 9.17 min Scan# 1205

Delta R.T. 0.00 min

Lab File: BF117106.D

Acq: 17 Sep 2019 15:04

Instrument :


BNA_F

ClientSampleId :

MW6-R2-1

Tot Ion:172 Resp: 734227




Ion	Ratio	Lower	Upper
172	100		
171	35.8	28.2	42.2
170	23.8	18.9	28.3

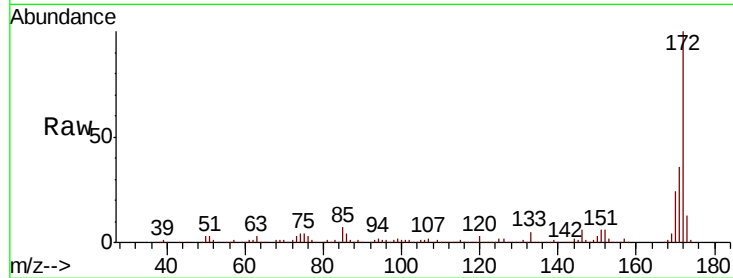

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

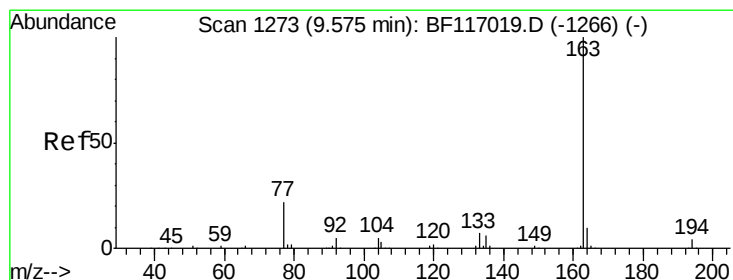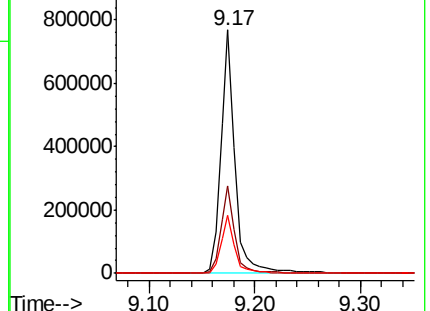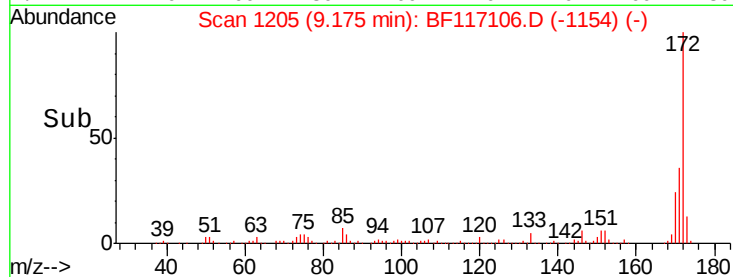

#50

Dimethylphthalate

Concen: 4.033 ng

RT: 9.57 min Scan# 1272


Delta R.T. -0.01 min

Lab File: BF117106.D

Acq: 17 Sep 2019 15:04

Tgt Ion:163 Resp: 37091



Ion	Ratio	Lower	Upper
163	100		
194	3.5	2.9	4.3
164	10.5	8.2	12.4

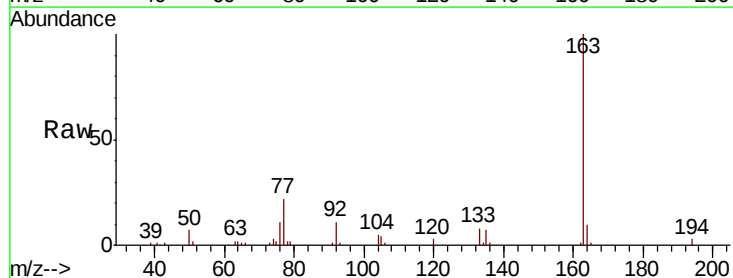


Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

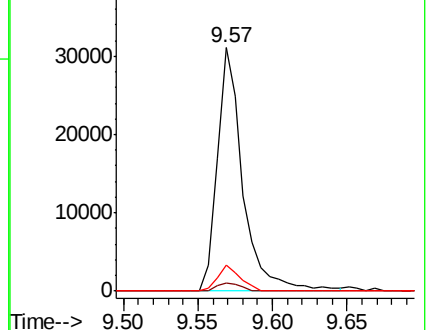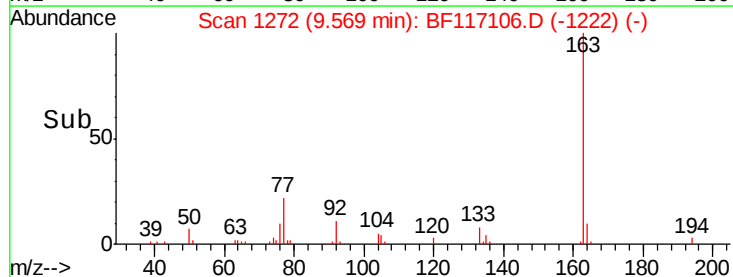


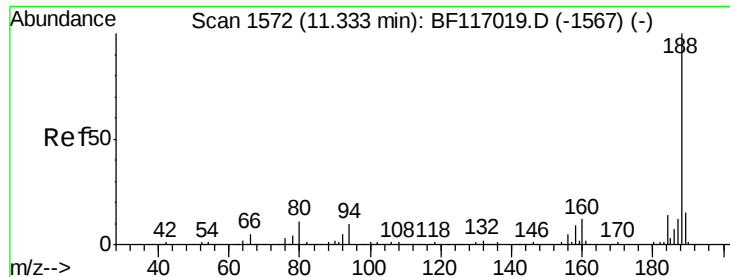




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.33 min Scan# 1572
Delta R.T. 0.00 min
Lab File: BF117106.D
Acq: 17 Sep 2019 15:04

Instrument :
BNA_F
ClientSampleId :
MW6-R2-1

Tot Ion	Ratio	Lower	Upper
188	100		
94	8.9	8.2	12.2
80	10.6	9.0	13.6

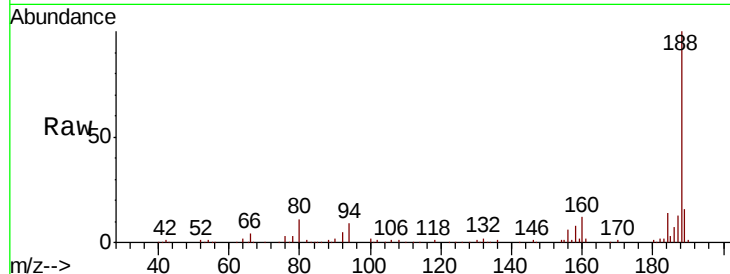


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

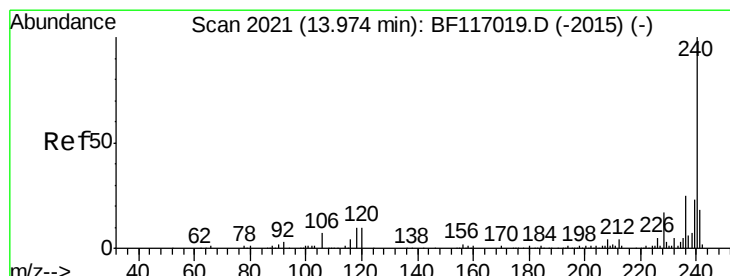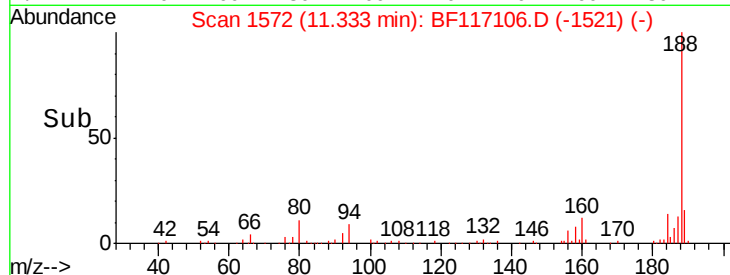
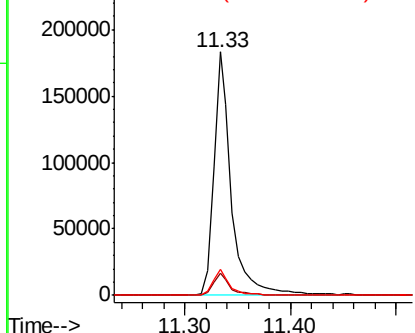



#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.97 min Scan# 2020
Delta R.T. -0.01 min
Lab File: BF117106.D
Acq: 17 Sep 2019 15:04

Tgt Ion	Ratio	Lower	Upper
240	100		
120	10.6	8.3	12.5
236	27.1	20.3	30.5

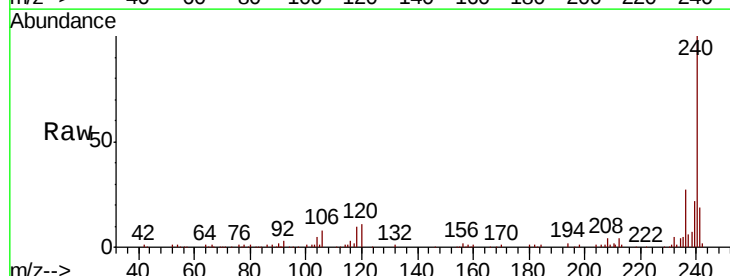

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

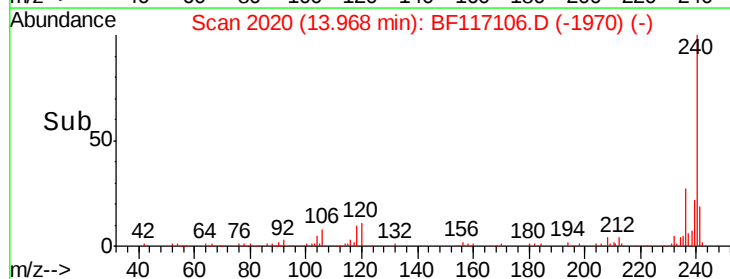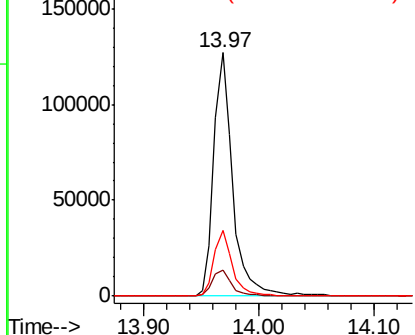


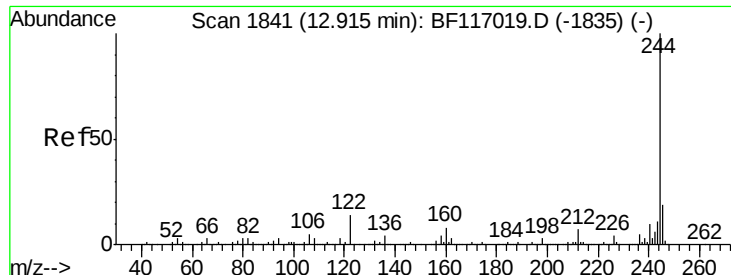




#79
 Terphenyl-d14
 Concen: 79.628 ng
 RT: 12.92 min Scan# 1841
 Delta R.T. 0.00 min
 Lab File: BF117106.D
 Acq: 17 Sep 2019 15:04

Instrument :
 BNA_F
 ClientSampleId :
 MW6-R2-1

Tot Ion:244 Resp: 621674
 Ion Ratio Lower Upper
 244 100
 212 7.0 5.8 8.8
 122 10.8 11.3 16.9#

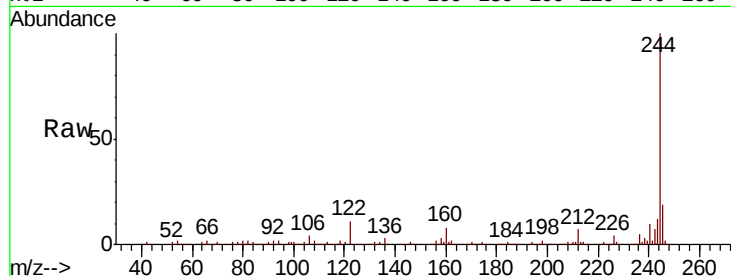


Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

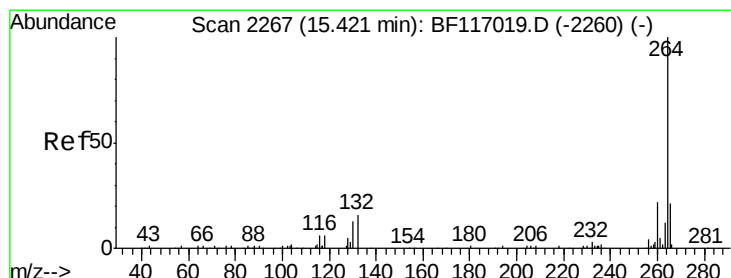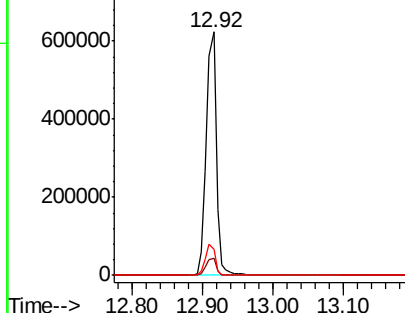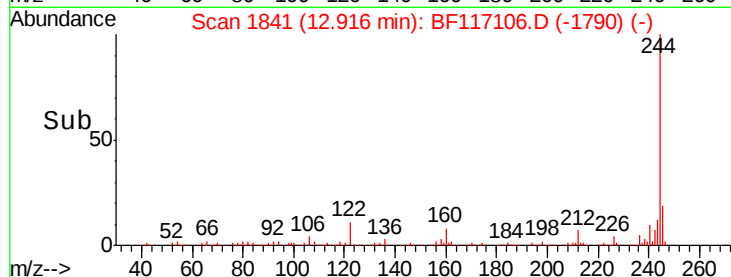

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.42 min Scan# 2267
 Delta R.T. 0.00 min
 Lab File: BF117106.D
 Acq: 17 Sep 2019 15:04

Tgt Ion:264 Resp: 121492
 Ion Ratio Lower Upper
 264 100
 260 23.4 17.6 26.4
 265 22.6 16.6 24.8

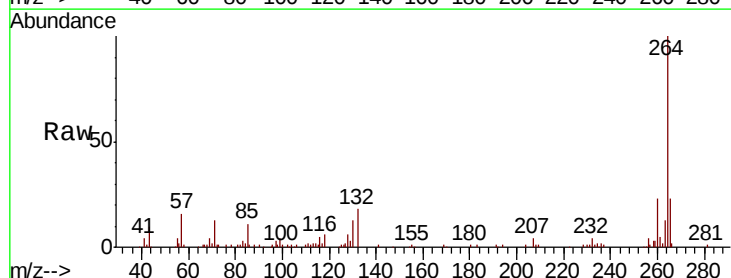

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

