


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091719\
 Data File : BF117093.D
 Acq On : 17 Sep 2019 8:05
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 13 16:23:17 2019

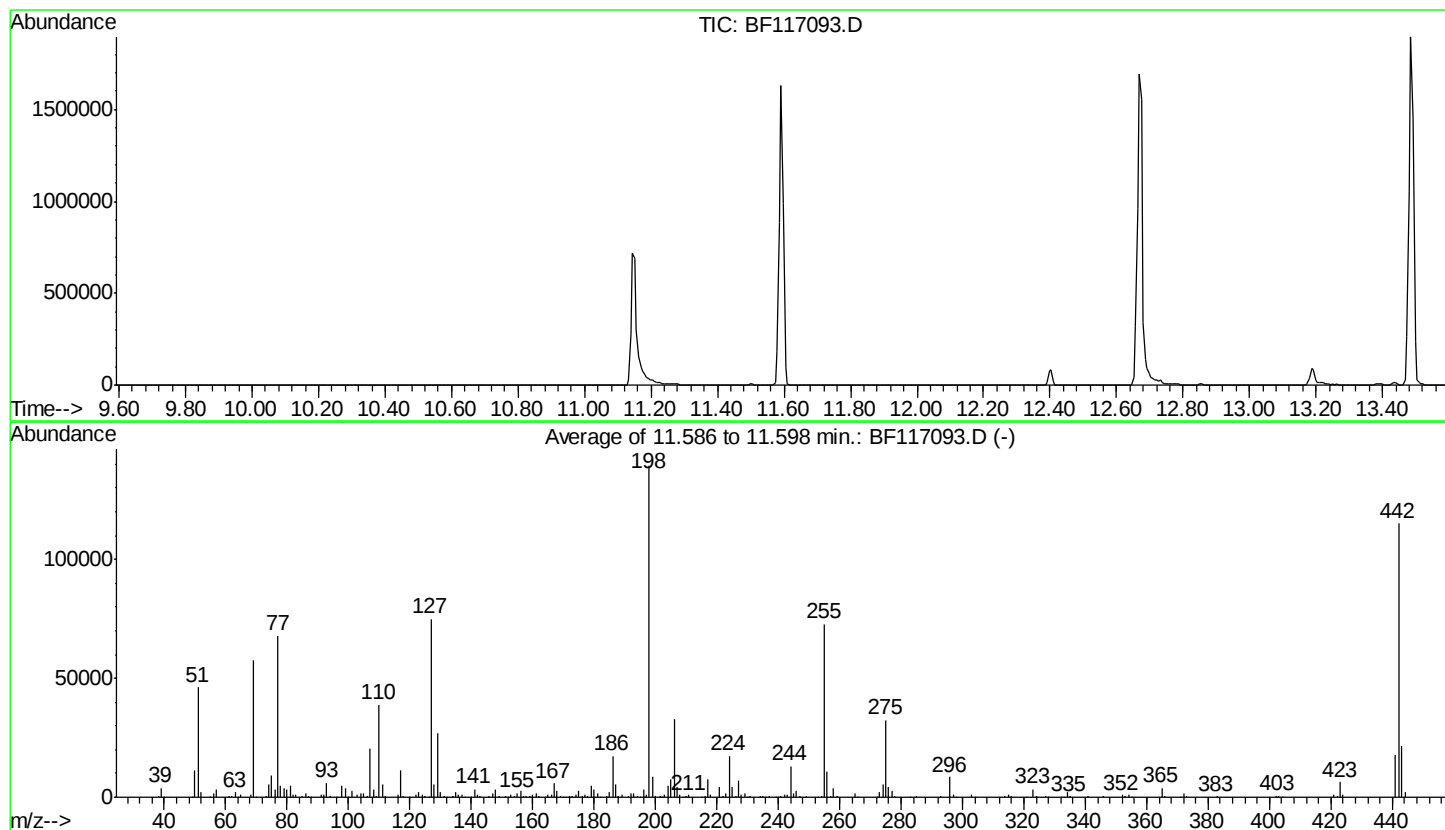

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	46074	PASS
68	69	0.00	2	1.6	913	PASS
69	198	0.00	100	41.3	57538	PASS
70	69	0.00	2	0.2	139	PASS
127	198	10	80	53.7	74877	PASS
197	198	0.00	2	0.8	1148	PASS
198	198	100	100	100.0	139421	PASS
199	198	5	9	6.2	8703	PASS
275	198	10	60	23.4	32576	PASS
365	198	1	100	2.8	3945	PASS
441	198	0.01	100	12.9	17969	PASS
442	198	50	100	82.5	115040	PASS
443	442	15	24	18.6	21417	PASS