

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091818\
 Data File : BF109120.D
 Acq On : 19 Sep 2018 2:54
 Operator : JU/SJ
 Sample : J4930-13
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Sep 19 04:07:11 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 14 13:26:52 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.72	152	120285	20.00	ng	0.00
21) Naphthalene-d8	8.00	136	413784	20.00	ng	0.00
38) Acenaphthene-d10	9.75	164	166540	20.00	ng	0.00
63) Phenanthrene-d10	11.23	188	292428	20.00	ng	0.00
75) Chrysene-d12	13.85	240	328485	20.00	ng	0.00
86) Perylene-d12	15.26	264	291117	20.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.32	112	292711	40.42	ng	0.00
7) Phenol-d6	6.35	99	232747	24.92	ng	-0.01
23) Nitrobenzene-d5	7.28	82	714125	96.80	ng	0.00
41) 2,4,6-Tribromophenol	10.54	330	163884	90.67	ng	0.00
44) 2-Fluorobiphenyl	9.08	172	1152969	108.47	ng	0.00
78) Terphenyl-d14	12.81	244	1160977	83.77	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
9) Benzaldehyde	6.49	77	12369	2.074	ng	# 74
19) n-Nitroso-di-n-propylamine	7.28	70	95489	15.469	ng	# 78
25) Isophorone	7.28	82	711633	56.116	ng	# 64
49) Dimethylphthalate	9.47	163	76229	6.404	ng	# 99
50) 2,6-Dinitrotoluene	9.75	165	20594	7.802	ng	# 26
56) 2,4-Dinitrotoluene	9.75	165	20594	5.965	ng	# 23
66) 4-Bromophenyl-phenylether	10.54	248	9801	2.973	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091818\
Data File : BF109120.D
Acq On : 19 Sep 2018 2:54
Operator : JU/SJ
Sample : J4930-13
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Sep 19 04:07:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 14 13:26:52 2018
Response via : Initial Calibration

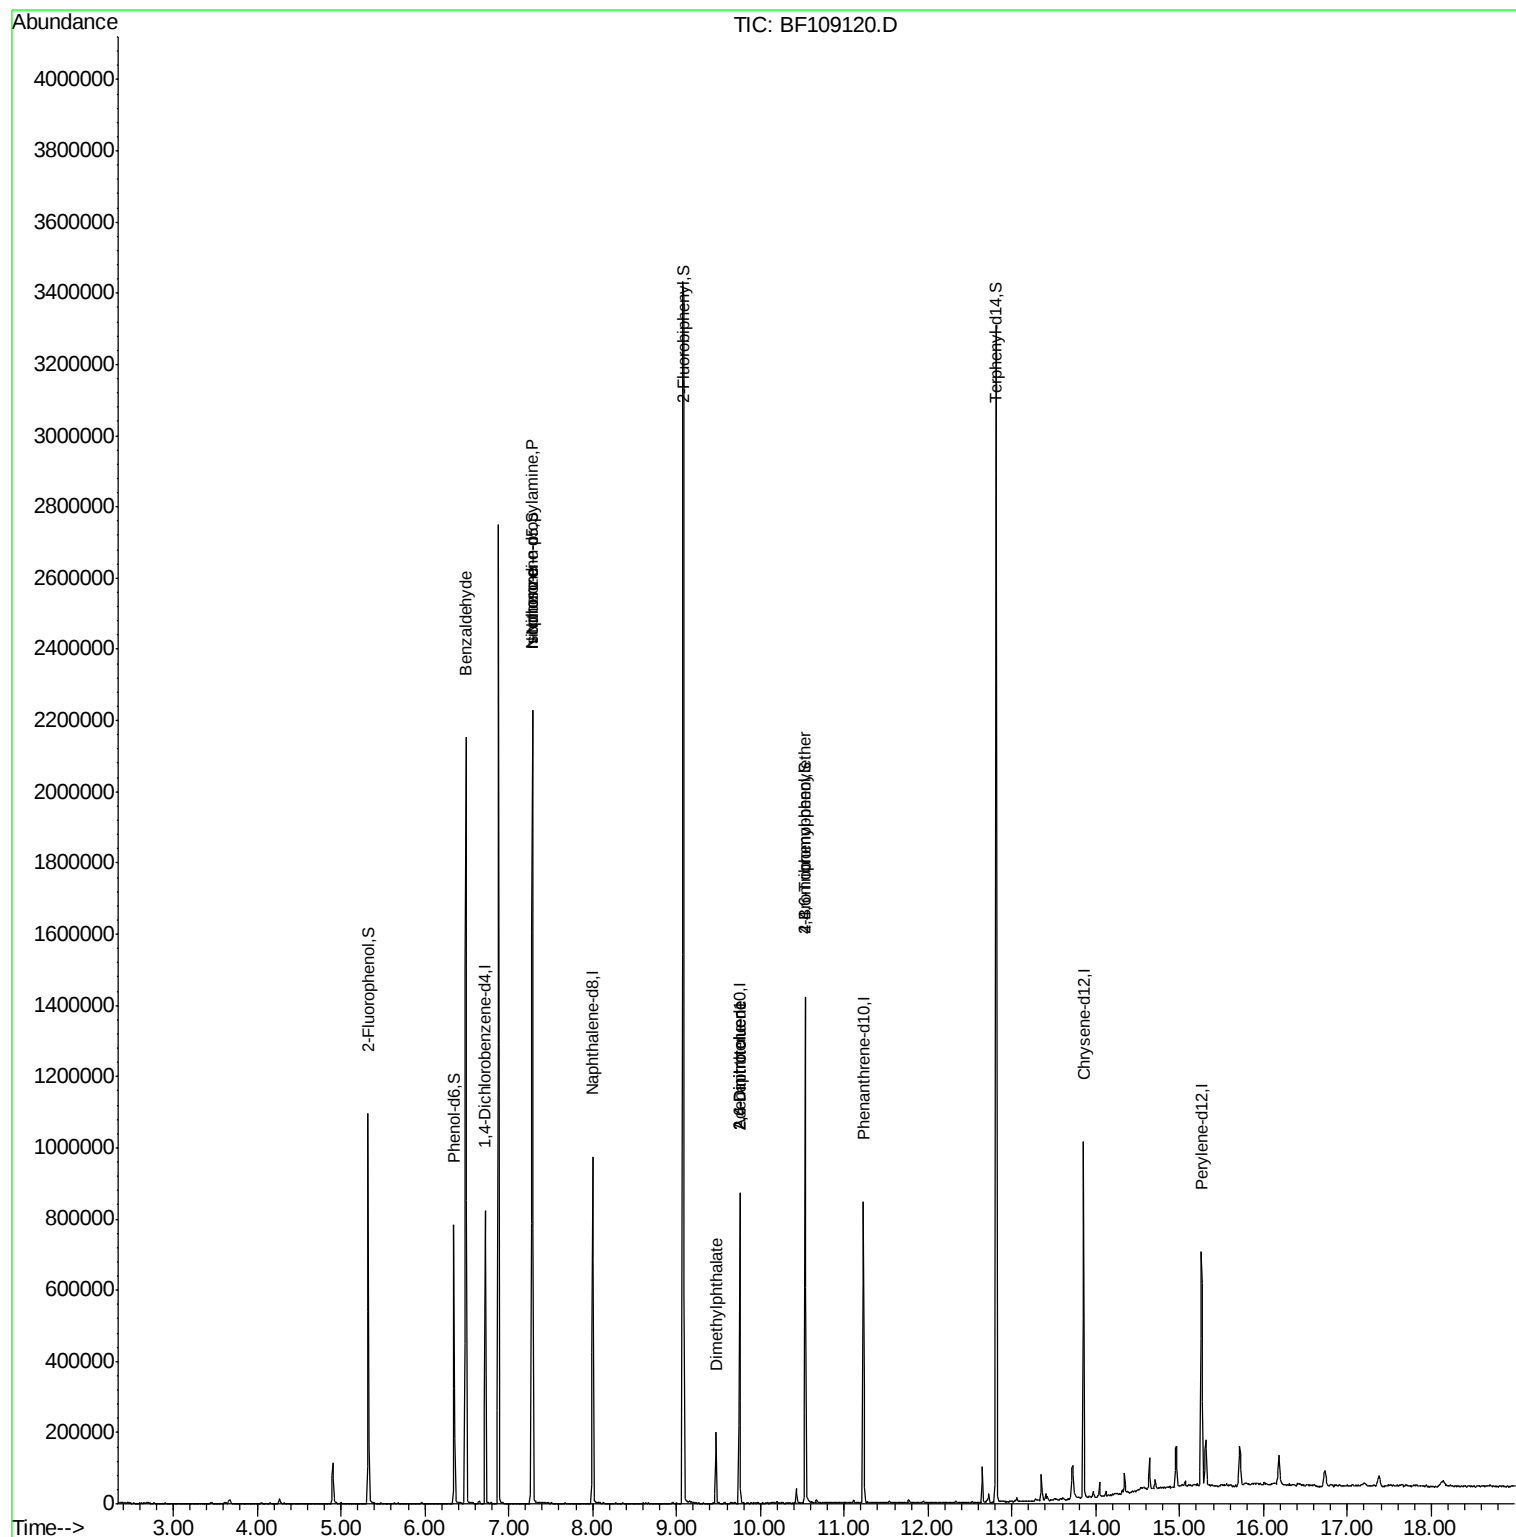

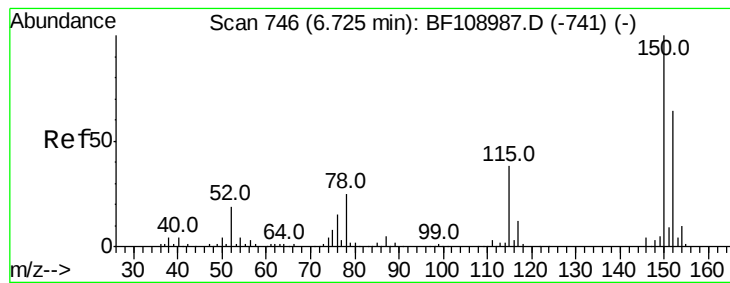


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.72 min Scan# 745
Delta R.T. -0.01 min
Lab File: BF109120.D
Acq: 19 Sep 2018 2:54

Instrument :
BNA_F
ClientSampled :

Tot Ion	Ratio	Lower	Upper
152	100		
150	158.5	124.6	186.8
115	62.0	50.1	75.1



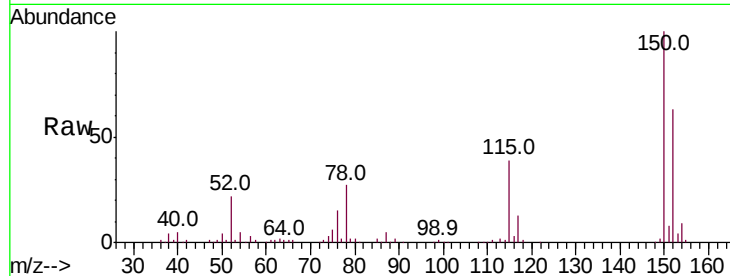


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

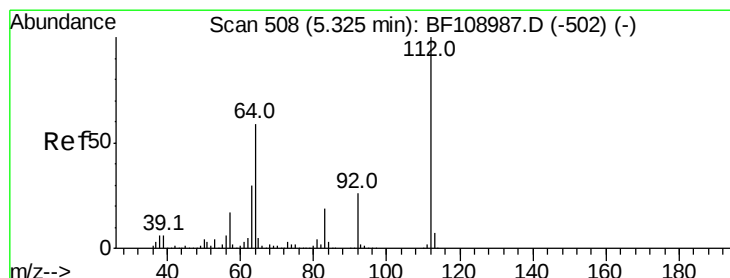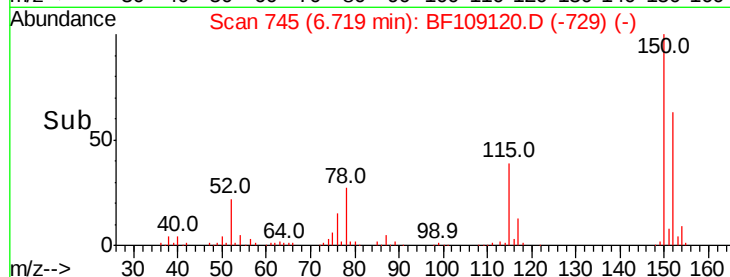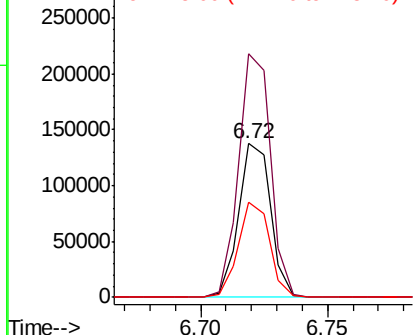

#5

2-Fluorophenol
Concen: 40.417 ng
RT: 5.32 min Scan# 508
Delta R.T. 0.00 min
Lab File: BF109120.D
Acq: 19 Sep 2018 2:54

Tgt Ion	Ratio	Lower	Upper
112	100		
64	58.8	47.9	71.9
63	30.2	23.7	35.5


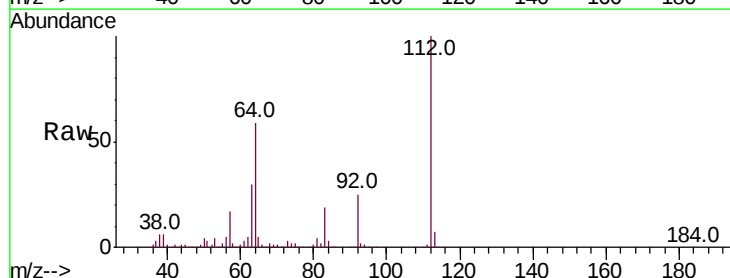



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

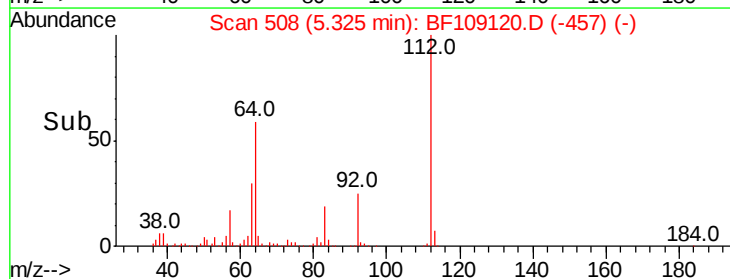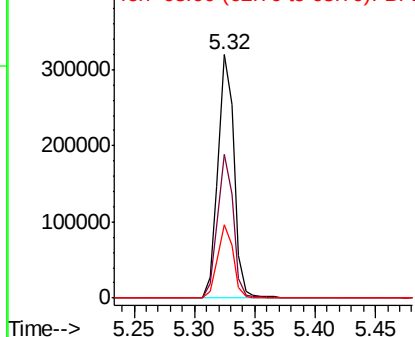

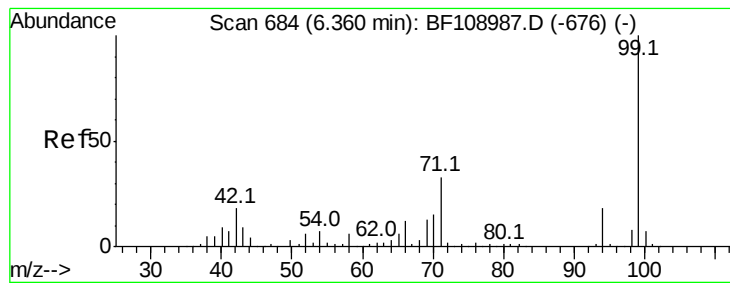

#7

Phenol-d6

Concen: 24.923 ng

RT: 6.35 min Scan# 682

Delta R.T. -0.01 min

Lab File: BF109120.D

Acq: 19 Sep 2018 2:54

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 232747

Ion Ratio Lower Upper




99 100

42 18.5 14.5 21.7

71 33.2 25.4 38.0

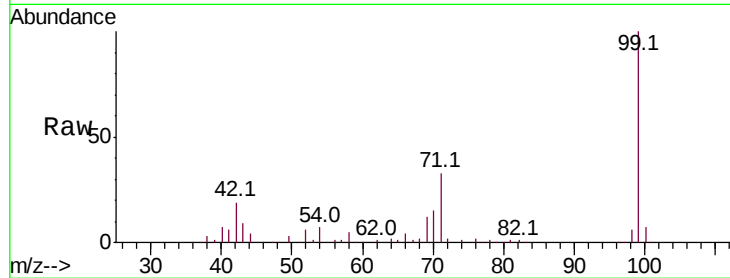

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

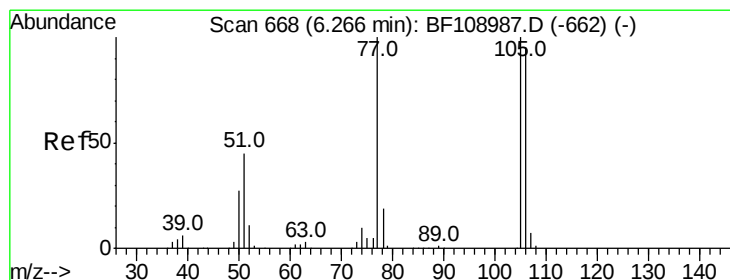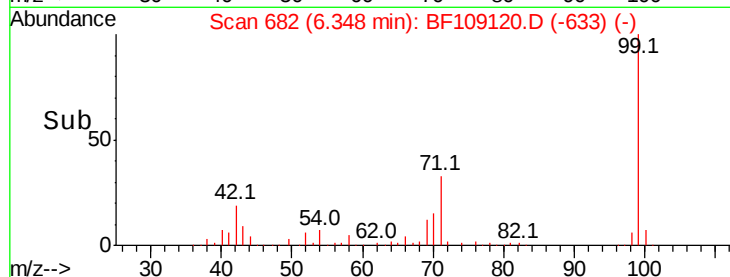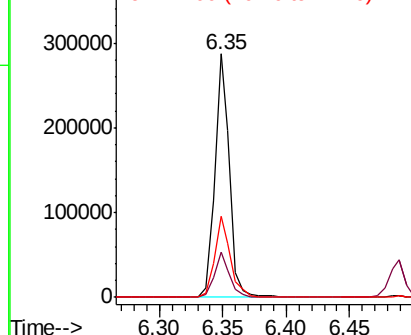

#9

Benzaldehyde

Concen: 2.074 ng

RT: 6.49 min Scan# 706

Delta R.T. 0.22 min

Lab File: BF109120.D

Acq: 19 Sep 2018 2:54


Tgt Ion: 77 Resp: 12369

Ion Ratio Lower Upper



77 100


105 78.9 81.1 121.1#

106 64.4 74.5 114.5#

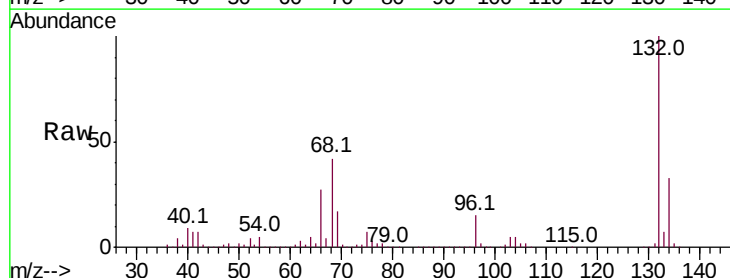

Abundance Ion 77.00 (76.70 to 77.70): BF1
Ion 105.00 (104.70 to 105.70): E
Ion 106.00 (105.70 to 106.70): E



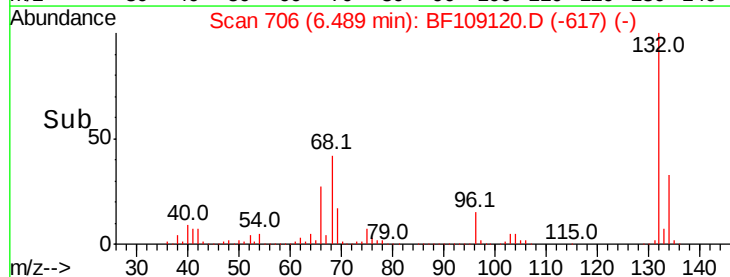
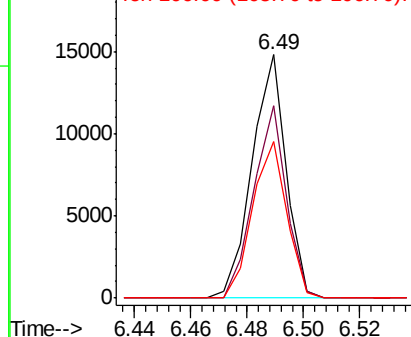




#19
n-Nitroso-di-n-propylamine
Concen: 15.469 ng
RT: 7.28 min Scan# 841
Delta R.T. 0.14 min
Lab File: BF109120.D
Acq: 19 Sep 2018 2:54




Instrument :
BNA_F
ClientSampleId :


Tot Ion:	70	Resp:	95489
Ion	Ratio	Lower	Upper
70	100		
42	48.3	47.5	71.3
101	0.0	7.4	11.2#
130	2.1	16.6	25.0#

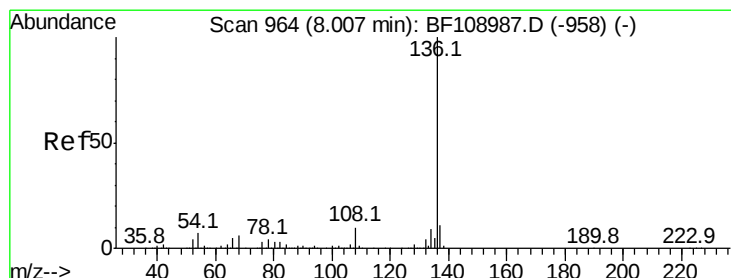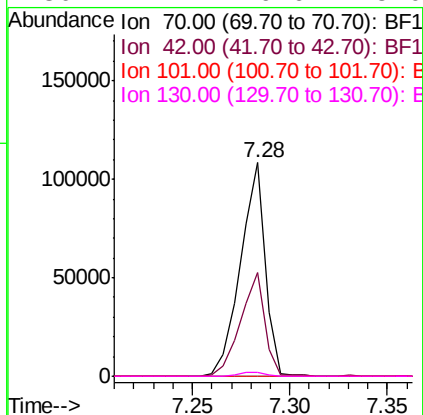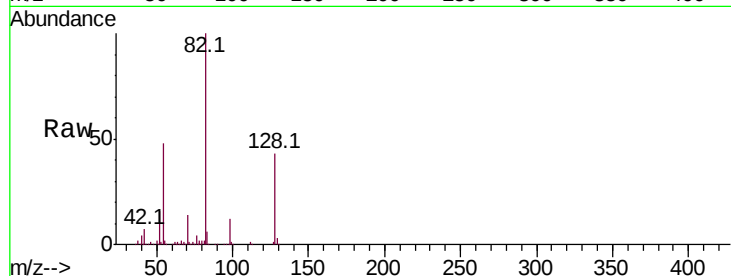

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.00 min Scan# 963
Delta R.T. -0.01 min
Lab File: BF109120.D
Acq: 19 Sep 2018 2:54

Tgt Ion:	136	Resp:	413784
Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.9	13.3
54	7.5	6.6	9.8
68	5.8	5.0	7.4

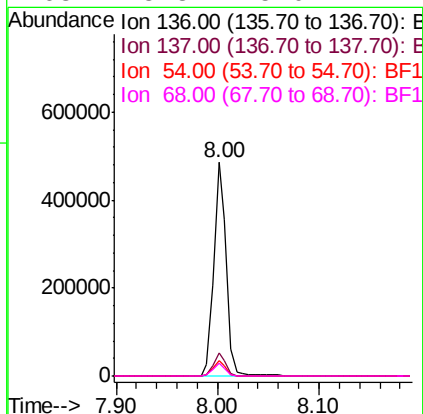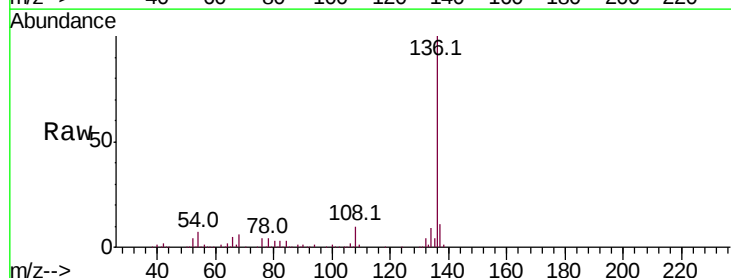

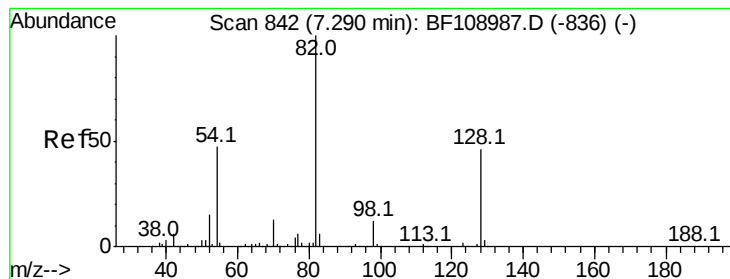

#23

Nitrobenzene-d5

Concen: 96.799 ng

RT: 7.28 min Scan# 841

Delta R.T. -0.01 min

Lab File: BF109120.D

Acq: 19 Sep 2018 2:54

Instrument :

BNA_F

ClientSampled :


Tot Ion: 82 Resp: 714125

Ion Ratio Lower Upper




82 100

128 43.3 36.1 54.1

54 48.4 41.4 62.2

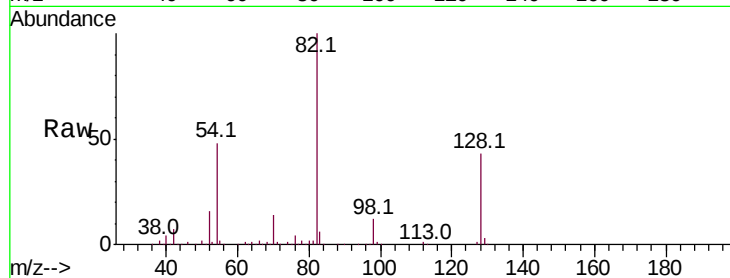

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1

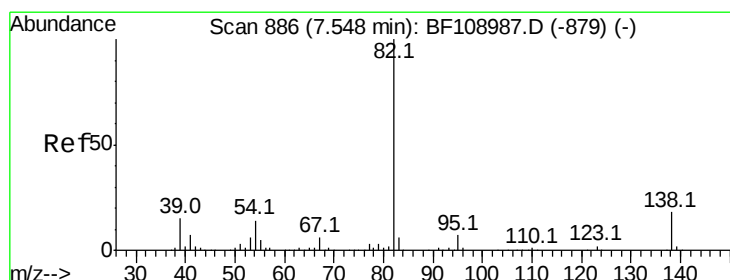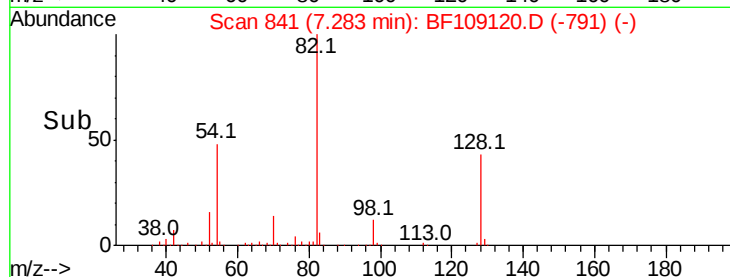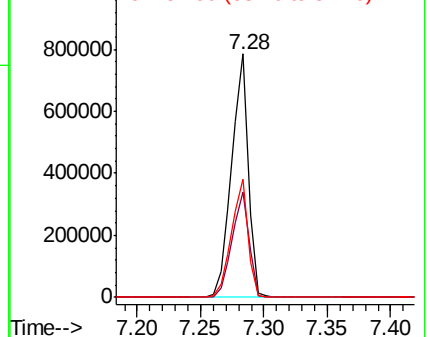

#25

Isophorone

Concen: 56.116 ng

RT: 7.28 min Scan# 841

Delta R.T. -0.26 min

Lab File: BF109120.D

Acq: 19 Sep 2018 2:54


Tgt Ion: 82 Resp: 711633

Ion Ratio Lower Upper



82 100


95 0.0 5.2 7.8#

138 0.0 14.9 22.3#

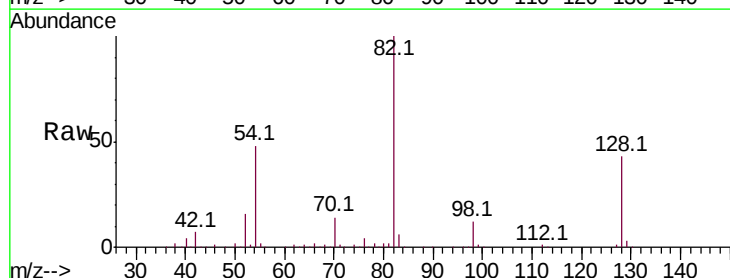

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 138.00 (137.70 to 138.70): BF1



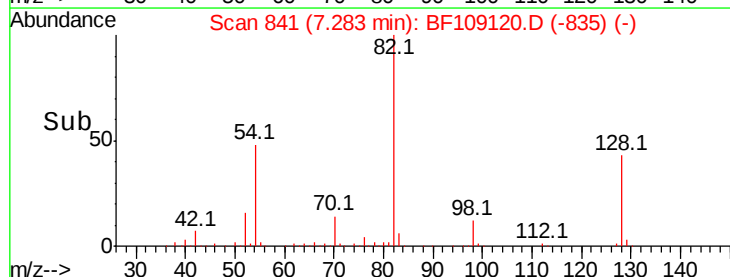
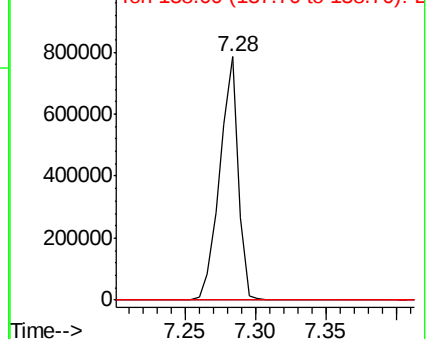


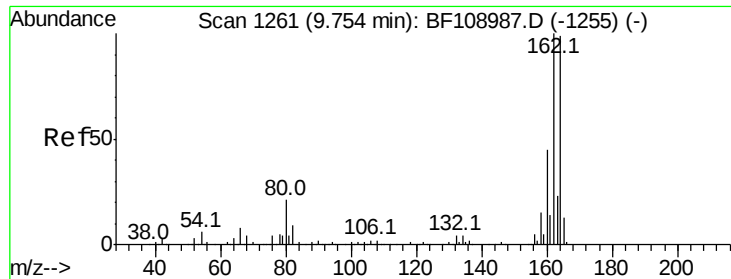

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.75 min Scan# 1261
 Delta R.T. -0.00 min
 Lab File: BF109120.D
 Acq: 19 Sep 2018 2:54




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
164	100		
162	103.2	86.1	129.1
160	48.4	38.3	57.5

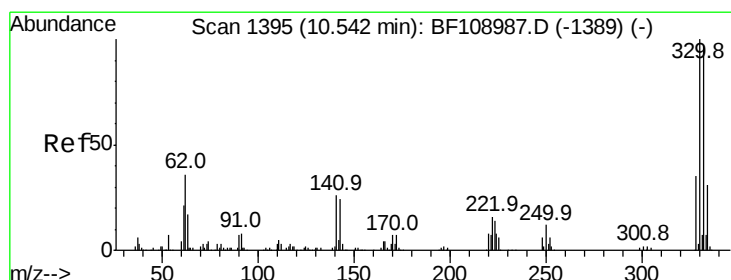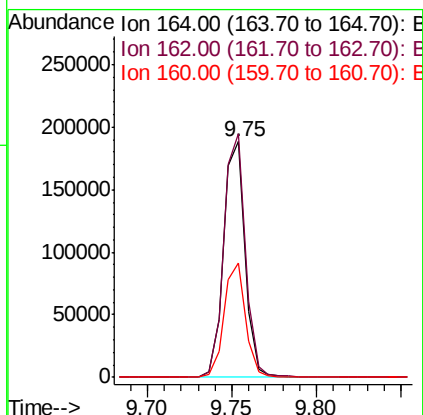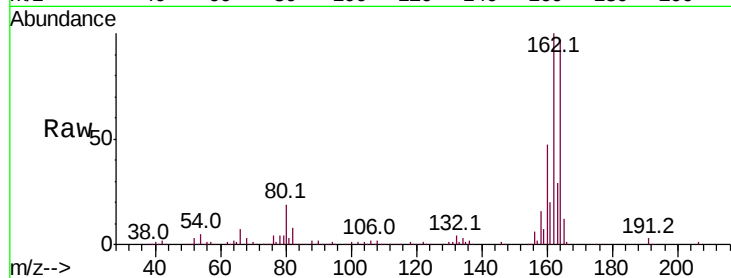

#41
 2,4,6-Tribromophenol
 Concen: 90.674 ng
 RT: 10.54 min Scan# 1394
 Delta R.T. -0.01 min
 Lab File: BF109120.D
 Acq: 19 Sep 2018 2:54

Tgt Ion	Ratio	Lower	Upper
330	100		
332	95.9	77.0	115.6
141	32.0	29.9	44.9

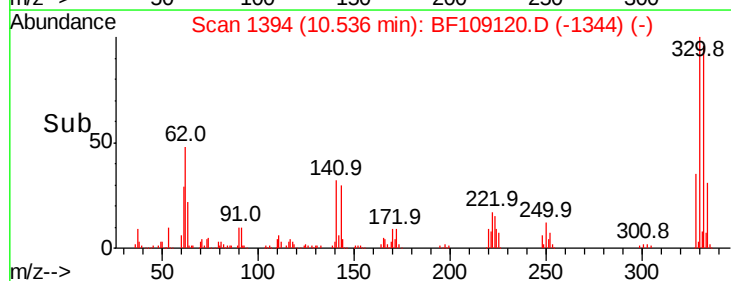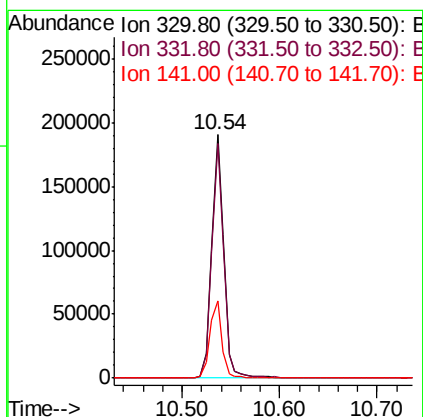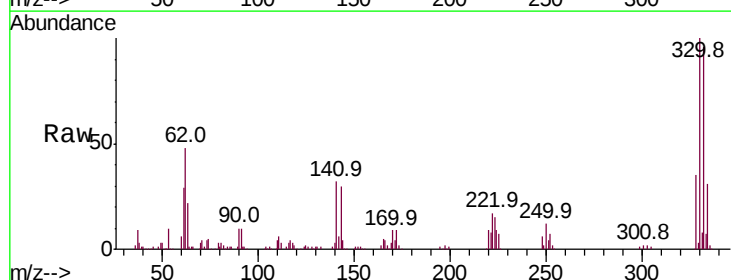


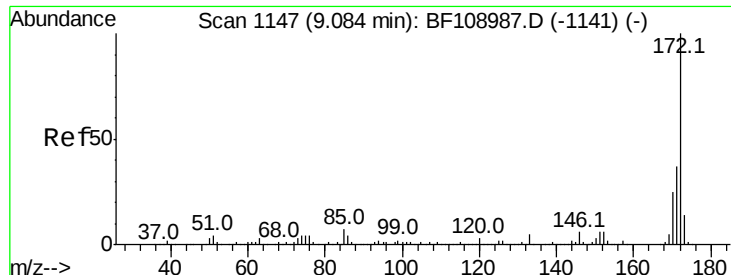




#44
2-Fluorobiphenyl
Concen: 108.466 ng
RT: 9.08 min Scan# 1147
Delta R.T. 0.00 min
Lab File: BF109120.D
Acq: 19 Sep 2018 2:54

Instrument :
BNA_F
ClientSampleId :

Tot Ion:172 Resp: 1152969
Ion Ratio Lower Upper
172 100
171 35.6 29.7 44.5
170 24.4 19.6 29.4

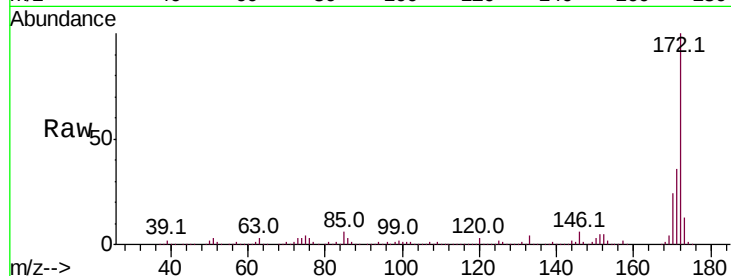


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

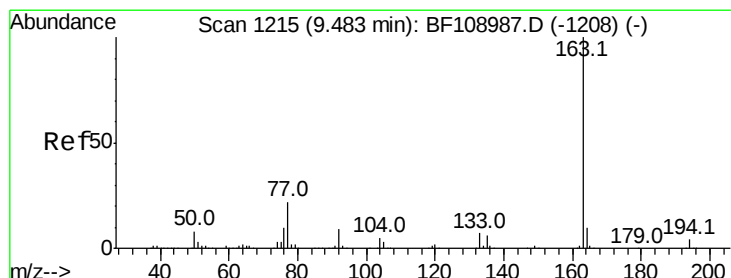
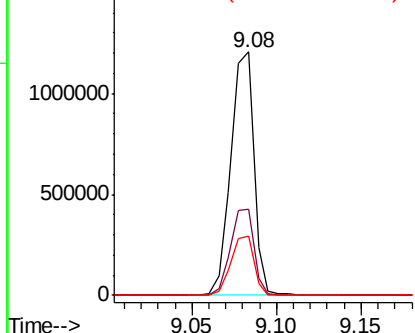



#49
Dimethylphthalate
Concen: 6.404 ng
RT: 9.47 min Scan# 1213
Delta R.T. -0.01 min
Lab File: BF109120.D
Acq: 19 Sep 2018 2:54

Tgt Ion:163 Resp: 76229
Ion Ratio Lower Upper
163 100
194 3.7 2.7 4.1
164 9.9 8.2 12.2

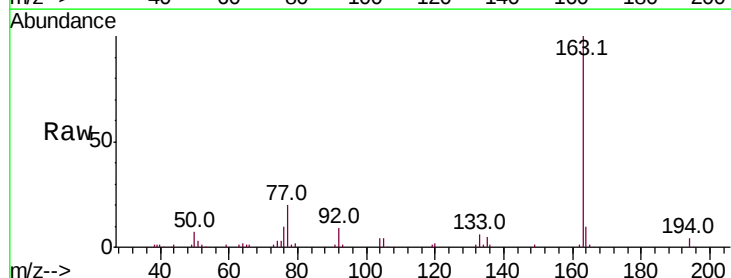

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

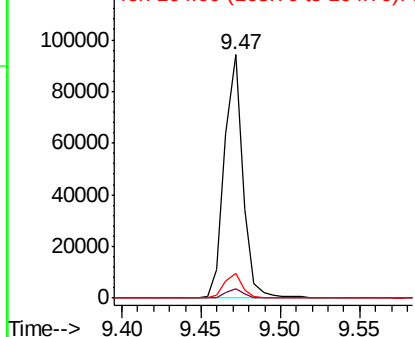


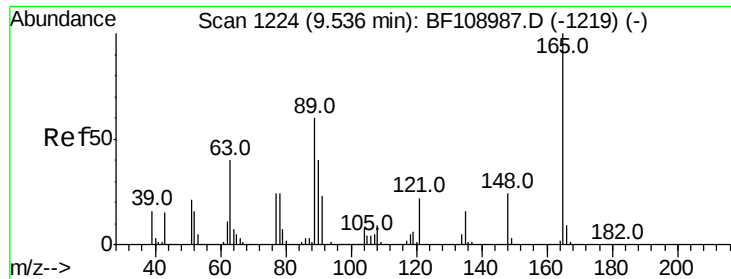




#50
 2,6-Dinitrotoluene
 Concen: 7.802 ng
 RT: 9.75 min Scan# 1261
 Delta R.T. 0.22 min
 Lab File: BF109120.D
 Acq: 19 Sep 2018 2:54

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
165	100		
63	1.3	44.7	67.1#
89	1.6	44.0	66.0#

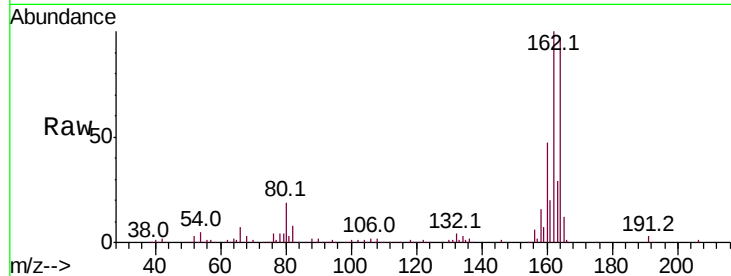




Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 89.00 (88.70 to 89.70): BF1

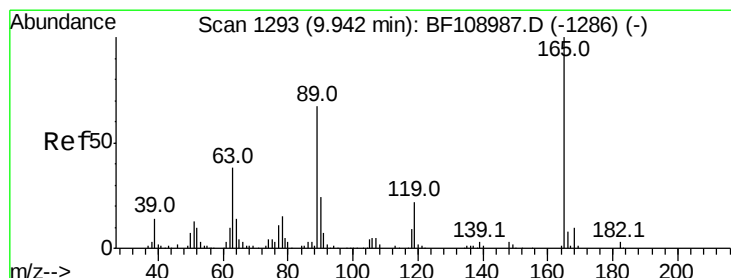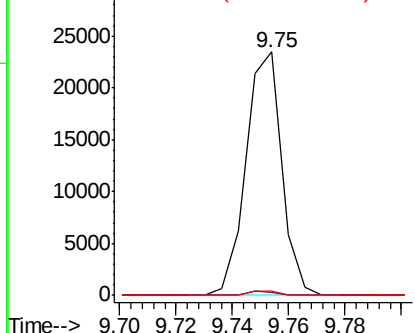


#56
 2,4-Dinitrotoluene
 Concen: 5.965 ng
 RT: 9.75 min Scan# 1261
 Delta R.T. -0.19 min
 Lab File: BF109120.D
 Acq: 19 Sep 2018 2:54

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.3	36.4	54.6#
89	1.6	57.8	86.6#
182	0.0	1.6	2.4#

Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 89.00 (88.70 to 89.70): BF1
 Ion 182.00 (181.70 to 182.70): E



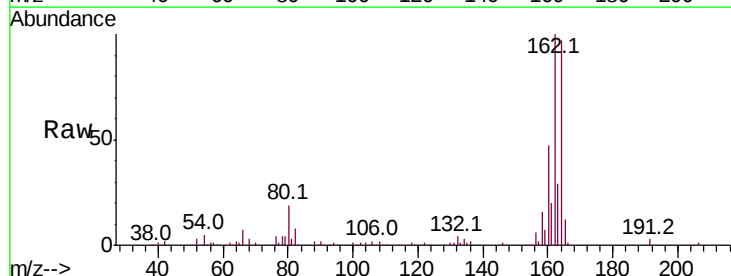
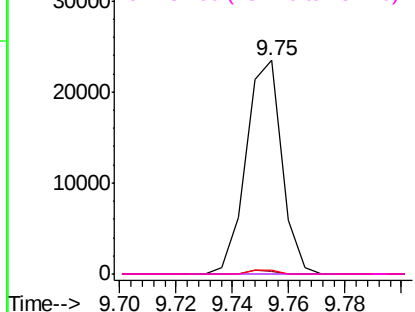


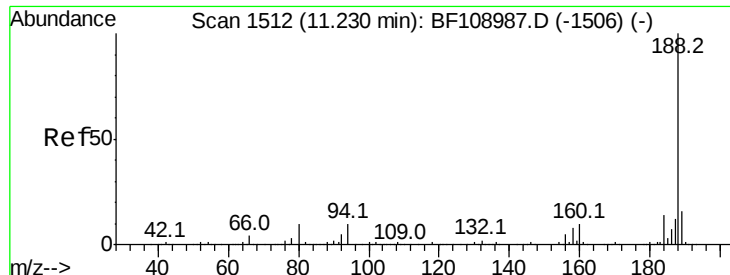

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.23 min Scan# 1512
Delta R.T. -0.00 min
Lab File: BF109120.D
Acq: 19 Sep 2018 2:54




Instrument :
BNA_F
ClientSampleId :


Tot Ion:188 Resp: 292428
Ion Ratio Lower Upper
188 100
94 9.3 8.5 12.7
80 9.7 9.2 13.8

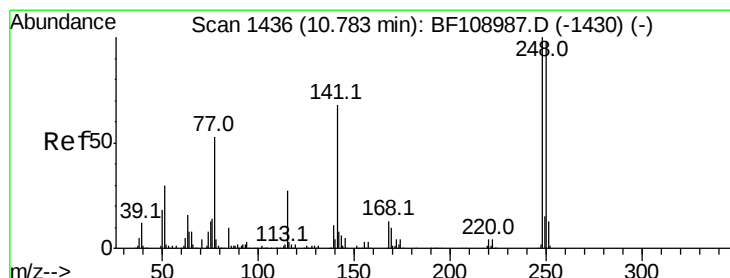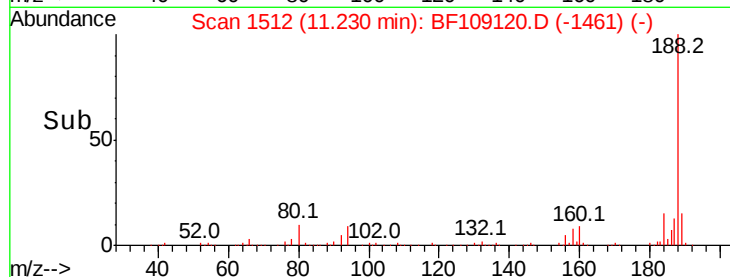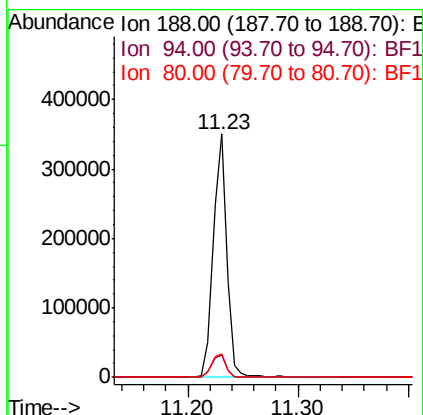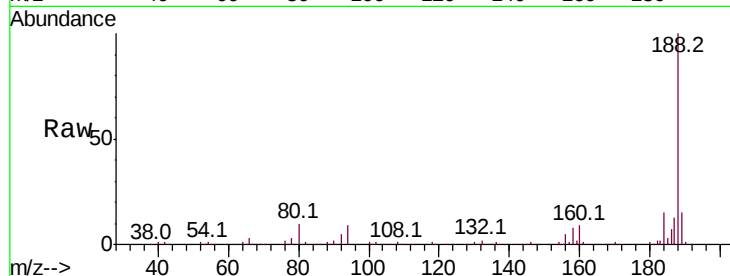

#66
4-Bromophenyl-phenylether
Concen: 2.973 ng
RT: 10.54 min Scan# 1394
Delta R.T. -0.25 min
Lab File: BF109120.D
Acq: 19 Sep 2018 2:54

Tgt Ion:248 Resp: 9801
Ion Ratio Lower Upper
248 100
250 194.0 76.9 115.3#
141 494.7 74.4 111.6#

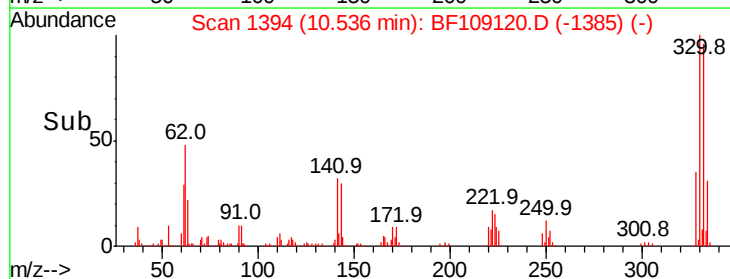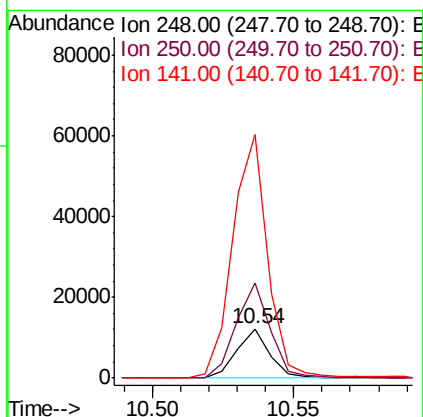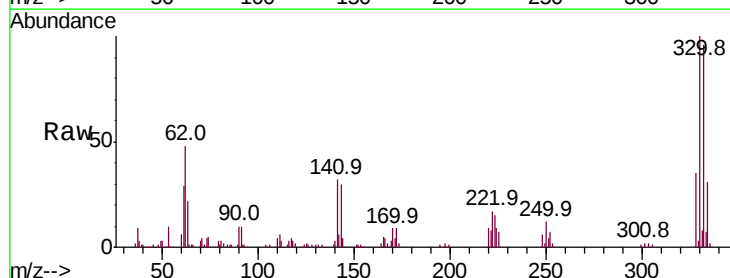



#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.85 min Scan# 1958

Delta R.T. -0.01 min

Lab File: BF109120.D

Acq: 19 Sep 2018 2:54

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 328485

Ion Ratio Lower Upper

240 100

120 12.1 9.5 14.3




236 26.2 20.7 31.1

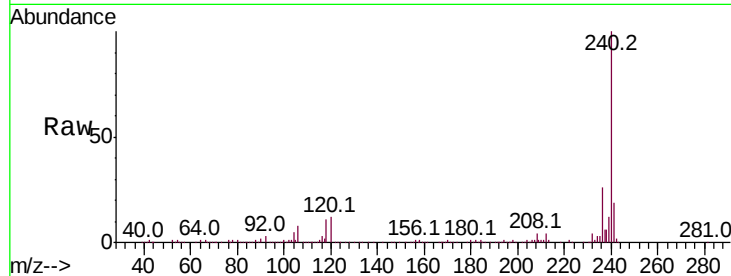

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

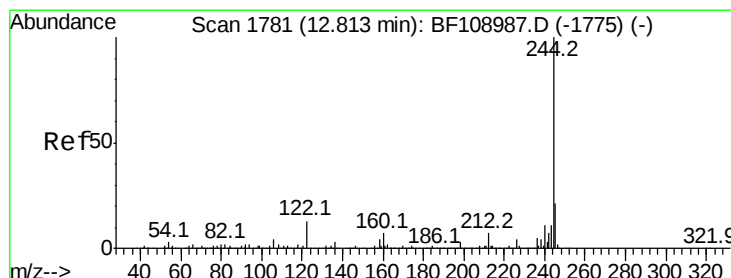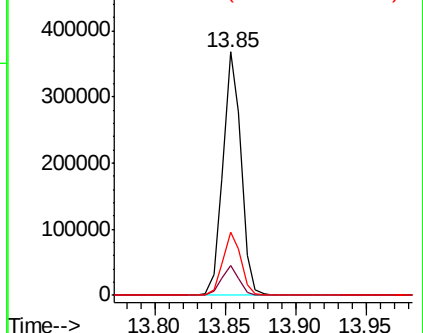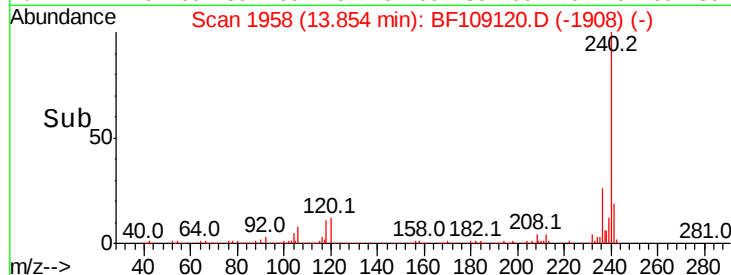

#78

Terphenyl-d14

Concen: 83.773 ng

RT: 12.81 min Scan# 1781

Delta R.T. -0.00 min

Lab File: BF109120.D

Acq: 19 Sep 2018 2:54


Tgt Ion:244 Resp: 1160977

Ion Ratio Lower Upper

244 100

212 7.4 5.4 8.0



122 12.6 11.0 16.4

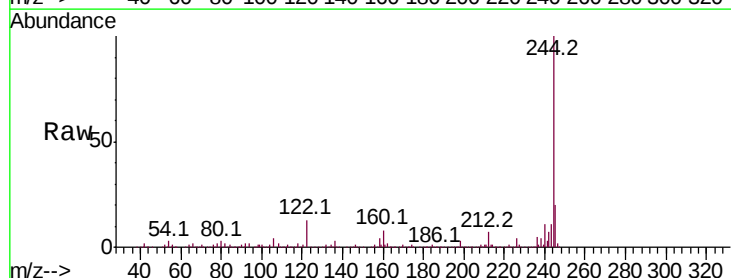


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

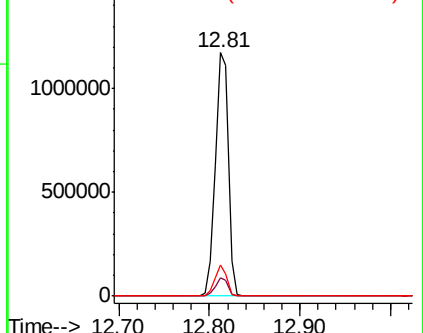

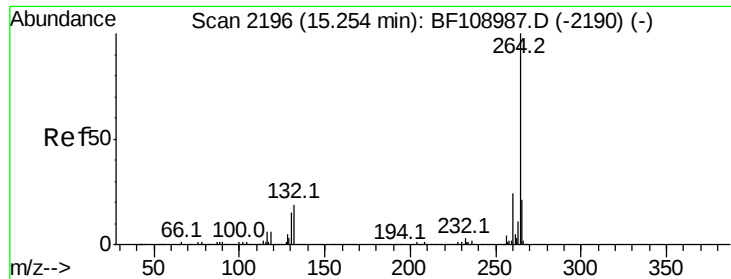

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.26 min Scan# 2197
Delta R.T. 0.01 min
Lab File: BF109120.D
Acq: 19 Sep 2018 2:54

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.9	19.2	28.8
265	21.4	17.5	26.3

