

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091818\
 Data File : BF109123.D
 Acq On : 19 Sep 2018 4:15
 Operator : JU/SJ
 Sample : J4930-07
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Sep 19 06:00:16 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 14 13:26:52 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.72	152	103354	20.00	ng	0.00
21) Naphthalene-d8	8.00	136	331327	20.00	ng	0.00
38) Acenaphthene-d10	9.75	164	131709	20.00	ng	0.00
63) Phenanthrene-d10	11.23	188	253799	20.00	ng	0.00
75) Chrysene-d12	13.85	240	306042	20.00	ng	0.00
86) Perylene-d12	15.26	264	241613	20.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.32	112	294393	47.31	ng	0.00
7) Phenol-d6	6.35	99	230968	28.78	ng	-0.01
23) Nitrobenzene-d5	7.28	82	628111	106.33	ng	0.00
41) 2,4,6-Tribromophenol	10.54	330	157409	110.12	ng	0.00
44) 2-Fluorobiphenyl	9.08	172	979190	116.48	ng	0.00
78) Terphenyl-d14	12.81	244	1183696	91.68	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
9) Benzaldehyde	6.49	77	11216	2.189	ng	# 75
19) n-Nitroso-di-n-propylamine	7.28	70	85164	16.057	ng	# 74
25) Isophorone	7.28	82	625182	61.568	ng	# 64
49) Dimethylphthalate	9.47	163	41255	4.382	ng	100
50) 2,6-Dinitrotoluene	9.75	165	16036	7.681	ng	# 25
56) 2,4-Dinitrotoluene	9.75	165	16036	5.874	ng	# 23
66) 4-Bromophenyl-phenylether	10.54	248	9390	3.282	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091818\
Data File : BF109123.D
Acq On : 19 Sep 2018 4:15
Operator : JU/SJ
Sample : J4930-07
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Sep 19 06:00:16 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 14 13:26:52 2018
Response via : Initial Calibration

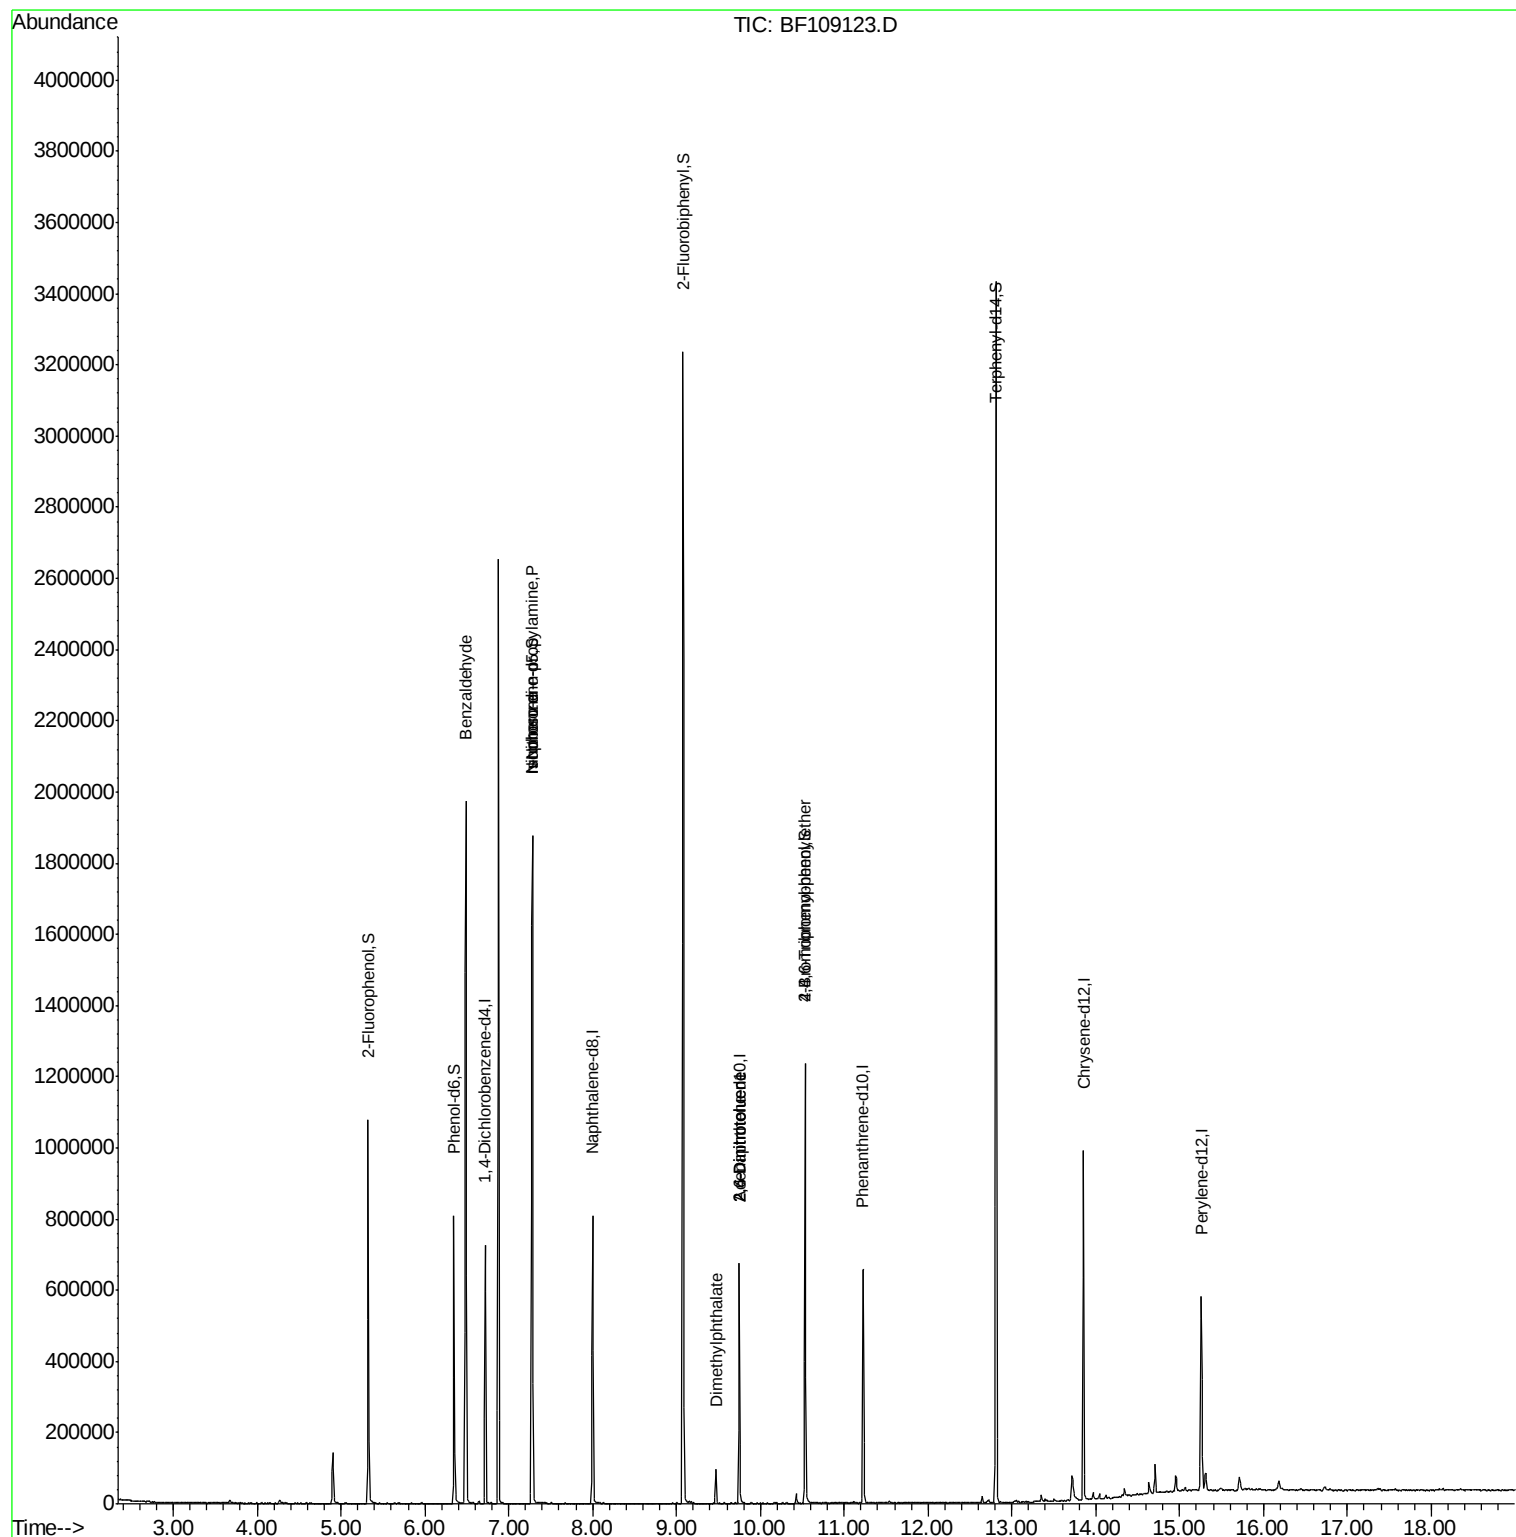

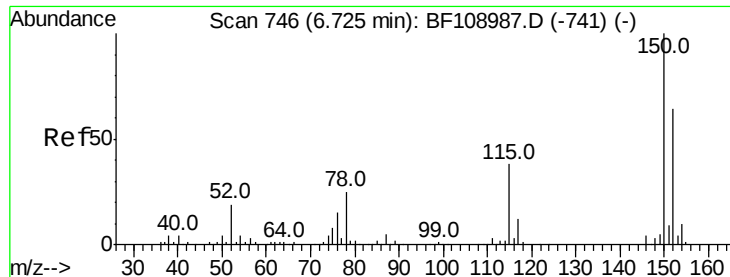


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.72 min Scan# 745
Delta R.T. -0.01 min
Lab File: BF109123.D
Acq: 19 Sep 2018 4:15

Instrument :
BNA_F
ClientSampled :

Tot Ion:152 Resp: 103354
Ion Ratio Lower Upper
152 100
150 161.1 124.6 186.8
115 63.6 50.1 75.1

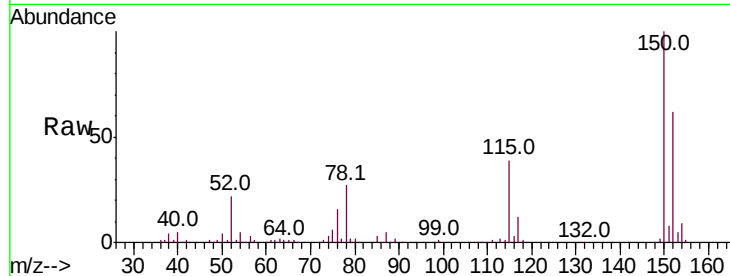


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

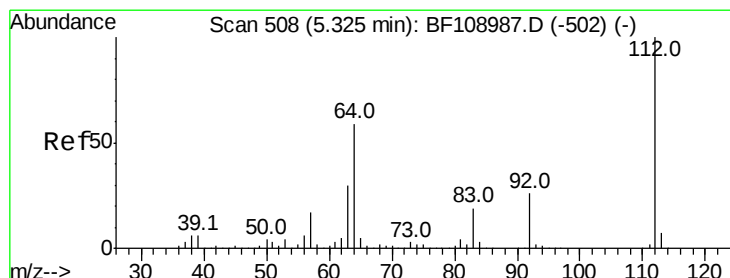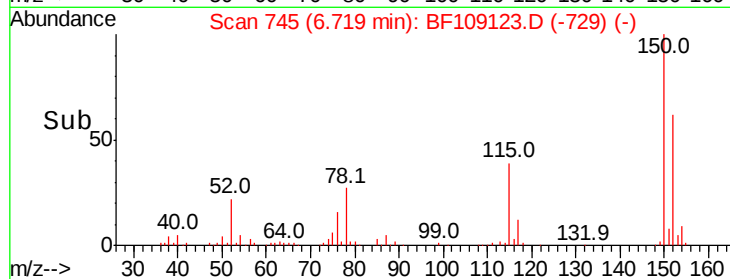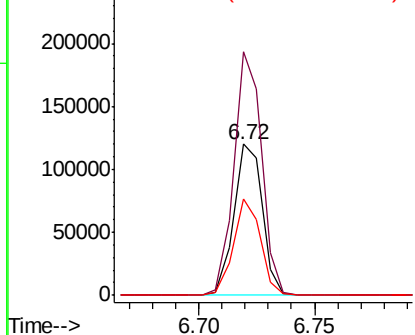



#5


2-Fluorophenol
Concen: 47.309 ng
RT: 5.32 min Scan# 508
Delta R.T. 0.00 min
Lab File: BF109123.D
Acq: 19 Sep 2018 4:15

Tgt Ion:112 Resp: 294393
Ion Ratio Lower Upper
112 100
64 59.1 47.9 71.9
63 30.3 23.7 35.5

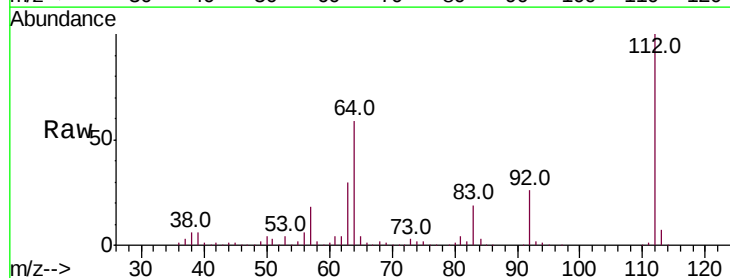

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

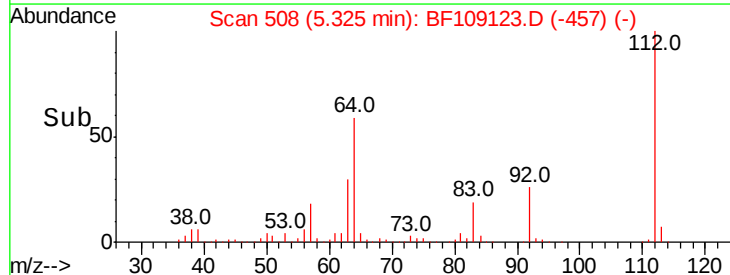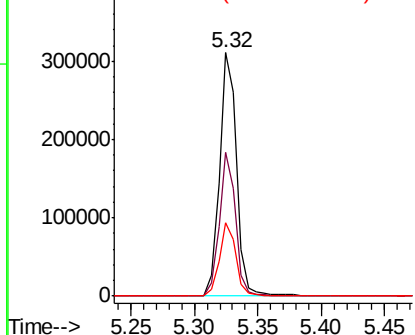

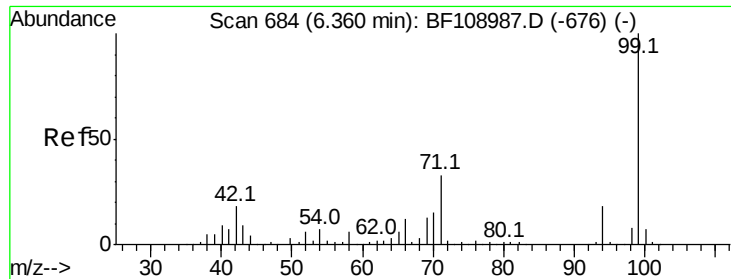

#7

Phenol-d6

Concen: 28.784 ng

RT: 6.35 min Scan# 682

Delta R.T. -0.01 min

Lab File: BF109123.D

Acq: 19 Sep 2018 4:15

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 230968

Ion Ratio Lower Upper




99 100

42 18.0 14.5 21.7

71 33.3 25.4 38.0

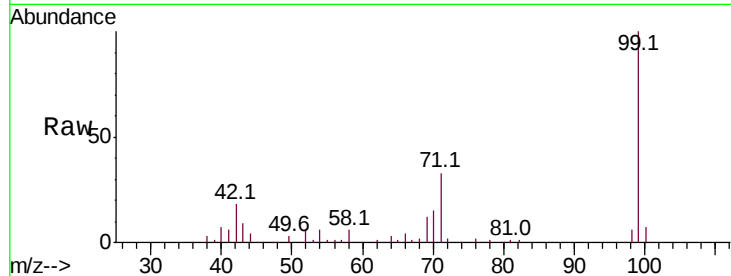

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

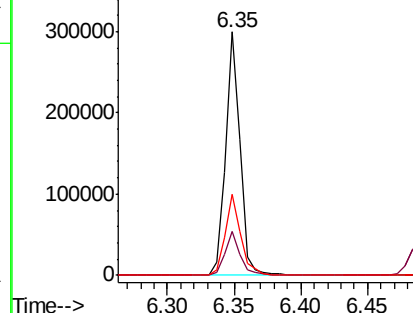

#9

Benzaldehyde

Concen: 2.189 ng

RT: 6.49 min Scan# 706

Delta R.T. 0.22 min

Lab File: BF109123.D

Acq: 19 Sep 2018 4:15


Tgt Ion: 77 Resp: 11216

Ion Ratio Lower Upper



77 100




105 77.2 81.1 121.1#

106 69.4 74.5 114.5#



Abundance Ion 77.00 (76.70 to 77.70): BF1
Ion 105.00 (104.70 to 105.70): E
Ion 106.00 (105.70 to 106.70): E



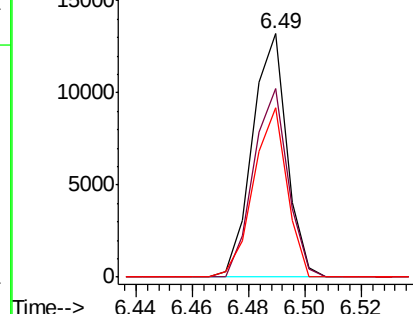



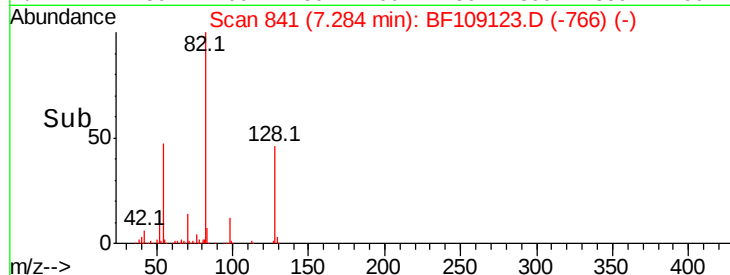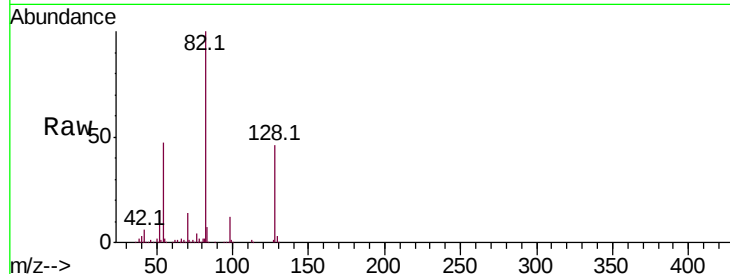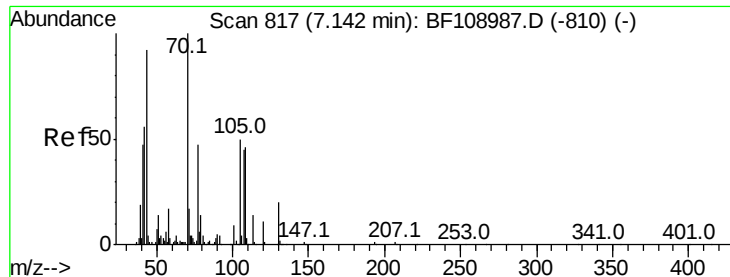

#19
n-Nitroso-di-n-propylamine
Concen: 16.057 ng
RT: 7.28 min Scan# 841
Delta R.T. 0.14 min
Lab File: BF109123.D
Acq: 19 Sep 2018 4:15


Instrument :
BNA_F
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
70	100		
42	43.4	47.5	71.3#
101	0.0	7.4	11.2#
130	2.0	16.6	25.0#

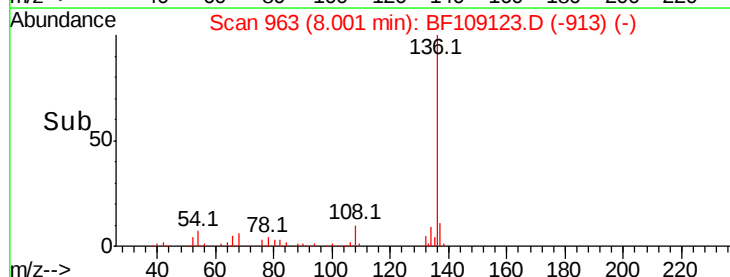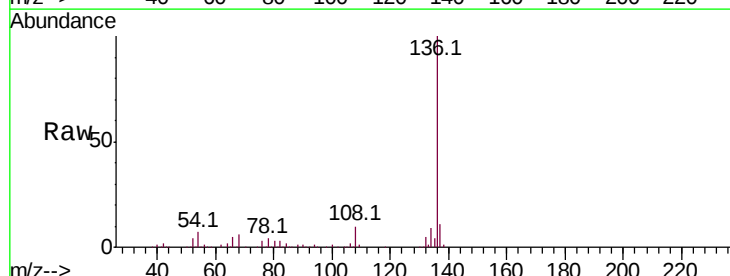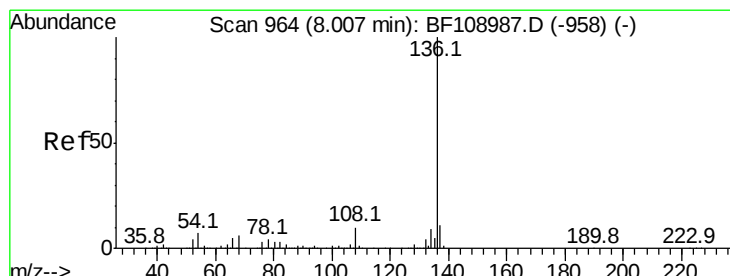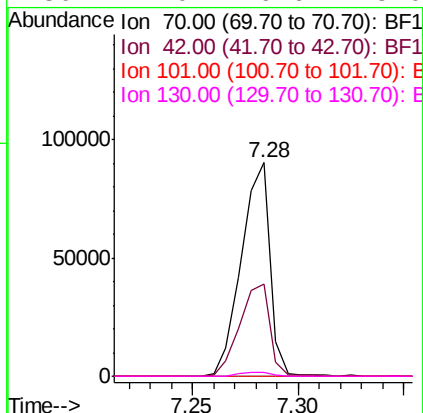

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.00 min Scan# 963
Delta R.T. -0.01 min
Lab File: BF109123.D
Acq: 19 Sep 2018 4:15

Tgt Ion	Ratio	Lower	Upper
136	100		
137	10.6	8.9	13.3
54	7.1	6.6	9.8
68	6.1	5.0	7.4




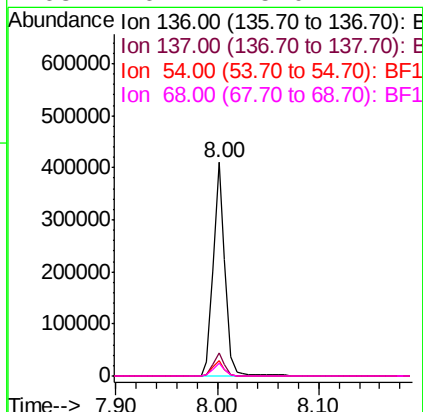




#23
Nitrobenzene-d5
Concen: 106.329 ng
RT: 7.28 min Scan# 841
Delta R.T. -0.01 min
Lab File: BF109123.D
Acq: 19 Sep 2018 4:15




Instrument :
BNA_F
ClientSampled :


Tot Ion: 82 Resp: 628111
Ion Ratio Lower Upper
82 100
128 45.9 36.1 54.1
54 47.1 41.4 62.2

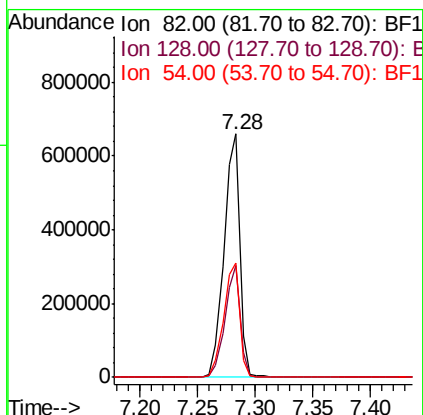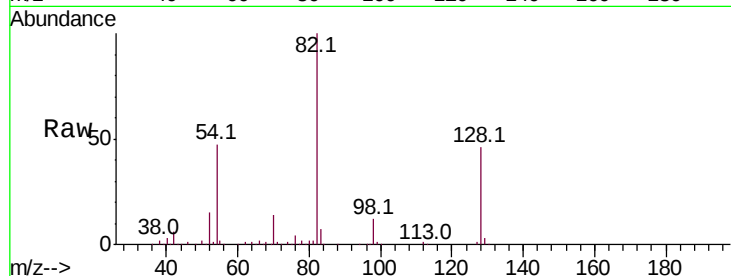

#25
Isophorone
Concen: 61.568 ng
RT: 7.28 min Scan# 841
Delta R.T. -0.26 min
Lab File: BF109123.D
Acq: 19 Sep 2018 4:15

Tgt Ion: 82 Resp: 625182
Ion Ratio Lower Upper
82 100
95 0.0 5.2 7.8#
138 0.0 14.9 22.3#


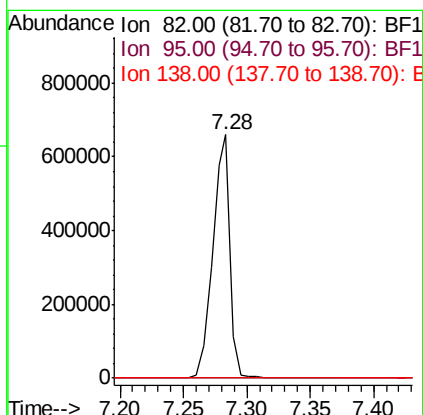




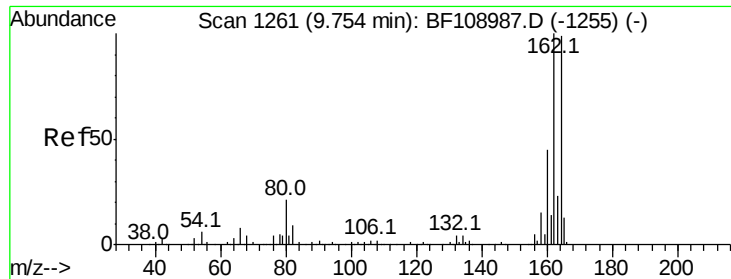

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.75 min Scan# 1260
 Delta R.T. -0.01 min
 Lab File: BF109123.D
 Acq: 19 Sep 2018 4:15




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion:164 Resp: 131709
 Ion Ratio Lower Upper
 164 100
 162 100.1 86.1 129.1
 160 45.6 38.3 57.5

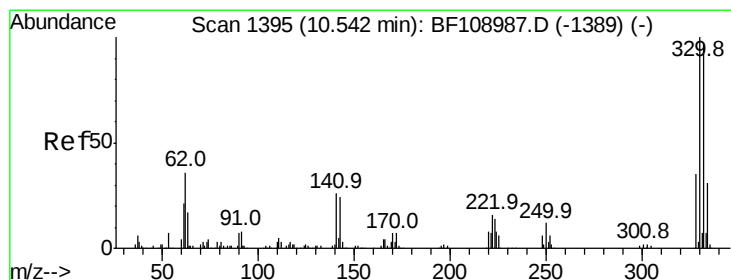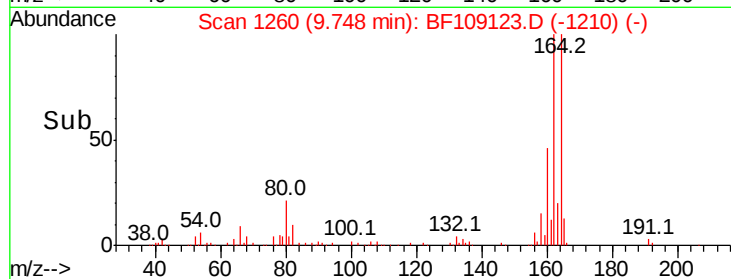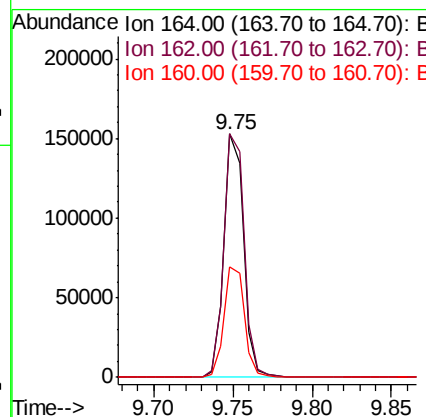

#41
 2,4,6-Tribromophenol
 Concen: 110.123 ng
 RT: 10.54 min Scan# 1394
 Delta R.T. -0.01 min
 Lab File: BF109123.D
 Acq: 19 Sep 2018 4:15

Tgt Ion:330 Resp: 157409
 Ion Ratio Lower Upper
 330 100
 332 97.8 77.0 115.6
 141 31.6 29.9 44.9

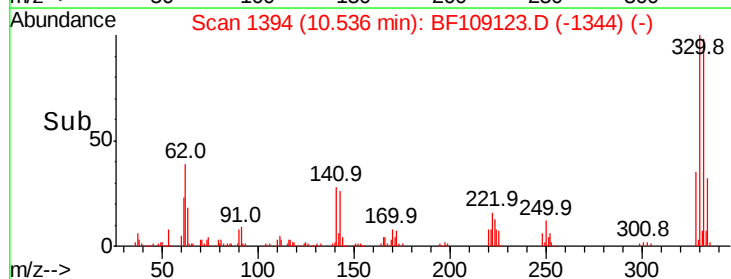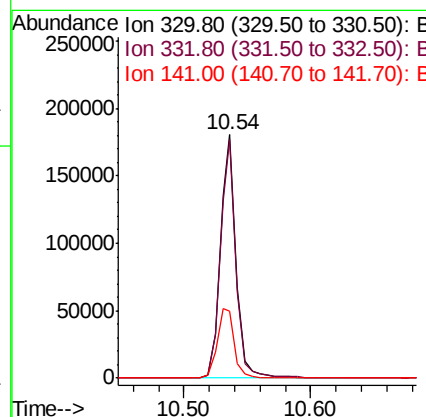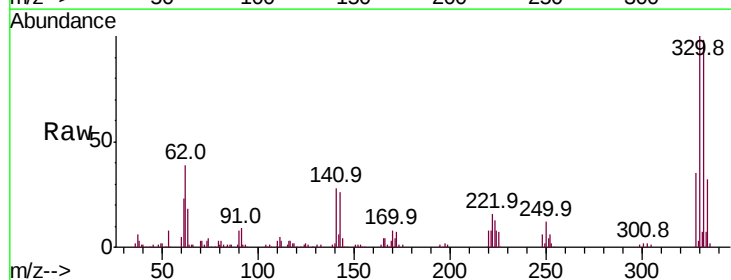


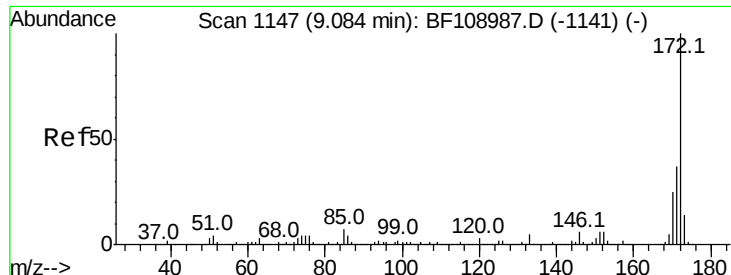




#44
 2-Fluorobiphenyl
 Concen: 116.478 ng
 RT: 9.08 min Scan# 1146
 Delta R.T. -0.01 min
 Lab File: BF109123.D
 Acq: 19 Sep 2018 4:15

Instrument :
 BNA_F
 ClientSampled :

Tot Ion:172 Resp: 979190
 Ion Ratio Lower Upper
 172 100
 171 35.7 29.7 44.5
 170 24.5 19.6 29.4

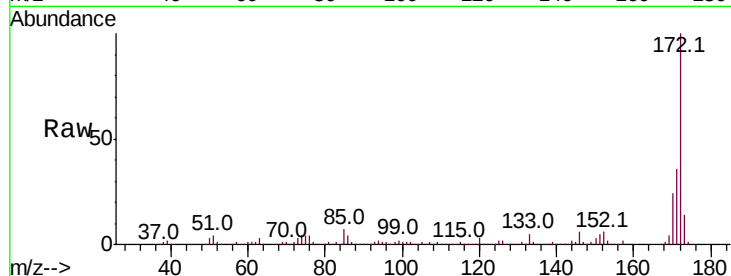


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

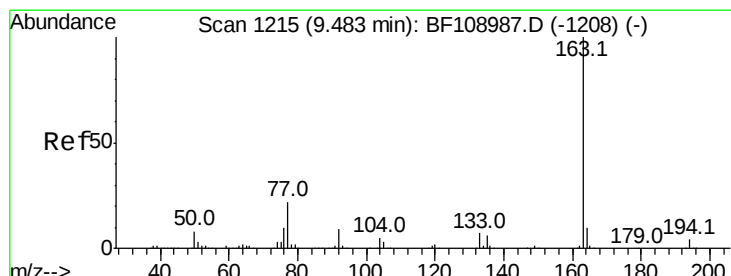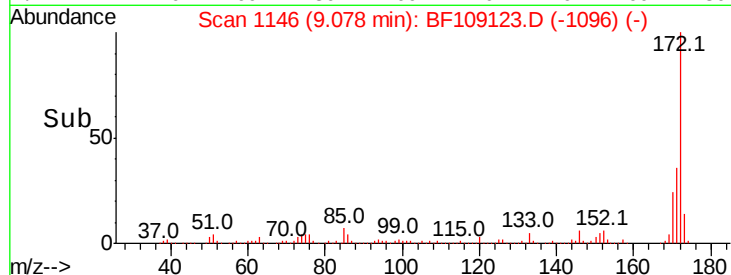
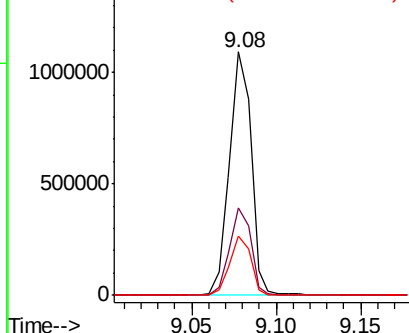



#49
 Dimethylphthalate
 Concen: 4.382 ng
 RT: 9.47 min Scan# 1213
 Delta R.T. -0.01 min
 Lab File: BF109123.D
 Acq: 19 Sep 2018 4:15

Tgt Ion:163 Resp: 41255
 Ion Ratio Lower Upper
 163 100
 194 3.5 2.7 4.1
 164 10.0 8.2 12.2

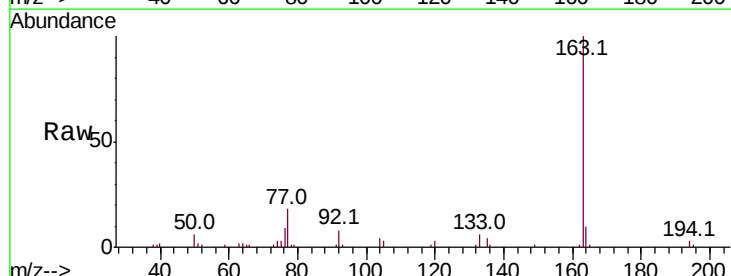

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E




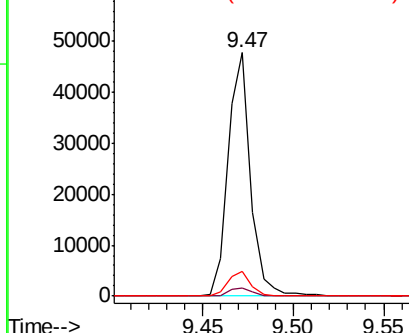


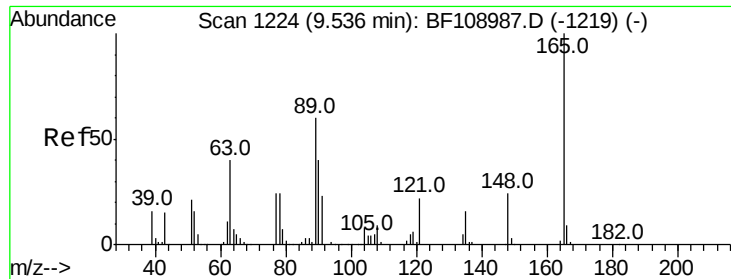

#50
 2,6-Dinitrotoluene
 Concen: 7.681 ng
 RT: 9.75 min Scan# 1260
 Delta R.T. 0.21 min
 Lab File: BF109123.D
 Acq: 19 Sep 2018 4:15




Instrument :
 BNA_F
 ClientSampled :


Tot Ion	Ratio	Lower	Upper
165	100		
63	0.0	44.7	67.1#
89	2.1	44.0	66.0#

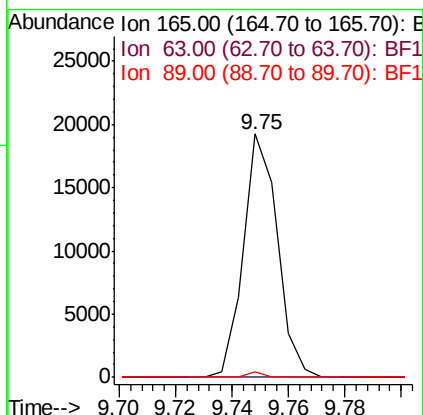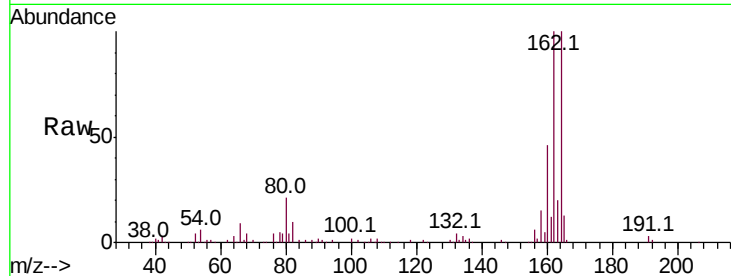

#56
 2,4-Dinitrotoluene
 Concen: 5.874 ng
 RT: 9.75 min Scan# 1260
 Delta R.T. -0.19 min
 Lab File: BF109123.D
 Acq: 19 Sep 2018 4:15

Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	36.4	54.6#
89	2.1	57.8	86.6#
182	0.0	1.6	2.4#

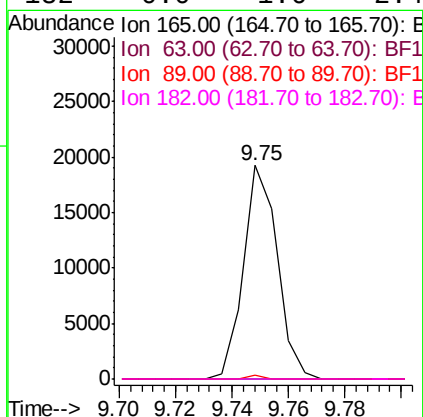


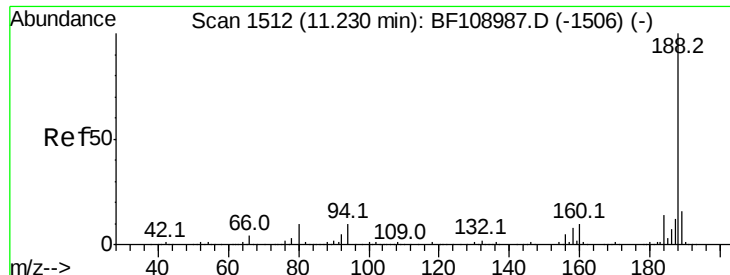




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.23 min Scan# 1512
Delta R.T. 0.00 min
Lab File: BF109123.D
Acq: 19 Sep 2018 4:15

Instrument :
BNA_F
ClientSampleId :

Tot Ion:188 Resp: 253799
Ion Ratio Lower Upper
188 100
94 8.7 8.5 12.7
80 9.2 9.2 13.8

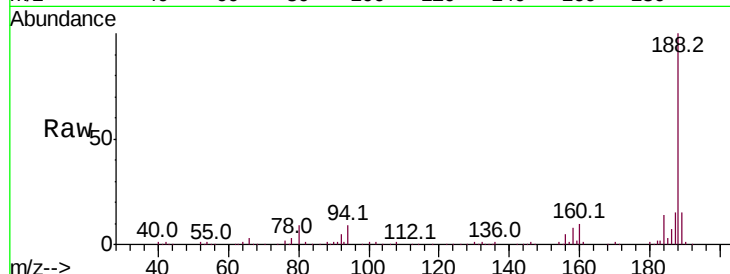


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

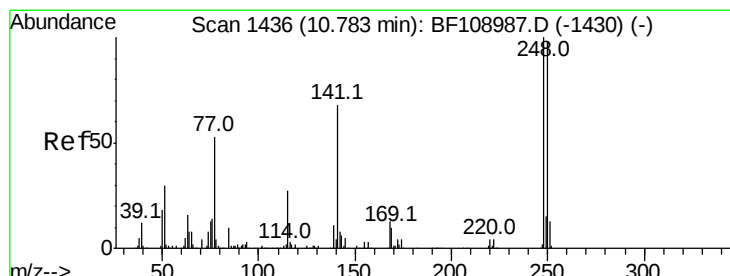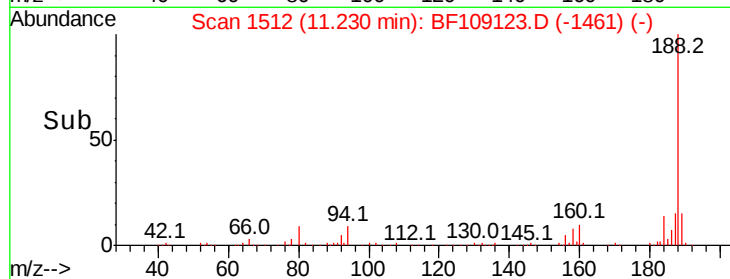
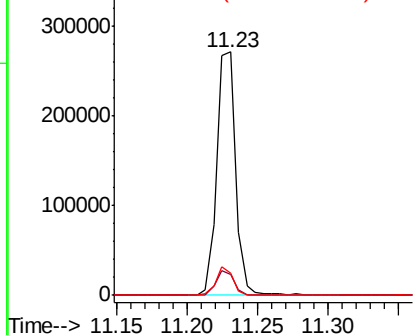



#66
4-Bromophenyl-phenylether
Concen: 3.282 ng
RT: 10.54 min Scan# 1394
Delta R.T. -0.25 min
Lab File: BF109123.D
Acq: 19 Sep 2018 4:15

Tgt Ion:248 Resp: 9390
Ion Ratio Lower Upper
248 100
250 201.1 76.9 115.3#
141 479.0 74.4 111.6#

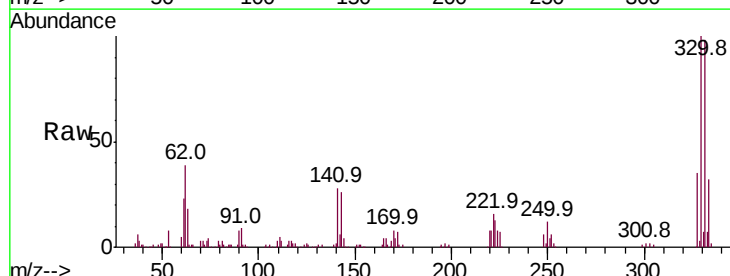

Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

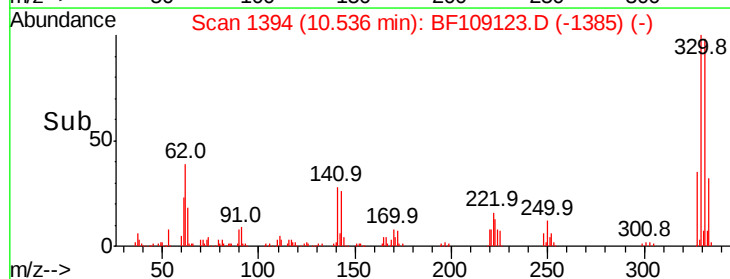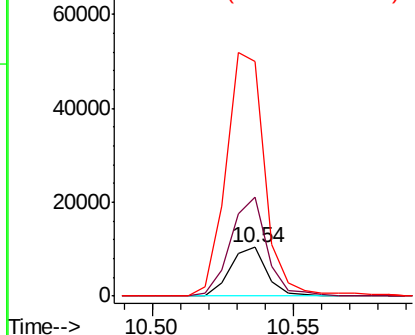



#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.85 min Scan# 1958

Delta R.T. -0.01 min

Lab File: BF109123.D

Acq: 19 Sep 2018 4:15

Instrument :

BNA_F

ClientSampleId :


Tot Ion:240 Resp: 306042

Ion Ratio Lower Upper

240 100

120 10.9 9.5 14.3




236 25.6 20.7 31.1

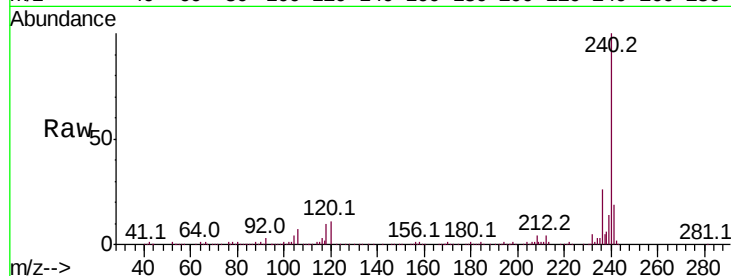

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

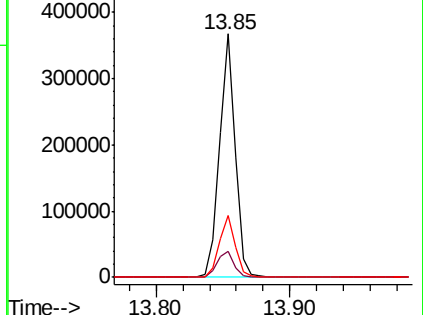

#78

Terphenyl-d14

Concen: 91.676 ng

RT: 12.81 min Scan# 1781

Delta R.T. 0.00 min

Lab File: BF109123.D

Acq: 19 Sep 2018 4:15


Tgt Ion:244 Resp: 1183696

Ion Ratio Lower Upper

244 100

212 7.3 5.4 8.0



122 11.6 11.0 16.4




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

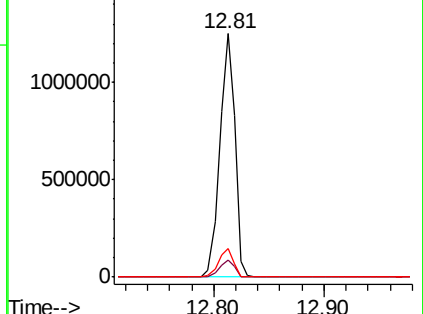


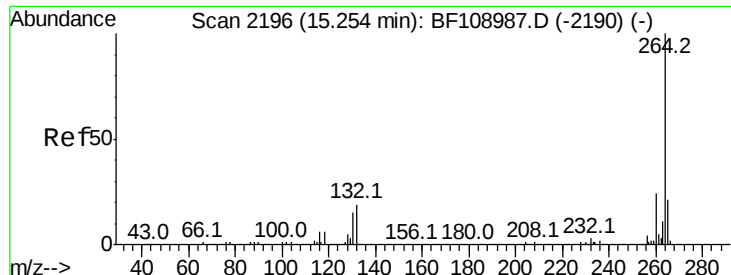

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.26 min Scan# 2197
Delta R.T. 0.01 min
Lab File: BF109123.D
Acq: 19 Sep 2018 4:15

Instrument :
BNA_F
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.1	19.2	28.8
265	21.1	17.5	26.3



Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

