

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091818\
 Data File : BF109128.D
 Acq On : 19 Sep 2018 6:30
 Operator : JU/SJ
 Sample : J4931-03
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 091418-SIDI-E-U-B

Quant Time: Sep 19 07:53:44 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 14 13:26:52 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.72	152	126987	20.00	ng	0.00
21) Naphthalene-d8	8.00	136	435488	20.00	ng	0.00
38) Acenaphthene-d10	9.75	164	177909	20.00	ng	0.00
63) Phenanthrene-d10	11.22	188	316972	20.00	ng	0.00
75) Chrysene-d12	13.85	240	340041	20.00	ng	0.00
86) Perylene-d12	15.26	264	285373	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	334492	43.75	ng	0.00
7) Phenol-d6	6.35	99	263077	26.68	ng	-0.01
23) Nitrobenzene-d5	7.28	82	778920	100.32	ng	0.00
41) 2,4,6-Tribromophenol	10.54	330	171720	88.94	ng	0.00
44) 2-Fluorobiphenyl	9.08	172	1261551	111.10	ng	0.00
78) Terphenyl-d14	12.81	244	1245429	86.81	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.47	163	59664	4.692	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091818\
Data File : BF109128.D
Acq On : 19 Sep 2018 6:30
Operator : JU/SJ
Sample : J4931-03
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
091418-SIDI-E-U-B

Quant Time: Sep 19 07:53:44 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 14 13:26:52 2018
Response via : Initial Calibration

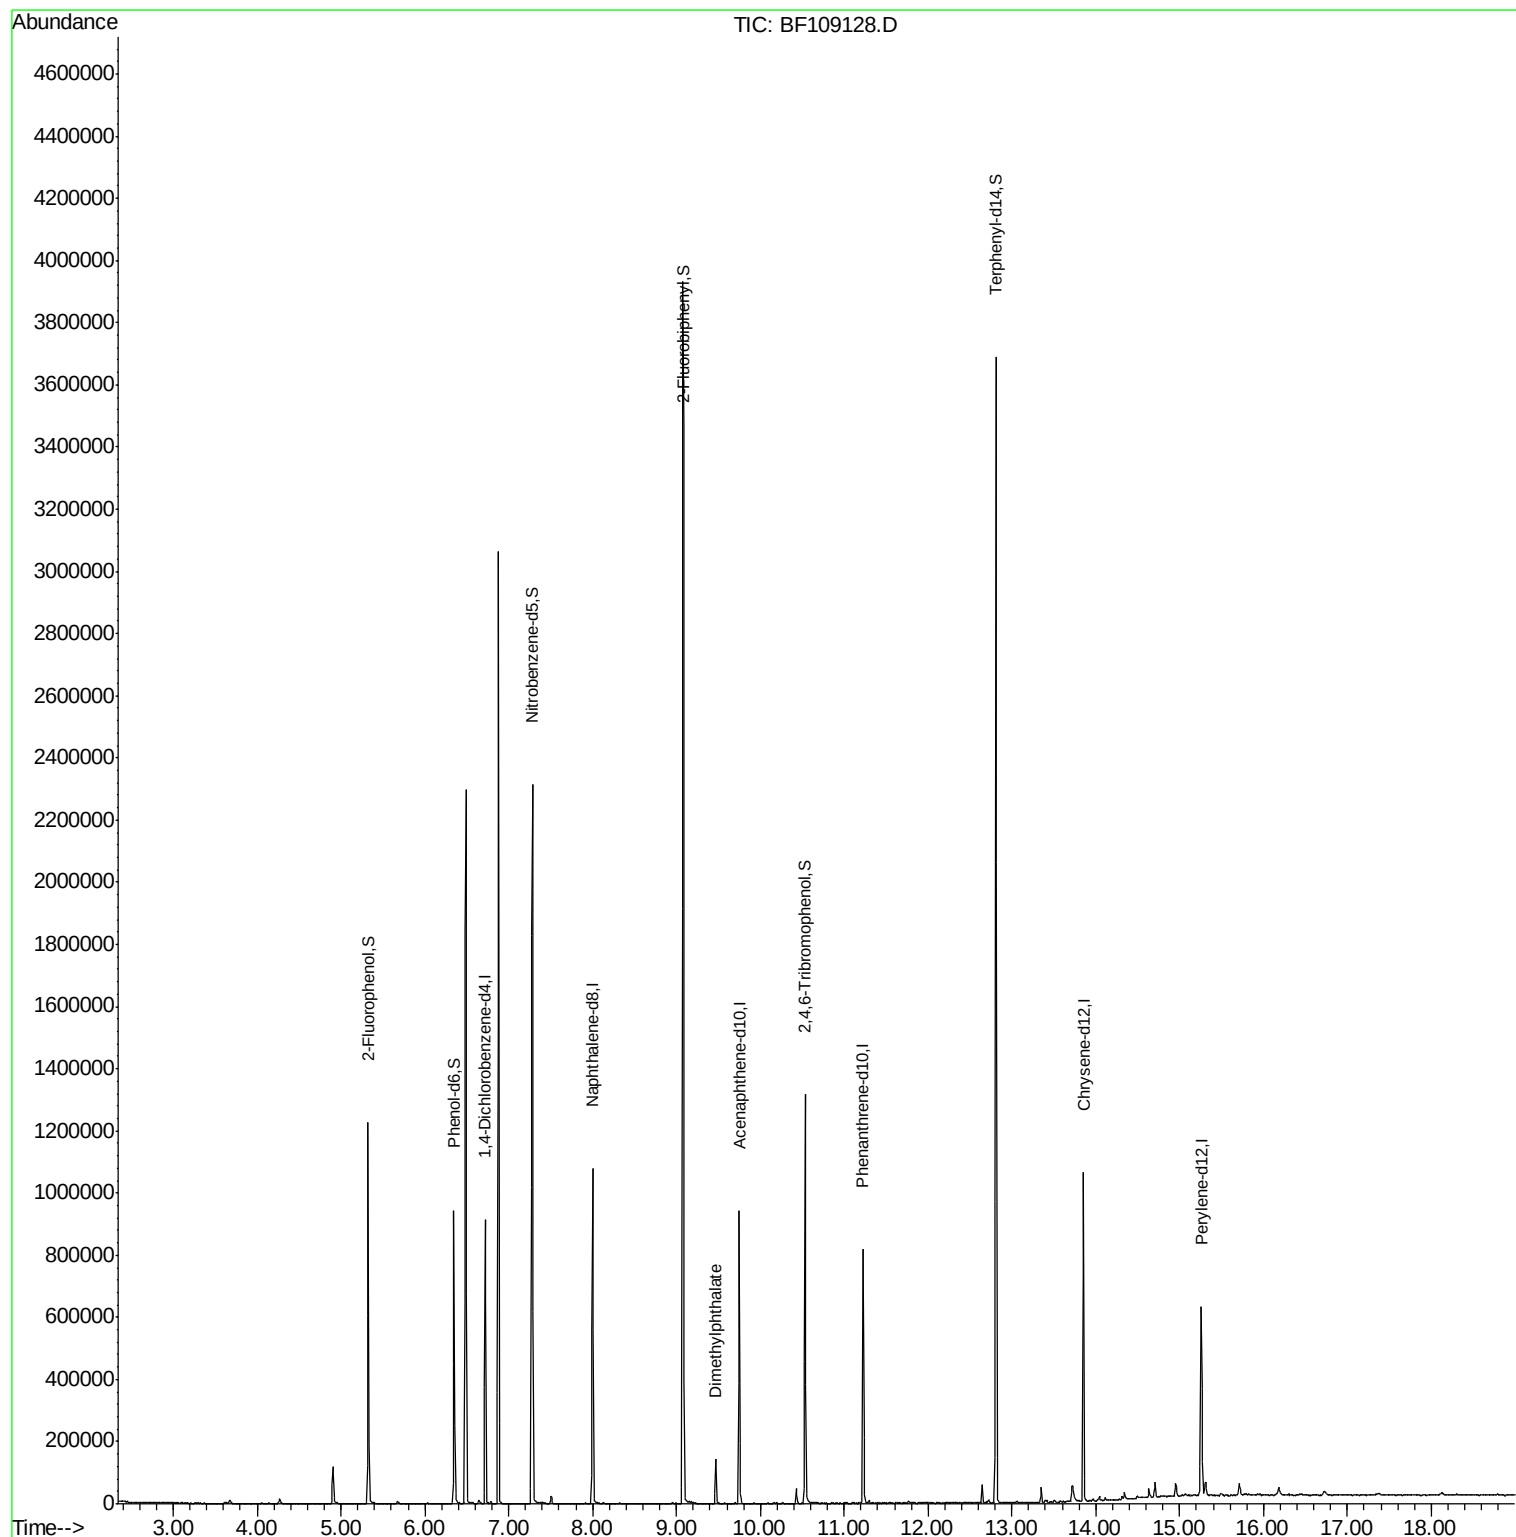




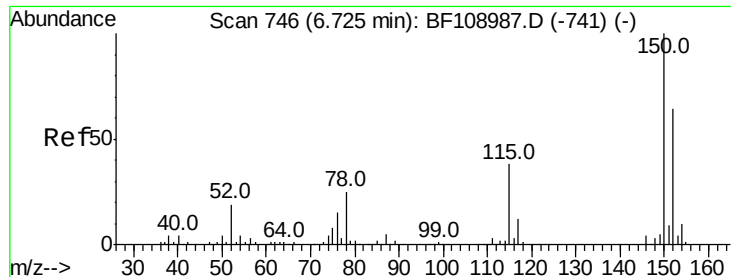


#1

1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.72 min Scan# 745
 Delta R.T. -0.01 min
 Lab File: BF109128.D
 Acq: 19 Sep 2018 6:30

Instrument :
 BNA_F
 ClientSampleId :
 091418-SIDI-E-U-B




Tot Ion	Ratio	Lower	Upper
152	100		
150	158.7	124.6	186.8
115	62.5	50.1	75.1

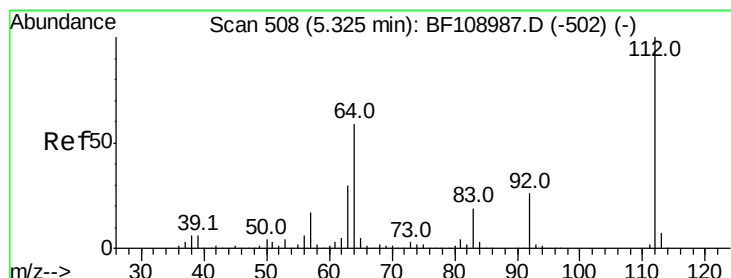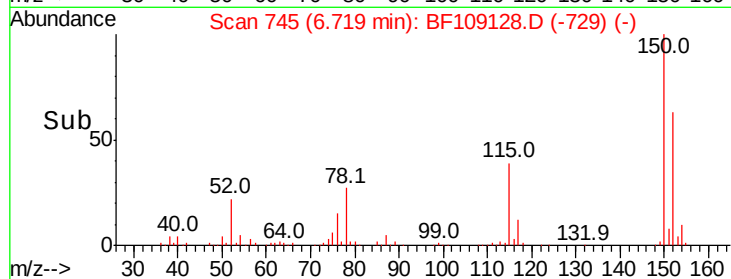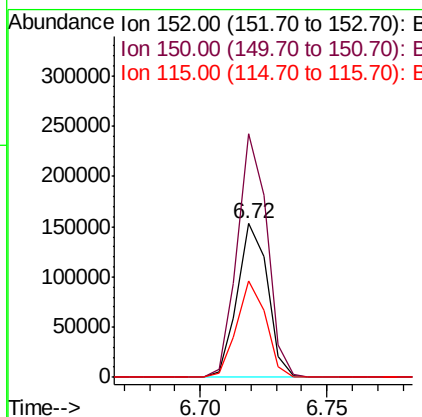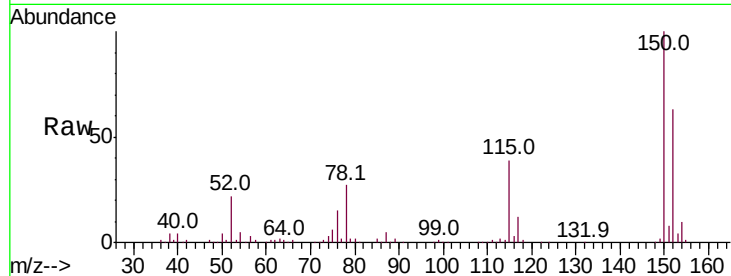


#5

2-Fluorophenol
 Concen: 43.749 ng
 RT: 5.32 min Scan# 508
 Delta R.T. 0.00 min
 Lab File: BF109128.D
 Acq: 19 Sep 2018 6:30

Tgt Ion	Ratio	Lower	Upper
112	100		
64	58.2	47.9	71.9
63	30.1	23.7	35.5

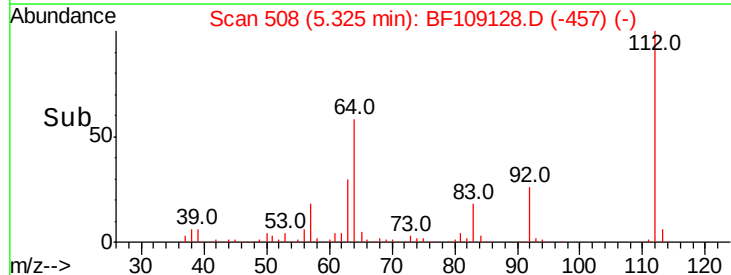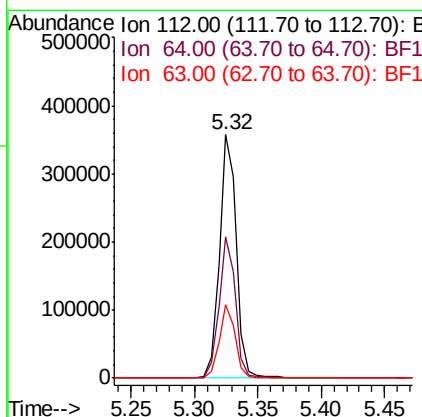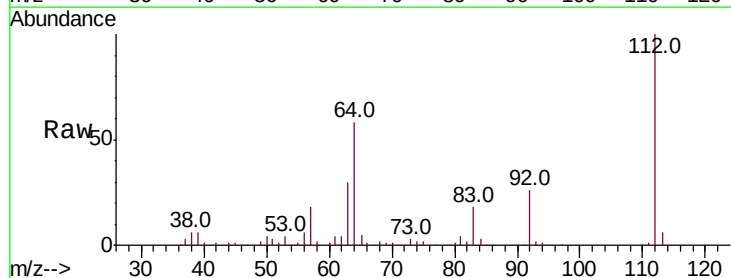

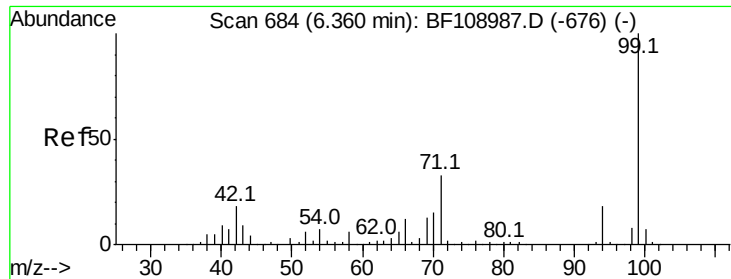

#7

Phenol-d6

Concen: 26.684 ng

RT: 6.35 min Scan# 682

Delta R.T. -0.01 min

Lab File: BF109128.D

Acq: 19 Sep 2018 6:30

Instrument :

BNA_F

ClientSampleId :

091418-SIDI-E-U-B


Tot Ion: 99 Resp: 263077

Ion Ratio Lower Upper




99 100

42 18.1 14.5 21.7

71 33.5 25.4 38.0

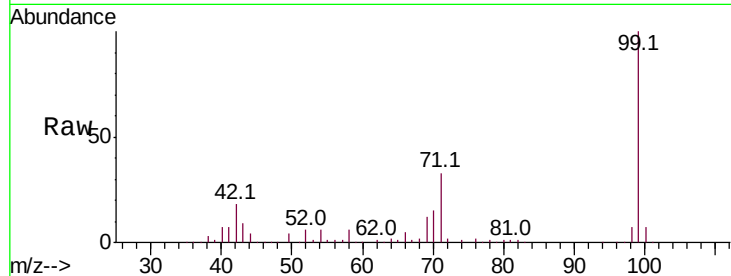

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

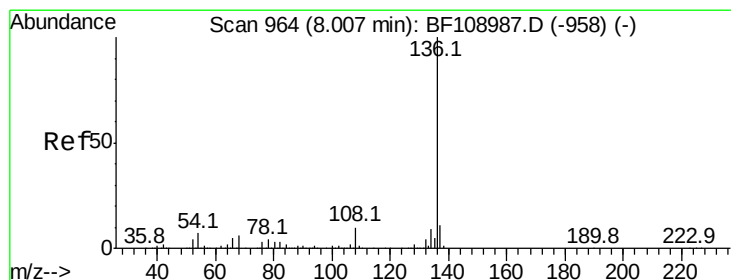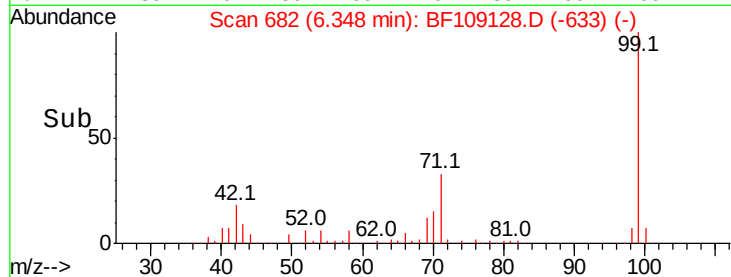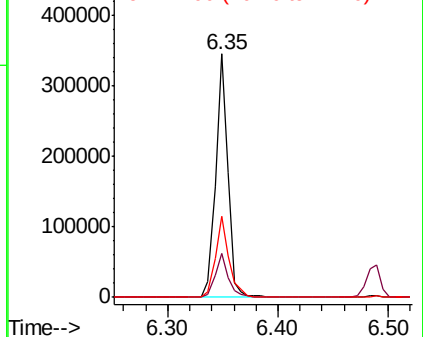

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.00 min Scan# 963

Delta R.T. -0.01 min

Lab File: BF109128.D

Acq: 19 Sep 2018 6:30

Tgt Ion: 136 Resp: 435488


Ion Ratio Lower Upper

136 100



137 11.3 8.9 13.3


54 7.2 6.6 9.8

68 5.7 5.0 7.4

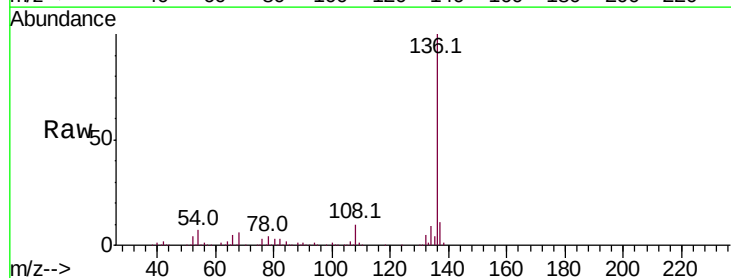

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

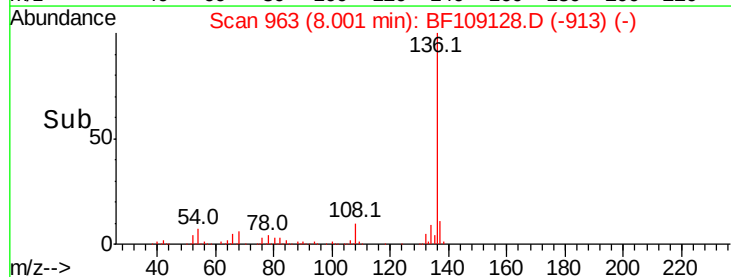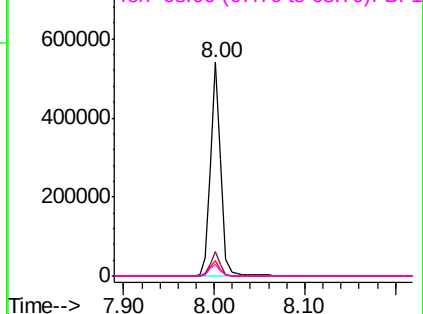


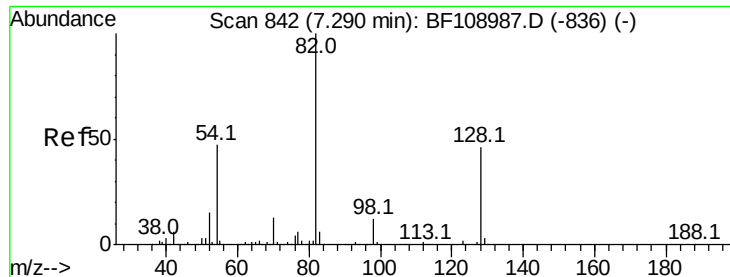




#23
 Nitrobenzene-d5
 Concen: 100.320 ng
 RT: 7.28 min Scan# 841
 Delta R.T. -0.01 min
 Lab File: BF109128.D
 Acq: 19 Sep 2018 6:30

Instrument :
 BNA_F
 ClientSampleId :
 091418-SIDI-E-U-B

Tot Ion: 82 Resp: 778920
 Ion Ratio Lower Upper
 82 100
 128 44.4 36.1 54.1
 54 47.7 41.4 62.2

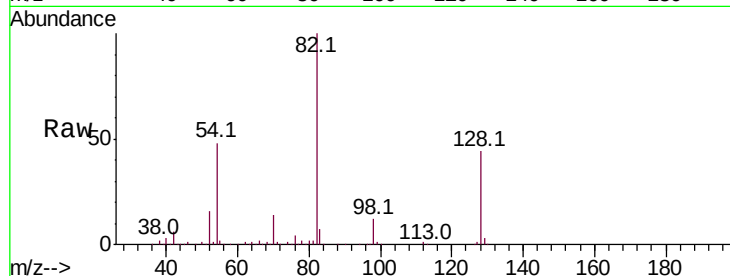


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

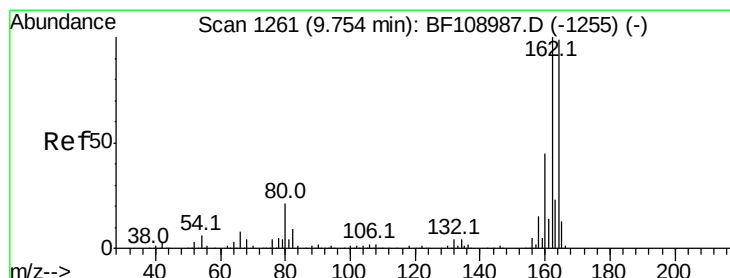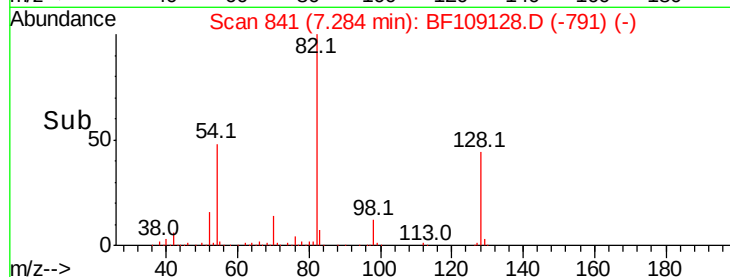
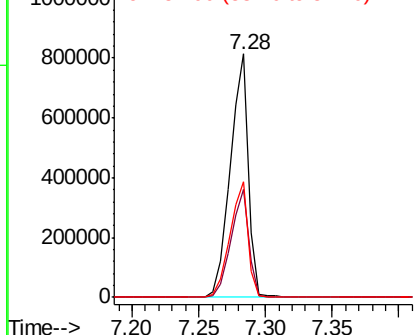



#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.75 min Scan# 1260
 Delta R.T. -0.01 min
 Lab File: BF109128.D
 Acq: 19 Sep 2018 6:30

Tgt Ion:164 Resp: 177909
 Ion Ratio Lower Upper
 164 100
 162 100.4 86.1 129.1
 160 45.7 38.3 57.5

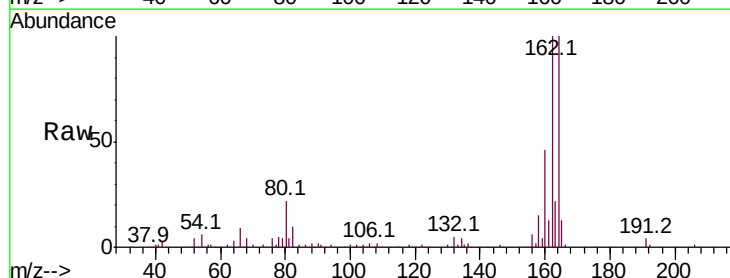

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

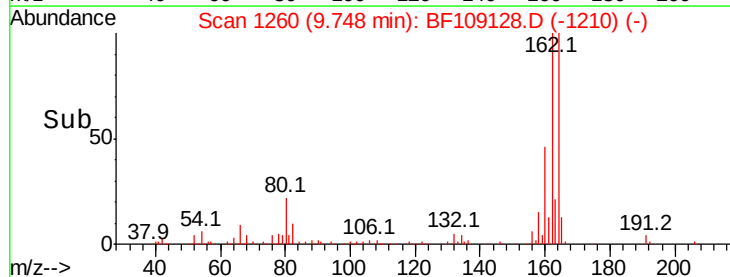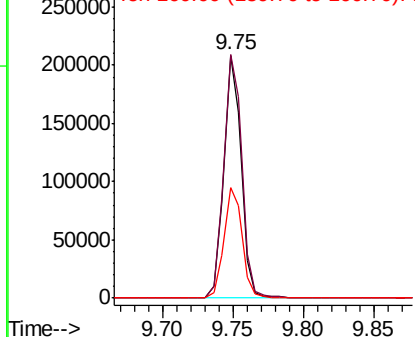


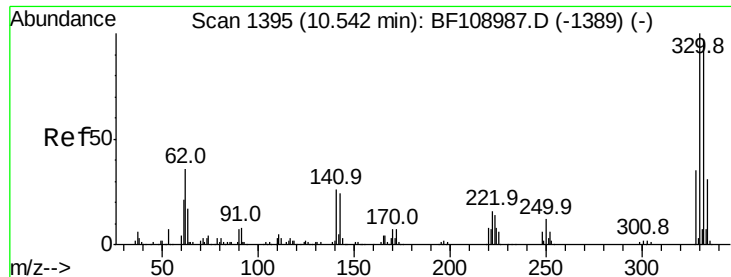

#41
 2,4,6-Tribromophenol
 Concen: 88.938 ng
 RT: 10.54 min Scan# 1394
 Delta R.T. -0.01 min
 Lab File: BF109128.D
 Acq: 19 Sep 2018 6:30

Instrument :
 BNA_F
 ClientSampleId :
 091418-SIDI-E-U-B

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.4	77.0	115.6
141	31.4	29.9	44.9



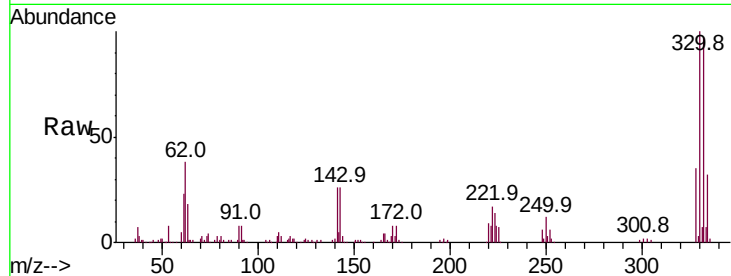


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

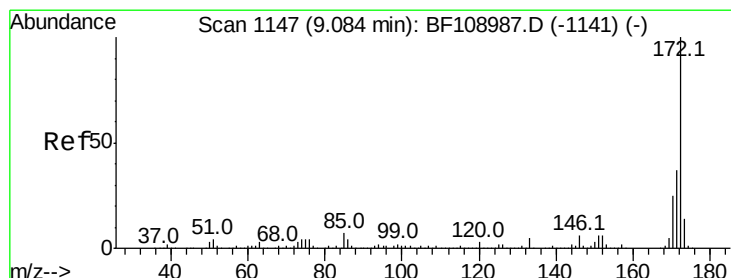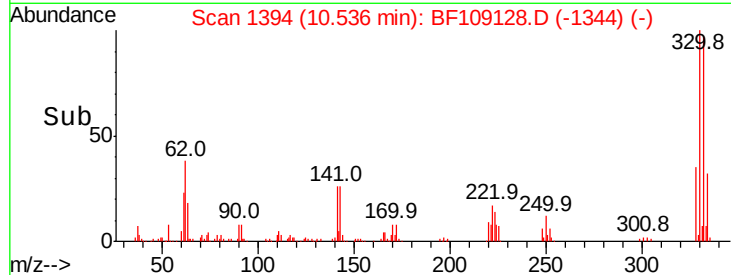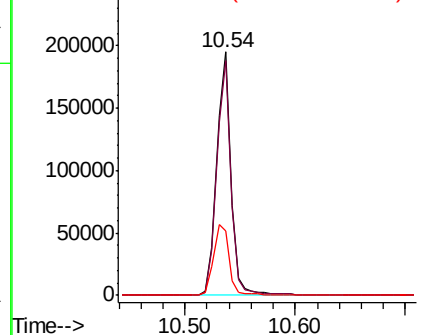

#44
 2-Fluorobiphenyl
 Concen: 111.097 ng
 RT: 9.08 min Scan# 1146
 Delta R.T. -0.01 min
 Lab File: BF109128.D
 Acq: 19 Sep 2018 6:30

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.2	29.7	44.5
170	24.5	19.6	29.4


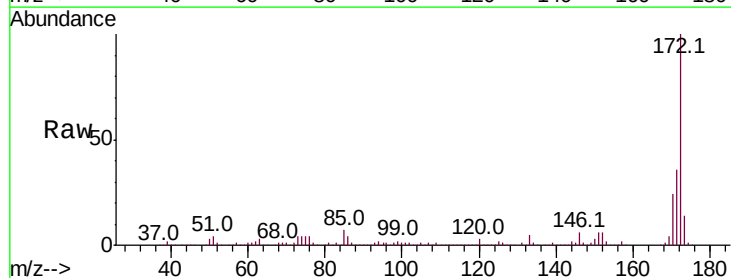



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

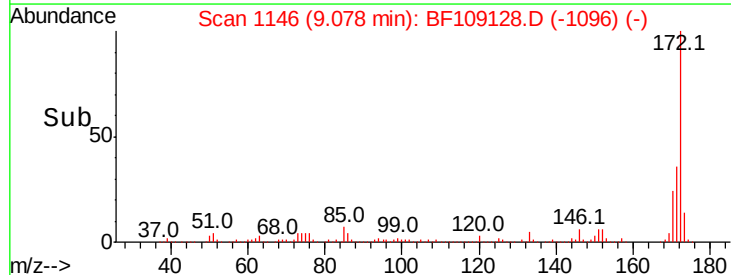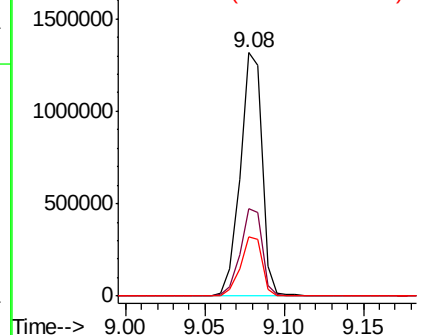

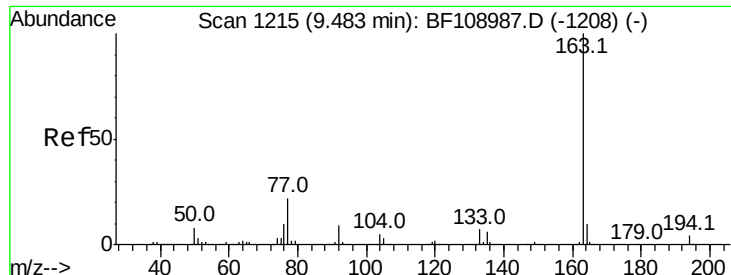

#49

Dimethylphthalate

Concen: 4.692 ng

RT: 9.47 min Scan# 1212

Delta R.T. -0.02 min

Lab File: BF109128.D

Acq: 19 Sep 2018 6:30

Instrument :

BNA_F

ClientSampleId :

091418-SIDI-E-U-B


Tot Ion:163 Resp: 59664

Ion Ratio Lower Upper




163 100

194 3.6 2.7 4.1

164 10.7 8.2 12.2

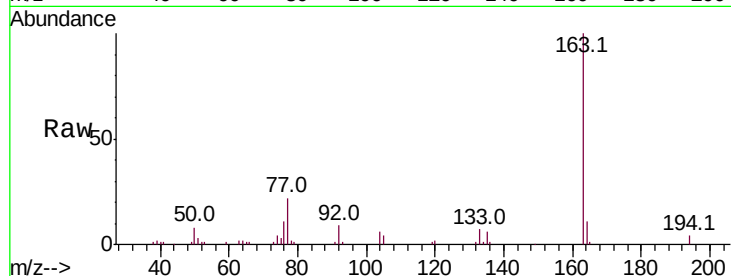

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

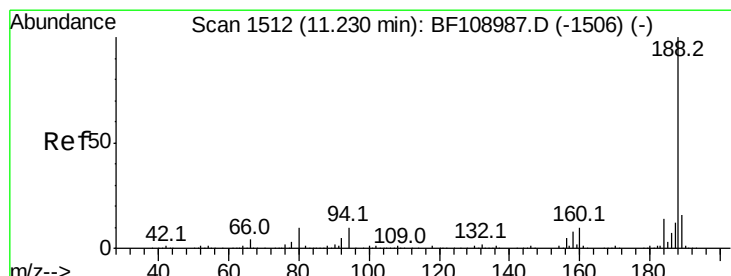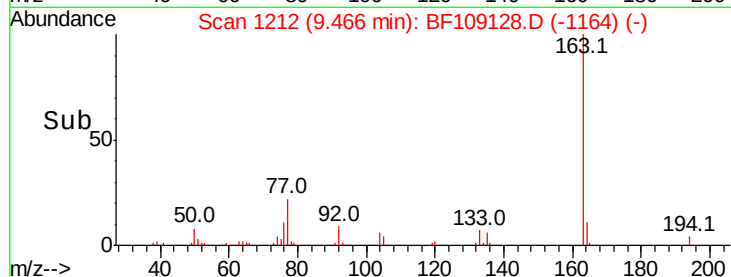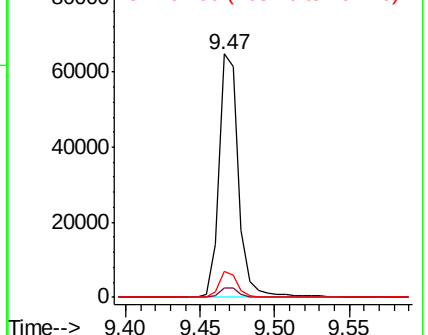

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.22 min Scan# 1511

Delta R.T. -0.01 min

Lab File: BF109128.D

Acq: 19 Sep 2018 6:30


Tgt Ion:188 Resp: 316972

Ion Ratio Lower Upper



188 100


94 10.6 8.5 12.7

80 10.6 9.2 13.8

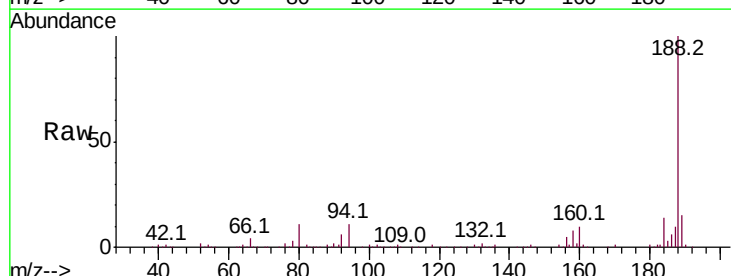

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

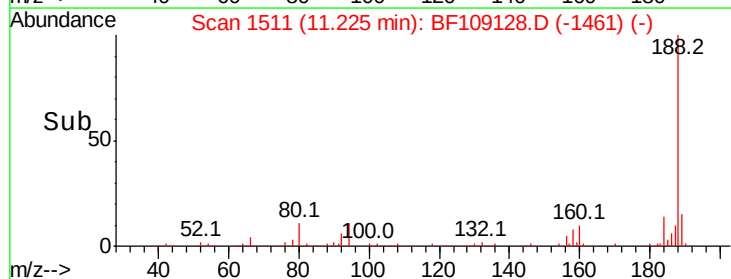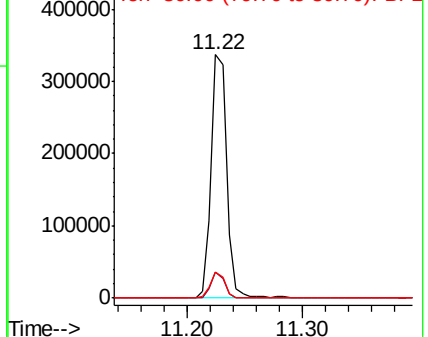

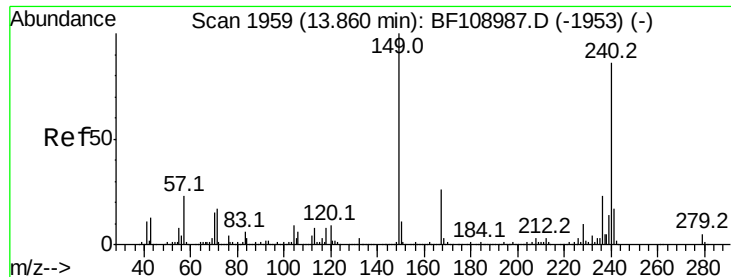

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.85 min Scan# 1958

Delta R.T. -0.01 min

Lab File: BF109128.D

Acq: 19 Sep 2018 6:30

Instrument :

BNA_F

ClientSampleId :

091418-SIDI-E-U-B


Tot Ion:240 Resp: 340041

Ion Ratio Lower Upper

240 100

120 11.0 9.5 14.3




236 25.5 20.7 31.1

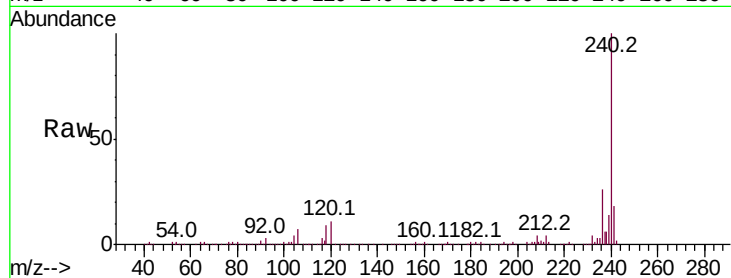

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

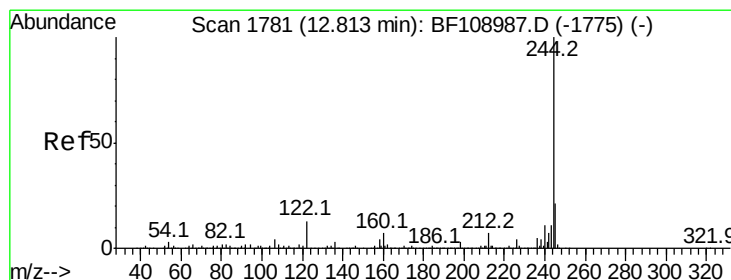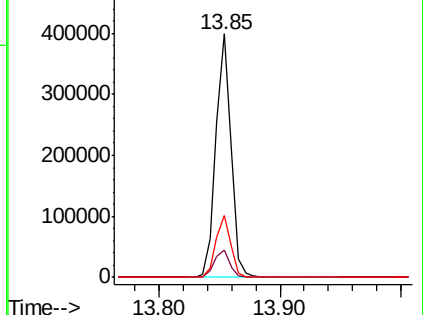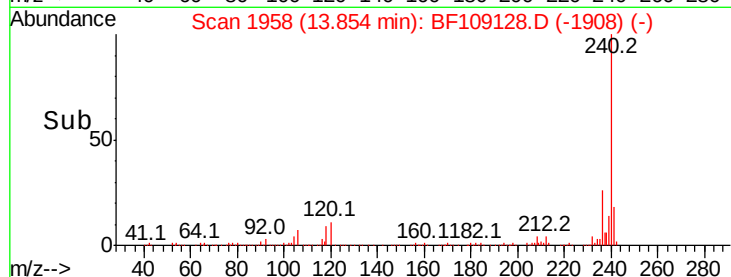

#78

Terphenyl-d14

Concen: 86.813 ng

RT: 12.81 min Scan# 1781

Delta R.T. 0.00 min

Lab File: BF109128.D

Acq: 19 Sep 2018 6:30


Tgt Ion:244 Resp: 1245429

Ion Ratio Lower Upper

244 100

212 7.2 5.4 8.0



122 12.1 11.0 16.4

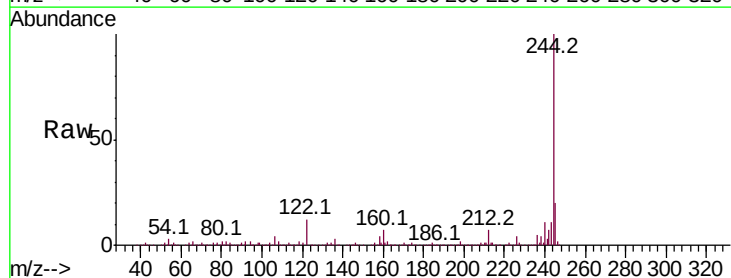


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

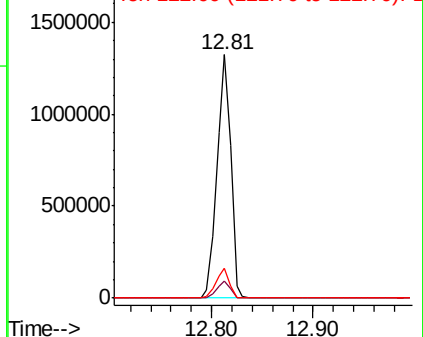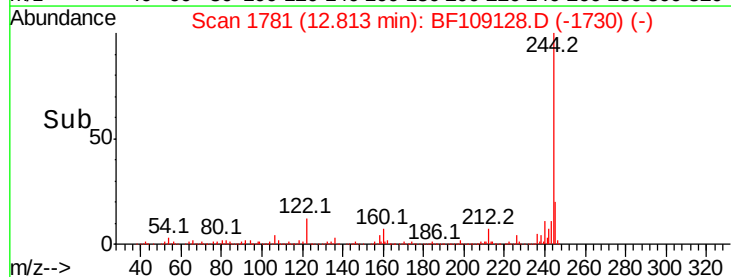


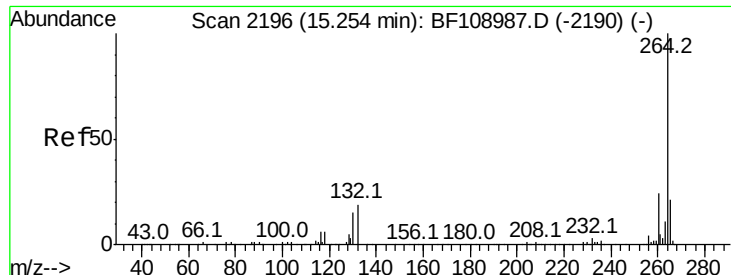

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.26 min Scan# 2197
Delta R.T. 0.01 min
Lab File: BF109128.D
Acq: 19 Sep 2018 6:30

Instrument :
BNA_F
ClientSampleId :
091418-SIDI-E-U-B

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.9	19.2	28.8
265	21.5	17.5	26.3

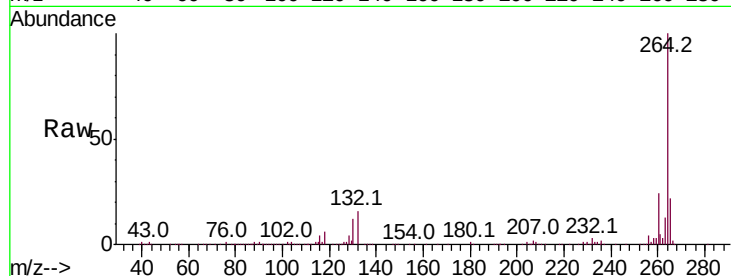

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

