


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091818\
 Data File : BF109091.D
 Acq On : 18 Sep 2018 13:15
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 14 13:26:52 2018

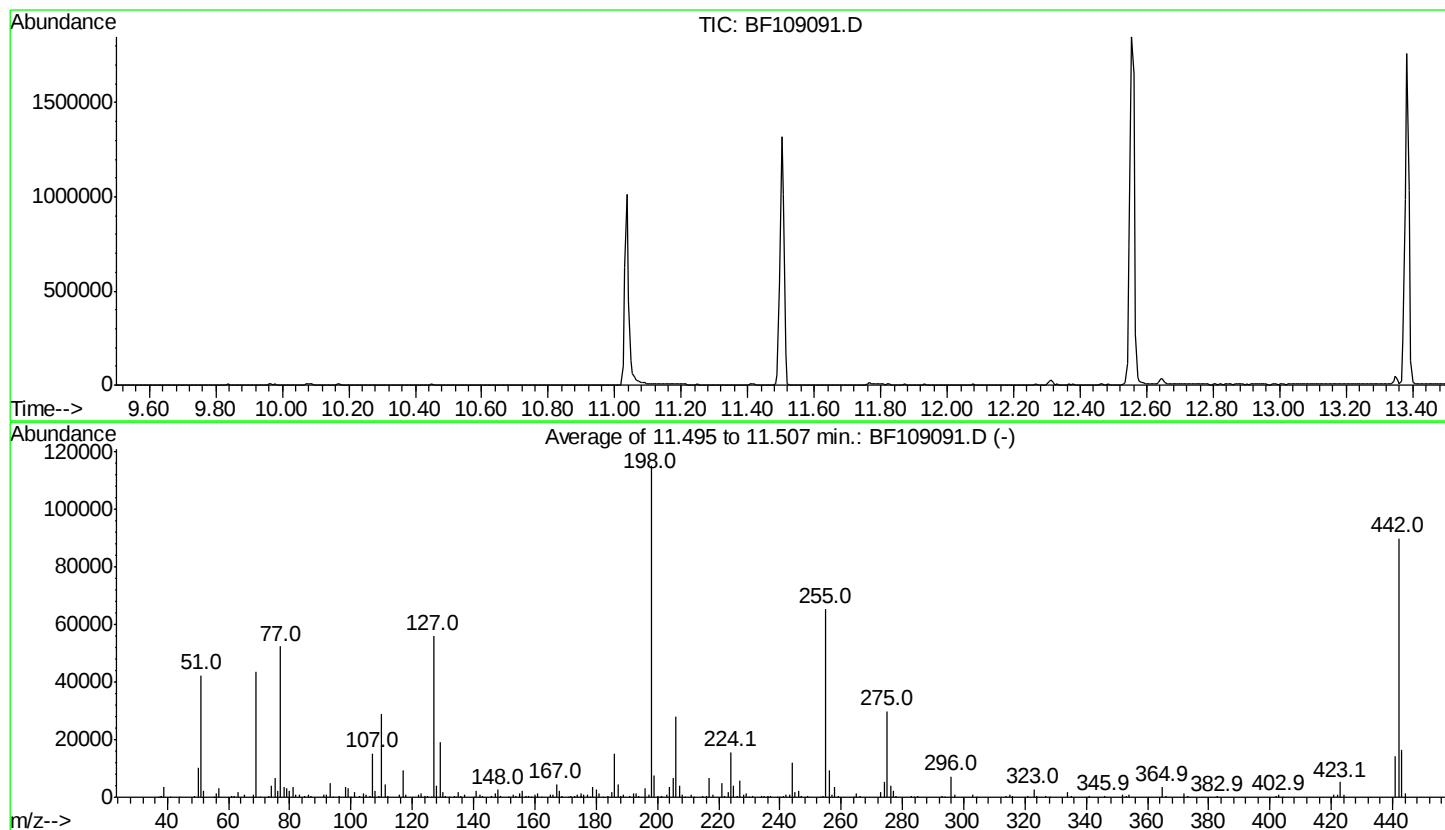

AutoFind: Scans 1557, 1558, 1559; Background Corrected with Scan 1552

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	42445	PASS
68	69	0.00	2	1.7	733	PASS
69	198	0.00	100	37.8	43520	PASS
70	69	0.00	2	0.3	146	PASS
127	198	10	80	48.7	56114	PASS
197	198	0.00	2	0.7	851	PASS
198	198	100	100	100.0	115216	PASS
199	198	5	9	6.5	7540	PASS
275	198	10	60	25.9	29893	PASS
365	198	1	100	3.1	3609	PASS
441	198	0.01	100	12.2	14042	PASS
442	198	50	100	78.1	89970	PASS
443	442	15	24	18.1	16279	PASS