


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091818\
 Data File : BF109118.D
 Acq On : 19 Sep 2018 1:53
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 14 13:26:52 2018

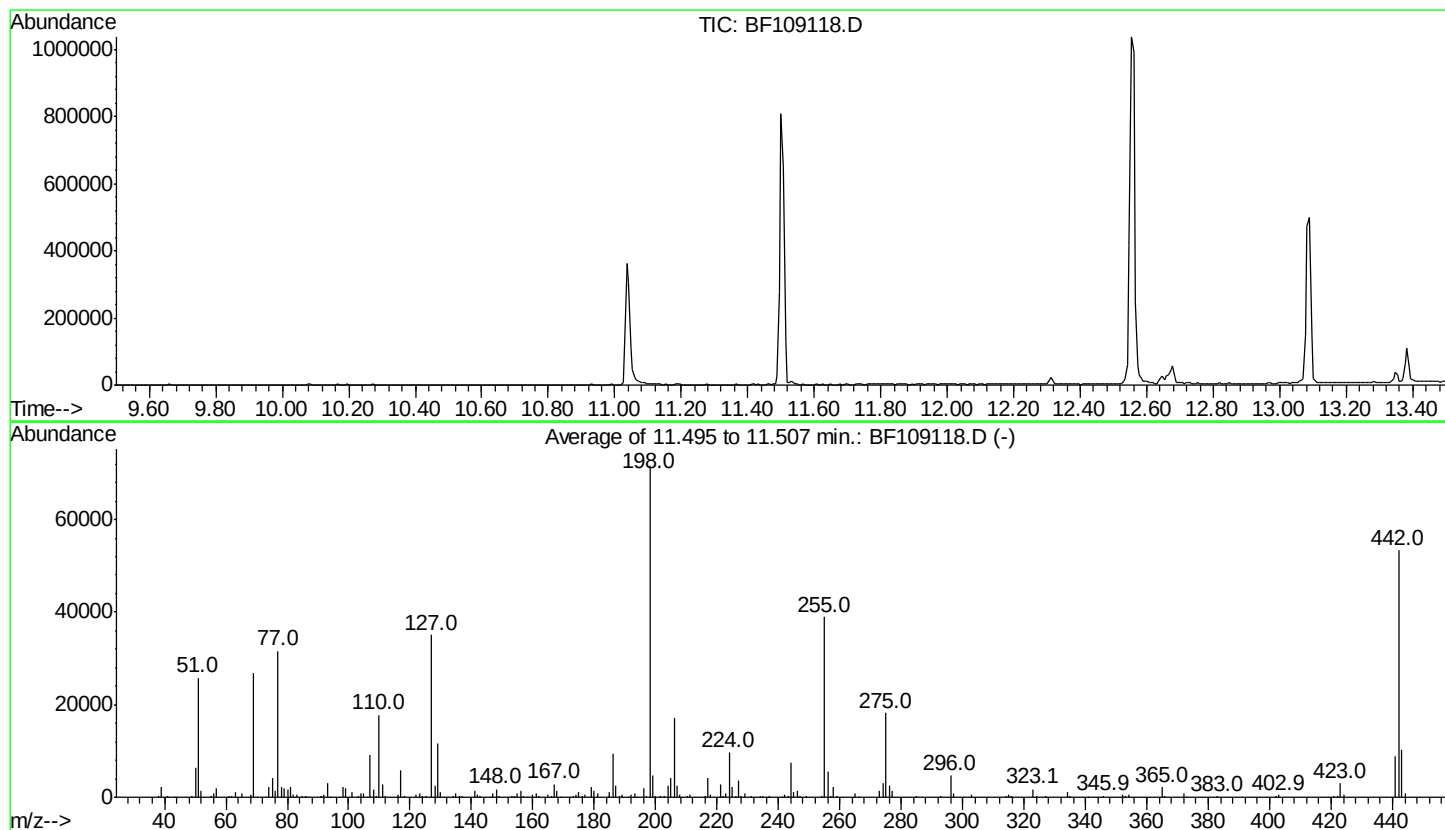

AutoFind: Scans 1557, 1558, 1559; Background Corrected with Scan 1553

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	25760	PASS
68	69	0.00	2	1.8	473	PASS
69	198	0.00	100	37.6	26906	PASS
70	69	0.00	2	0.5	122	PASS
127	198	10	80	49.0	35085	PASS
197	198	0.00	2	0.2	170	PASS
198	198	100	100	100.0	71650	PASS
199	198	5	9	6.7	4806	PASS
275	198	10	60	25.3	18137	PASS
365	198	1	100	3.0	2151	PASS
441	198	0.01	100	12.4	8857	PASS
442	198	50	100	74.4	53317	PASS
443	442	15	24	19.4	10318	PASS