

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091819\
 Data File : BF117140.D
 Acq On : 18 Sep 2019 11:34
 Operator : HP/JU
 Sample : PB123161BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Sep 19 05:11:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 13 16:23:17 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.82	152	77806	20.00	ng	0.00
21) Naphthalene-d8	8.10	136	310128	20.00	ng	0.00
39) Acenaphthene-d10	9.85	164	161010	20.00	ng	0.00
64) Phenanthrene-d10	11.33	188	265348	20.00	ng	0.00
76) Chrysene-d12	13.97	240	168898	20.00	ng	0.00
87) Perylene-d12	15.42	264	133876	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.46	112	617641	123.94	ng	0.02
7) Phenol-d6	6.46	99	856356	132.96	ng	0.00
23) Nitrobenzene-d5	7.39	82	543307	92.05	ng	0.00
42) 2,4,6-Tribromophenol	10.64	330	186816	138.83	ng	0.00
45) 2-Fluorobiphenyl	9.17	172	970906	94.29	ng	0.00
79) Terphenyl-d14	12.92	244	975195	107.93	ng	0.00
Target Compounds						
9) Benzaldehyde	6.46	77	1176	Below Cal	Qvalue	# 1
19) n-Nitroso-di-n-propylamine	7.39	70	72085	18.380 ng	#	78
25) Isophorone	7.39	82	543304	51.987 ng	#	66
51) 2,6-Dinitrotoluene	9.85	165	19908	8.574 ng	#	25
57) 2,4-Dinitrotoluene	9.85	165	19908	6.605 ng	#	19
65) 4,6-Dinitro-2-methylphenol	10.64	198	295	7.111 ng	#	1
67) 4-Bromophenyl-phenylether	10.64	248	12349	4.557 ng	#	1
77) Benzidine	12.92	184	13244	2.434 ng	#	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091819\
Data File : BF117140.D
Acq On : 18 Sep 2019 11:34
Operator : HP/JU
Sample : PB123161BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Sep 19 05:11:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 13 16:23:17 2019
Response via : Initial Calibration

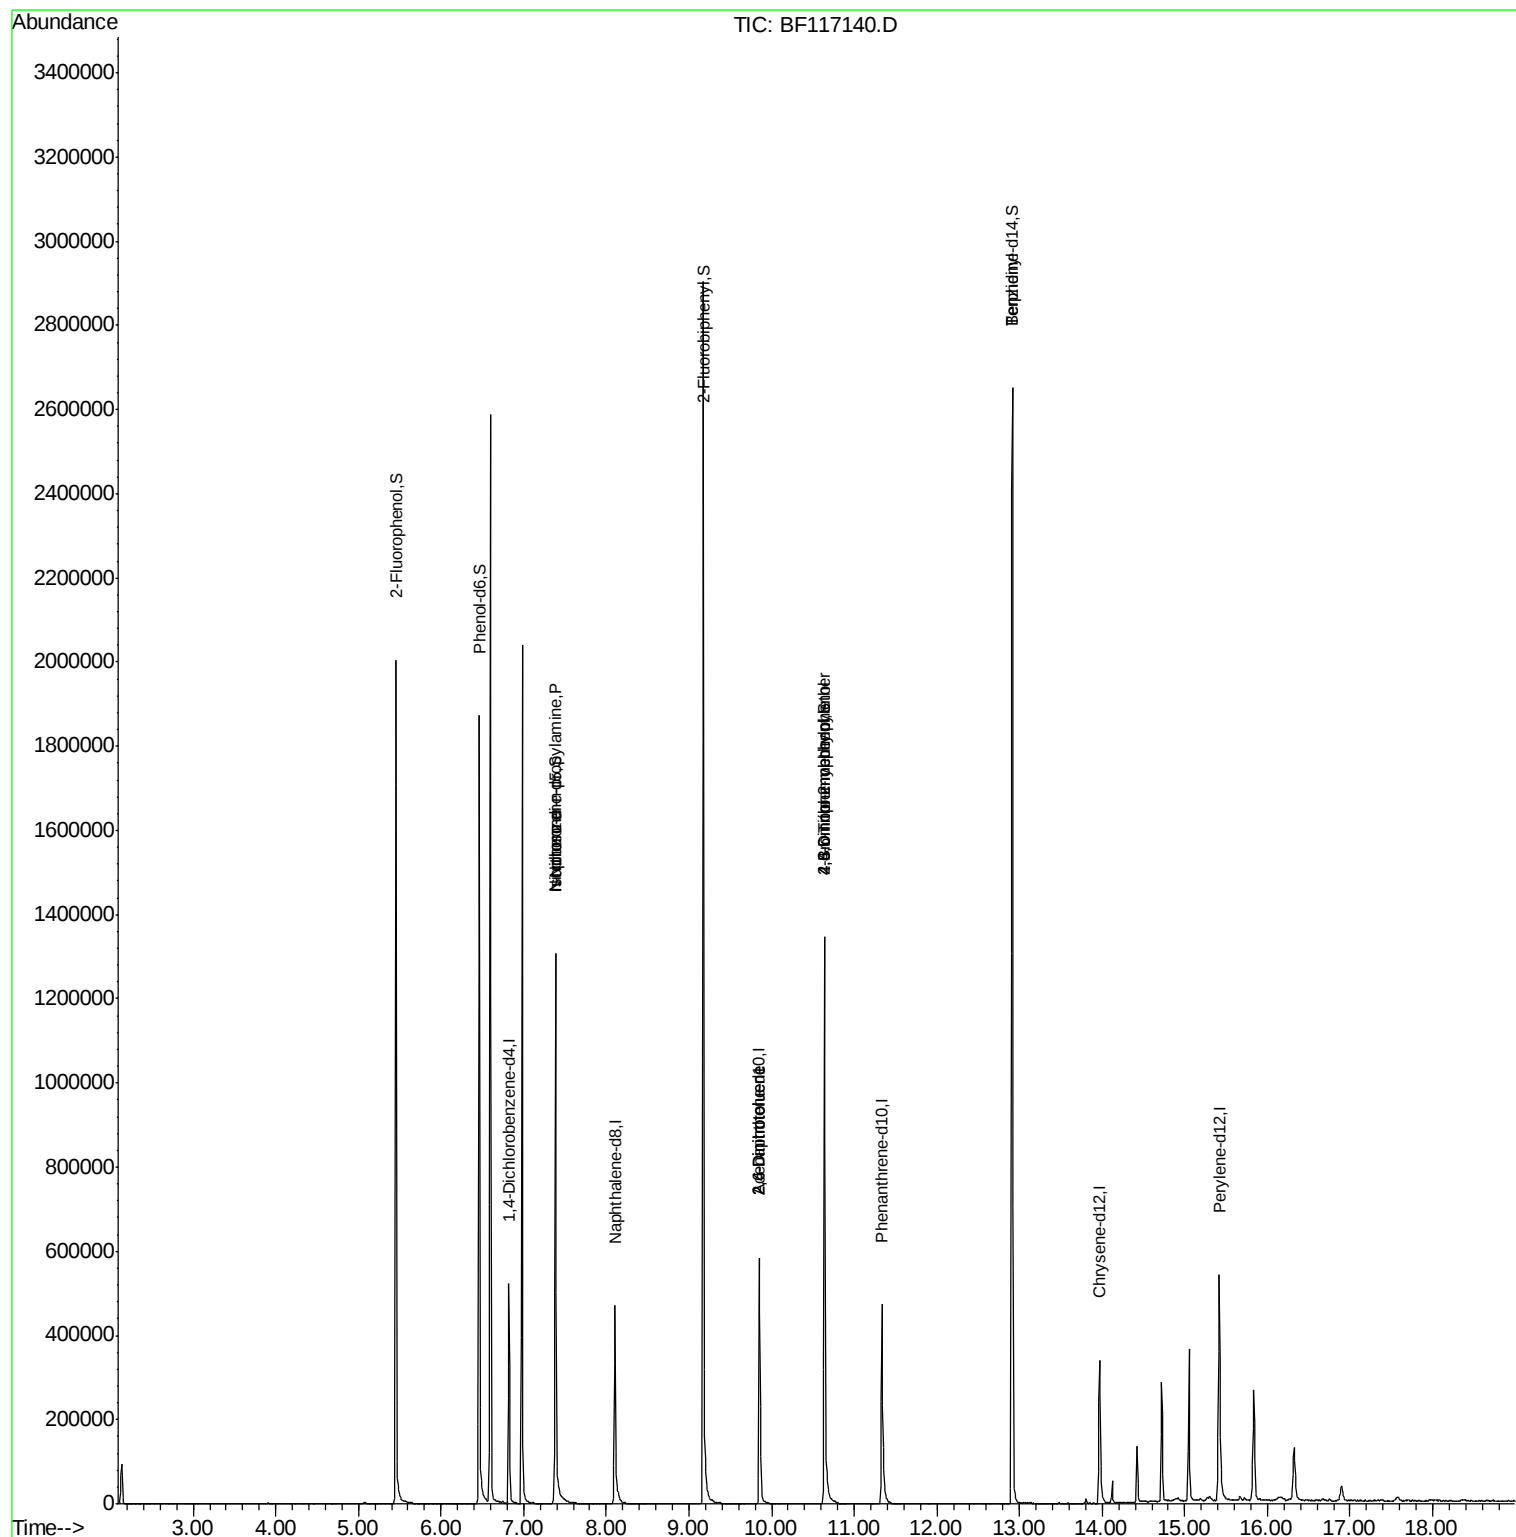




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.82 min Scan# 805
Delta R.T. -0.00 min
Lab File: BF117140.D
Acq: 18 Sep 2019 11:34

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 77806
Ion Ratio Lower Upper
152 100
150 158.0 127.5 191.3
115 64.3 55.0 82.4

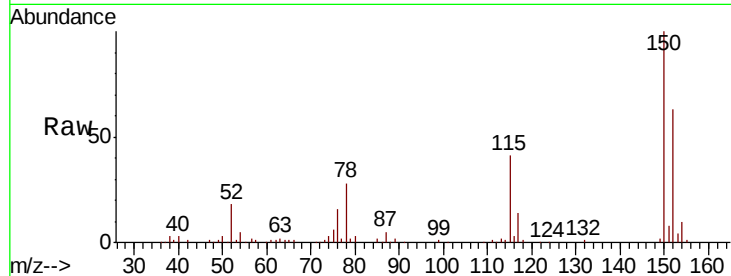


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

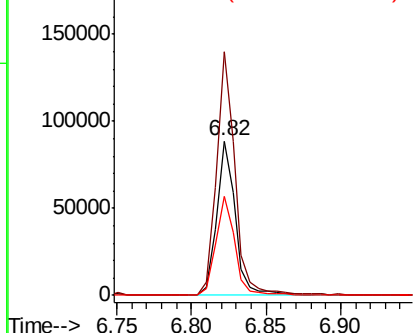



#5


2-Fluorophenol
Concen: 123.935 ng
RT: 5.46 min Scan# 573
Delta R.T. 0.02 min
Lab File: BF117140.D
Acq: 18 Sep 2019 11:34

Tgt Ion:112 Resp: 617641
Ion Ratio Lower Upper
112 100
64 57.1 45.7 68.5
63 30.7 24.9 37.3



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

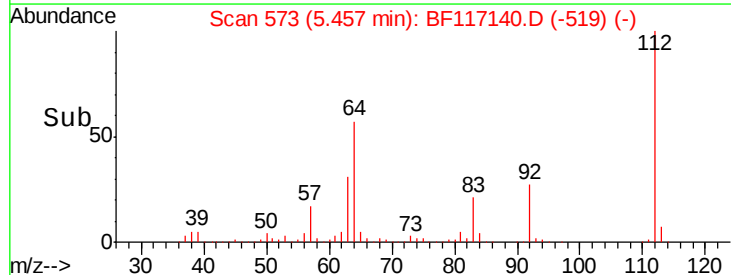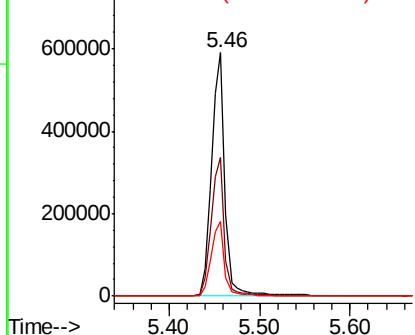

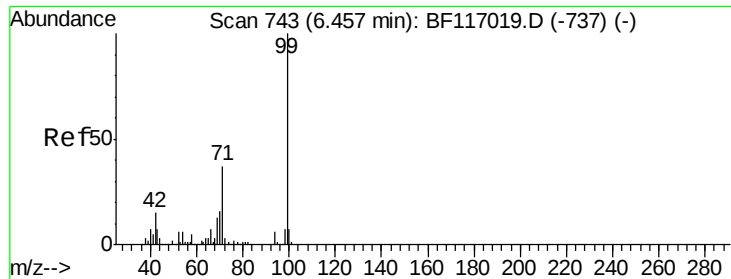

#7

Phenol-d6

Concen: 132.963 ng

RT: 6.46 min Scan# 744

Delta R.T. 0.01 min

Lab File: BF117140.D

Acq: 18 Sep 2019 11:34

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 856356

Ion Ratio Lower Upper

99 100

42 16.1 12.2 18.2




71 38.2 29.8 44.8



Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

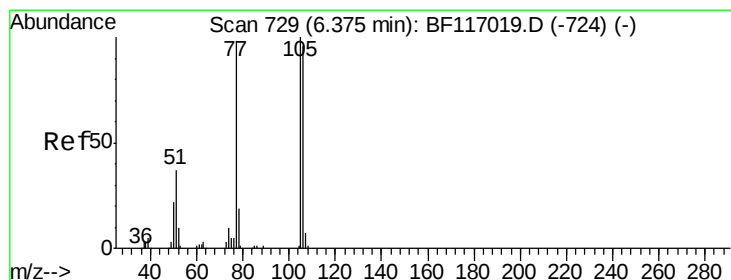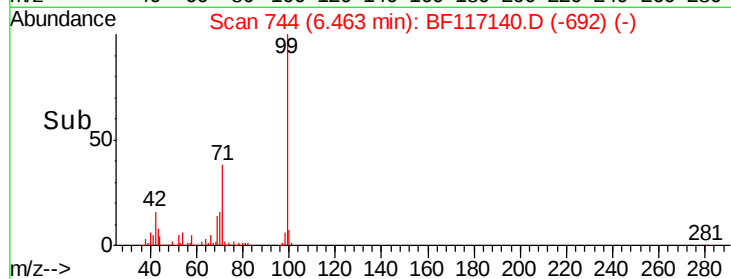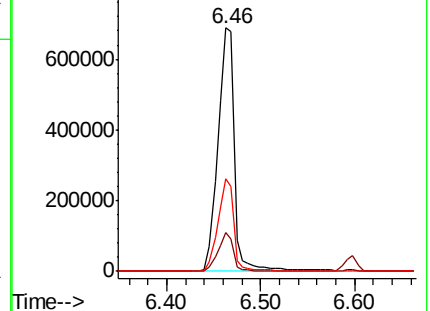

#9

Benzaldehyde

Concen: Below Cal

RT: 6.46 min Scan# 744

Delta R.T. 0.09 min

Lab File: BF117140.D

Acq: 18 Sep 2019 11:34


Tgt Ion: 77 Resp: 1176

Ion Ratio Lower Upper

77 100

105 0.0 81.8 121.8#



106 0.0 77.3 117.3#



Abundance Ion 77.00 (76.70 to 77.70): BF1

Ion 105.00 (104.70 to 105.70): E

Ion 106.00 (105.70 to 106.70): E

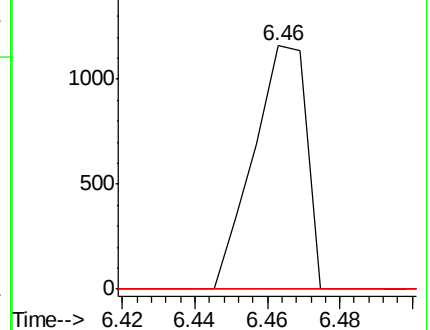



#19

n-Nitroso-di-n-propylamine

Concen: 18.380 ng

RT: 7.39 min Scan# 901

Delta R.T. 0.15 min

Lab File: BF117140.D

Acq: 18 Sep 2019 11:34

Instrument :



BNA_F

ClientSampleId :

Tot Ion: 70 Resp: 72085

Ion Ratio Lower Upper

70	100		
42	36.4	34.0	51.0
101	0.0	7.8	11.6#
130	1.8	17.8	26.8#

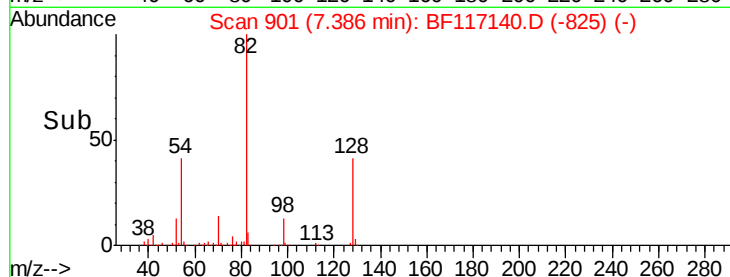
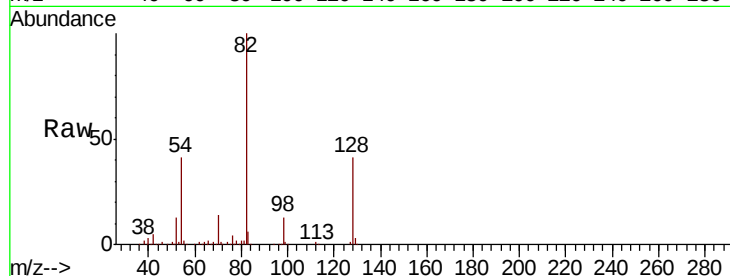


Abundance Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1

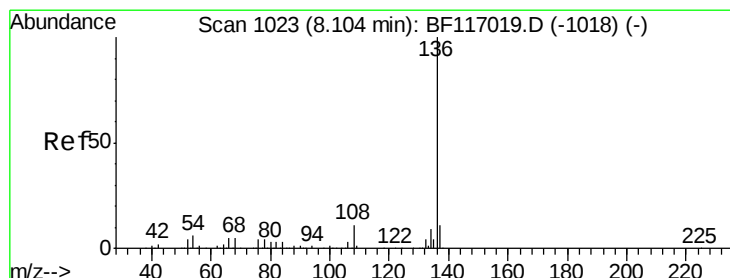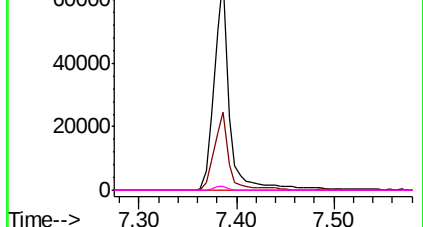

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.10 min Scan# 1023

Delta R.T. -0.00 min



Lab File: BF117140.D

Acq: 18 Sep 2019 11:34

Tgt Ion: 136 Resp: 310128

Ion Ratio Lower Upper

136	100		
137	10.4	9.0	13.4
54	5.5	4.5	6.7
68	4.6	4.0	6.0

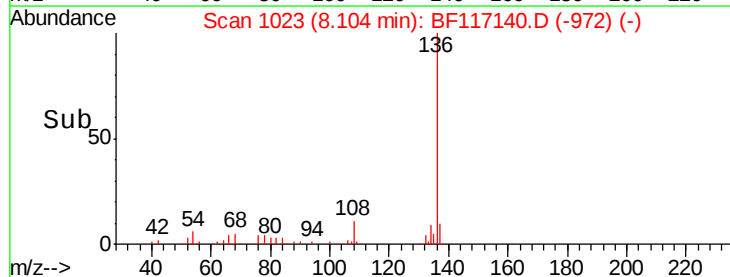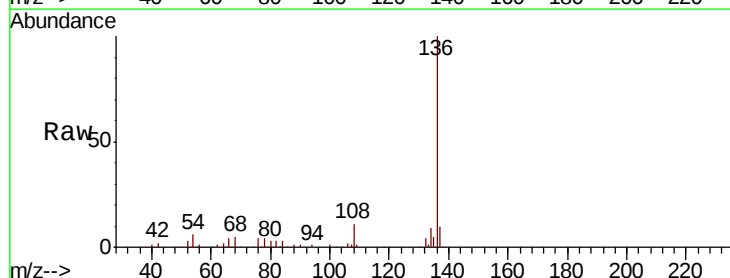


Abundance Ion 136.00 (135.70 to 136.70): BF1

Ion 137.00 (136.70 to 137.70): BF1

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1




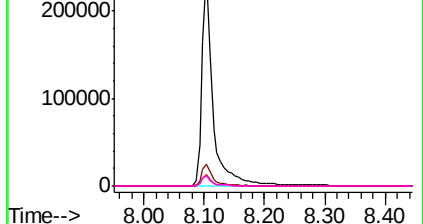




#23
 Nitrobenzene-d5
 Concen: 92.048 ng
 RT: 7.39 min Scan# 901
 Delta R.T. -0.00 min
 Lab File: BF117140.D
 Acq: 18 Sep 2019 11:34




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion	82	Resp	543307
Ion Ratio	Lower	Upper	
82	100		
128	41.1	32.3	48.5
54	40.6	33.3	49.9

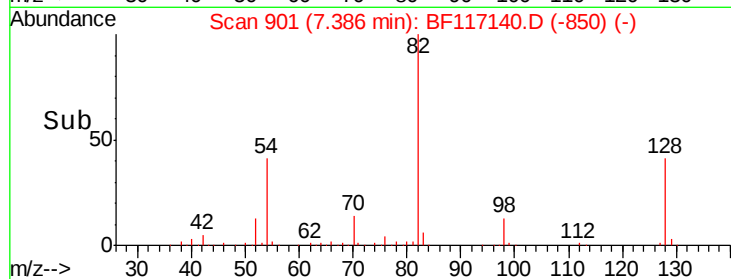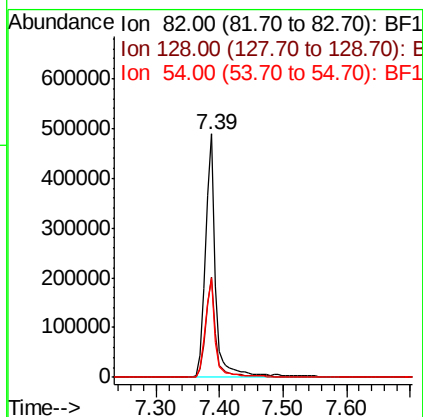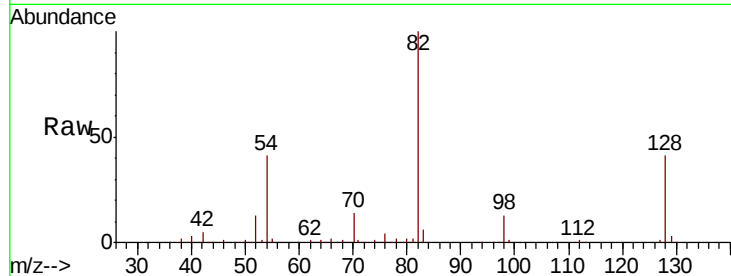

#25
 Isophorone
 Concen: 51.987 ng
 RT: 7.39 min Scan# 901
 Delta R.T. -0.26 min
 Lab File: BF117140.D
 Acq: 18 Sep 2019 11:34

Tgt Ion	82	Resp	543304
Ion Ratio	Lower	Upper	
82	100		
95	0.0	5.8	8.6#
138	0.0	13.5	20.3#

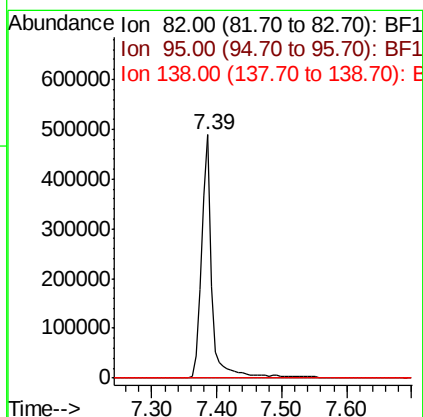

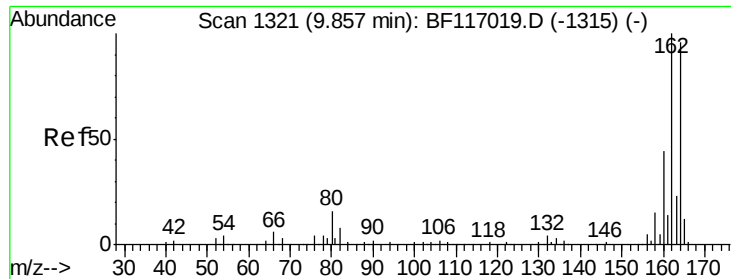

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.85 min Scan# 1320

Delta R.T. -0.01 min

Lab File: BF117140.D

Acq: 18 Sep 2019 11:34

Instrument :

BNA_F

ClientSampleId :


Tot Ion:164 Resp: 161010

Ion Ratio Lower Upper

164 100

162 104.7 83.4 125.2




160 45.7 36.4 54.6



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

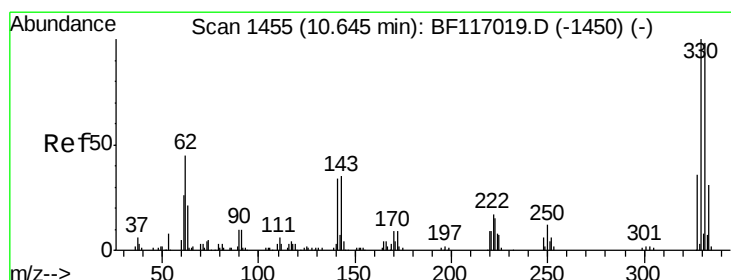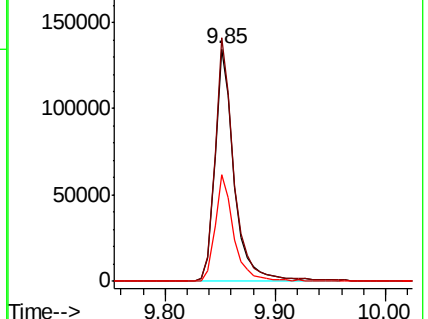

#42

2,4,6-Tribromophenol

Concen: 138.827 ng

RT: 10.64 min Scan# 1454

Delta R.T. -0.01 min

Lab File: BF117140.D

Acq: 18 Sep 2019 11:34


Tgt Ion:330 Resp: 186816

Ion Ratio Lower Upper

330 100

332 96.3 78.0 117.0



141 43.3 35.8 53.6



Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



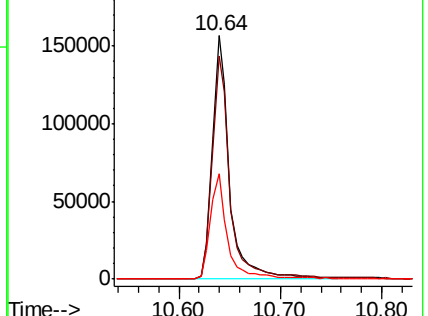





#45
 2-Fluorobiphenyl
 Concen: 94.285 ng
 RT: 9.17 min Scan# 1205
 Delta R.T. -0.00 min
 Lab File: BF117140.D
 Acq: 18 Sep 2019 11:34




Instrument :
 BNA_F
 ClientSampled :

Tot Ion	Ratio	Lower	Upper
172	100		
171	35.0	28.2	42.2
170	23.5	18.9	28.3

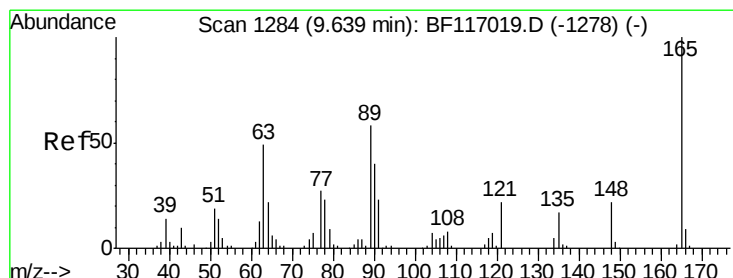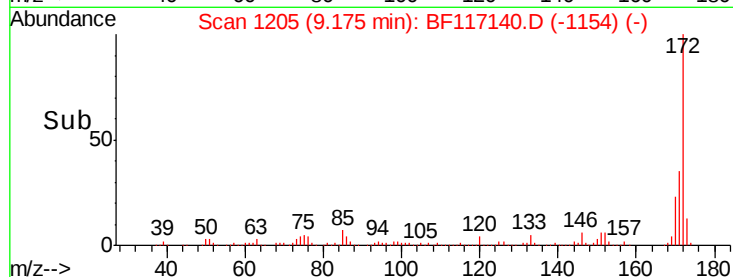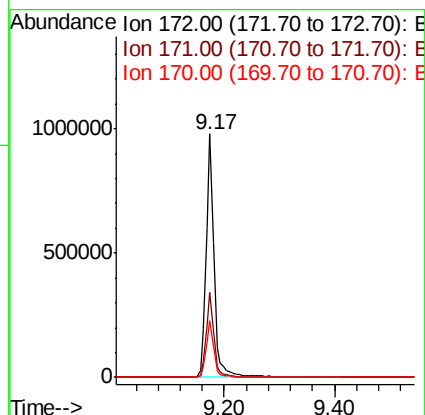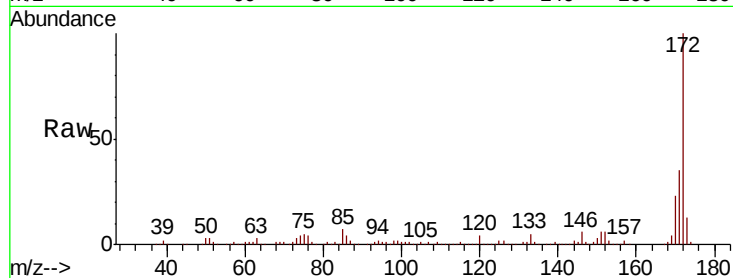

#51
 2,6-Dinitrotoluene
 Concen: 8.574 ng
 RT: 9.85 min Scan# 1320
 Delta R.T. 0.21 min
 Lab File: BF117140.D
 Acq: 18 Sep 2019 11:34

Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	41.8	62.8#
89	2.0	46.5	69.7#


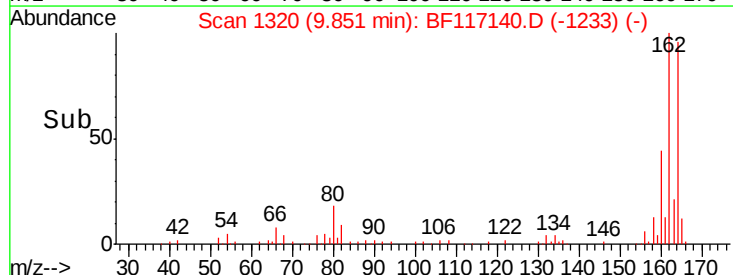
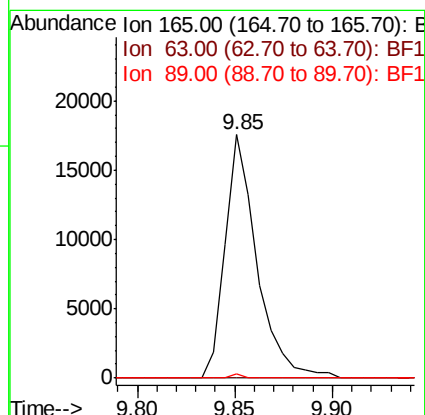
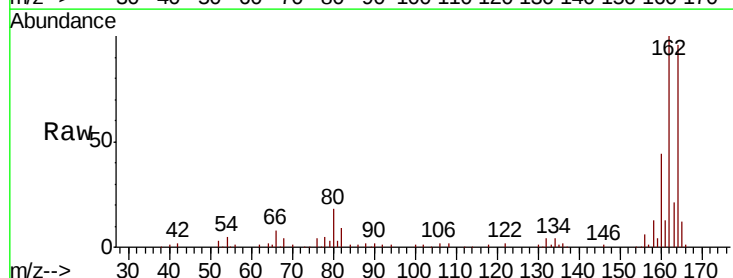




#57
 2,4-Dinitrotoluene
 Concen: 6.605 ng
 RT: 9.85 min Scan# 1320
 Delta R.T. -0.19 min
 Lab File: BF117140.D
 Acq: 18 Sep 2019 11:34




Instrument :
 BNA_F
 ClientSampled :


Tot Ion:165 Resp: 19908
 Ion Ratio Lower Upper
 165 100
 63 0.0 35.0 52.4#
 89 2.0 66.1 99.1#
 182 0.0 2.0 3.0#

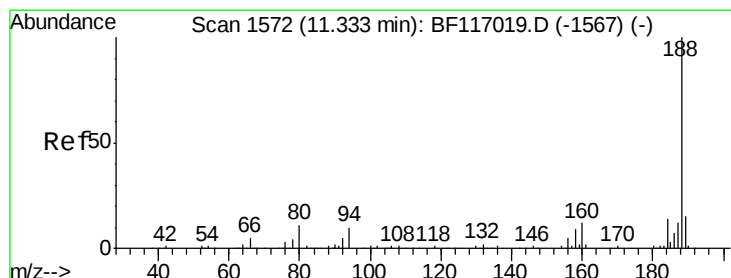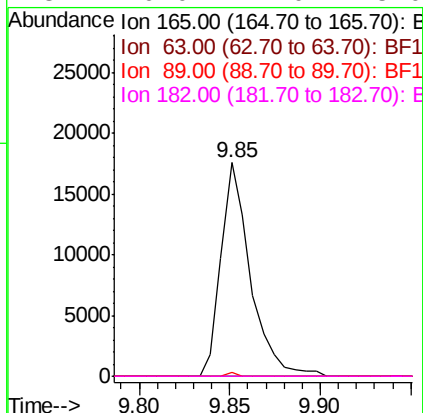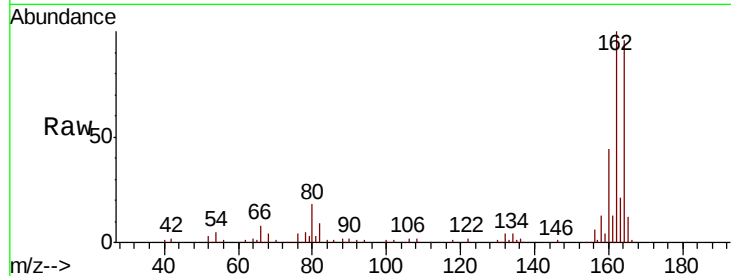

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.33 min Scan# 1572
 Delta R.T. -0.00 min
 Lab File: BF117140.D
 Acq: 18 Sep 2019 11:34

Tgt Ion:188 Resp: 265348
 Ion Ratio Lower Upper
 188 100
 94 9.8 8.2 12.2
 80 10.5 9.0 13.6

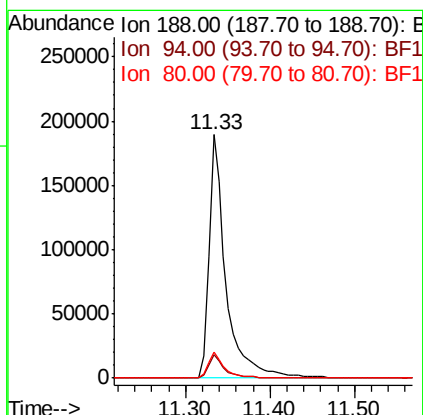


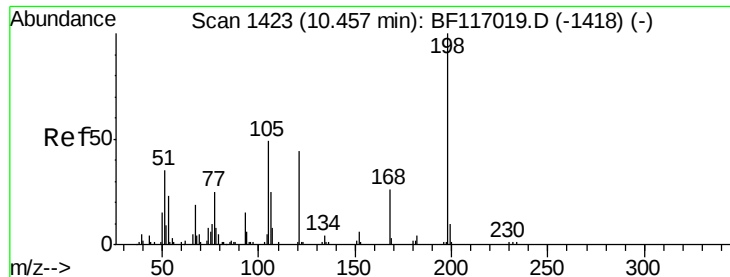




#65
 4,6-Dinitro-2-methylphenol
 Concen: 7.111 ng
 RT: 10.64 min Scan# 1454
 Delta R.T. 0.18 min
 Lab File: BF117140.D
 Acq: 18 Sep 2019 11:34

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:198 Resp: 295
 Ion Ratio Lower Upper
 198 100
 51 146.8 18.7 58.7#
 105 189.3 30.2 70.2#

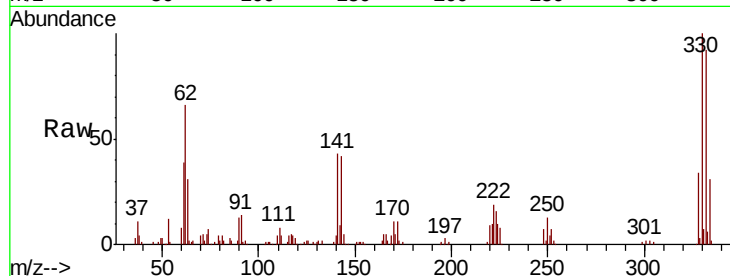


Abundance Ion 198.00 (197.70 to 198.70): E
 Ion 51.00 (50.70 to 51.70): BF1
 Ion 105.00 (104.70 to 105.70): E

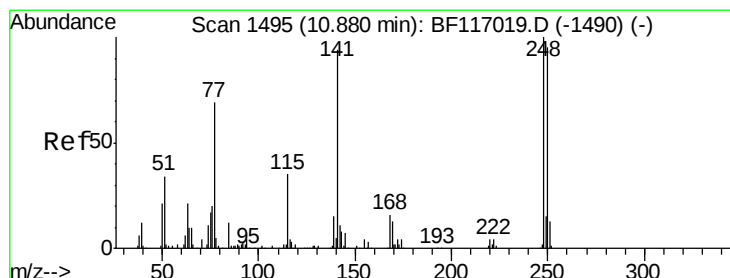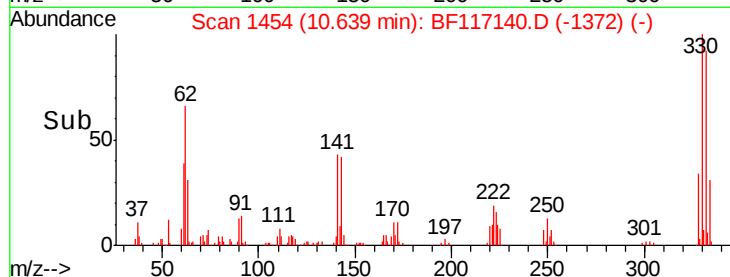
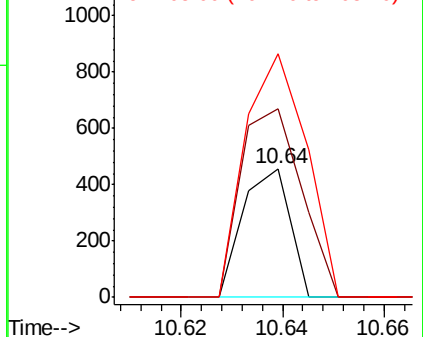



#67
 4-Bromophenyl-phenylether
 Concen: 4.557 ng
 RT: 10.64 min Scan# 1454
 Delta R.T. -0.24 min
 Lab File: BF117140.D
 Acq: 18 Sep 2019 11:34

Tgt Ion:248 Resp: 12349
 Ion Ratio Lower Upper
 248 100
 250 197.6 76.2 114.4#
 141 640.6 75.0 112.4#

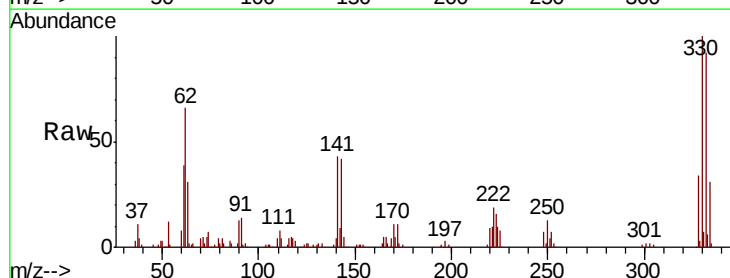

Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E



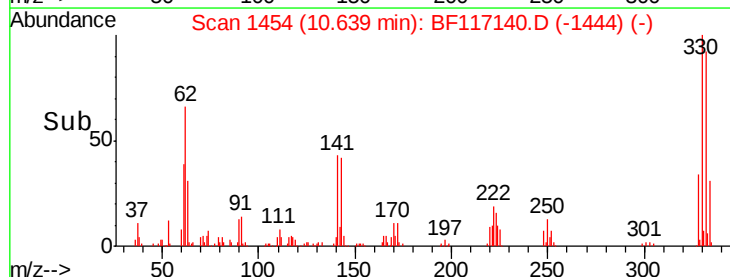
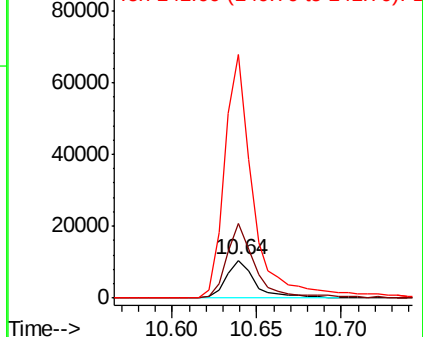


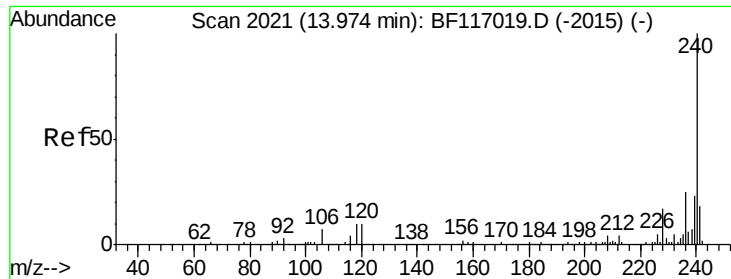

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.97 min Scan# 2020
Delta R.T. -0.01 min
Lab File: BF117140.D
Acq: 18 Sep 2019 11:34




Instrument :
BNA_F
ClientSampleId :


Tot Ion:240 Resp: 168898
Ion Ratio Lower Upper
240 100
120 10.5 8.3 12.5
236 25.2 20.3 30.5

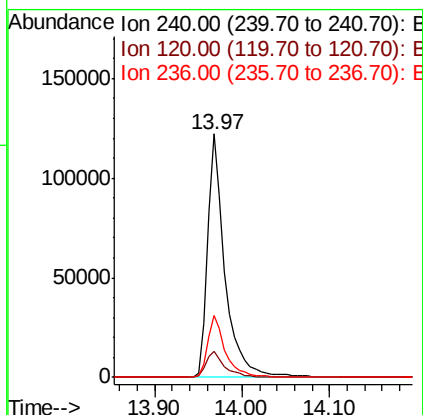

#77
Benzidine
Concen: 2.434 ng
RT: 12.92 min Scan# 1841
Delta R.T. 0.25 min
Lab File: BF117140.D
Acq: 18 Sep 2019 11:34

Tgt Ion:184 Resp: 13244
Ion Ratio Lower Upper
184 100
185 18.6 11.6 17.4#
183 10.6 9.0 13.4


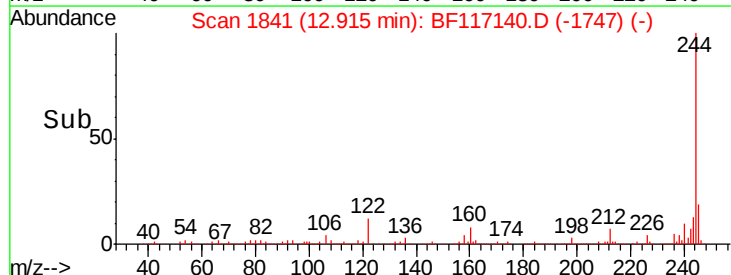
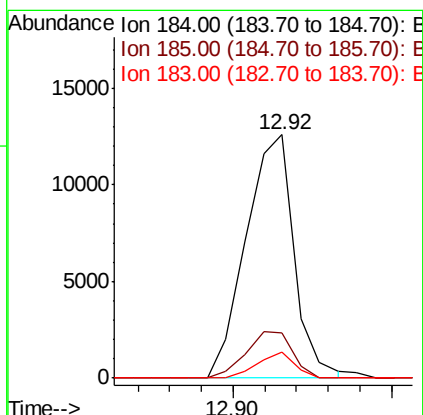



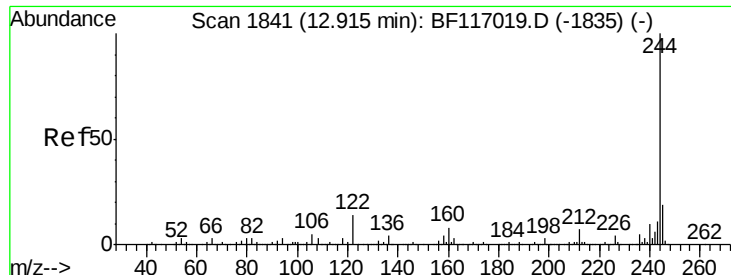

#79
 Terphenyl-d14
 Concen: 107.926 ng
 RT: 12.92 min Scan# 1841
 Delta R.T. -0.00 min
 Lab File: BF117140.D
 Acq: 18 Sep 2019 11:34

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:244 Resp: 975195
 Ion Ratio Lower Upper
 244 100
 212 7.1 5.8 8.8
 122 12.5 11.3 16.9

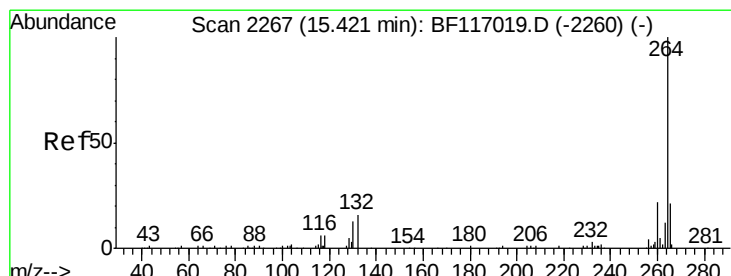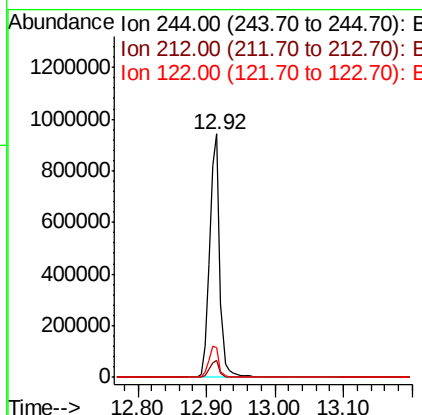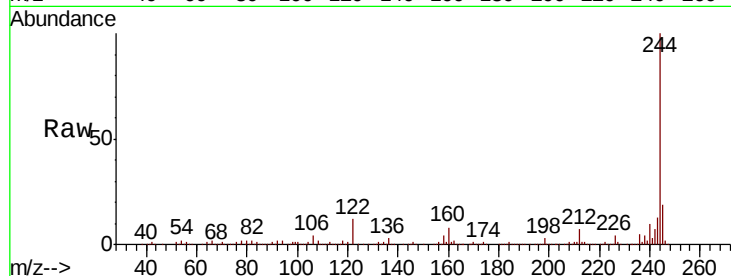

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.42 min Scan# 2266
 Delta R.T. -0.01 min
 Lab File: BF117140.D
 Acq: 18 Sep 2019 11:34

Tgt Ion:264 Resp: 133876
 Ion Ratio Lower Upper
 264 100
 260 23.6 17.6 26.4
 265 20.9 16.6 24.8

