


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091819\
 Data File : BF117135.D
 Acq On : 18 Sep 2019 8:51
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 13 16:23:17 2019

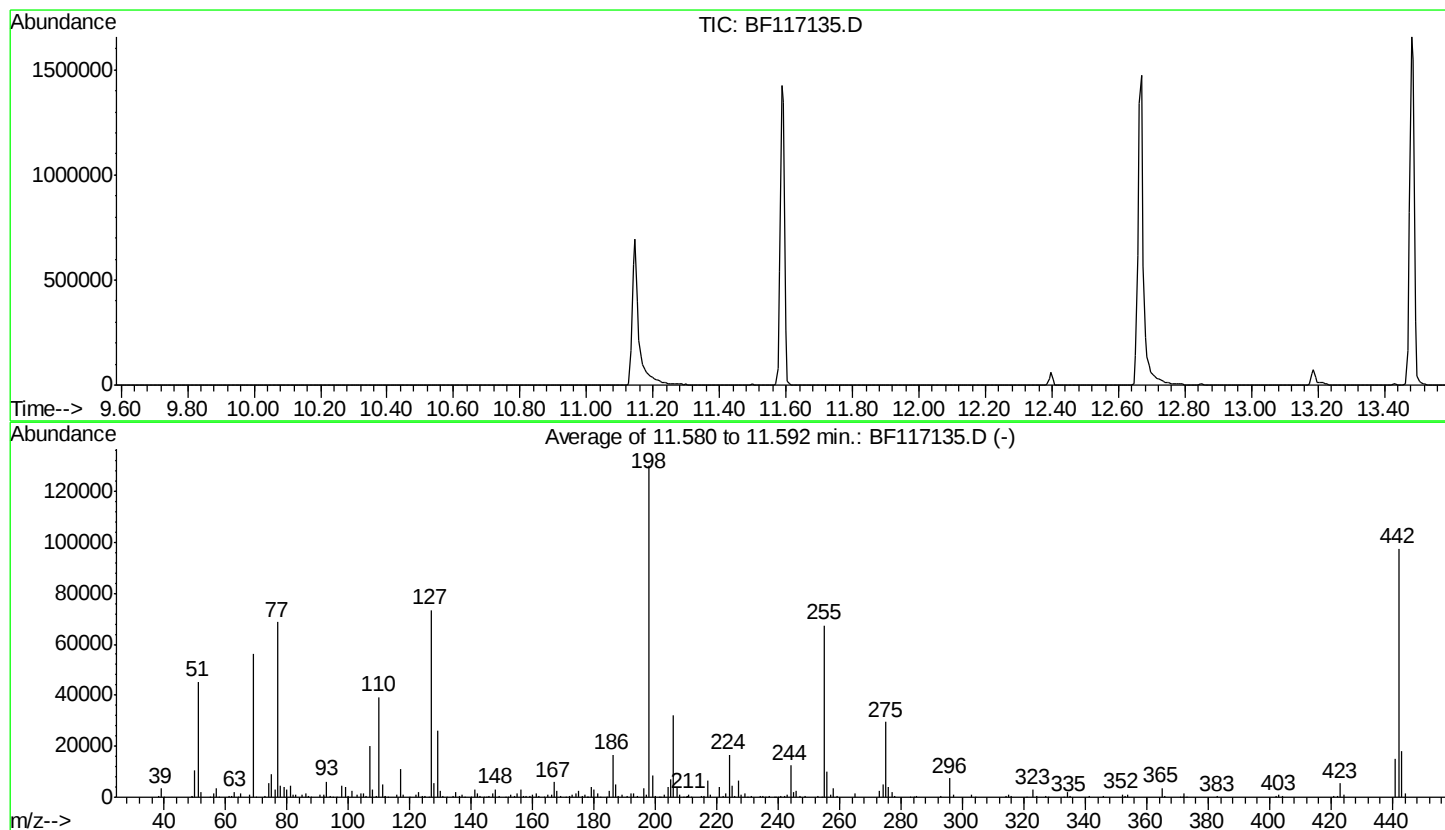

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	45250	PASS
68	69	0.00	2	1.6	880	PASS
69	198	0.00	100	43.1	56050	PASS
70	69	0.00	2	0.2	119	PASS
127	198	10	80	56.5	73480	PASS
197	198	0.00	2	0.8	1001	PASS
198	198	100	100	100.0	130050	PASS
199	198	5	9	6.7	8726	PASS
275	198	10	60	22.7	29560	PASS
365	198	1	100	2.8	3650	PASS
441	198	0.01	100	11.7	15240	PASS
442	198	50	100	75.1	97648	PASS
443	442	15	24	18.7	18295	PASS