


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091819\
 Data File : BF117148.D
 Acq On : 18 Sep 2019 16:49
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 13 16:23:17 2019

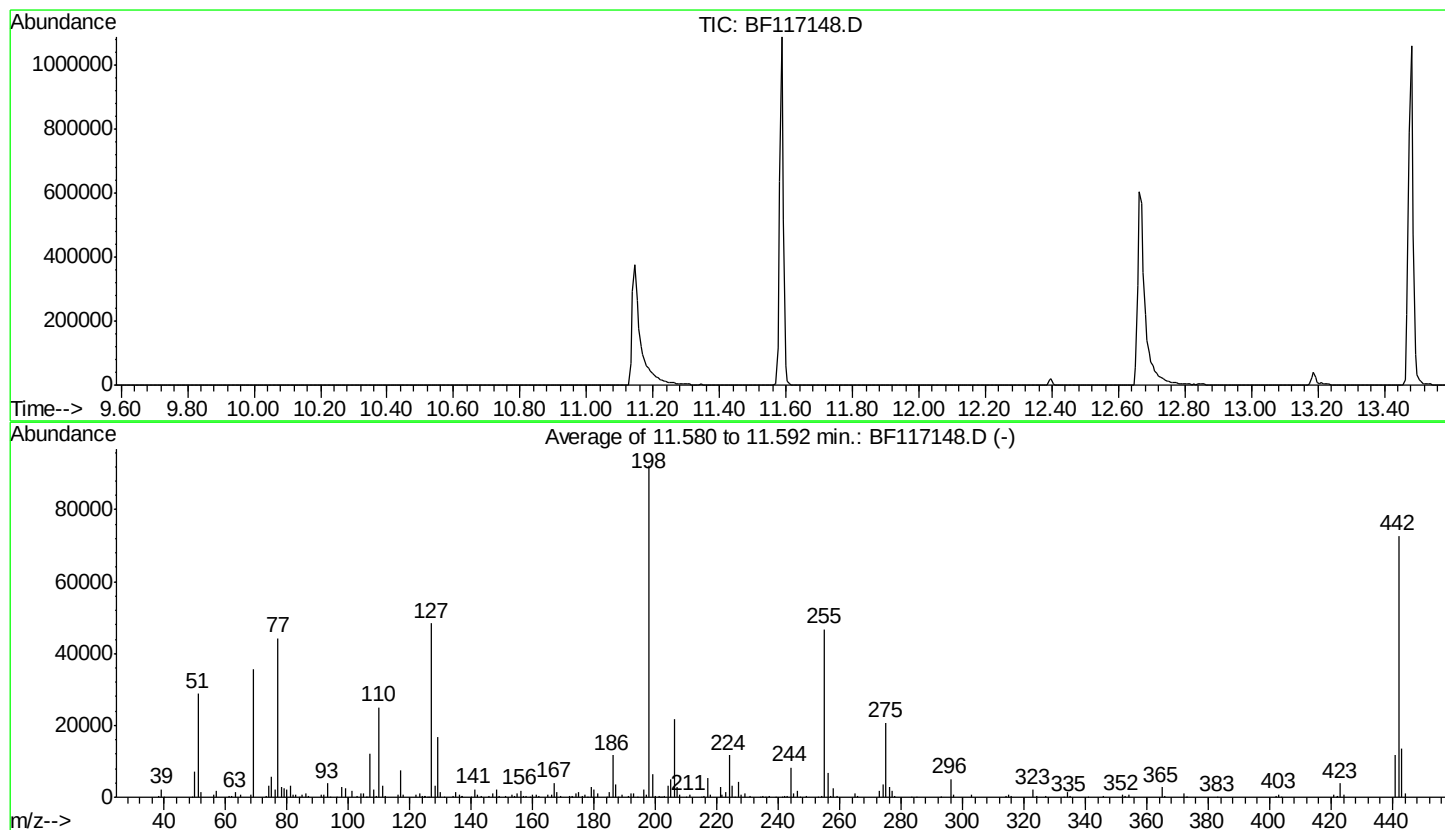

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.1	28707	PASS
68	69	0.00	2	1.8	631	PASS
69	198	0.00	100	38.8	35817	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.5	48445	PASS
197	198	0.00	2	0.7	678	PASS
198	198	100	100	100.0	92298	PASS
199	198	5	9	6.8	6319	PASS
275	198	10	60	22.6	20840	PASS
365	198	1	100	3.0	2744	PASS
441	198	0.01	100	12.6	11634	PASS
442	198	50	100	78.9	72813	PASS
443	442	15	24	18.7	13619	PASS