
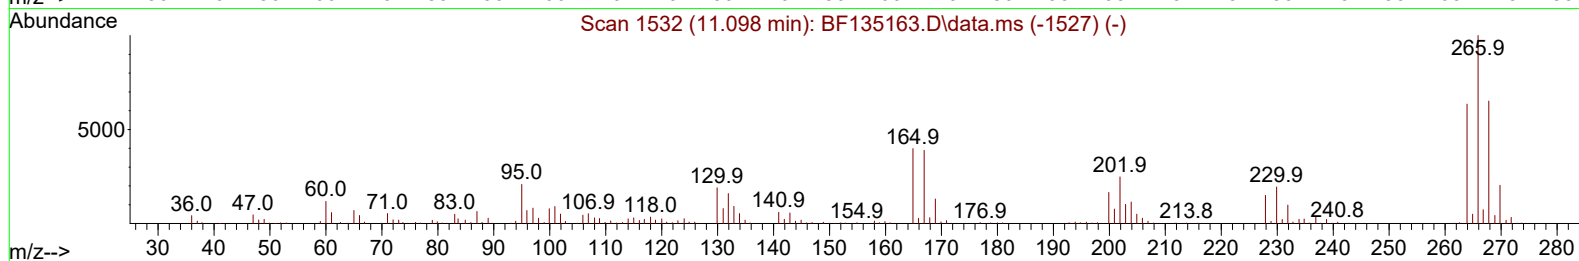
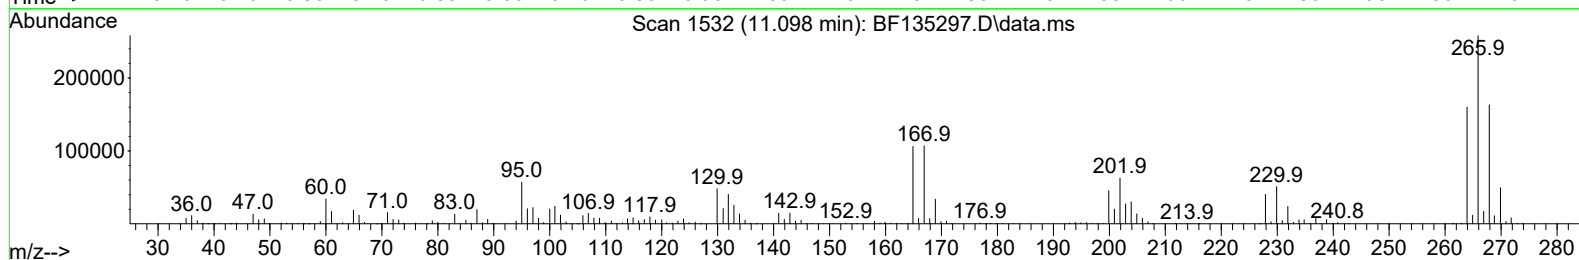


Quant Time: Sep 19 03:02:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

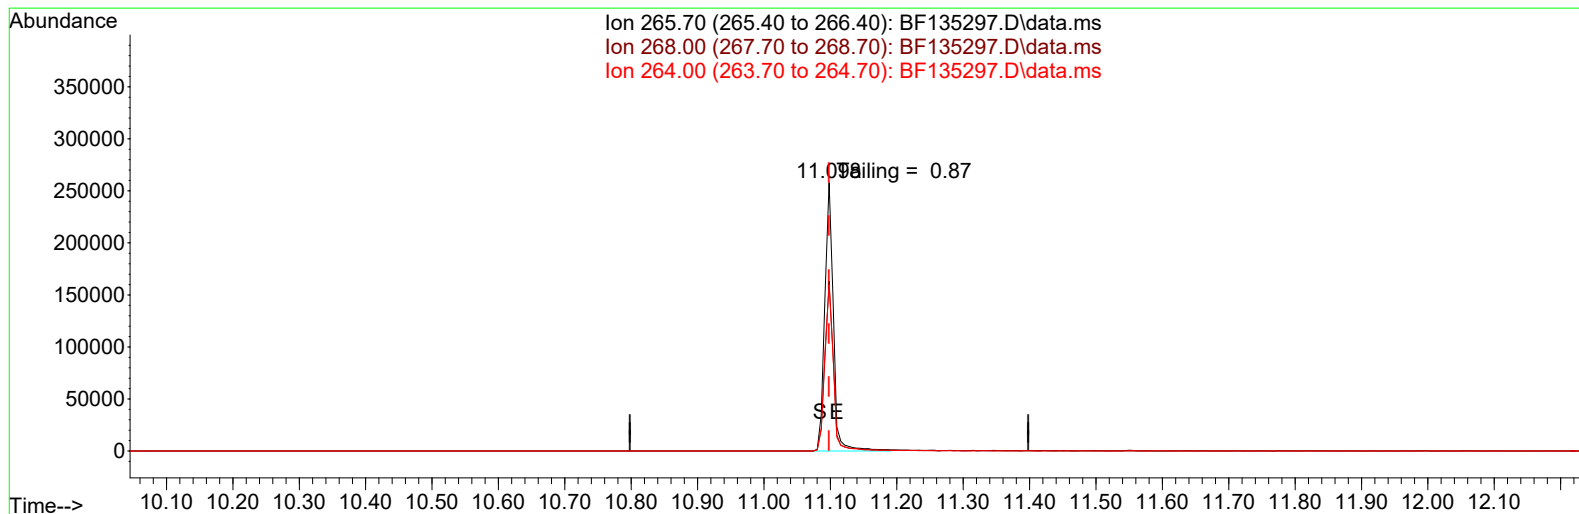

TIC: BF135297.D\data.ms

(70) Pentachlorophenol (C)




11.098min (+ 0.000) 300624.26 ng

response **235096**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	63.23
264.00	63.50	61.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091823\
Data File : BF135297.D
Acq On : 18 Sep 2023 10:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 19 03:02:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

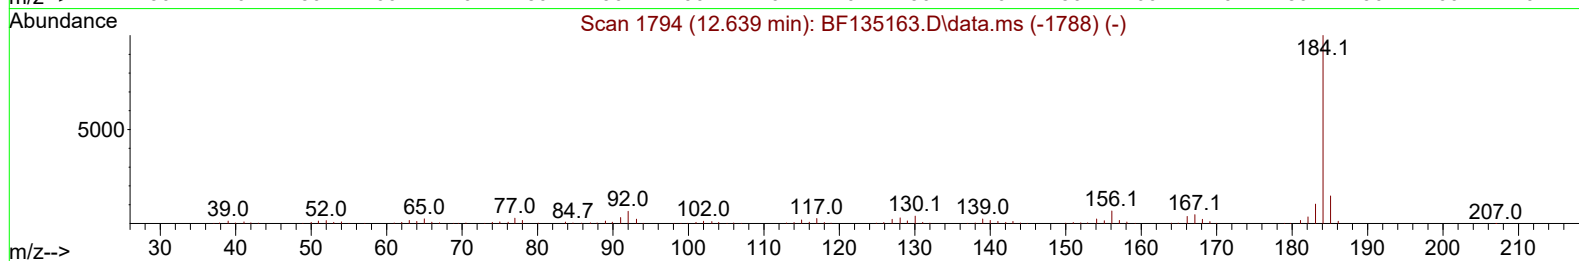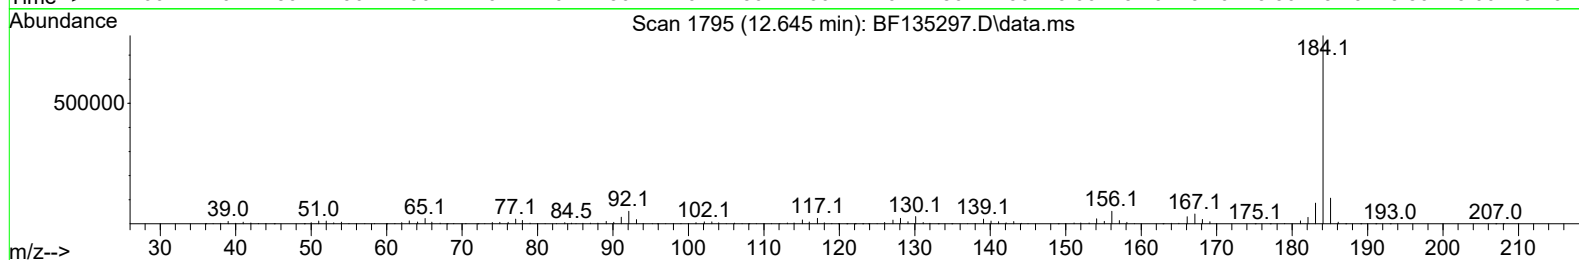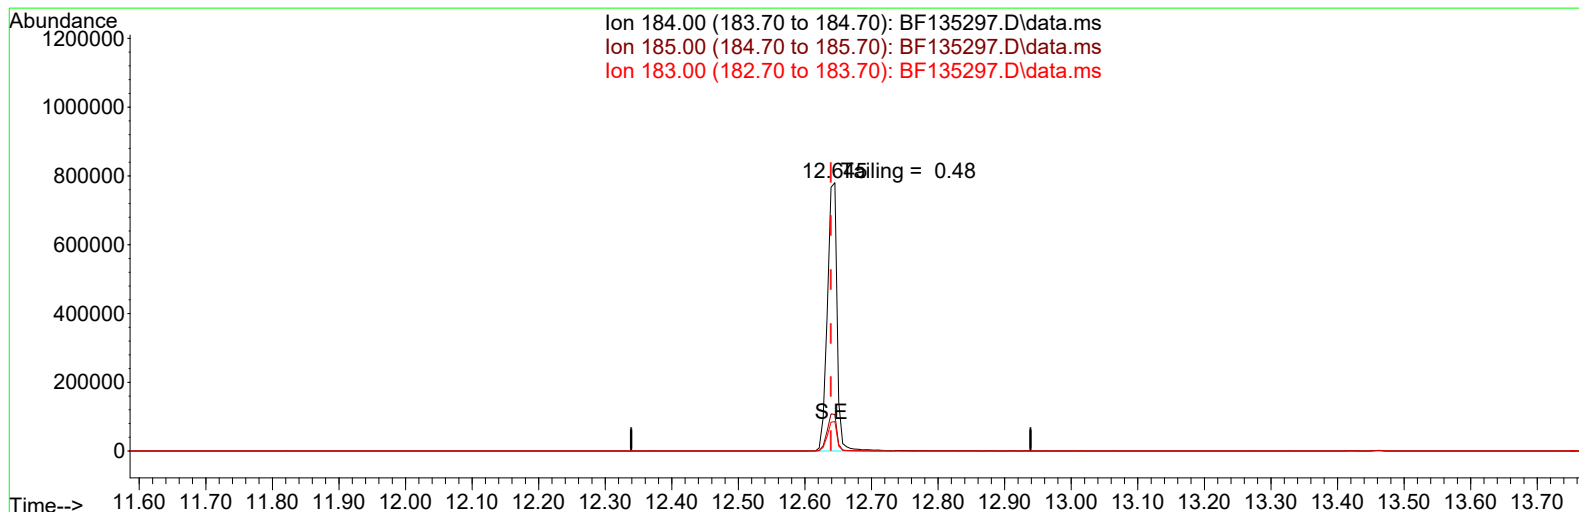

TIC: BF135297.D\data.ms

(77) Benzidine

12.645min (+ 0.006) 61581.99 ng

response 799867

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.63
183.00	10.30	11.02
0.00	0.00	0.00