
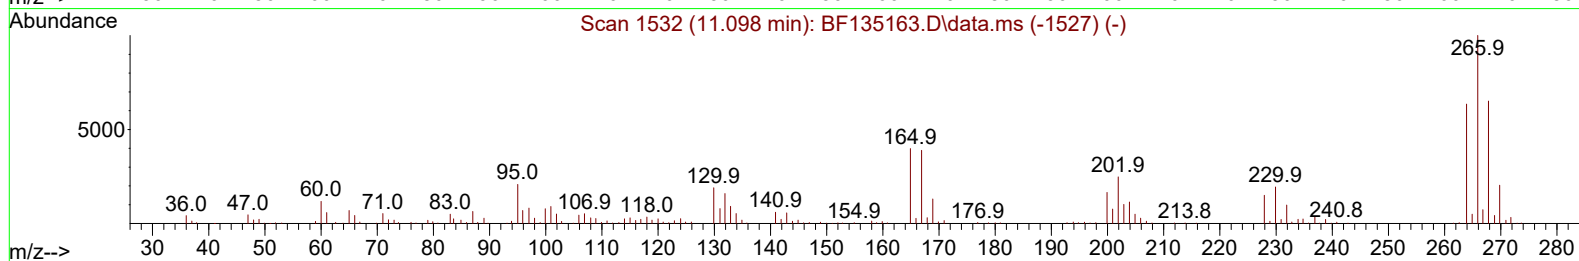
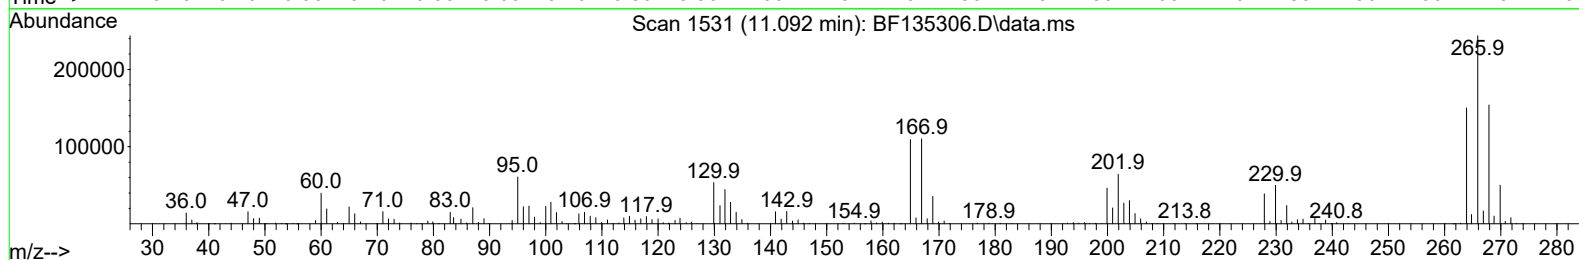


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091823\
 Data File : BF135306.D
 Acq On : 18 Sep 2023 14:55
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 19:31:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 12 00:19:07 2023
 Response via : Initial Calibration

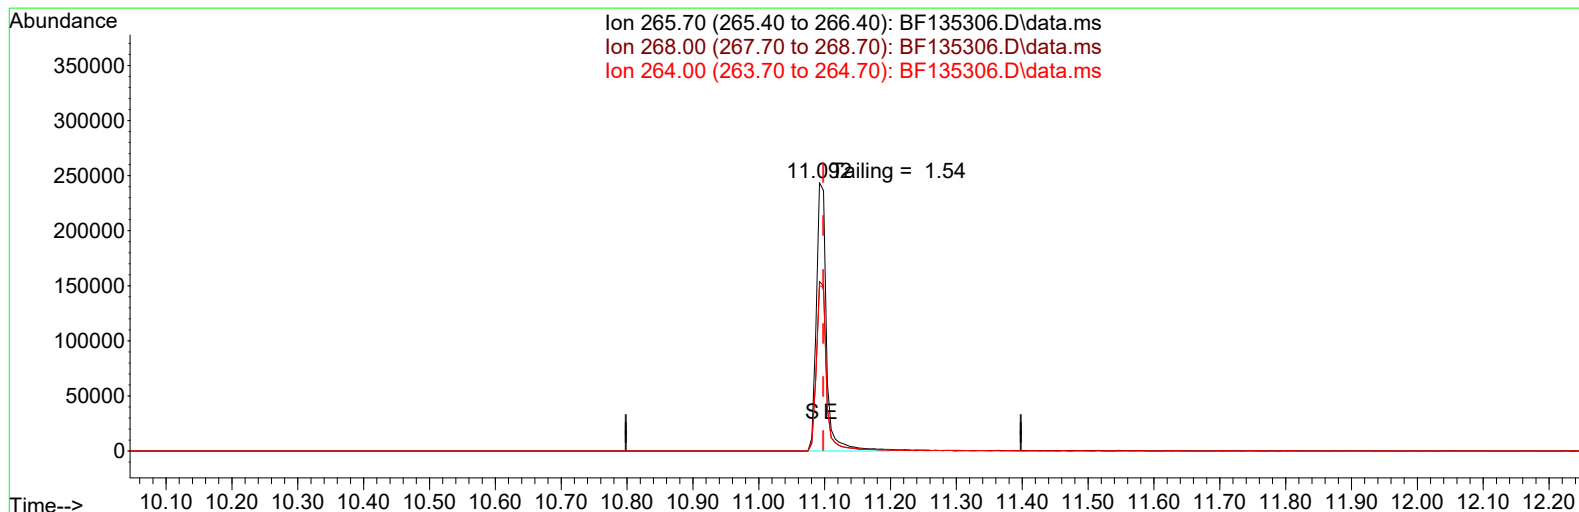

TIC: BF135306.D\data.ms

(70) Pentachlorophenol (C)




11.092min (-0.006) 236146.89 ng

response 261978

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	63.17
264.00	63.50	61.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091823\
Data File : BF135306.D
Acq On : 18 Sep 2023 14:55
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 19:31:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

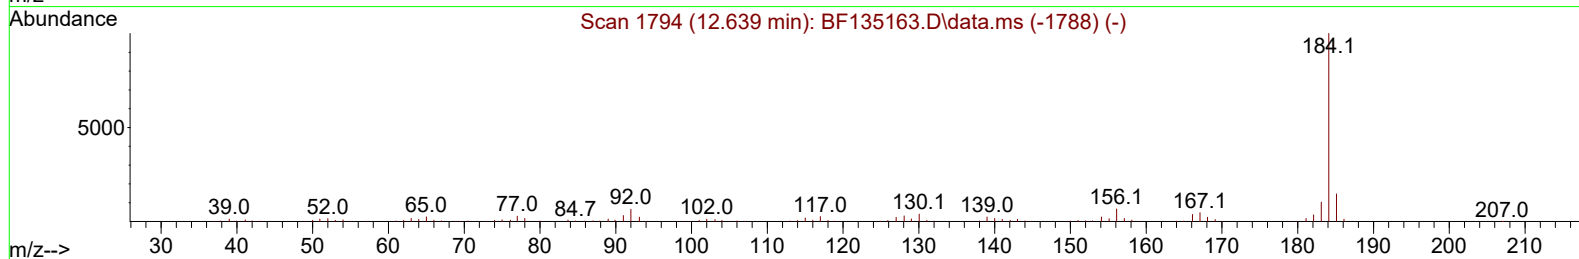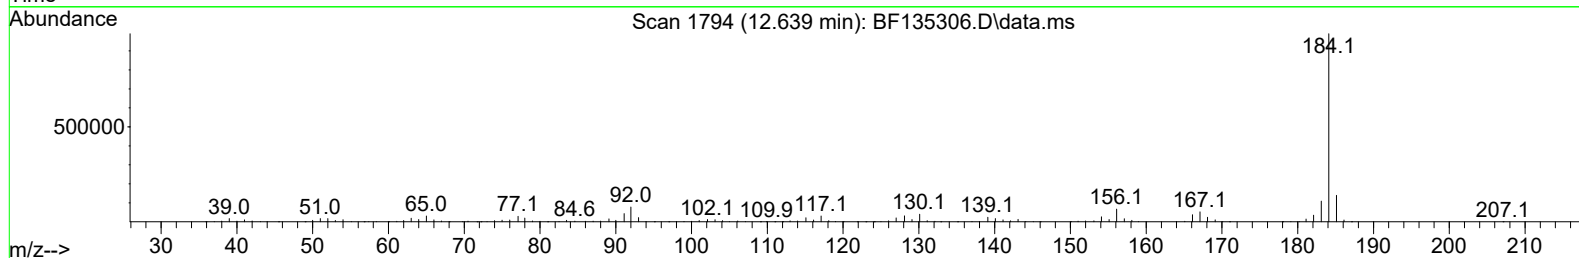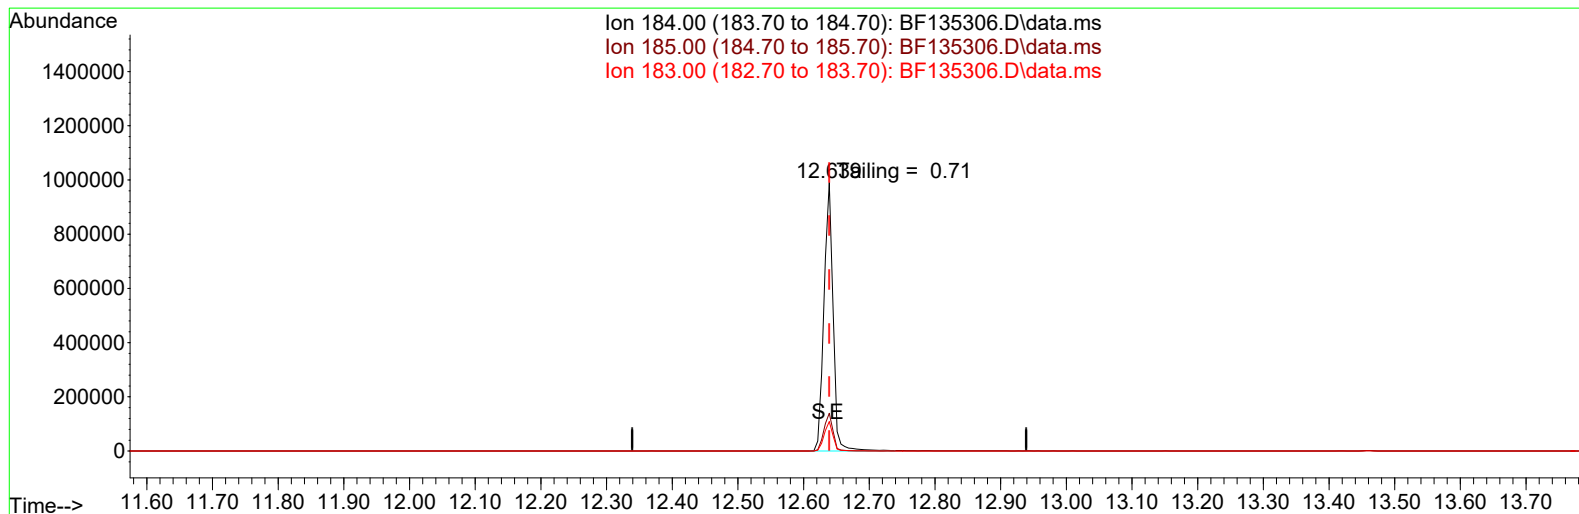

TIC: BF135306.D\data.ms

(77) Benzidine

12.639min (+ 0.000) 175132.49 ng

response 957972

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.09
183.00	10.30	11.00
0.00	0.00	0.00