

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091823\
 Data File : BF135303.D
 Acq On : 18 Sep 2023 13:20
 Operator : CG\JU
 Sample : PB155524BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB155524BL

Quant Time: Sep 18 16:12:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 12 00:19:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.757	152	96747	20.000	ng	0.00
21) Naphthalene-d8	8.034	136	370864	20.000	ng	-0.01
39) Acenaphthene-d10	9.792	164	191670	20.000	ng	-0.01
64) Phenanthrene-d10	11.286	188	377901	20.000	ng	0.00
76) Chrysene-d12	13.939	240	180506	20.000	ng	0.00
86) Perylene-d12	15.409	264	204329	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.398	112	1076990	181.056	ng	0.01
7) Phenol-d6	6.404	99	993848	131.397	ng	0.00
23) Nitrobenzene-d5	7.322	82	623726	91.372	ng	-0.01
42) 2,4,6-Tribromophenol	10.592	330	282503	148.316	ng	0.00
45) 2-Fluorobiphenyl	9.116	172	1169584	92.063	ng	-0.01
79) Terphenyl-d14	12.886	244	1220080	104.781	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091823\
Data File : BF135303.D
Acq On : 18 Sep 2023 13:20
Operator : CG\JU
Sample : PB155524BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155524BL

Quant Time: Sep 18 16:12:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration




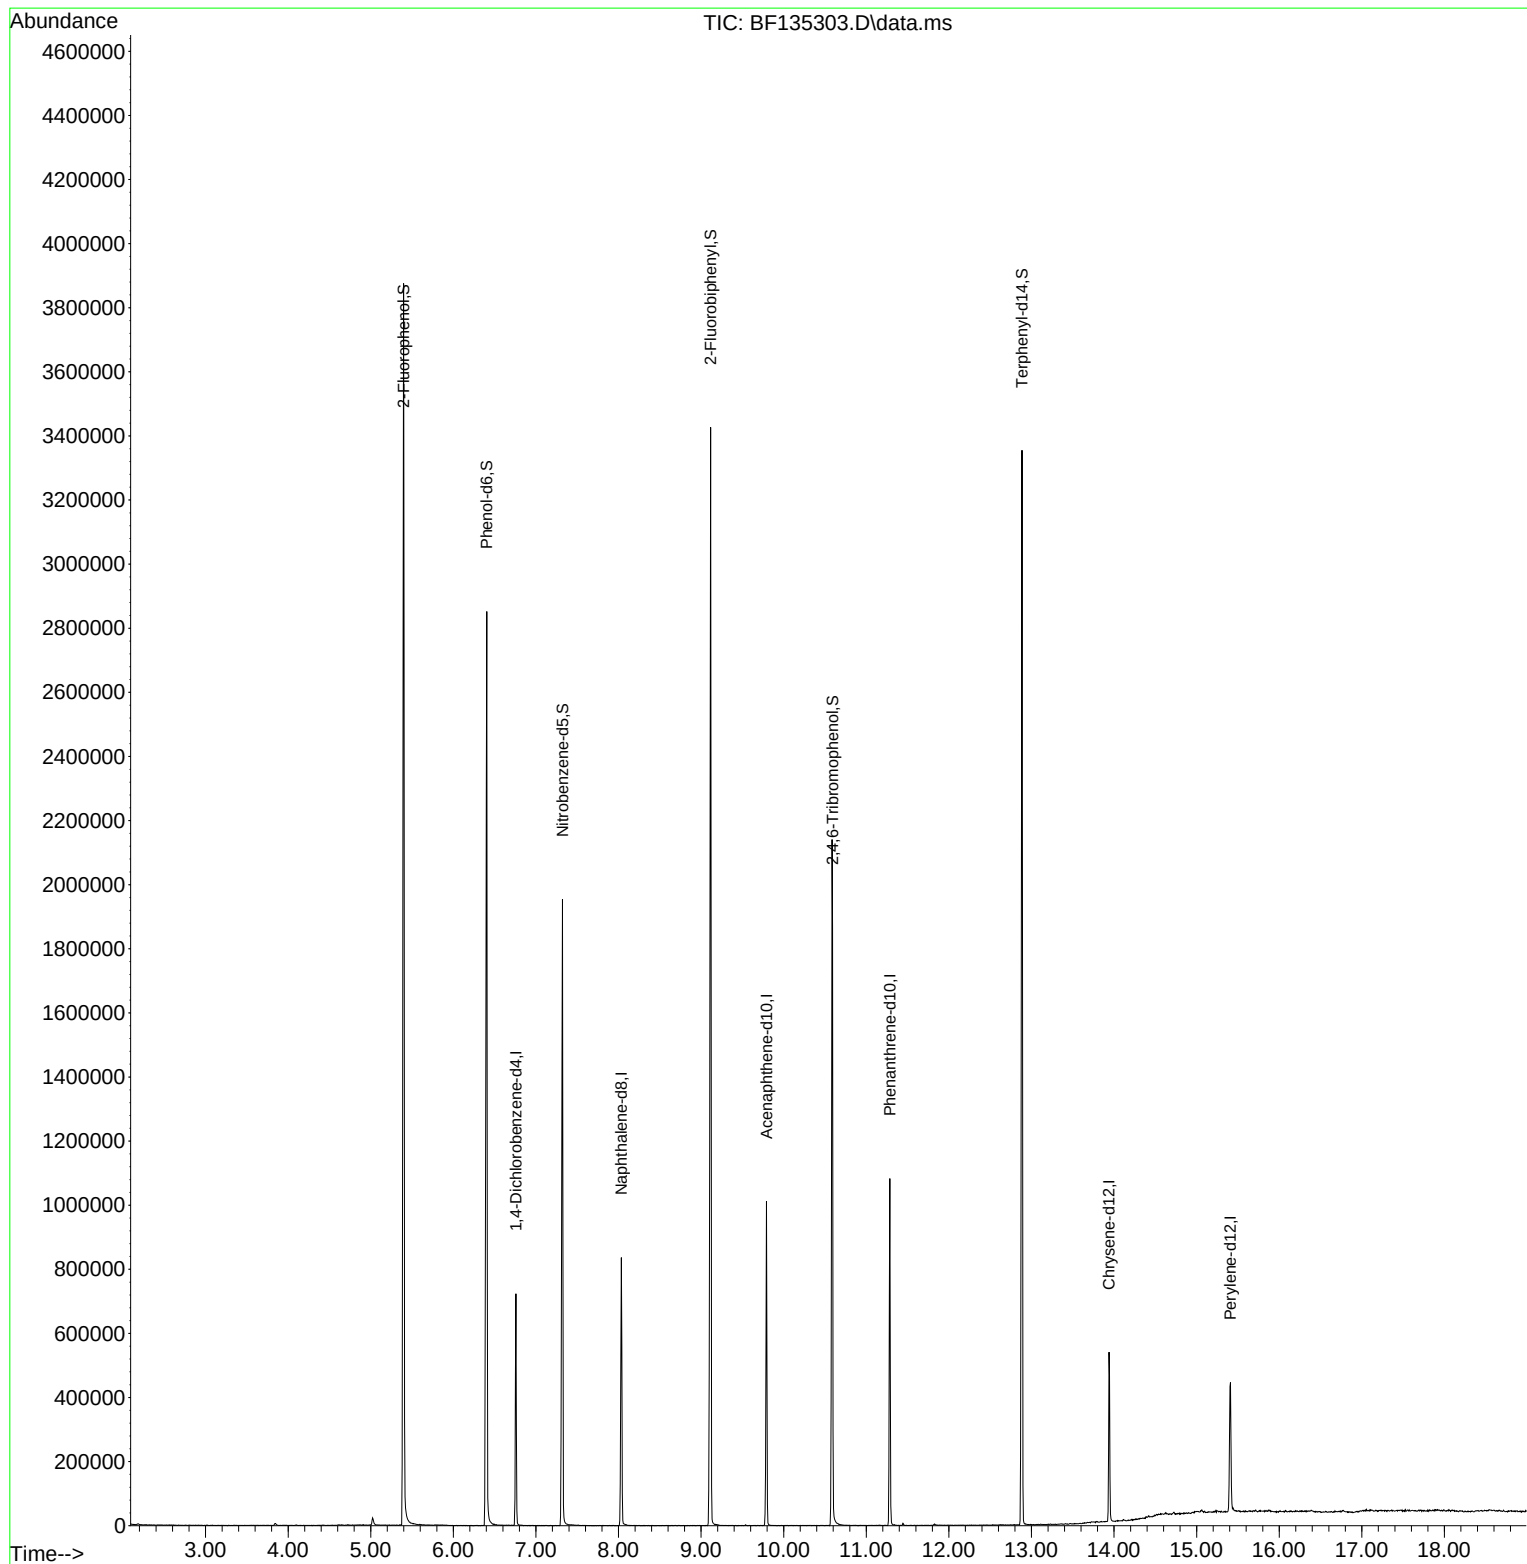


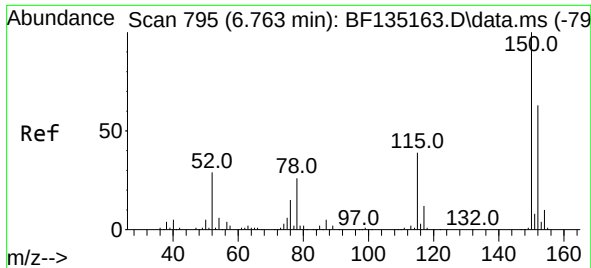

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.757 min Scan# 795
 Delta R.T. -0.006 min
 Lab File: BF135303.D
 Acq: 18 Sep 2023 13:20




Instrument :
 BNA_F
 ClientSampleId :
 PB155524BL


Tgt Ion:152 Resp: 96747
 Ion Ratio Lower Upper
 152 100
 150 157.9 127.8 191.6
 115 57.8 49.8 74.8

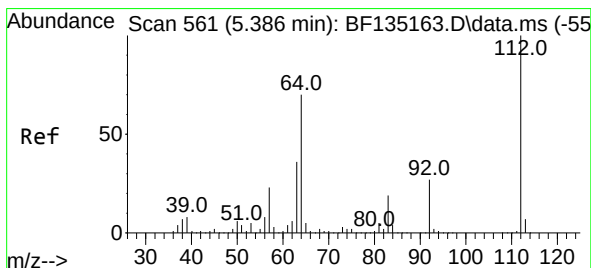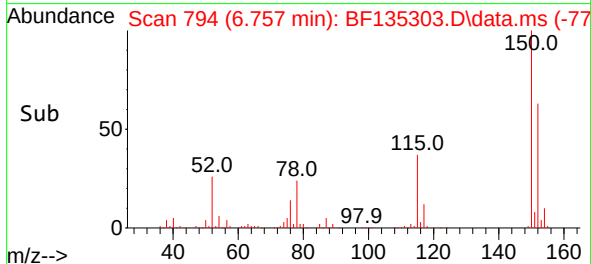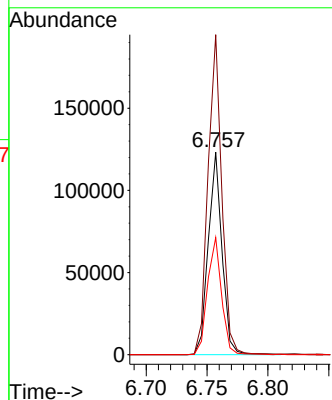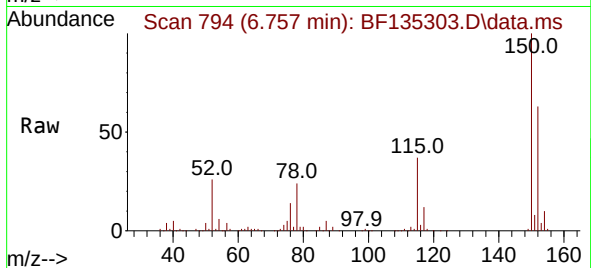

#5
 2-Fluorophenol
 Concen: 181.056 ng
 RT: 5.398 min Scan# 563
 Delta R.T. 0.012 min
 Lab File: BF135303.D
 Acq: 18 Sep 2023 13:20

Tgt Ion:112 Resp: 1076990
 Ion Ratio Lower Upper
 112 100
 64 69.4 55.9 83.9
 63 36.3 29.0 43.6


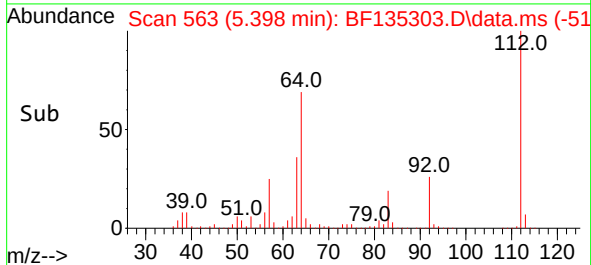
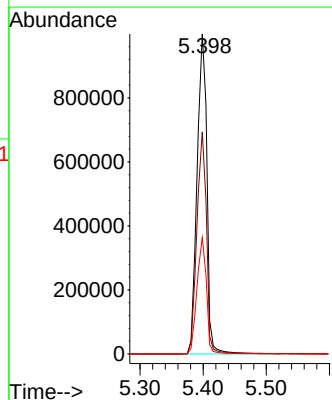
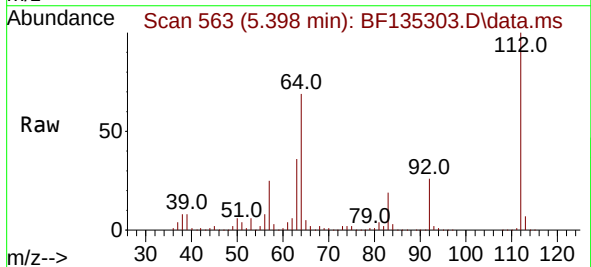


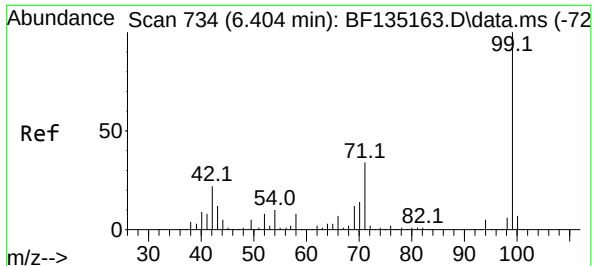

#7
Phenol-d6
Concen: 131.397 ng
RT: 6.404 min Scan# 71
Delta R.T. 0.000 min
Lab File: BF135303.D
Acq: 18 Sep 2023 13:20




Instrument :
BNA_F
ClientSampleId :
PB155524BL


Tgt Ion: 99 Resp: 993848
Ion Ratio Lower Upper
99 100
42 22.9 17.9 26.9
71 34.7 27.0 40.6

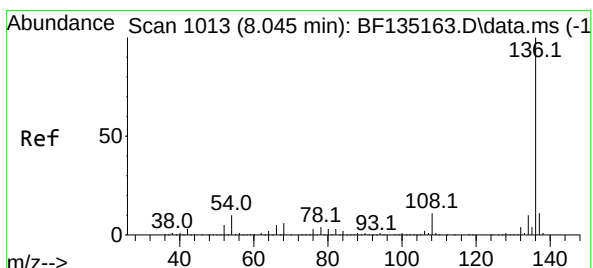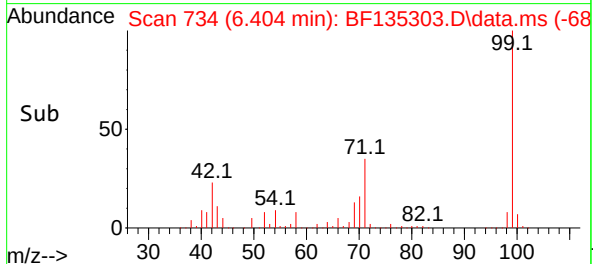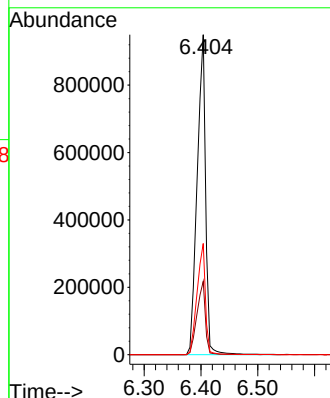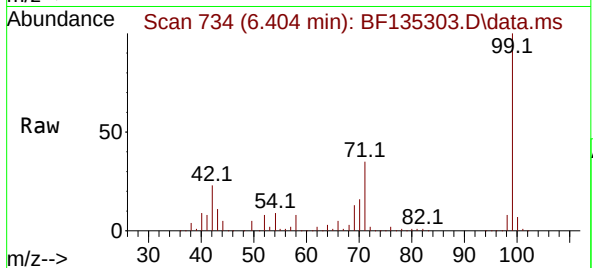

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.034 min Scan# 1011
Delta R.T. -0.012 min
Lab File: BF135303.D
Acq: 18 Sep 2023 13:20

Tgt Ion: 136 Resp: 370864
Ion Ratio Lower Upper
136 100
137 10.8 8.8 13.2
54 10.2 7.7 11.5
68 5.8 4.6 6.8

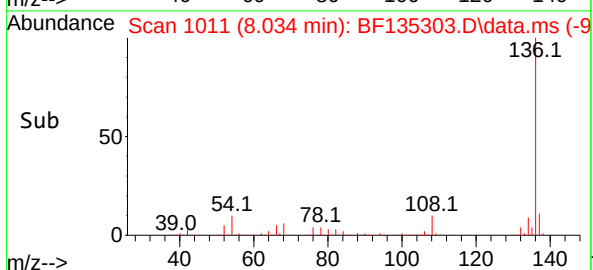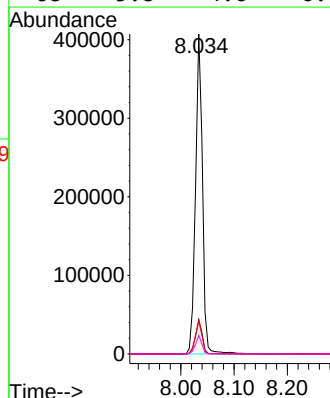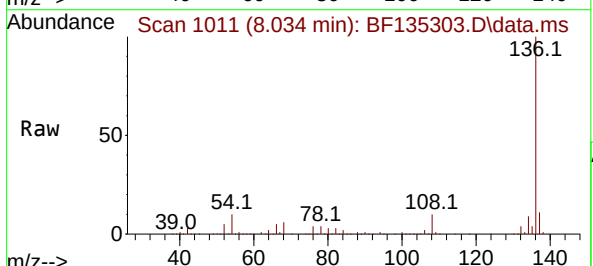

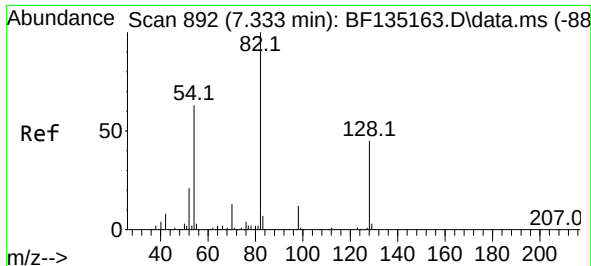

#23

Nitrobenzene-d5

Concen: 91.372 ng

RT: 7.322 min Scan# 89

Delta R.T. -0.012 min

Lab File: BF135303.D

Acq: 18 Sep 2023 13:20

Instrument :

BNA_F

ClientSampleId :

PB155524BL





Tgt Ion: 82 Resp: 623726

Ion Ratio Lower Upper

82 100

128 44.5 35.8 53.6

54 64.0 50.6 76.0

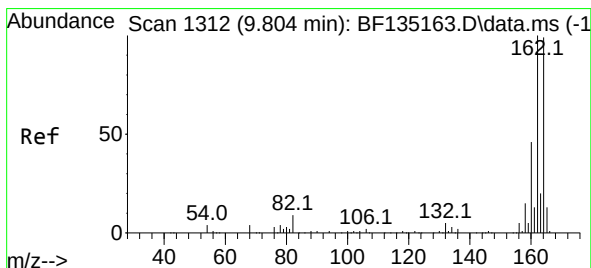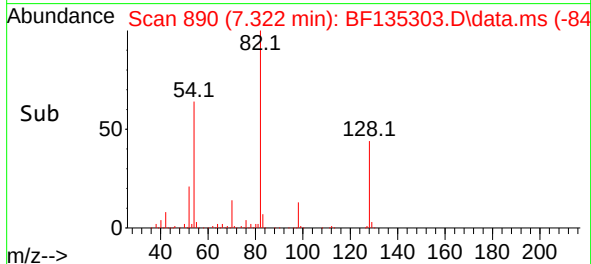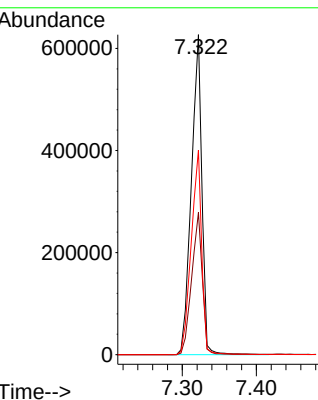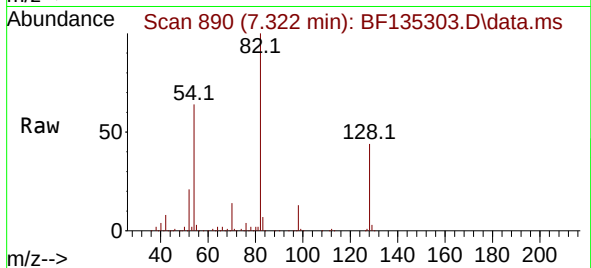

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.792 min Scan# 1310

Delta R.T. -0.012 min

Lab File: BF135303.D

Acq: 18 Sep 2023 13:20




Tgt Ion: 164 Resp: 191670


Ion Ratio Lower Upper

164 100

162 103.5 81.0 121.4

160 45.1 37.0 55.4

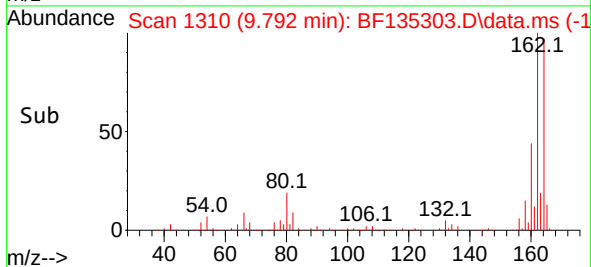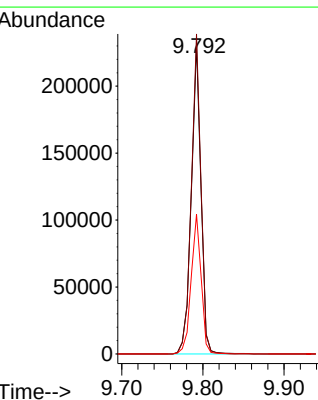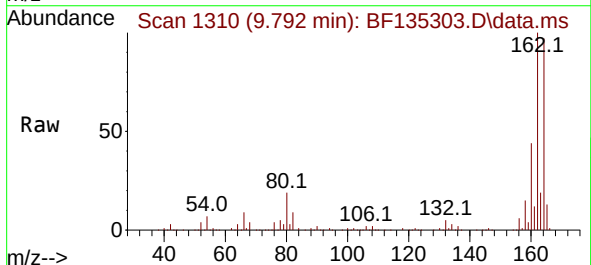

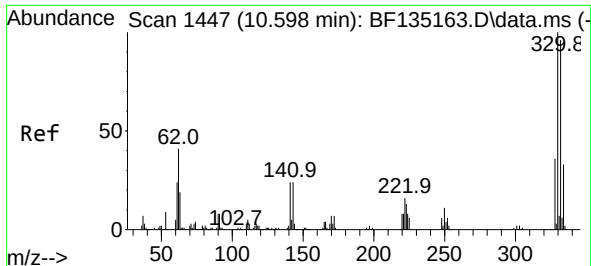

#42

2,4,6-Tribromophenol

Concen: 148.316 ng

RT: 10.592 min Scan# 1446

Delta R.T. -0.006 min

Lab File: BF135303.D

Acq: 18 Sep 2023 13:20

Instrument :

BNA_F

ClientSampleId :

PB155524BL





Tgt Ion:330 Resp: 282503

Ion Ratio Lower Upper

330 100

332 97.1 77.3 115.9

141 30.6 25.8 38.8

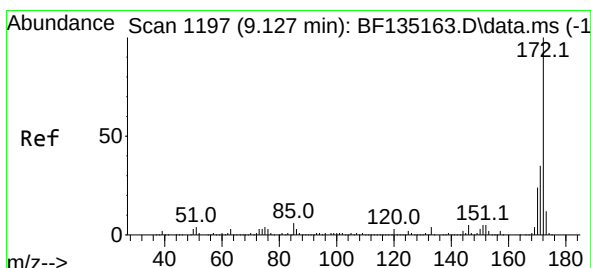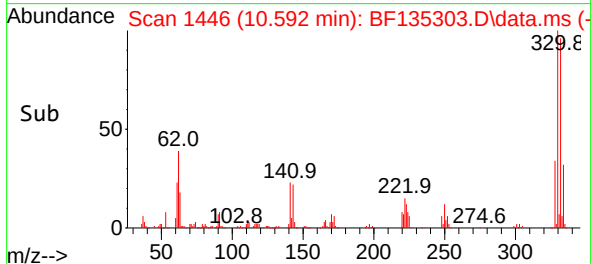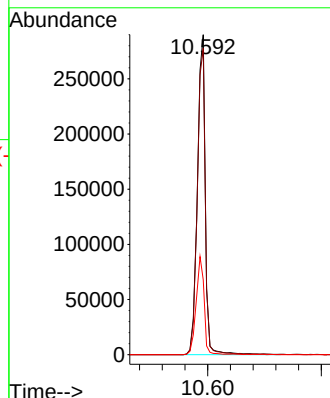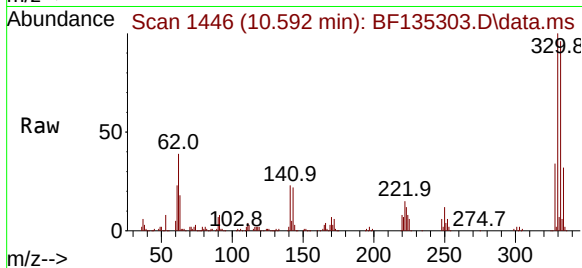

#45

2-Fluorobiphenyl

Concen: 92.063 ng

RT: 9.116 min Scan# 1195

Delta R.T. -0.012 min

Lab File: BF135303.D

Acq: 18 Sep 2023 13:20




Tgt Ion:172 Resp: 1169584


Ion Ratio Lower Upper

172 100

171 36.4 28.4 42.6

170 23.9 19.0 28.4

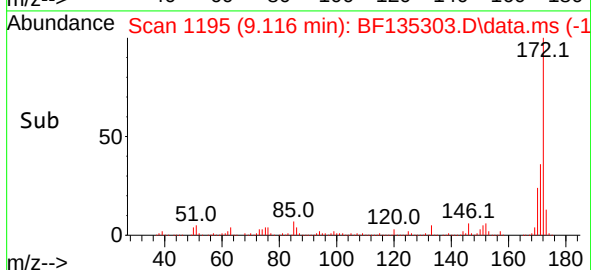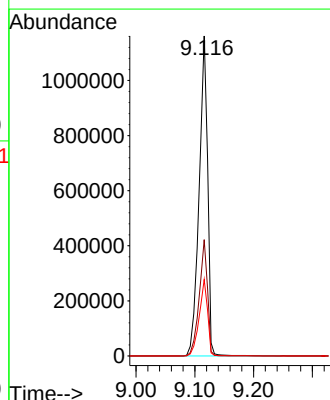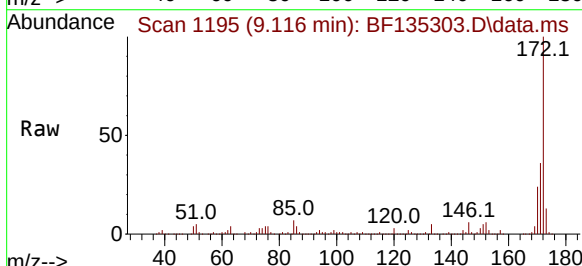

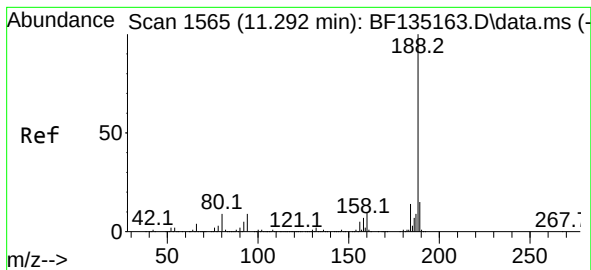

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.286 min Scan# 11

Delta R.T. -0.006 min

Lab File: BF135303.D

Acq: 18 Sep 2023 13:20

Instrument :

BNA_F

ClientSampleId :

PB155524BL





Tgt Ion:188 Resp: 377901

Ion Ratio Lower Upper

188 100

94 8.4 7.0 10.6

80 8.9 7.5 11.3

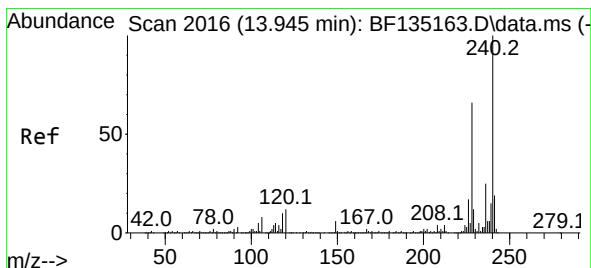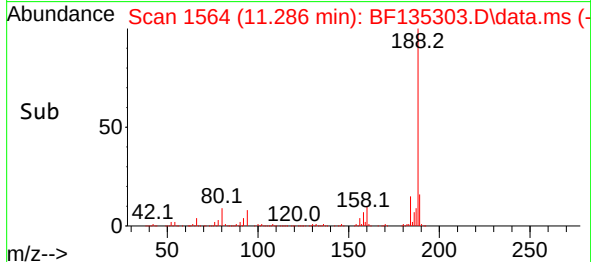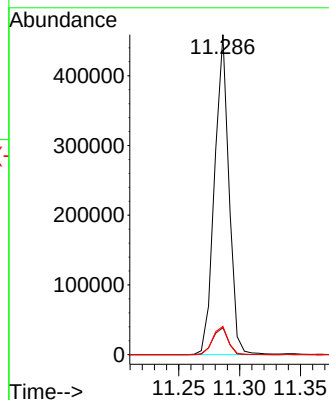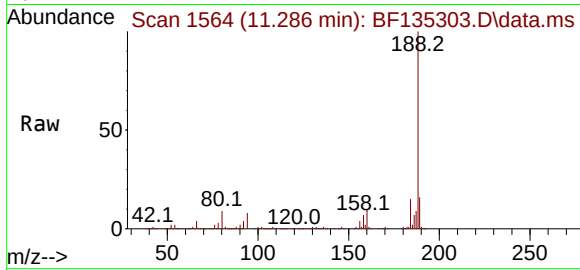

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.939 min Scan# 2015

Delta R.T. -0.006 min

Lab File: BF135303.D

Acq: 18 Sep 2023 13:20




Tgt Ion:240 Resp: 180506


Ion Ratio Lower Upper

240 100

120 10.8 9.4 14.2


236 24.9 19.8 29.8

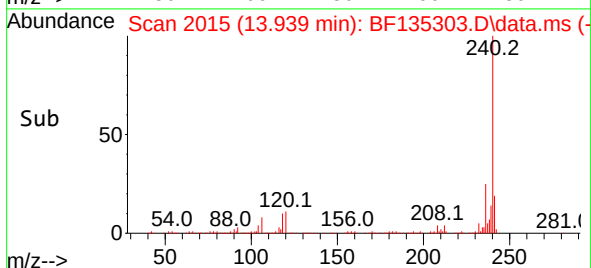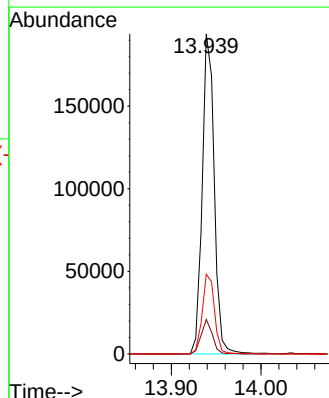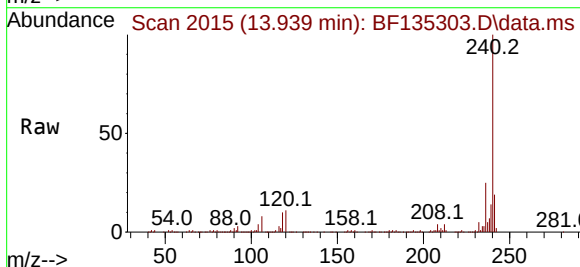



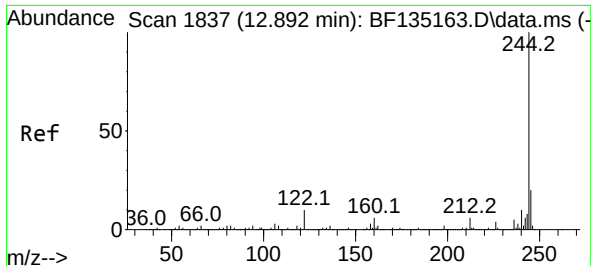


#79
 Terphenyl-d14
 Concen: 104.781 ng
 RT: 12.886 min Scan# 1836
 Delta R.T. -0.006 min
 Lab File: BF135303.D
 Acq: 18 Sep 2023 13:20

Instrument :
 BNA_F
 ClientSampleId :
 PB155524BL

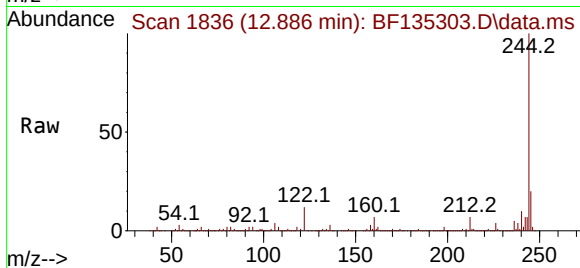

Tgt Ion:244 Resp: 1220080
 Ion Ratio Lower Upper
 244 100
 212 6.9 5.1 7.7
 122 11.7 7.9 11.9

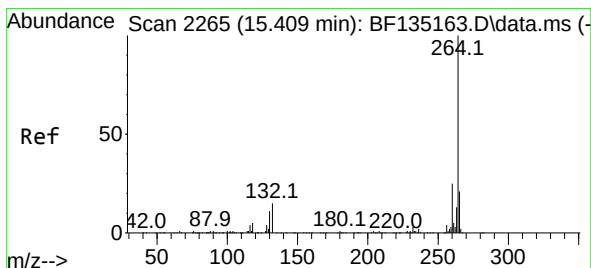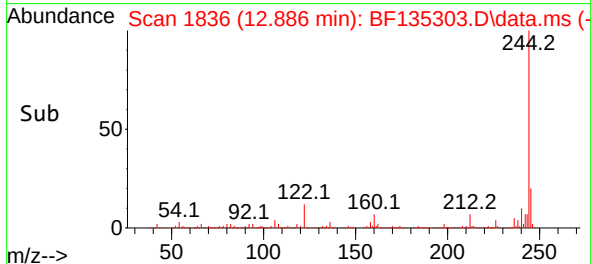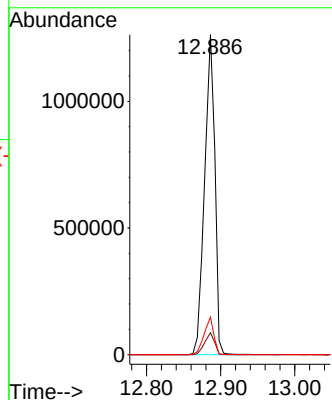

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.409 min Scan# 2265
 Delta R.T. 0.000 min
 Lab File: BF135303.D
 Acq: 18 Sep 2023 13:20

Tgt Ion:264 Resp: 204329
 Ion Ratio Lower Upper
 264 100
 260 24.3 19.8 29.6
 265 21.9 17.0 25.4

