

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091823\
 Data File : BF135303.D
 Acq On : 18 Sep 2023 13:20
 Operator : CG\JU
 Sample : PB155524BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB155524BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135303.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.398	558	563	566	rBV	3873607	3978643	100.00%	18.435%
2	6.404	729	734	737	rBV	2851165	2930040	73.64%	13.576%
3	6.757	790	794	804	rBV	722875	581412	14.61%	2.694%
4	7.322	885	890	893	rBV	1952582	1920041	48.26%	8.896%
5	8.034	1007	1011	1015	rBV	835920	745104	18.73%	3.452%
6	9.116	1189	1195	1198	rBV	3426002	3358820	84.42%	15.563%
7	9.792	1305	1310	1313	rBV	1011891	839054	21.09%	3.888%
8	10.586	1440	1445	1449	rBV	2140805	2145154	53.92%	9.939%
9	11.286	1560	1564	1567	rBV	1081379	894570	22.48%	4.145%
10	12.886	1831	1836	1839	rBV	3352324	3178219	79.88%	14.726%
11	13.939	2011	2015	2025	rBV	528703	499323	12.55%	2.314%
12	15.409	2260	2265	2269	rBV	400652	511788	12.86%	2.371%




Sum of corrected areas: 21582168

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091823\
Data File : BF135303.D
Acq On : 18 Sep 2023 13:20
Operator : CG\JU
Sample : PB155524BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155524BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

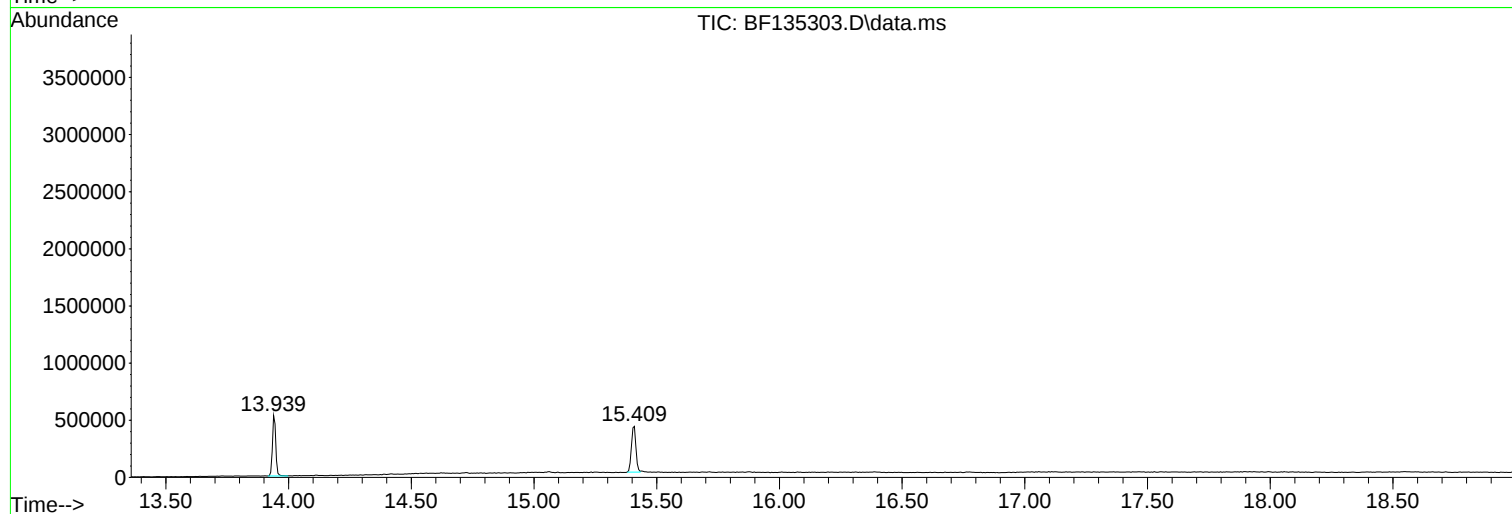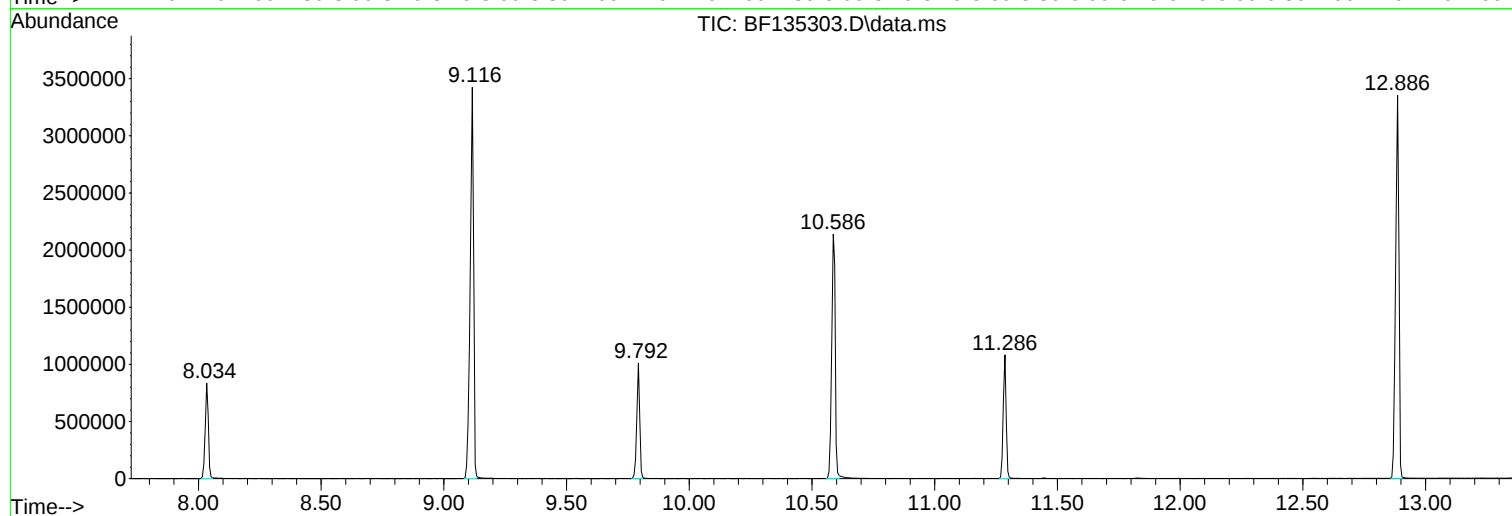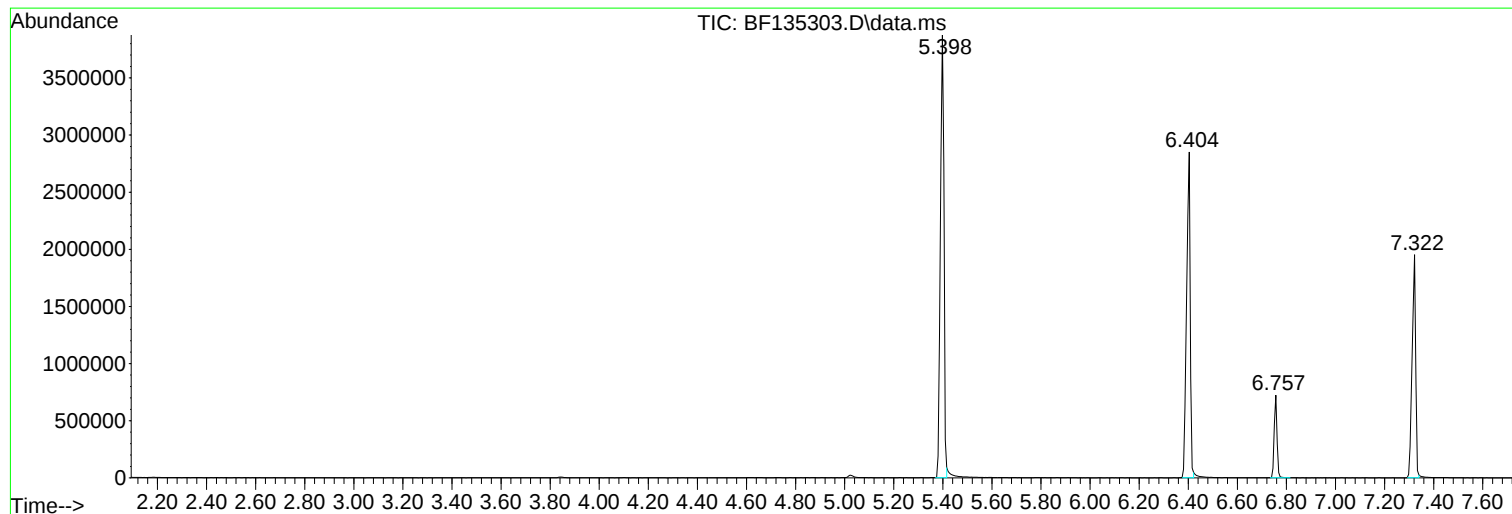

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091823\
Data File : BF135303.D
Acq On : 18 Sep 2023 13:20
Operator : CG\JU
Sample : PB155524BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155524BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091823\
Data File : BF135303.D
Acq On : 18 Sep 2023 13:20
Operator : CG\JU
Sample : PB155524BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155524BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------