

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091823\
 Data File : BF135308.D
 Acq On : 18 Sep 2023 15:59
 Operator : CG\JU
 Sample : PB155592BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB155592BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135308.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.169	9	14	22	rVB	59428	81236	1.81%	0.290%
2	5.016	492	498	507	rVB	67441	100454	2.24%	0.359%
3	5.398	558	563	566	rBV	3991923	4148163	92.50%	14.818%
4	6.404	729	734	737	rBV	3727852	4148464	92.51%	14.819%
5	6.757	790	794	802	rBV	1187581	962276	21.46%	3.437%
6	7.322	885	890	893	rBV	2684258	2795902	62.35%	9.987%
7	8.034	1007	1011	1015	rBV	1371450	1244092	27.74%	4.444%
8	9.116	1189	1195	1198	rBV	4383905	4484526	100.00%	16.019%
9	9.792	1305	1310	1314	rBV	1566833	1357050	30.26%	4.847%
10	10.586	1441	1445	1449	rBV	2367767	2426317	54.10%	8.667%
11	11.286	1560	1564	1567	rBV	1500276	1251155	27.90%	4.469%
12	12.886	1831	1836	1839	rBV	3530741	3553697	79.24%	12.694%
13	13.939	2011	2015	2025	rBV	706239	693380	15.46%	2.477%
14	15.410	2260	2265	2281	rVB	579036	748181	16.68%	2.673%




Sum of corrected areas: 27994893

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091823\
Data File : BF135308.D
Acq On : 18 Sep 2023 15:59
Operator : CG\JU
Sample : PB155592BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155592BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

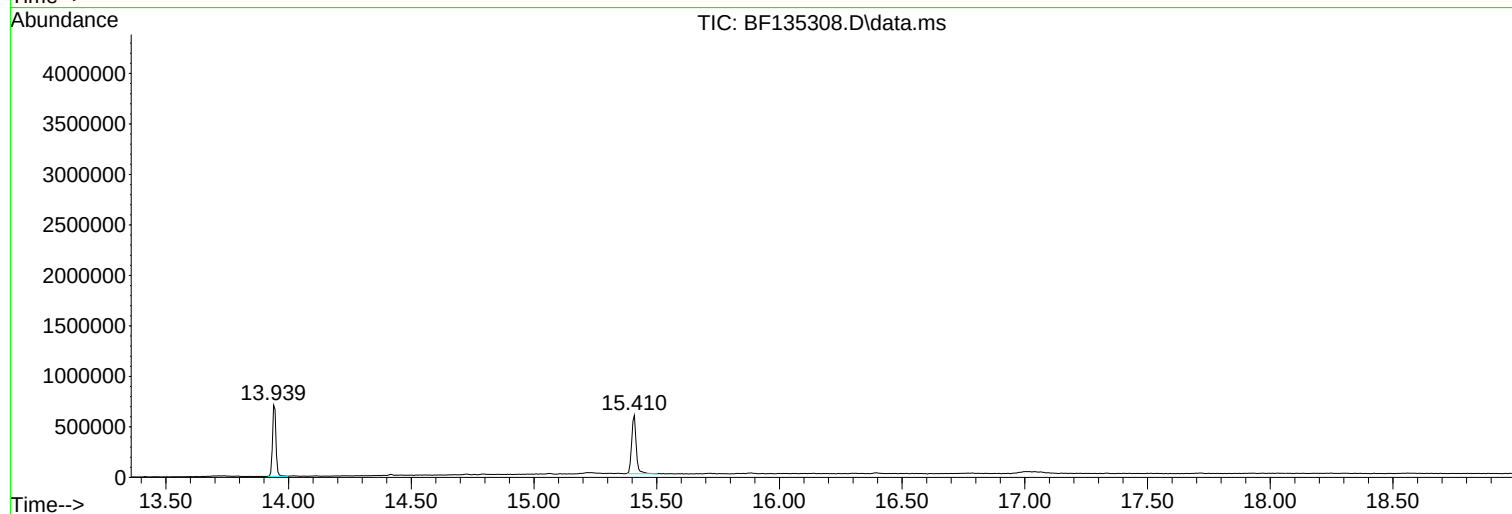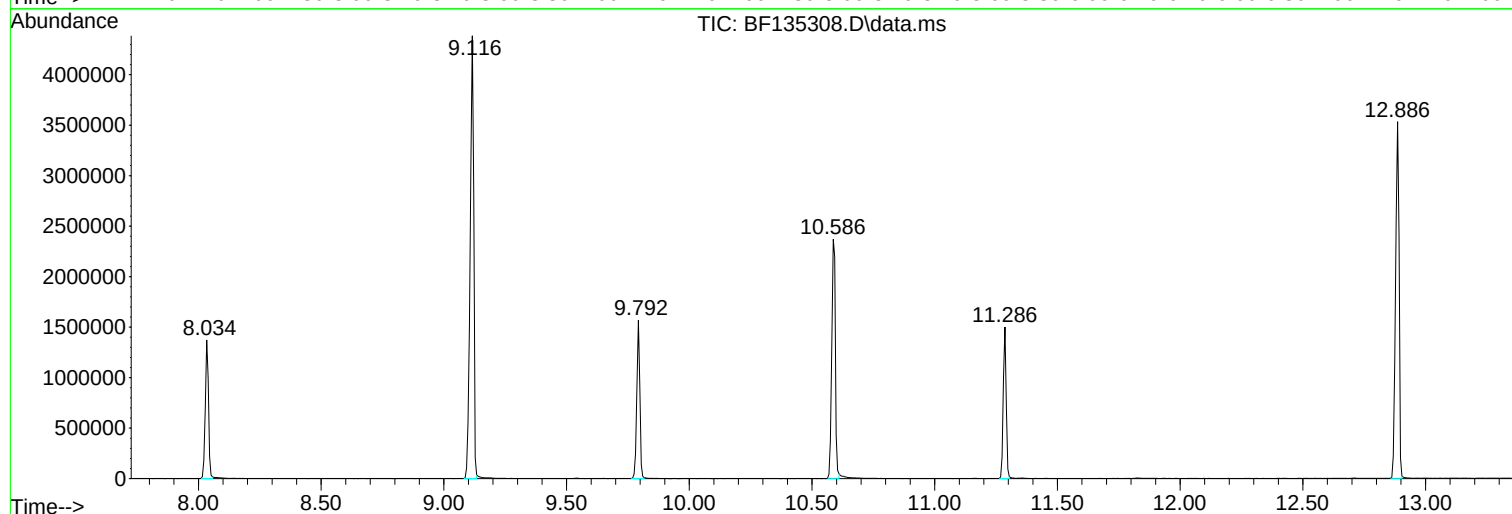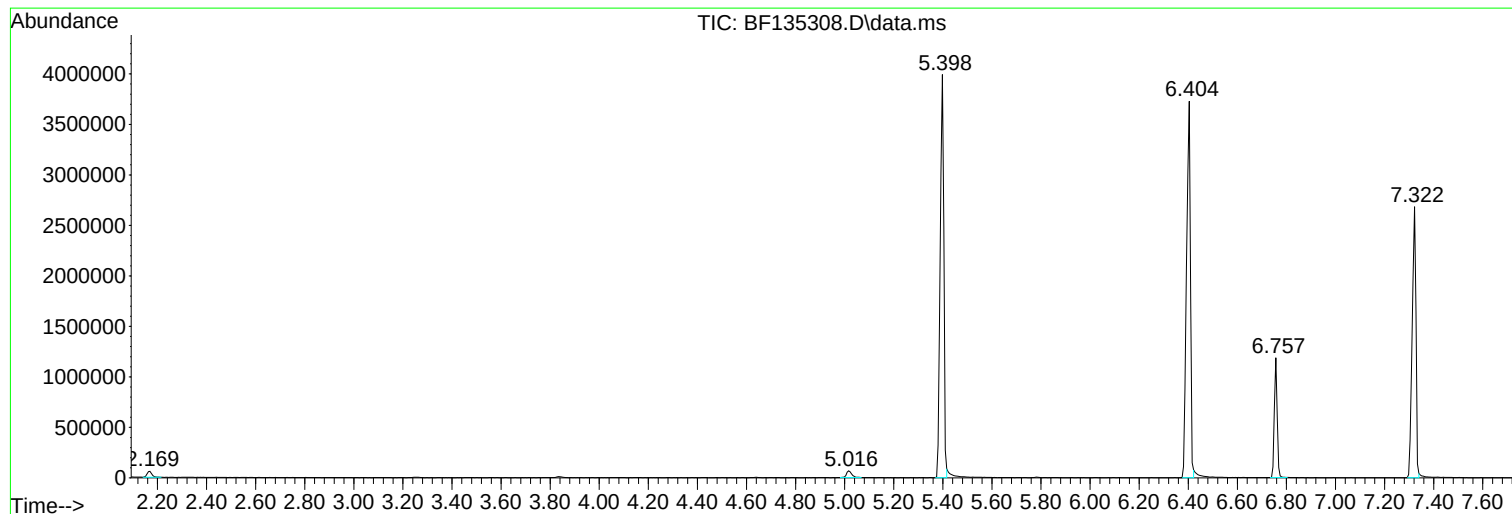

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091823\
Data File : BF135308.D
Acq On : 18 Sep 2023 15:59
Operator : CG\JU
Sample : PB155592BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155592BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.016	2.09 ng	100454	1,4-Dichlorobenzene-d4	6.757

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59		
2	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	38		
3	2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	28		
4	Butyl aldoxime, 3-methyl-, syn-	101	C5H11NO	005780-40-5	23		
5	Propane, 2-ethoxy-2-methyl-	102	C6H14O	000637-92-3	23		

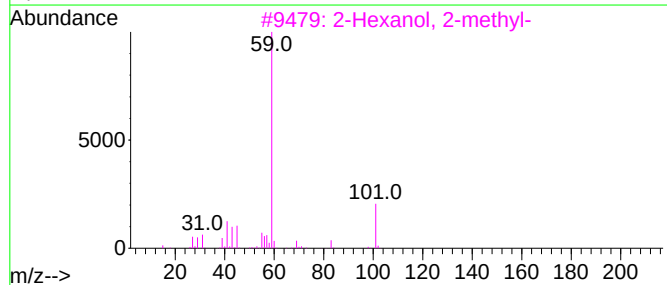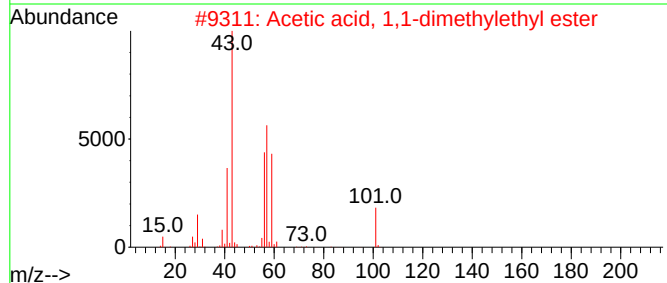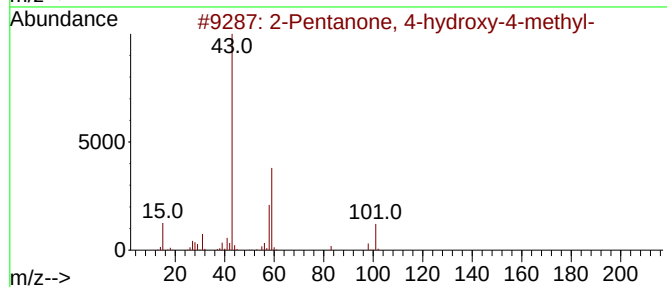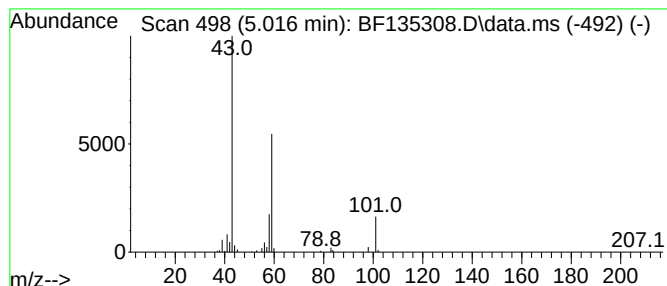

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091823\
Data File : BF135308.D
Acq On : 18 Sep 2023 15:59
Operator : CG\JU
Sample : PB155592BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155592BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.016	2.1	ng	100454	1	6.757	962276	20.0