


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091823\
Data File : BF135297.D
Acq On : 18 Sep 2023 10:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 12 00:19:07 2023

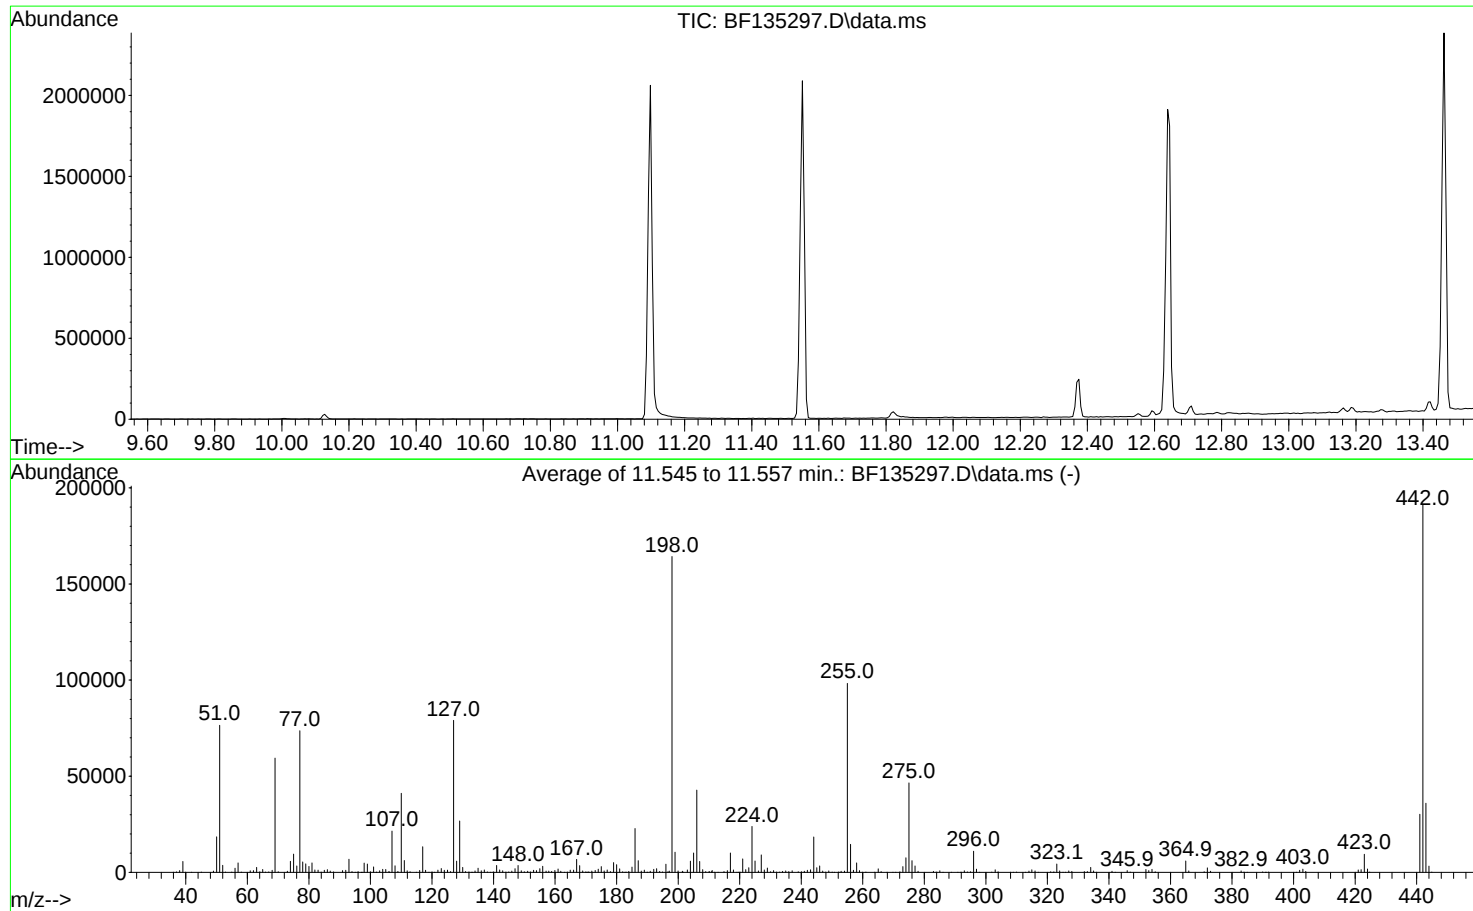




AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.6	76483	PASS
68	69	0.00	2	1.8	1059	PASS
69	198	0.00	100	36.2	59400	PASS
70	69	0.00	2	0.6	378	PASS
127	198	10	80	48.1	79043	PASS
197	198	0.00	2	0.4	654	PASS
198	198	100	100	100.0	164291	PASS
199	198	5	9	6.4	10459	PASS
275	198	10	60	28.3	46485	PASS
365	198	1	100	3.6	5922	PASS
441	198	0.01	100	18.4	30238	PASS
442	442	50	100	100.0	191328	PASS
443	442	15	24	18.8	35989	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091823\
Data File : BF135297.D
Acq On : 18 Sep 2023 10:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 19 03:02:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

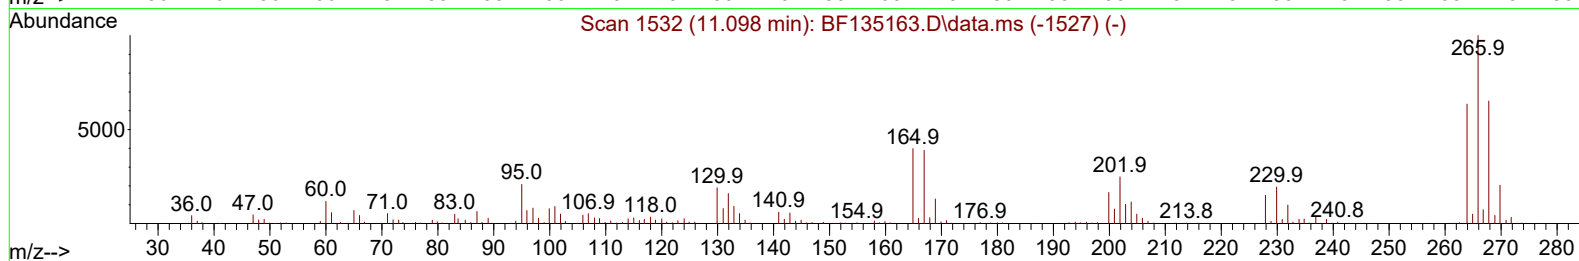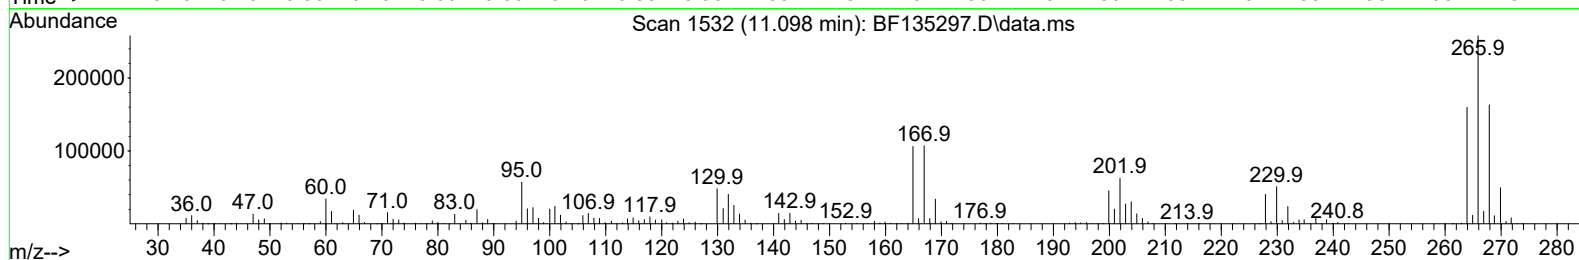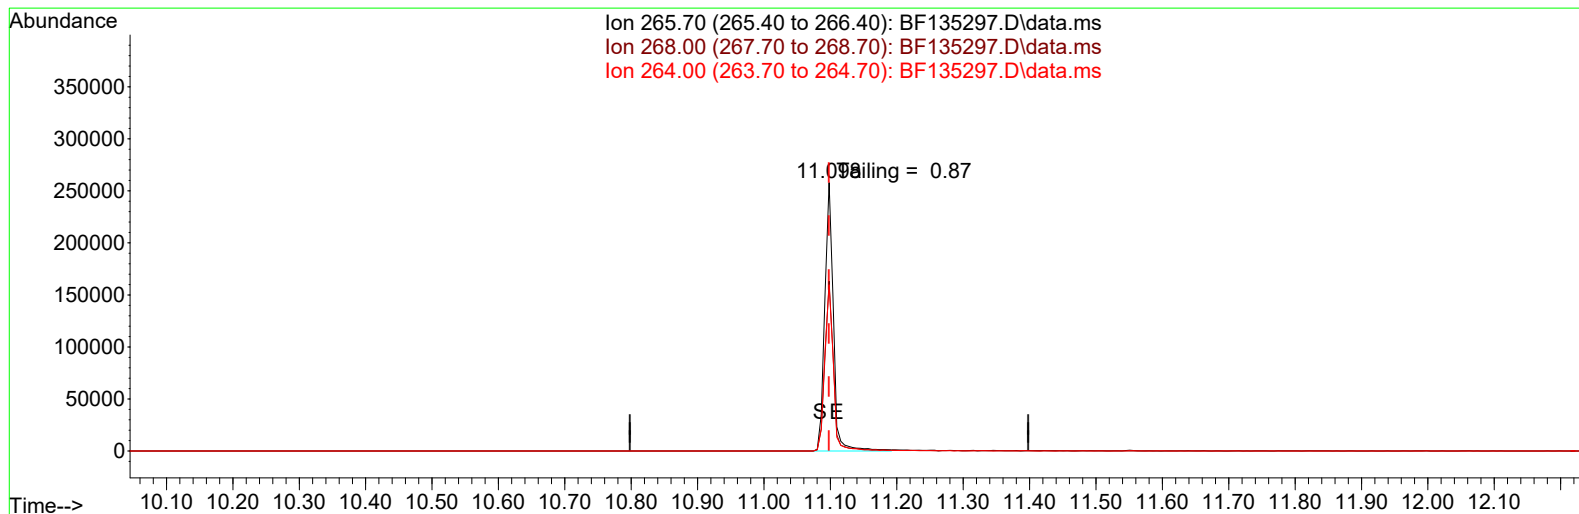

TIC: BF135297.D\data.ms

(70) Pentachlorophenol (C)

11.098min (+ 0.000) 300624.26 ng




response 235096

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	63.23
264.00	63.50	61.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091823\
Data File : BF135297.D
Acq On : 18 Sep 2023 10:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 19 03:02:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

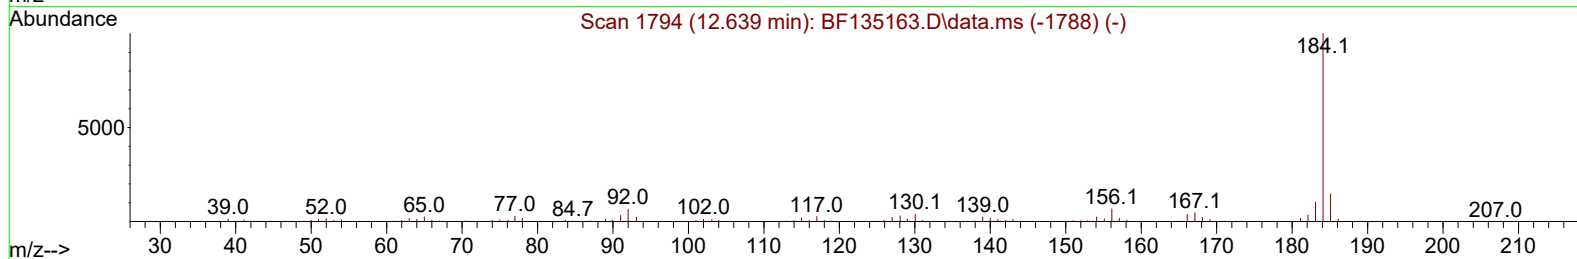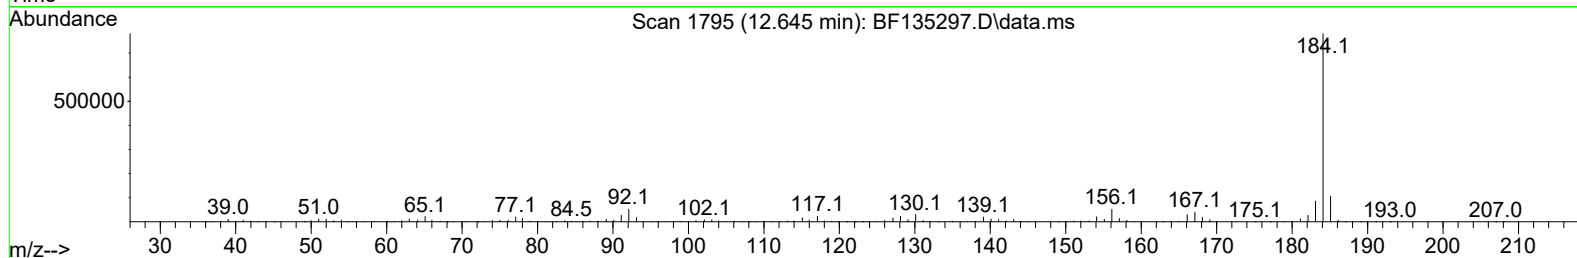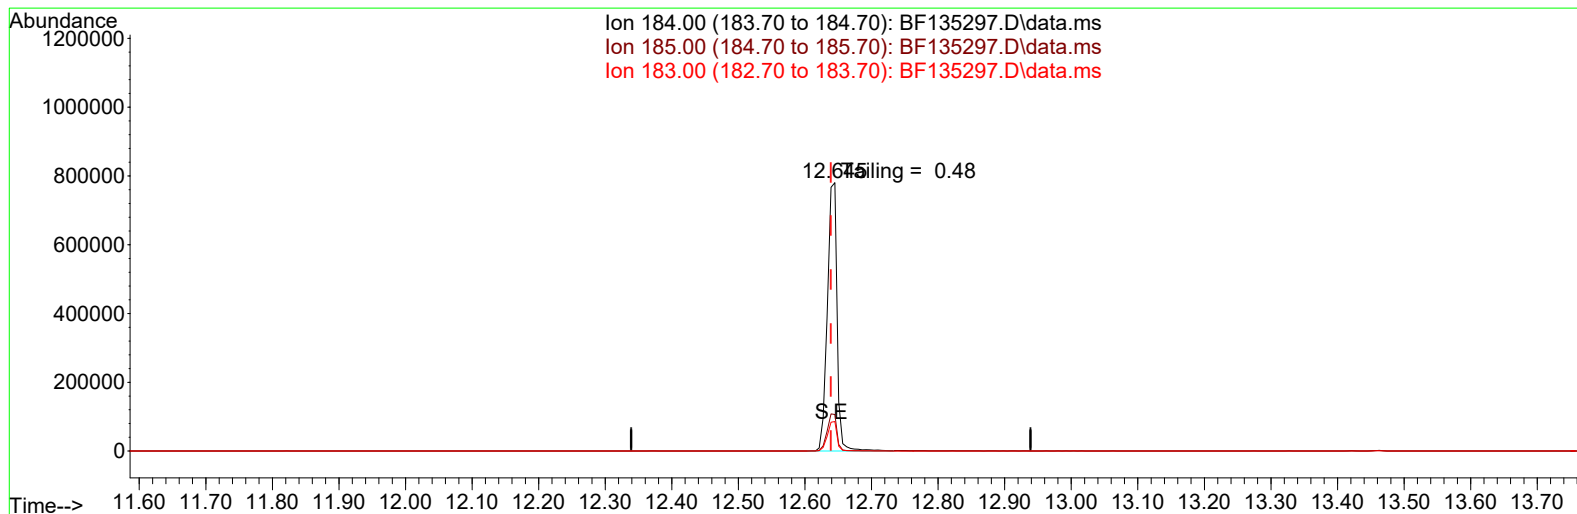

TIC: BF135297.D\data.ms

(77) Benzidine

12.645min (+ 0.006) 61581.99 ng

response 799867

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.63
183.00	10.30	11.02
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/18/2023	BNA_F	<u>BF135297.D</u>
Compound Name	Response	Retention Time
DDT	397755	13.463
DDD	10225	13.163
DDE	1021	12.821
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11246	409001	2.75

Instrument :
BNA_F
ClientSampleId :
DFTPP