
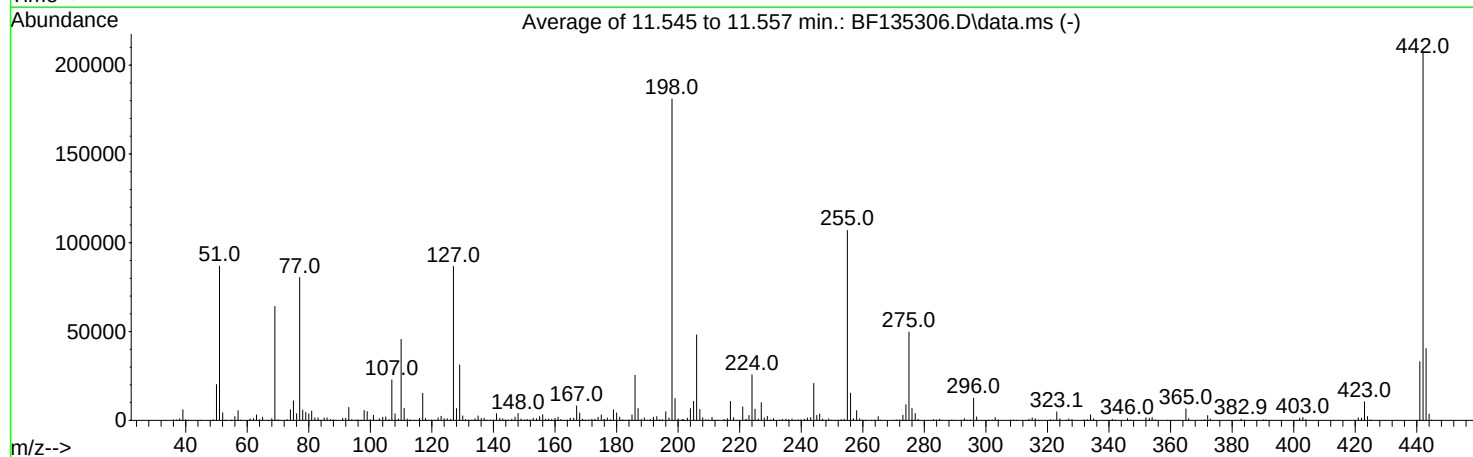


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091823\
Data File : BF135306.D
Acq On : 18 Sep 2023 14:55
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 12 00:19:07 2023

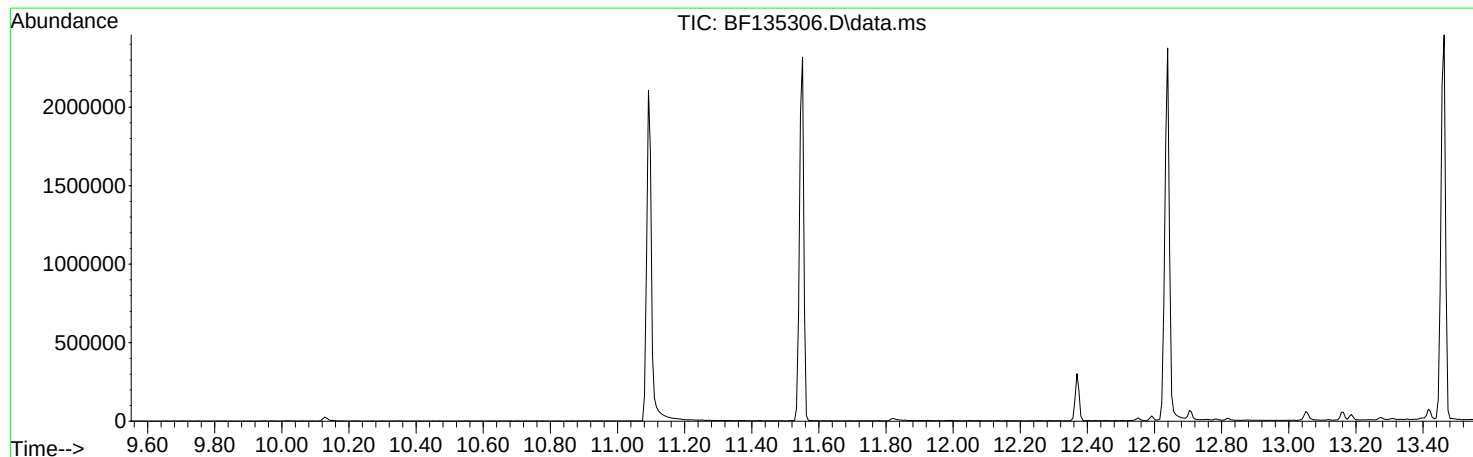




AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.0	86861	PASS
68	69	0.00	2	1.6	1002	PASS
69	198	0.00	100	35.4	64098	PASS
70	69	0.00	2	0.5	349	PASS
127	198	10	80	47.9	86656	PASS
197	198	0.00	2	0.8	1361	PASS
198	198	100	100	100.0	180869	PASS
199	198	5	9	6.8	12387	PASS
275	198	10	60	27.5	49765	PASS
365	198	1	100	3.6	6513	PASS
441	198	0.01	100	18.2	32931	PASS
442	442	50	100	100.0	207104	PASS
443	442	15	24	19.5	40421	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091823\
 Data File : BF135306.D
 Acq On : 18 Sep 2023 14:55
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 18 19:31:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 12 00:19:07 2023
 Response via : Initial Calibration

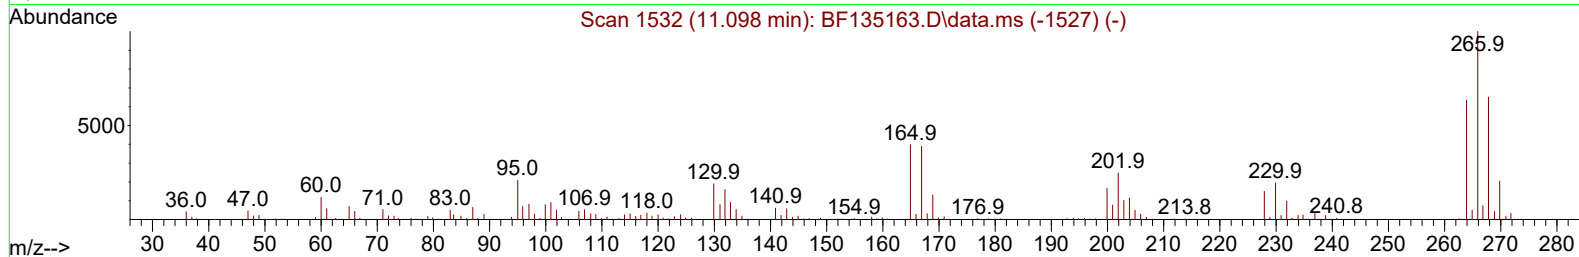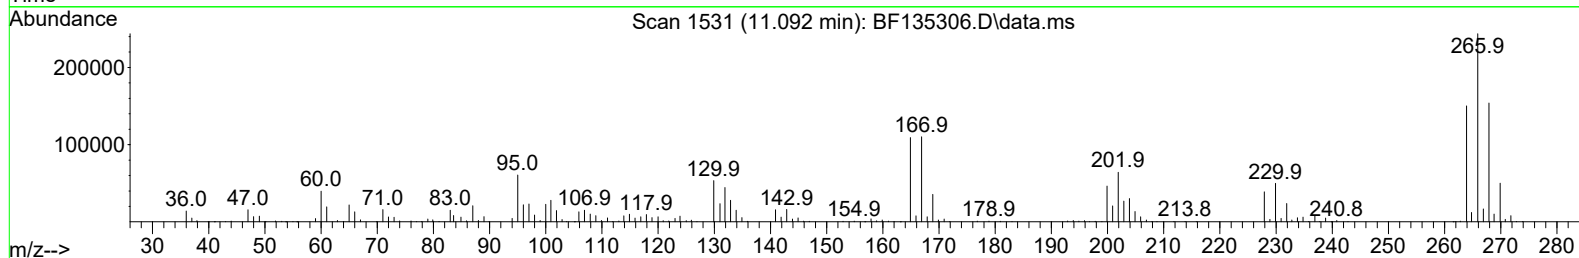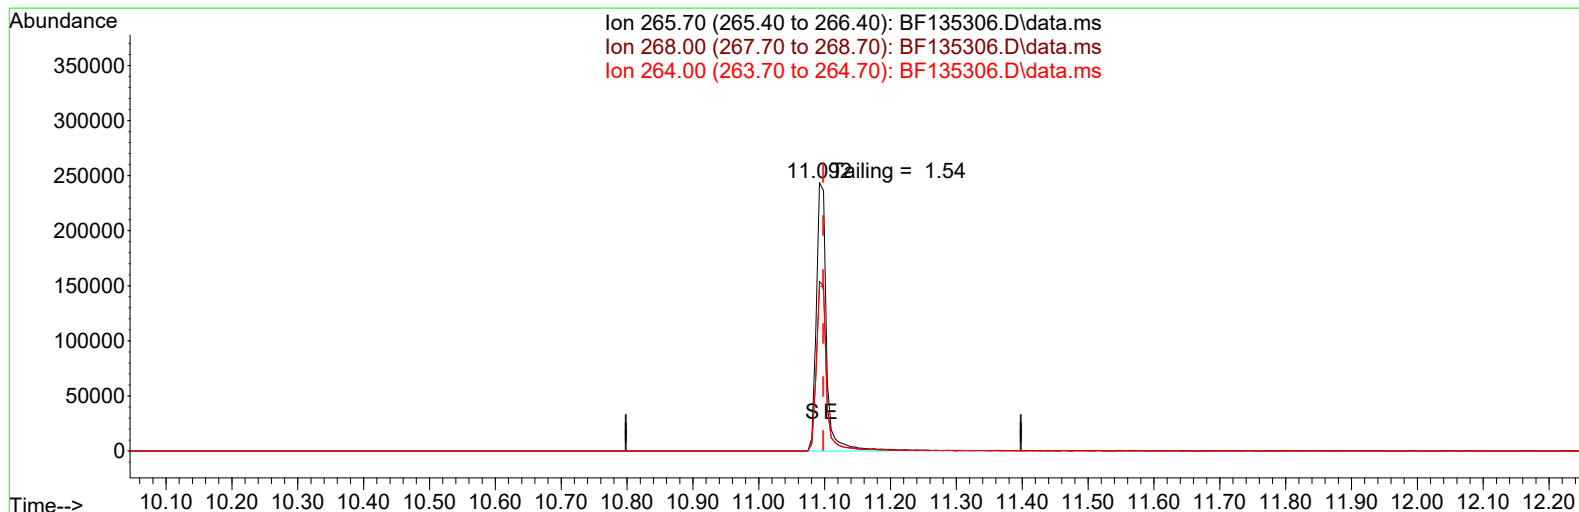

TIC: BF135306.D\data.ms

(70) Pentachlorophenol (C)

11.092min (-0.006) 236146.89 ng




response 261978

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	63.17
264.00	63.50	61.62
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091823\  
Data File : BF135306.D  
Acq On    : 18 Sep 2023  14:55  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 18 19:31:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 00:19:07 2023
Response via : Initial Calibration

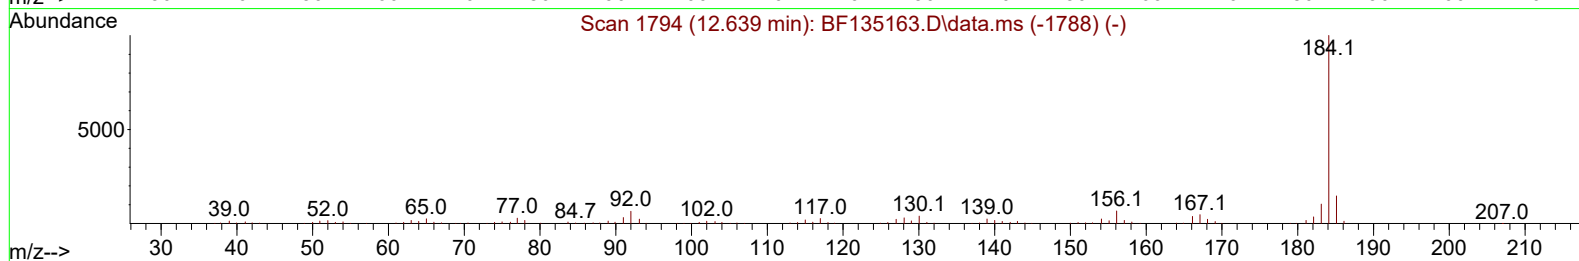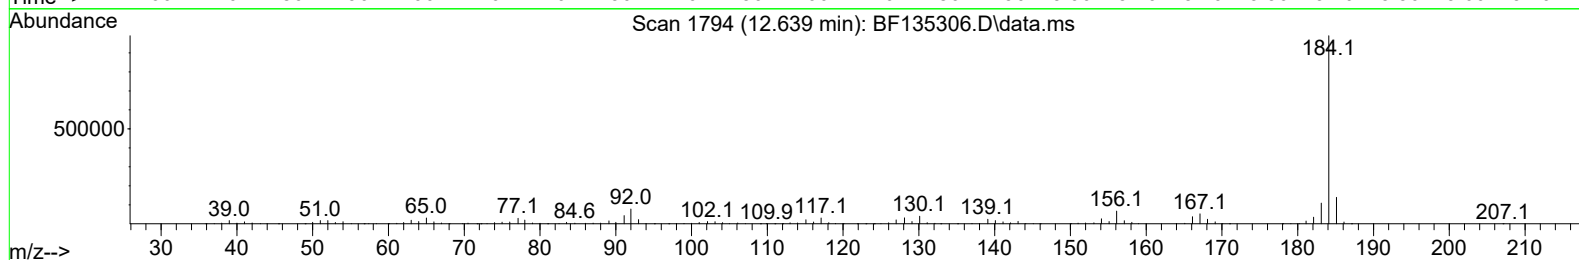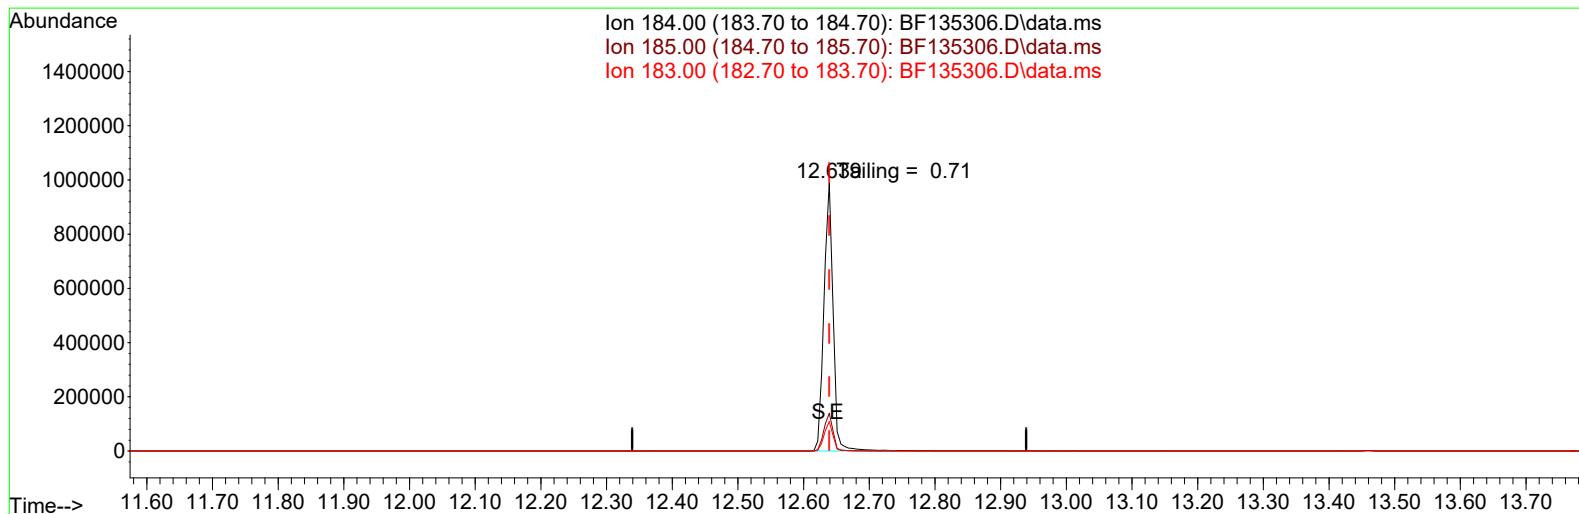

TIC: BF135306.D\data.ms

(77) Benzidine

12.639min (+ 0.000) 175132.49 ng

response **957972**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.09
183.00	10.30	11.00
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/18/2023	BNA_F	<u>BF135306.D</u>
Compound Name	Response	Retention Time
DDT	459902	13.463
DDD	16173	13.163
DDE	1759	12.822
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17932	477834	3.75

Instrument :
BNA_F
ClientSampleId :
DFTPP