


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091919\
 Data File : BF117171.D
 Acq On : 19 Sep 2019 12:35
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 13 16:23:17 2019

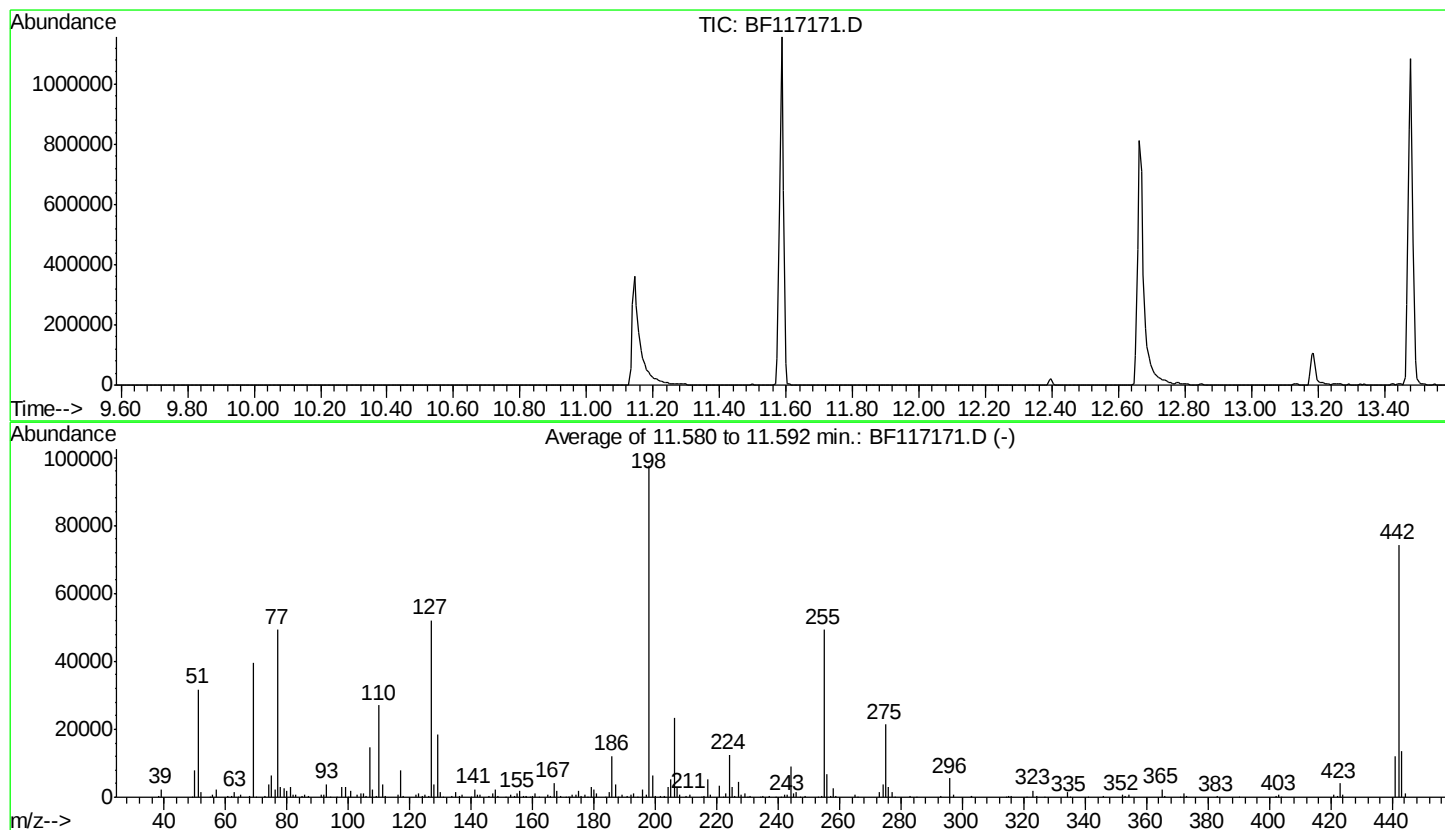

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.5	31765	PASS
68	69	0.00	2	1.4	536	PASS
69	198	0.00	100	40.5	39554	PASS
70	69	0.00	2	0.3	135	PASS
127	198	10	80	53.3	52040	PASS
197	198	0.00	2	0.9	870	PASS
198	198	100	100	100.0	97602	PASS
199	198	5	9	6.5	6323	PASS
275	198	10	60	22.0	21425	PASS
365	198	1	100	2.5	2454	PASS
441	198	0.01	100	12.4	12074	PASS
442	198	50	100	76.2	74328	PASS
443	442	15	24	18.4	13684	PASS