

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091922\
 Data File : BF130315.D
 Acq On : 19 Sep 2022 11:45
 Operator : CG\JU
 Sample : PB147728BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB147728BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130315.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.269	536	541	544	rBV	2733854	2988598	54.79%	11.082%
2	6.298	710	716	719	rBV	2659711	2933897	53.79%	10.879%
3	6.657	773	777	780	rBV	885980	689040	12.63%	2.555%
4	7.228	868	874	877	rBV	2431681	2929133	53.70%	10.862%
5	7.940	990	995	998	rBV	1051206	934862	17.14%	3.467%
6	9.022	1172	1179	1182	rBV	5647927	5454847	100.00%	20.228%
7	9.686	1287	1292	1296	rBV	1122141	1036568	19.00%	3.844%
8	10.475	1420	1426	1429	rBV	2658909	2479943	45.46%	9.196%
9	11.169	1540	1544	1547	rBV	1235502	977084	17.91%	3.623%
10	12.763	1809	1815	1818	rBV	5576591	5274301	96.69%	19.558%
11	13.798	1986	1991	1994	rBV	757157	724310	13.28%	2.686%
12	15.186	2221	2227	2232	rBV	479187	544777	9.99%	2.020%




Sum of corrected areas: 26967360

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091922\
Data File : BF130315.D
Acq On : 19 Sep 2022 11:45
Operator : CG\JU
Sample : PB147728BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147728BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

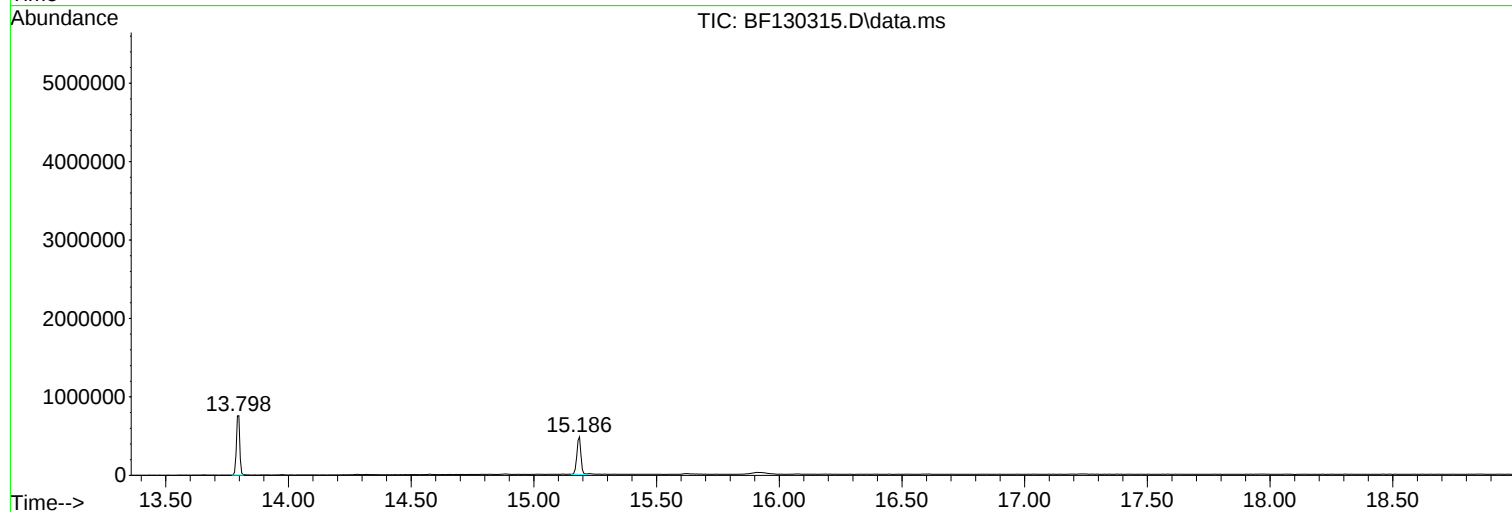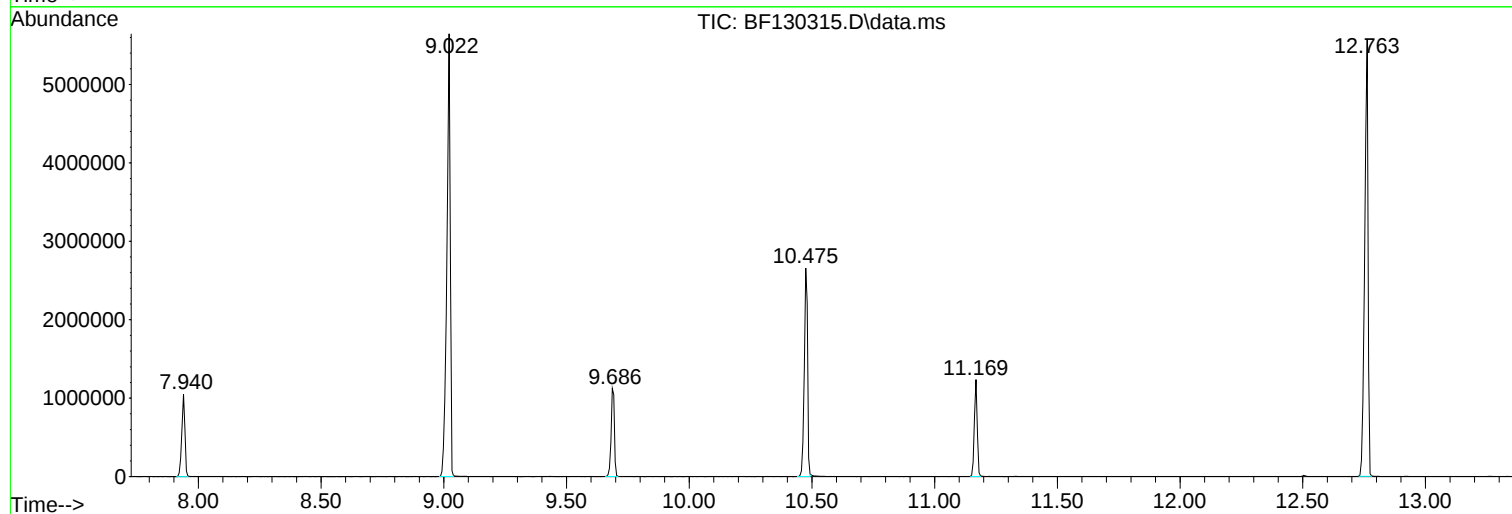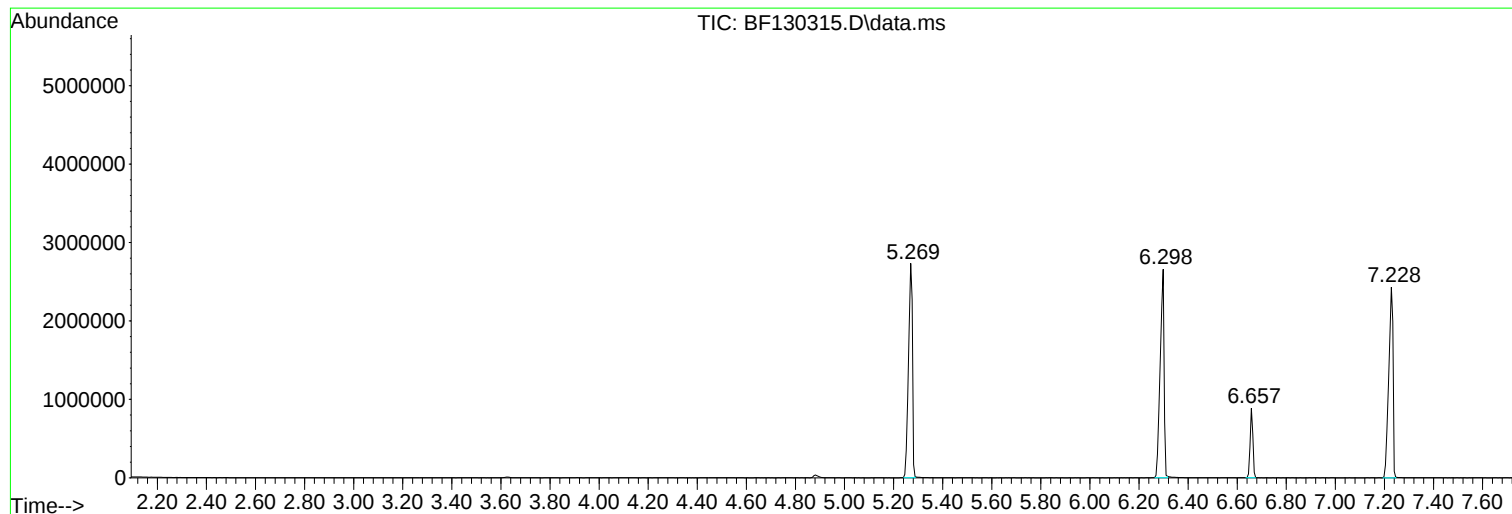

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091922\
Data File : BF130315.D
Acq On : 19 Sep 2022 11:45
Operator : CG\JU
Sample : PB147728BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147728BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091922\
Data File : BF130315.D
Acq On : 19 Sep 2022 11:45
Operator : CG\JU
Sample : PB147728BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147728BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------