


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091922\
 Data File : BF130313.D
 Acq On : 19 Sep 2022 10:41
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 19 15:06:14 2022

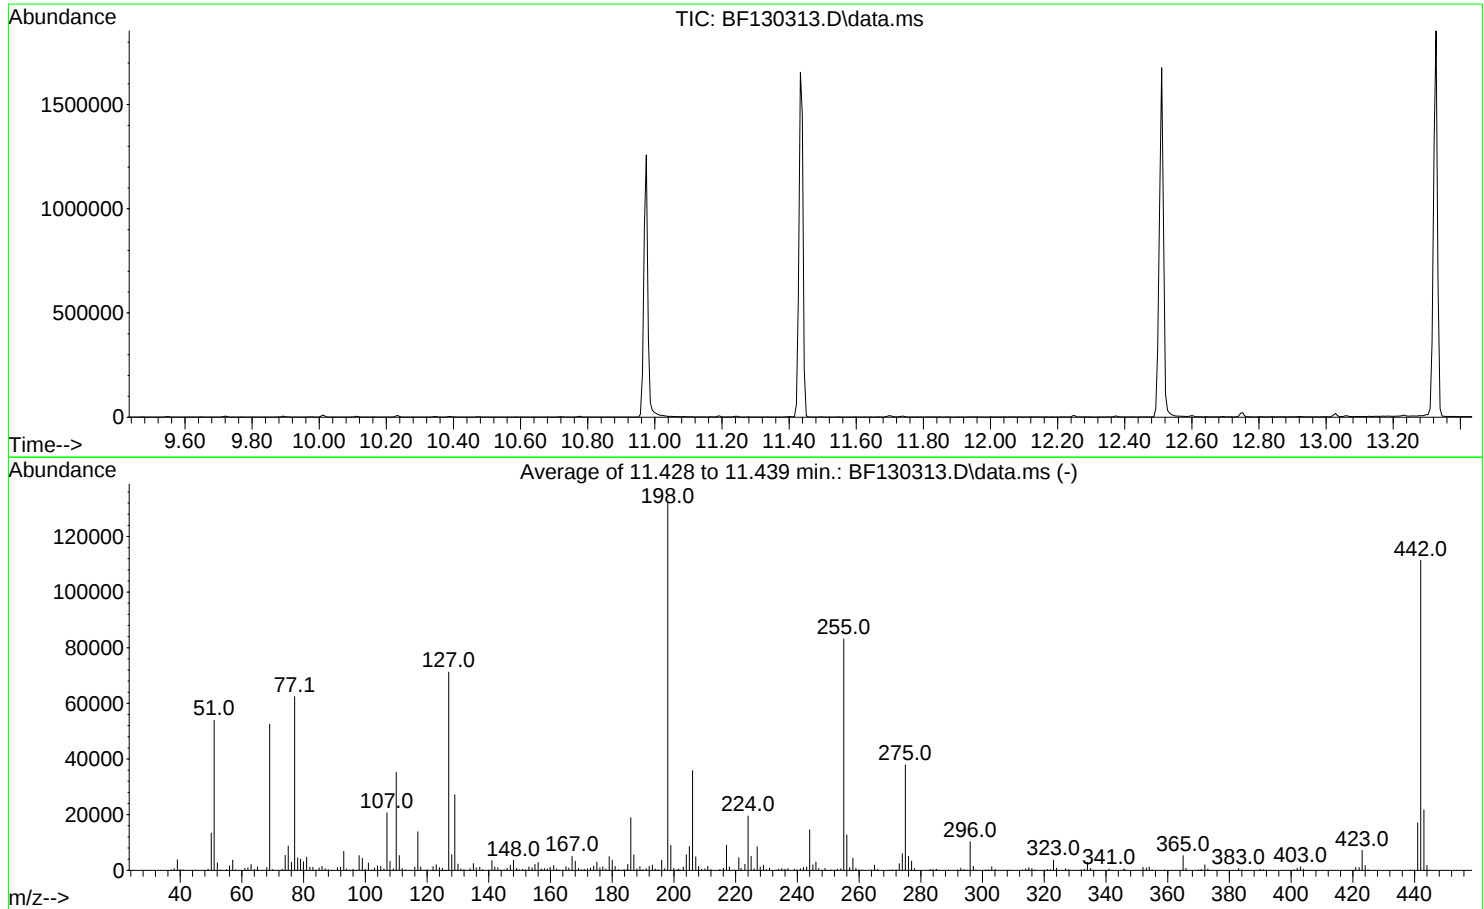




AutoFind: Scans 1588, 1589, 1590; Background Corrected with Scan 1583

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.8	53925	PASS
68	69	0.00	2	1.9	1017	PASS
69	198	0.00	100	39.7	52507	PASS
70	69	0.00	2	0.6	341	PASS
127	198	10	80	53.9	71213	PASS
197	198	0.00	2	0.4	590	PASS
198	198	100	100	100.0	132229	PASS
199	198	5	9	6.8	8941	PASS
275	198	10	60	28.6	37855	PASS
365	198	1	100	4.0	5252	PASS
441	198	0.01	100	12.9	17052	PASS
442	442	50	100	100.0	111397	PASS
443	442	15	24	19.5	21703	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091922\  
Data File : BF130313.D  
Acq On    : 19 Sep 2022  10:41  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 19 17:57:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 19 15:06:14 2022
Response via : Initial Calibration

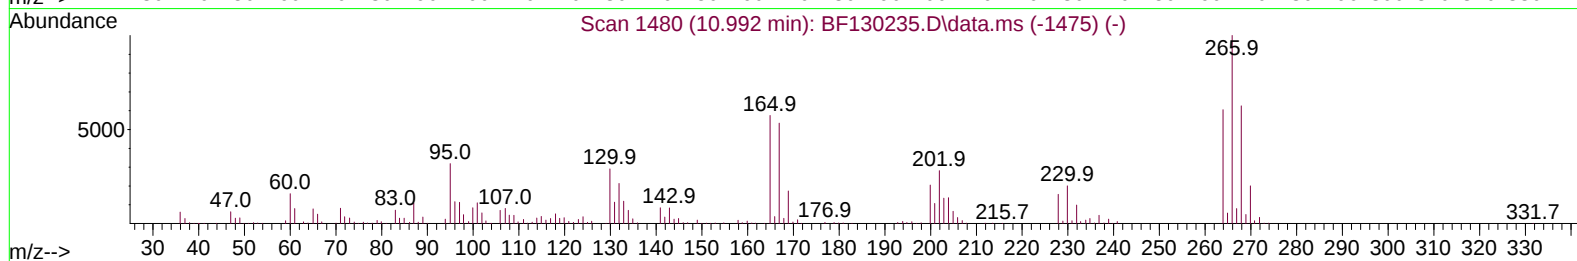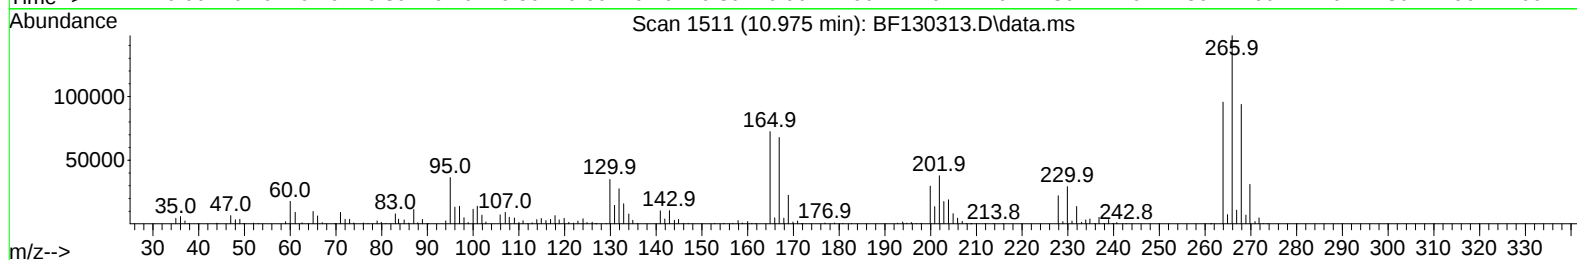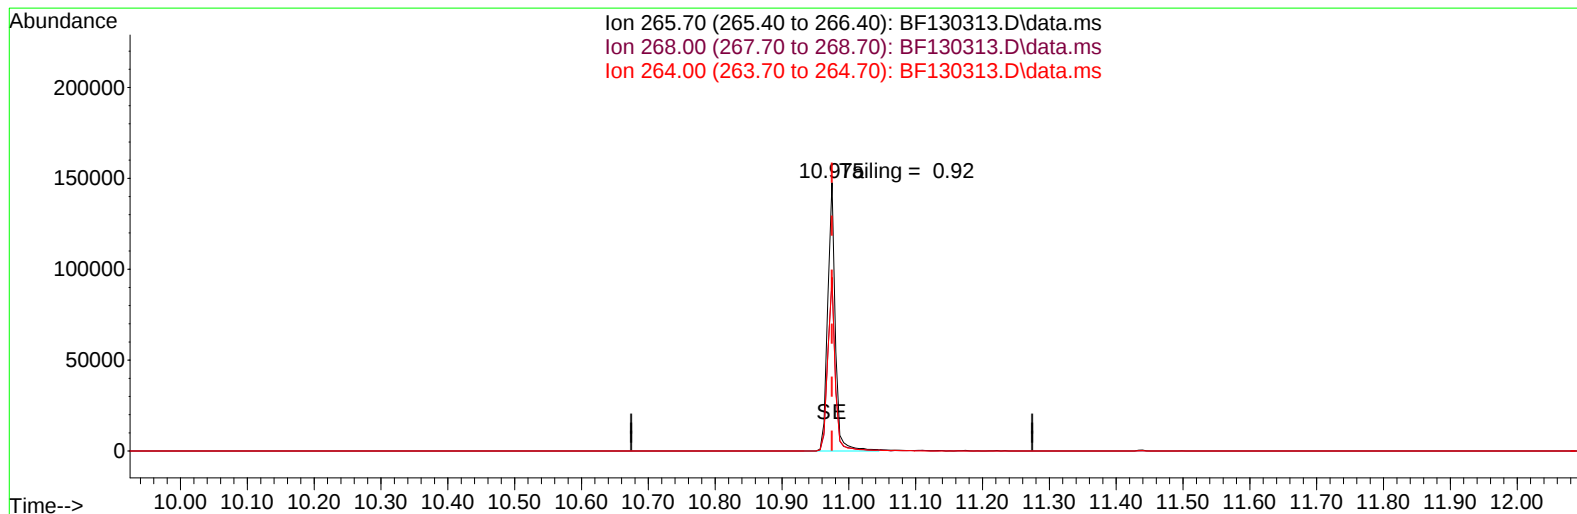

TIC: BF130313.D\data.ms

(70) Pentachlorophenol (C)

10.975min (+ 0.000) 30018.50 ng




response **118058**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.50
264.00	63.10	64.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091922\
 Data File : BF130313.D
 Acq On : 19 Sep 2022 10:41
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 19 17:57:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 19 15:06:14 2022
 Response via : Initial Calibration

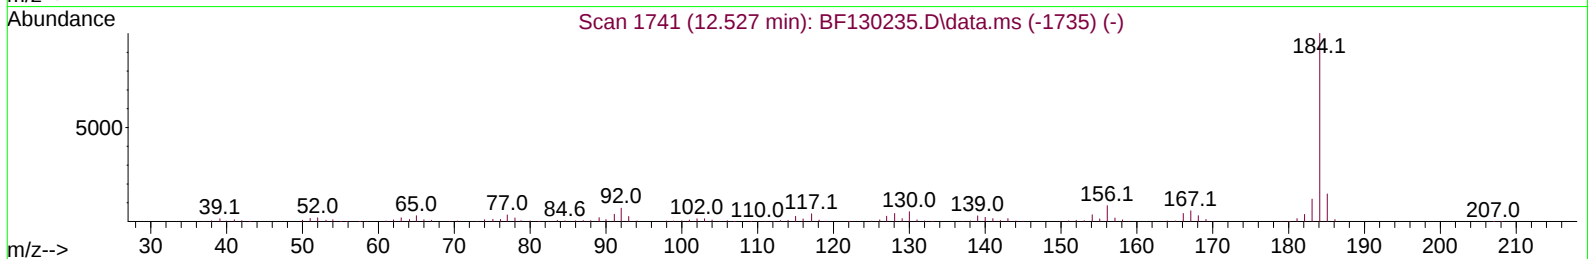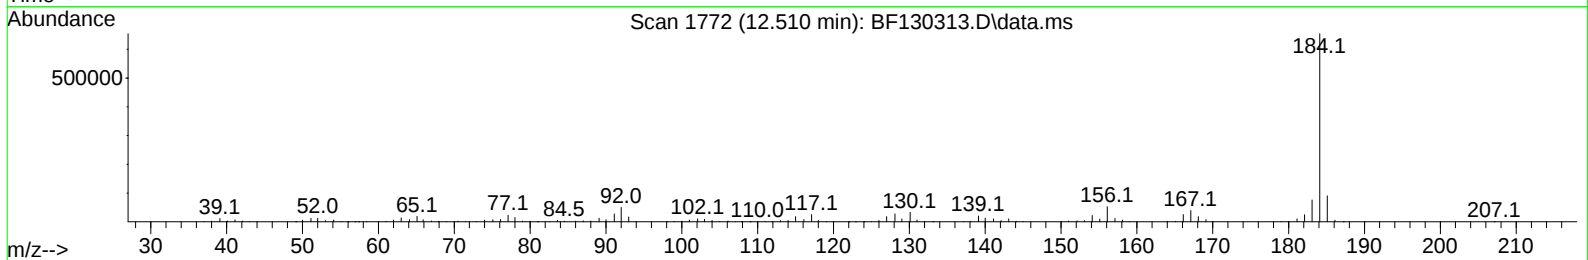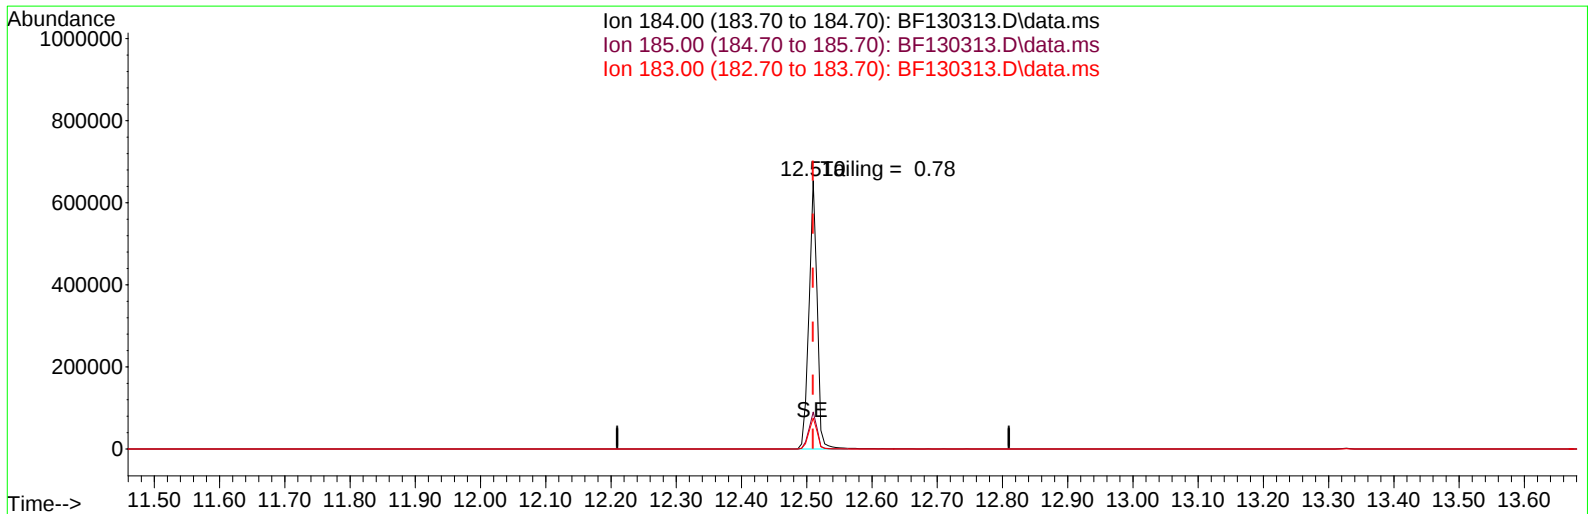

TIC: BF130313.D\data.ms

(77) Benzidine

12.510min (+ 0.000) 0.00 ng

response 572035

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.78
183.00	11.40	11.61
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/19/2022	BNA_F	<u>BF130313.D</u>
Compound Name	Response	Retention Time
DDT	277891	13.32
DDD	2739	13.02
DDE	378	12.69
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3117	281008	1.11

Instrument :
BNA_F
ClientSampleId :
DFTPP